

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042219\
 Data File : BN005206.D
 Acq On : 23 Apr 2019 10:15
 Operator : JU/SJ
 Sample : K2455-13
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GAHR3

Quant Time: Apr 23 10:52:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 23 03:50:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	266498	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	1267320	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	819972	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	1793951	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	1522354	20.00	ng/ul	0.00
85) Perylene-d12	23.43	264	1653846	20.00	ng/ul	0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	76769	13.91	ng/uL	0.00
5) Phenol-d5	6.78	99	931676	44.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	584190	44.74	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	755637	47.17	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	735165	44.93	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	364527	46.73	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	396648	50.16	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	741040	40.88	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	939886	50.28	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	2203137	37.01	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	2717201	37.17	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	336247	35.78	ng/ul	0.00
57) Fluorene-d10	15.23	176	1826558	36.56	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	121027	15.00	ng/ul	0.00
70) Anthracene-d10	17.09	188	2725180	36.24	ng/ul	0.00
78) Pyrene-d10	19.40	212	2835658	36.41	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.30	264	2671370	36.96	ng/ul	0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.70	163	474646	8.003	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042219\
Data File : BN005206.D
Acq On : 23 Apr 2019 10:15
Operator : JU/SJ
Sample : K2455-13
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GAHR3

Quant Time: Apr 23 10:52:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 03:50:45 2019
Response via : Initial Calibration

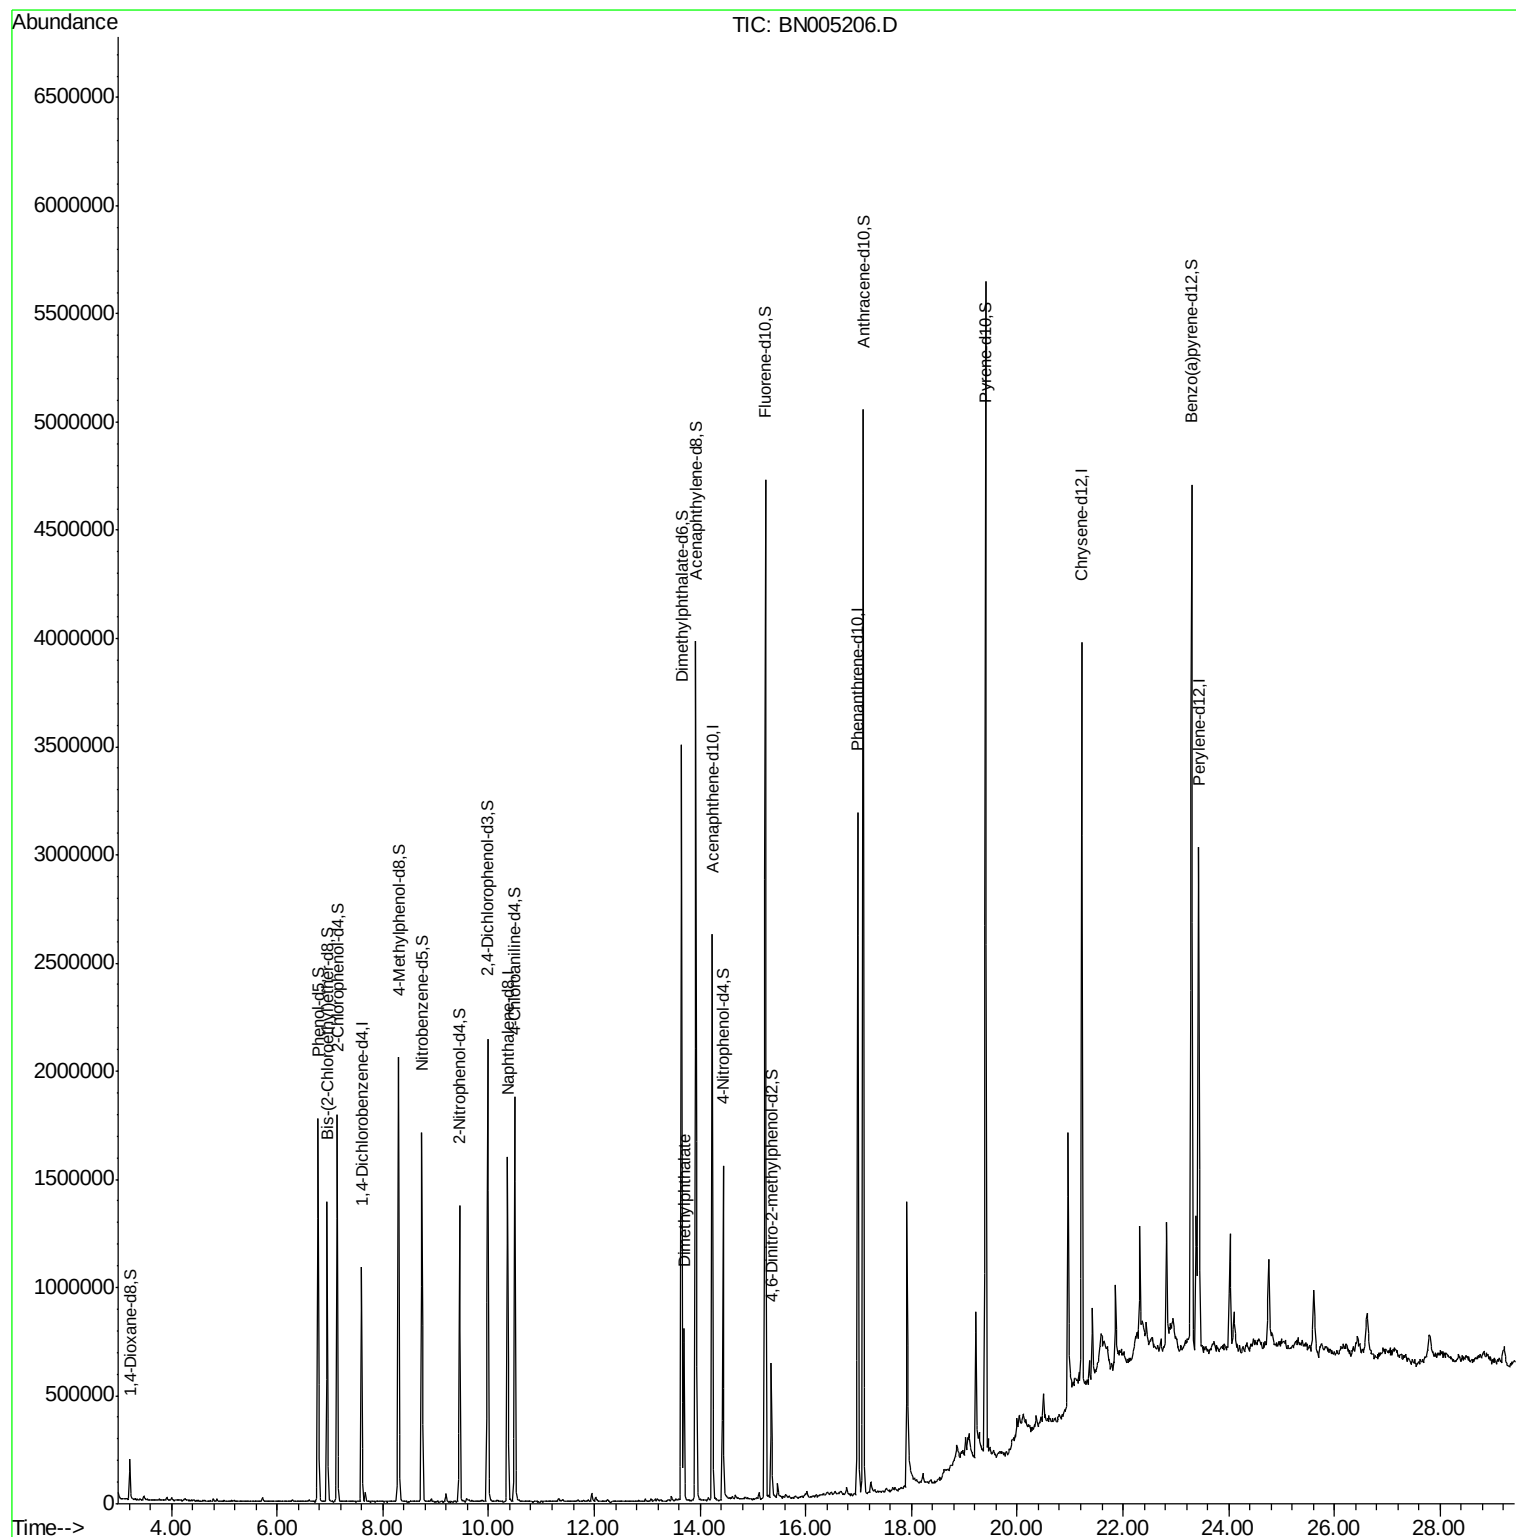

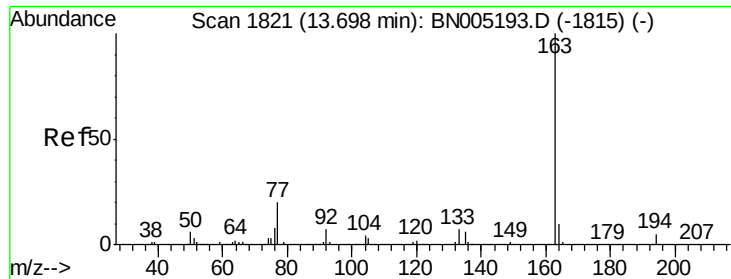

#44
 Dimethylphthalate
 Concen: 8.003 ng/ul
 RT: 13.70 min Scan# 1821
 Delta R.T. -0.01 min
 Lab File: BN005206.D
 Acq: 23 Apr 2019 10:15

Instrument :
 BNA_N
 ClientSampleId :
 GAHR3

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.6	3.4	5.0
164	10.4	8.1	12.1

