

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042221\
 Data File : BN014349.D
 Acq On : 21 Apr 2021 10:21
 Operator : CG/JU
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Quant Time: Apr 21 12:50:15 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 21 12:48:18 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.692	152	7833	0.40	ng	0.00
7) Naphthalene-d8	10.467	136	27271	0.40	ng	0.00
13) Acenaphthene-d10	14.321	164	13854	0.40	ng	0.00
19) Phenanthrene-d10	17.067	188	29978	0.40	ng	0.00
29) Chrysene-d12	21.258	240	26881	0.40	ng	0.00
36) Perylene-d12	23.486	264	26326	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.292	112	3175	0.18	ng	0.00
5) Phenol-d6	6.863	99	3830	0.18	ng	0.00
8) Nitrobenzene-d5	8.832	82	4366	0.26	ng	0.00
11) 2-Methylnaphthalene-d10	12.057	152	8018	0.19	ng	0.00
14) 2,4,6-Tribromophenol	15.818	330	797	0.16	ng	0.00
15) 2-Fluorobiphenyl	12.938	172	10665	0.20	ng	0.00
27) Fluoranthene-d10	19.101	212	14686	0.18	ng	0.00
31) Terphenyl-d14	19.707	244	11231	0.20	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.255	88	1905	0.19	ng	98
3) n-Nitrosodimethylamine	3.601	42	799	0.15	ng	# 87
6) bis(2-Chloroethyl)ether	7.120	93	3873	0.20	ng	100
9) Naphthalene	10.518	128	13317	0.19	ng	99
10) Hexachlorobutadiene	10.809	225	2943	0.22	ng	# 100
12) 2-Methylnaphthalene	12.133	142	8591	0.19	ng	99
16) Acenaphthylene	14.042	152	11134	0.21	ng	100
17) Acenaphthene	14.384	154	7465	0.19	ng	99
18) Fluorene	15.374	166	9182	0.19	ng	100
20) 4,6-Dinitro-2-methylph...	15.450	198	575	0.18	ng	# 51
21) 4-Bromophenyl-phenylether	16.264	248	3149	0.20	ng	99
22) Hexachlorobenzene	16.373	284	4404	0.22	ng	99
23) Atrazine	16.532	200	1729	0.18	ng	99
24) Pentachlorophenol	16.714	266	699	0.13	ng	99
25) Phenanthrene	17.104	178	15933	0.19	ng	100
26) Anthracene	17.201	178	11774	0.18	ng	99
28) Fluoranthene	19.131	202	16030	0.17	ng	100
30) Pyrene	19.498	202	15908	0.21	ng	100
32) Benzo(a)anthracene	21.247	228	12971	0.18	ng	99
33) Chrysene	21.300	228	16535	0.19	ng	99
34) Bis(2-ethylhexyl)phtha...	21.183	149	4924	0.24	ng	98
35) Indeno(1,2,3-cd)pyrene	25.722	276	20585	0.20	ng	99
37) Benzo(b)fluoranthene	22.863	252	18365	0.16	ng	94
38) Benzo(k)fluoranthene	22.863	252	18365	0.17	ng	95
39) Benzo(a)pyrene	23.394	252	15604	0.18	ng	# 77
40) Dibenzo(a,h)anthracene	25.739	278	16702	0.17	ng	97
41) Benzo(g,h,i)perylene	26.406	276	17202	0.16	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042221\
 Data File : BN014349.D
 Acq On : 21 Apr 2021 10:21
 Operator : CG/JU
 Sample : SSTDIC0.2
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDIC0.2

Quant Time: Apr 21 12:50:15 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 21 12:48:18 2021
 Response via : Initial Calibration




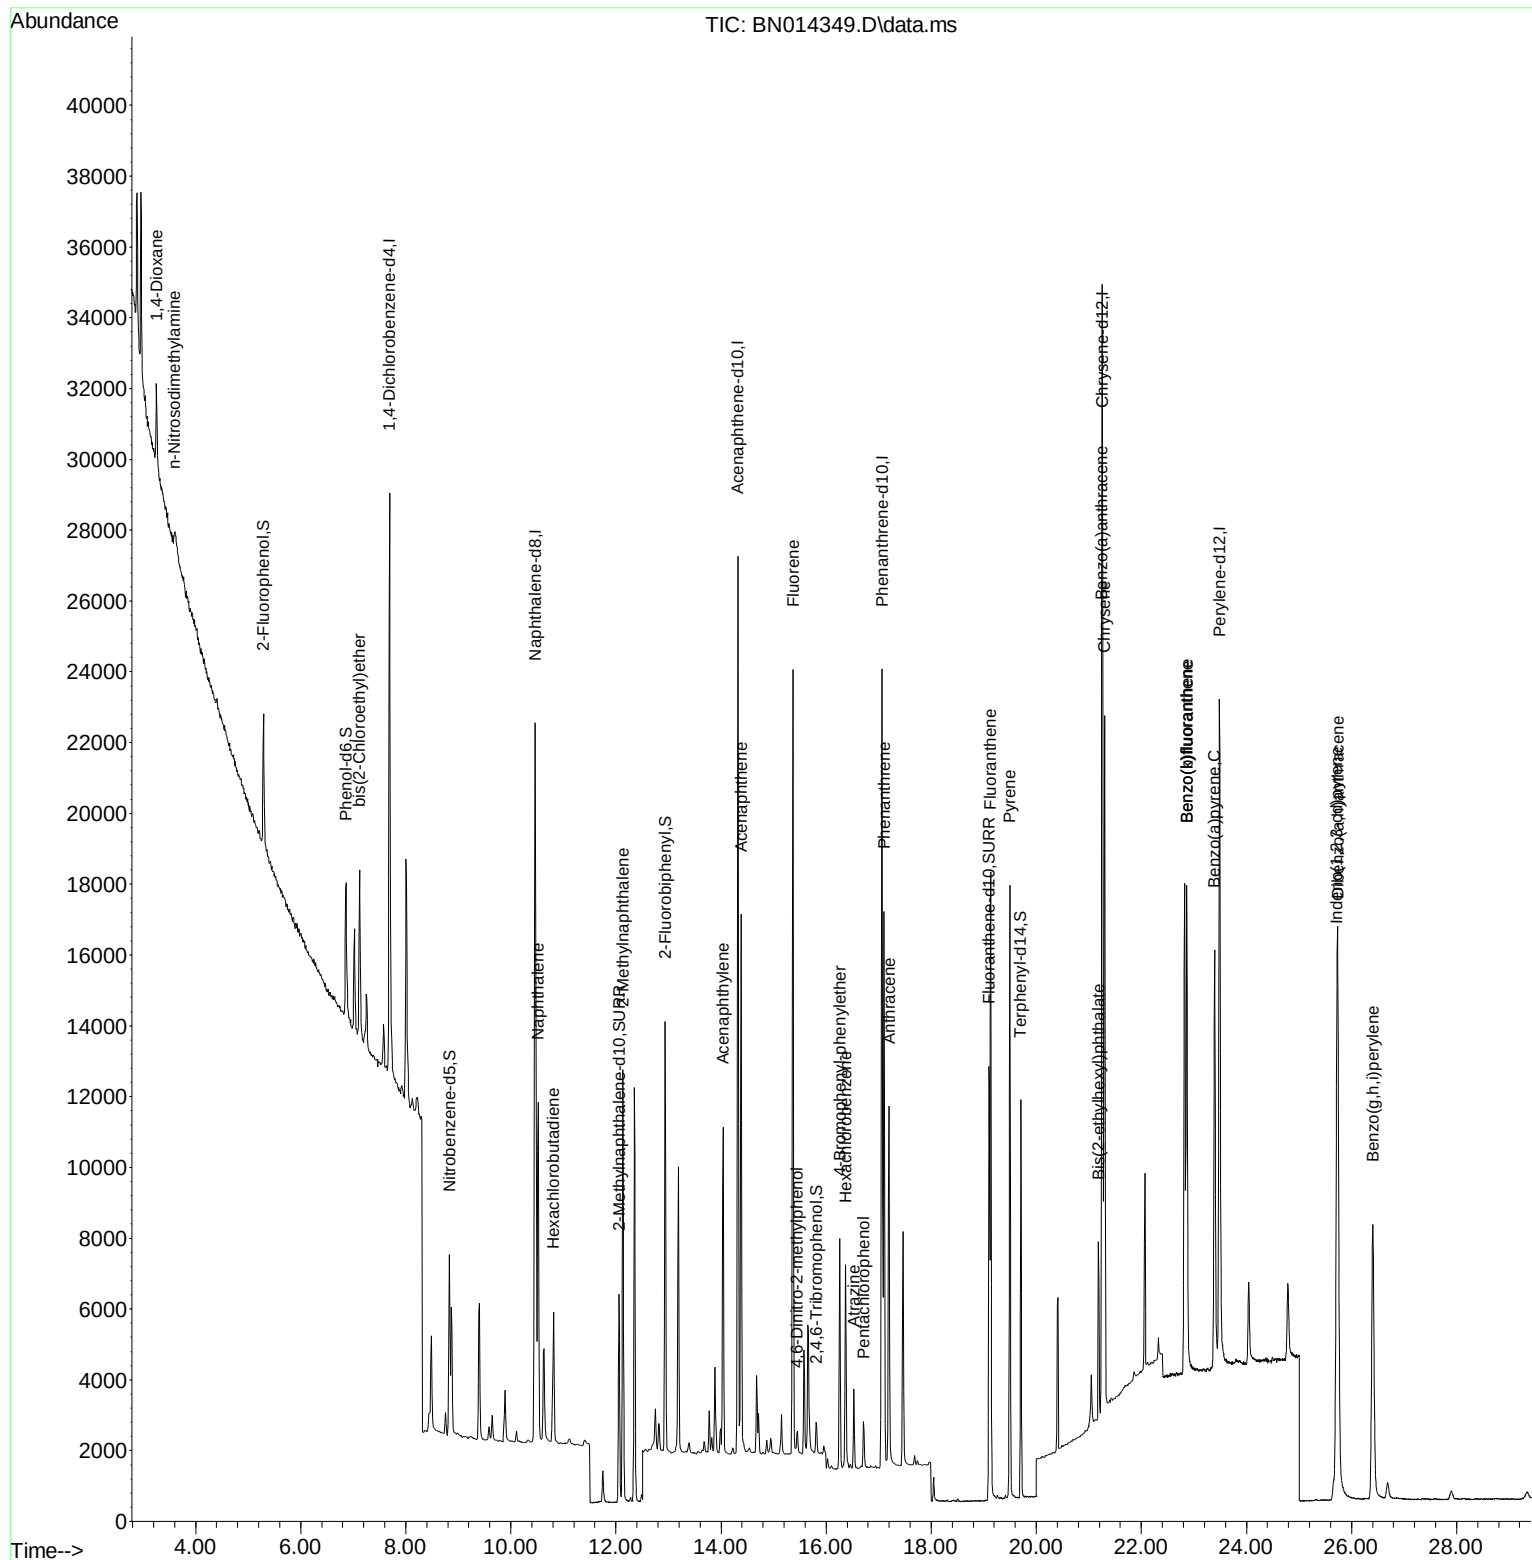


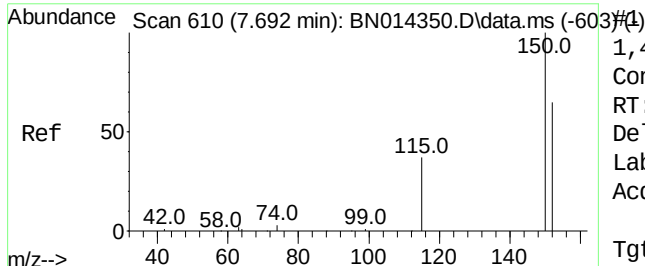

1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.692 min Scan# 610
 Delta R.T. 0.000 min
 Lab File: BN014349.D
 Acq: 21 Apr 2021 10:21




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2


Tgt Ion:	152	Resp:	7833
Ion	Ratio	Lower	Upper
152	100		
150	151.6	123.4	185.2
115	57.8	47.5	71.3

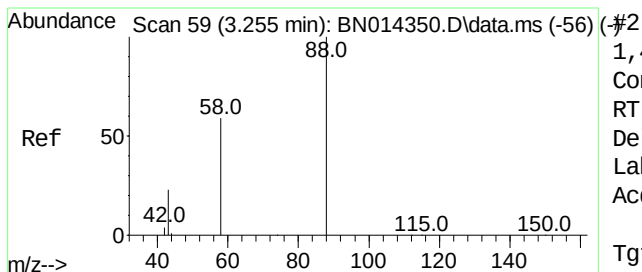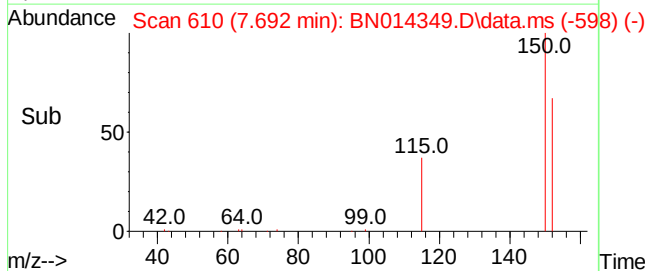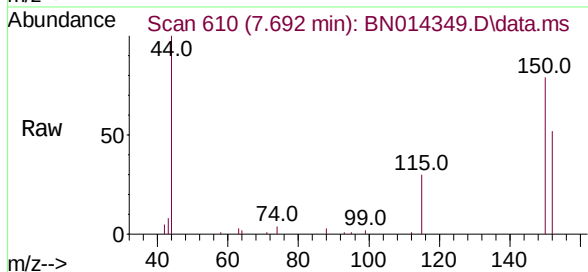

1,4-Dioxane
 Concen: 0.19 ng
 RT: 3.255 min Scan# 59
 Delta R.T. -0.000 min
 Lab File: BN014349.D
 Acq: 21 Apr 2021 10:21

Tgt Ion:	88	Resp:	1905
Ion	Ratio	Lower	Upper
88	100		
58	65.7	52.2	78.2
43	27.8	20.6	30.8


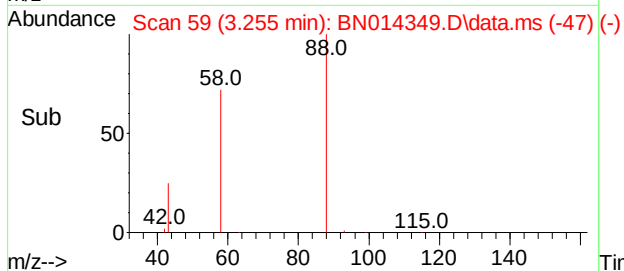




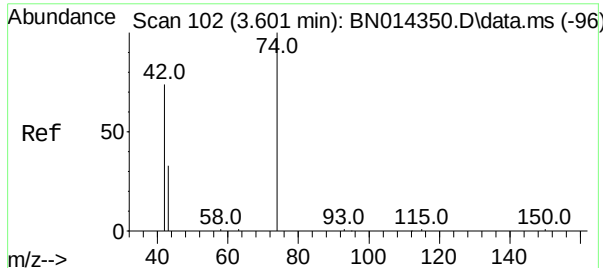

n-Nitrosodimethylamine
 Concen: 0.15 ng
 RT: 3.601 min Scan# 102
 Delta R.T. -0.000 min
 Lab File: BN014349.D
 Acq: 21 Apr 2021 10:21




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2


Tgt Ion:	42	Resp:	799
Ion	Ratio	Lower	Upper
42	100		
74	151.1	108.0	162.0
44	0.0	0.0	0.0

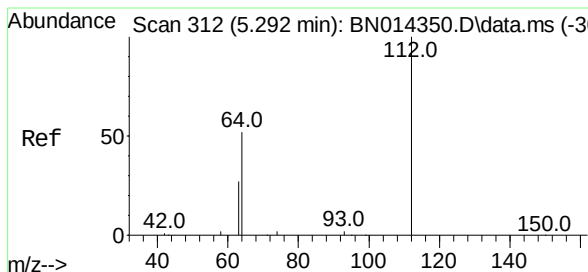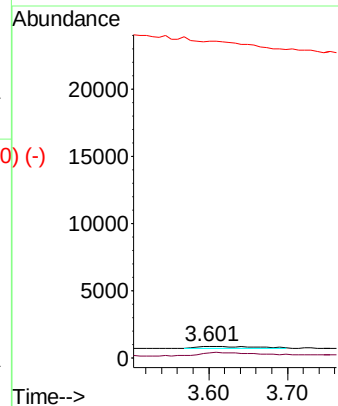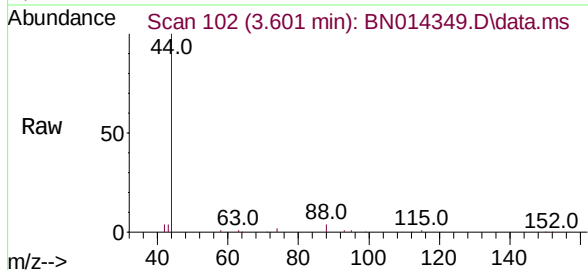

2-Fluorophenol
 Concen: 0.18 ng
 RT: 5.292 min Scan# 312
 Delta R.T. -0.000 min
 Lab File: BN014349.D
 Acq: 21 Apr 2021 10:21

Tgt Ion:	112	Resp:	3175
Ion	Ratio	Lower	Upper
112	100		
64	54.1	43.0	64.6
63	29.7	23.4	35.0



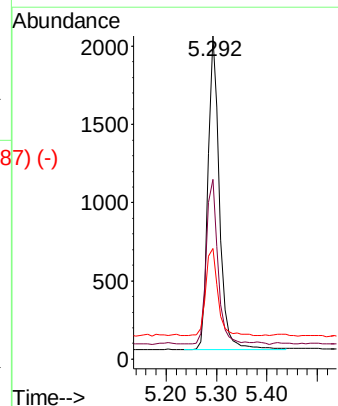



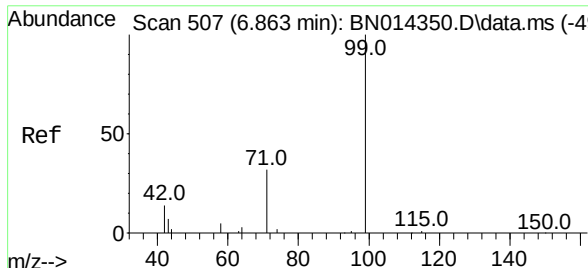

Phenol-d6
 Concen: 0.18 ng
 RT: 6.863 min Scan# 507
 Delta R.T. -0.000 min
 Lab File: BN014349.D
 Acq: 21 Apr 2021 10:21




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Tgt Ion:	99	Resp:	3830
Ion	Ratio	Lower	Upper
99	100		
42	18.4	16.0	24.0
71	35.8	27.8	41.8

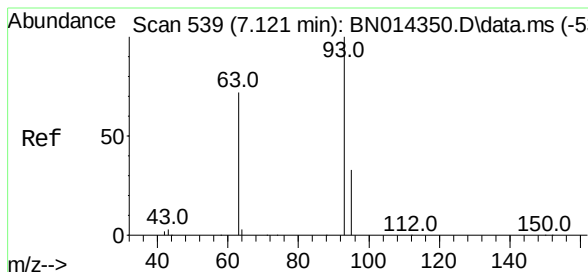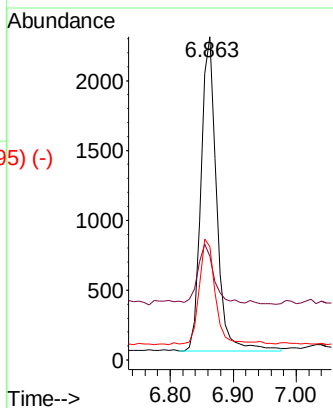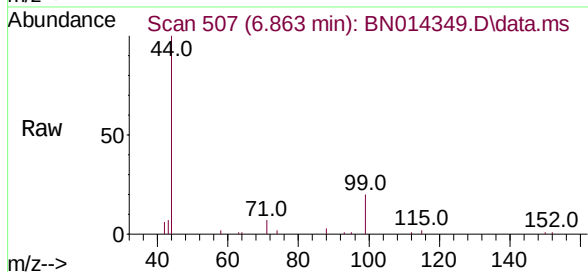

bis(2-Chloroethyl)ether
 Concen: 0.20 ng
 RT: 7.120 min Scan# 539
 Delta R.T. -0.000 min
 Lab File: BN014349.D
 Acq: 21 Apr 2021 10:21


Tgt Ion:	93	Resp:	3873
Ion	Ratio	Lower	Upper
93	100		
63	73.8	59.4	89.2
95	33.8	27.0	40.4






Abundance Scan 857 (10.467 min): BN014350.D\data.ms (-857) (-)

Naphthalene-d8
Concen: 0.40 ng
RT: 10.467 min Scan# 857
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

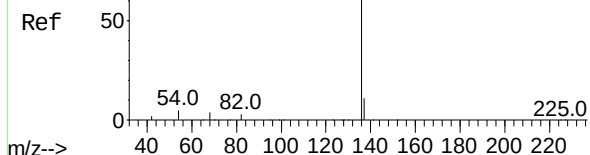




Tgt Ion:	136	Resp:	27271
Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.0	13.6
54	5.4	4.4	6.6
68	5.0	3.9	5.9

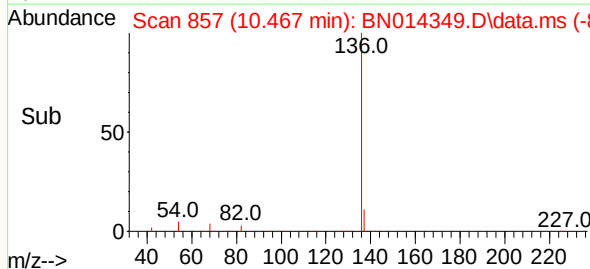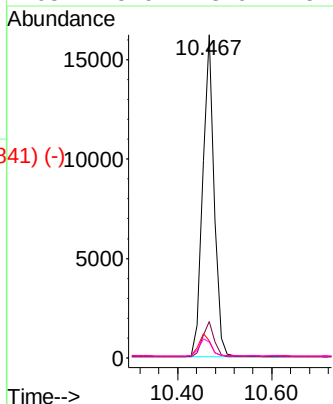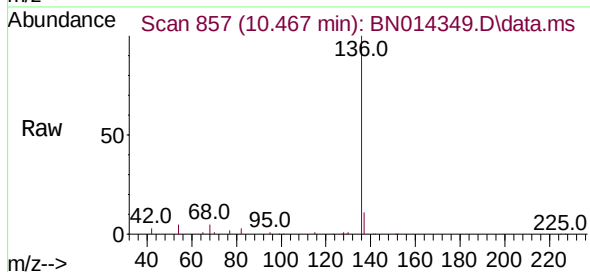

Abundance Scan 728 (8.832 min): BN014350.D\data.ms (-725) (-)

Nitrobenzene-d5
Concen: 0.26 ng
RT: 8.832 min Scan# 728
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21


Tgt Ion:	82	Resp:	4366
Ion	Ratio	Lower	Upper
82	100		
128	38.4	30.3	45.5
54	46.8	35.8	53.8

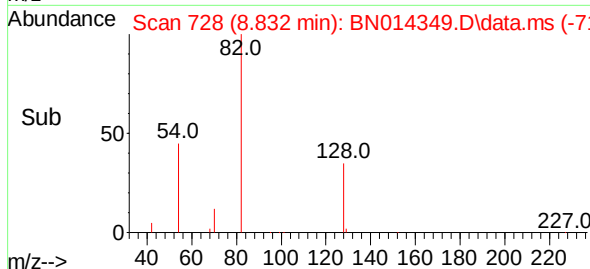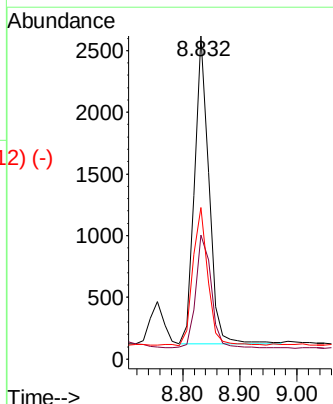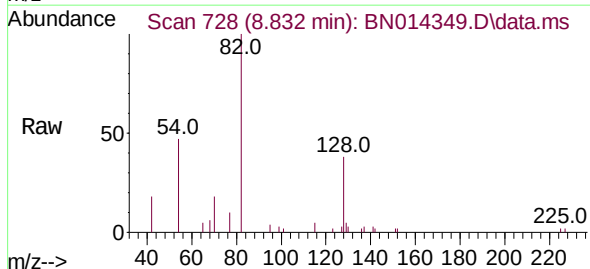




Abundance Scan 861 (10.518 min): BN014350.D\data.ms (-855) (-)

Naphthalene
Concen: 0.19 ng
RT: 10.518 min Scan# 861
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

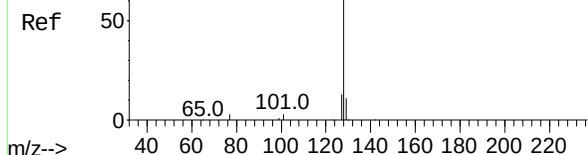


Tgt Ion:	128	Resp:	13317
Ion	Ratio	Lower	Upper
128	100		
129	11.8	9.0	13.6
127	13.3	10.3	15.5


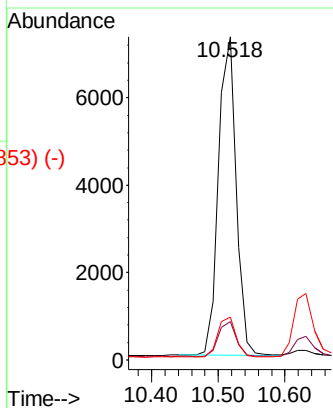
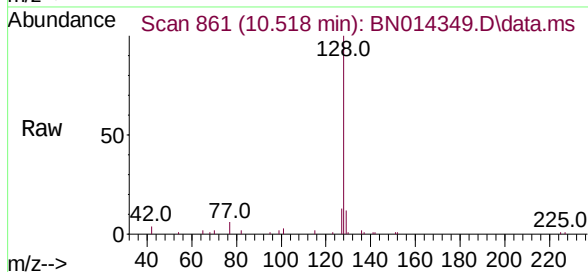



Abundance Scan 884 (10.809 min): BN014350.D\data.ms (-876) (-)

Hexachlorobutadiene
Concen: 0.22 ng
RT: 10.809 min Scan# 884
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21

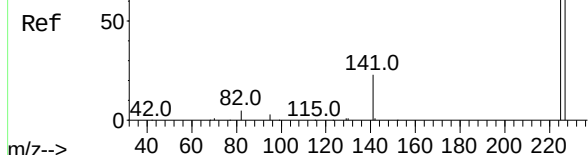

Tgt Ion:	225	Resp:	2943
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.5	50.6	75.8


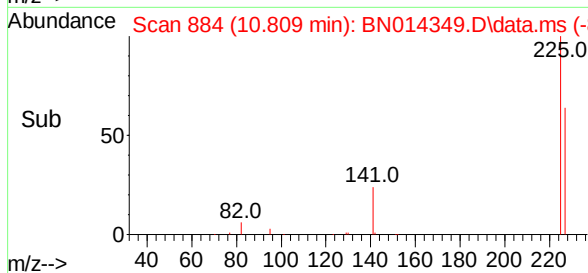




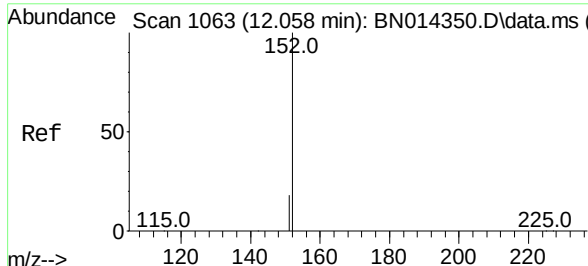

Scan 1063 (12.058 min): BN014350.D\data.ms (-1031) (-)
 2-Methylnaphthalene-d10
 Concen: 0.19 ng
 RT: 12.057 min Scan# 1063
 Delta R.T. -0.000 min
 Lab File: BN014349.D
 Acq: 21 Apr 2021 10:21




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Tgt Ion:	152	Resp:	8018
Ion Ratio	Lower	Upper	
152	100		
151	20.2	16.3	24.5

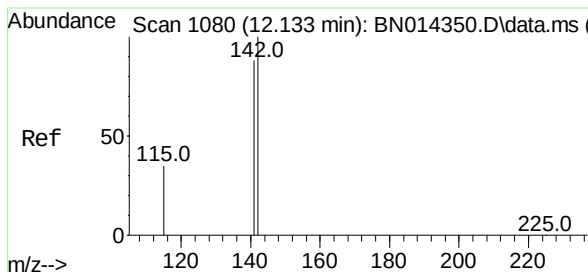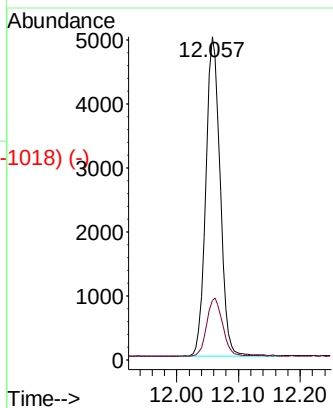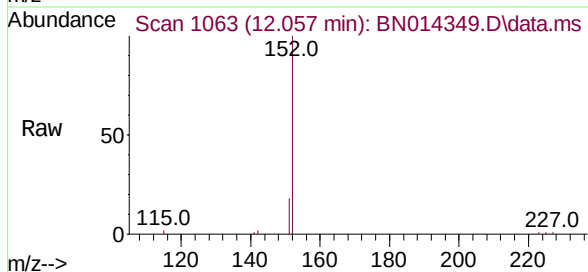

Scan 1080 (12.133 min): BN014350.D\data.ms (-1071) (-)
 2-Methylnaphthalene
 Concen: 0.19 ng
 RT: 12.133 min Scan# 1080
 Delta R.T. -0.000 min
 Lab File: BN014349.D
 Acq: 21 Apr 2021 10:21


Tgt Ion:	142	Resp:	8591
Ion Ratio	Lower	Upper	
142	100		
141	88.2	70.6	105.8
115	37.9	29.0	43.6






Abundance Scan 1307 (14.321 min): BN014350.D\data.ms (-1291) (-)

Acenaphthene-d10
Concen: 0.40 ng
RT: 14.321 min Scan# 1307
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

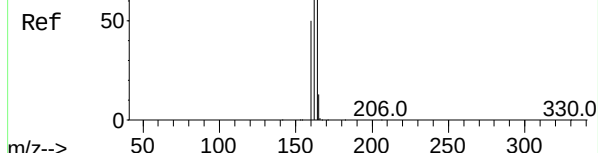


Tgt Ion:	164	Resp:	13854
Ion Ratio	Lower	Upper	
164	100		
162	101.1	81.0	121.6
160	50.9	40.7	61.1

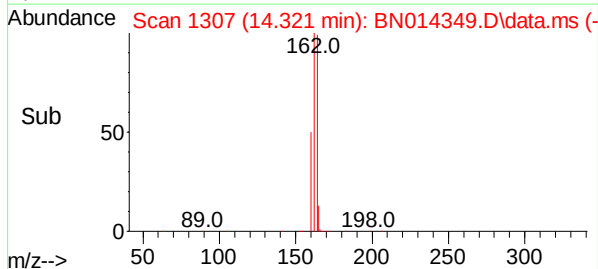

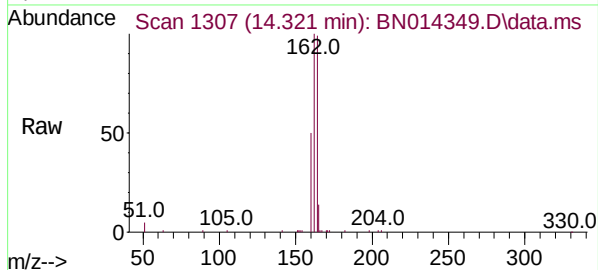


Abundance Scan 1425 (15.818 min): BN014350.D\data.ms (-1417) (-)

2,4,6-Tribromophenol
Concen: 0.16 ng
RT: 15.818 min Scan# 1425
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21

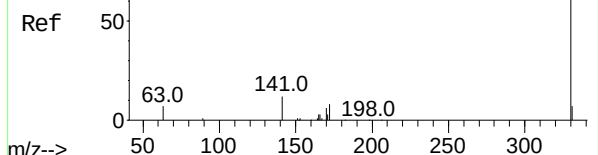


Tgt Ion:	330	Resp:	797
Ion Ratio	Lower	Upper	
330	100		
332	0.0	0.0	0.0
141	37.4	26.2	39.2

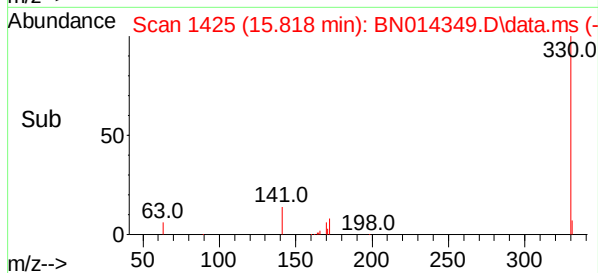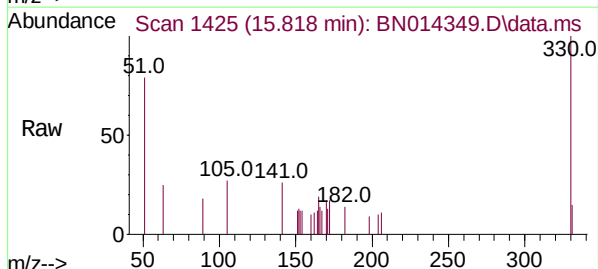




Abundance Scan 1198 (12.938 min): BN014350.D\data.ms (-1198) (-)

2-Fluorobiphenyl
Concen: 0.20 ng
RT: 12.938 min Scan# 1198
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

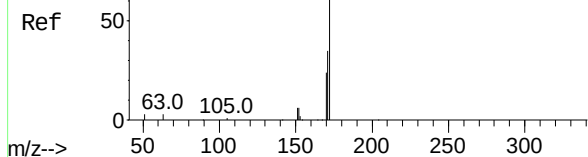


Tgt Ion:	172	Resp:	10665
Ion Ratio	Lower	Upper	
172	100		
171	35.9	28.2	42.2
170	25.5	19.6	29.4


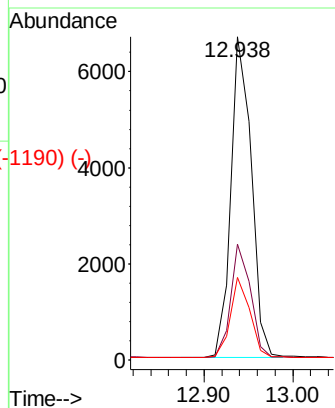
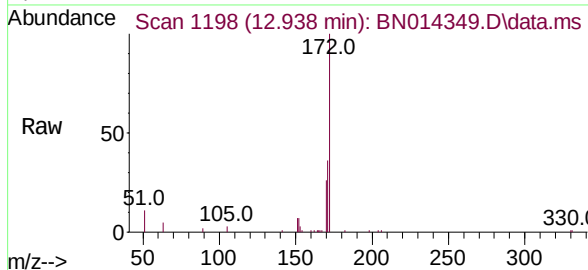



Abundance Scan 1285 (14.042 min): BN014350.D\data.ms (-1285) (-)

Acenaphthylene
Concen: 0.21 ng
RT: 14.042 min Scan# 1285
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21

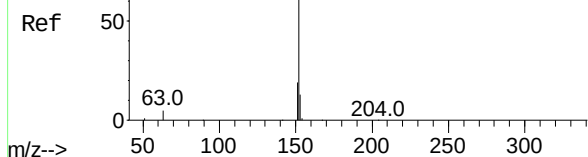

Tgt Ion:	152	Resp:	11134
Ion Ratio	Lower	Upper	
152	100		
151	19.5	15.6	23.4
153	13.1	10.5	15.7



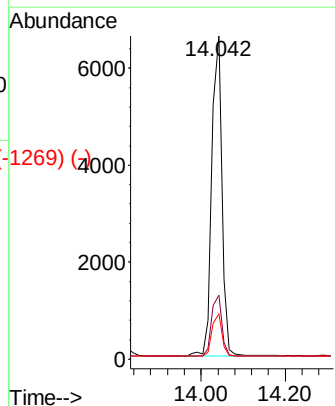



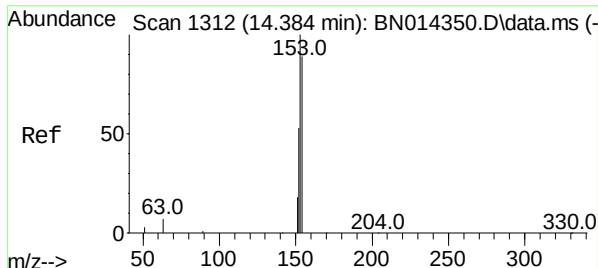

Acenaphthene
Concen: 0.19 ng
RT: 14.384 min Scan# 1312
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Tgt Ion:	154	Resp:	7465
Ion	Ratio	Lower	Upper
154	100		
153	112.4	89.2	133.8
152	61.8	49.0	73.4

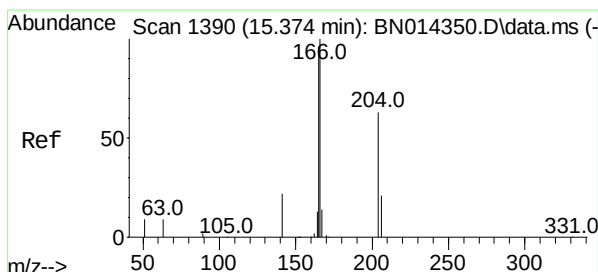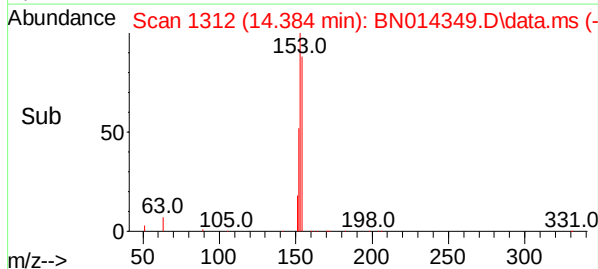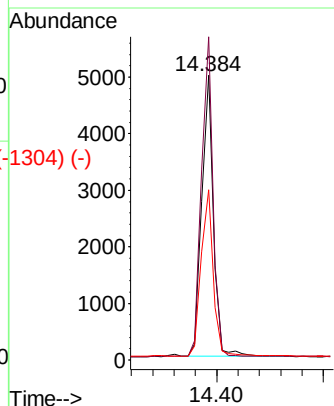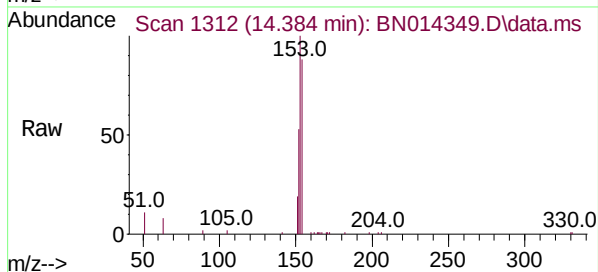

Fluorene
Concen: 0.19 ng
RT: 15.374 min Scan# 1390
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21


Tgt Ion:	166	Resp:	9182
Ion	Ratio	Lower	Upper
166	100		
165	98.7	78.6	118.0
167	13.5	10.9	16.3

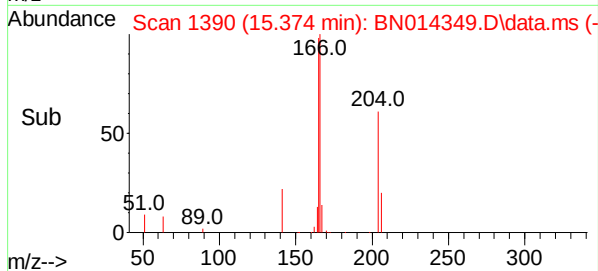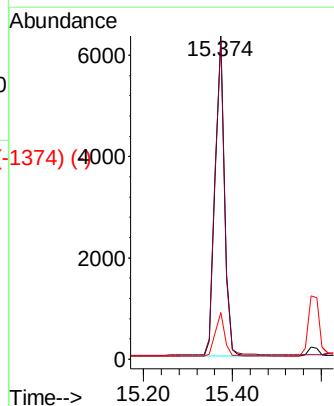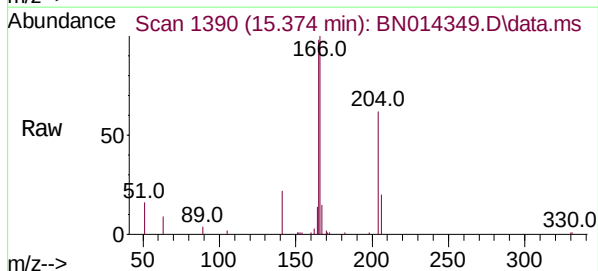



Abundance Scan 1527 (17.067 min): BN014350.D\data.ms (-1511) (-)

Phenanthrene-d10
Concen: 0.40 ng
RT: 17.067 min Scan# 1527
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

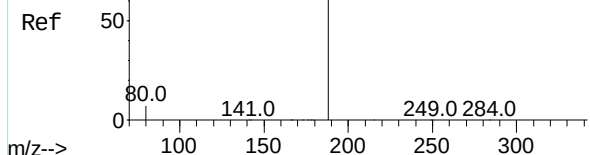

Tgt Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	7.6	6.2	9.4

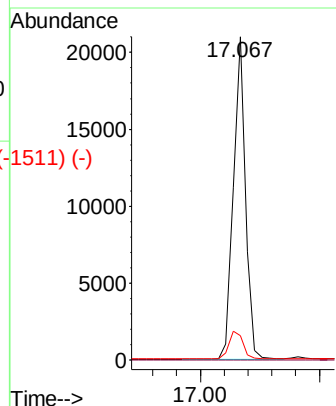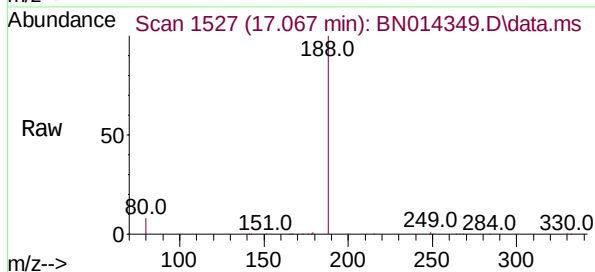




Abundance Scan 1527 (17.067 min): BN014349.D\data.ms (-1511) (-)

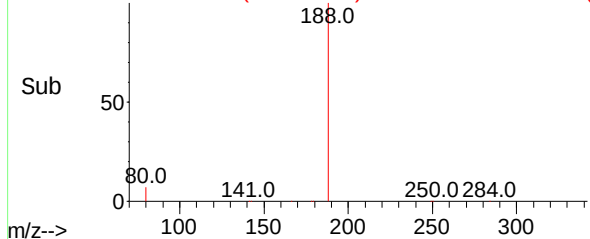


Abundance Scan 1396 (15.450 min): BN014350.D\data.ms (-1320) (-)

4,6-Dinitro-2-methylphenol
Concen: 0.18 ng
RT: 15.450 min Scan# 1396
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21

Tgt Ion	Ratio	Lower	Upper
198	100		
51	127.0	60.0	90.0#
105	55.3	31.5	47.3#

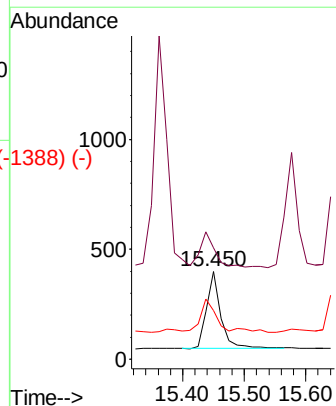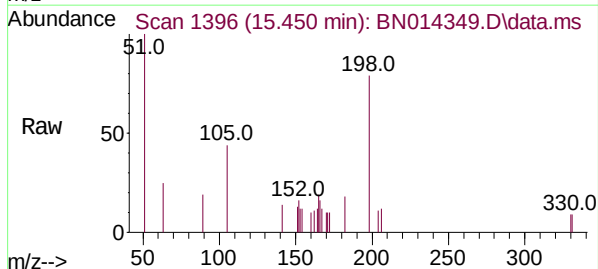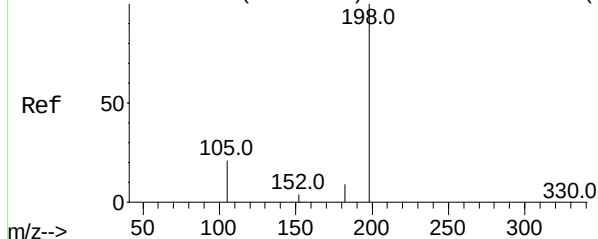


Abundance Scan 1396 (15.450 min): BN014349.D\data.ms (-1388) (-)

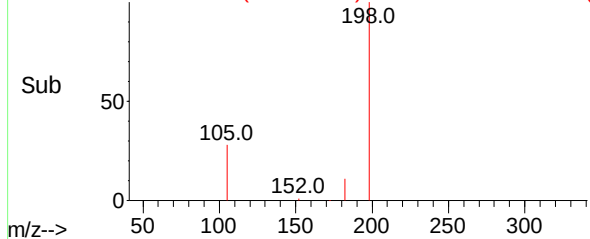




Abundance Scan 1461 (16.264 min): BN014350.D\data.ms (-1427) (-)

4-Bromophenyl-phenylether
Concen: 0.20 ng
RT: 16.264 min Scan# 1461
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

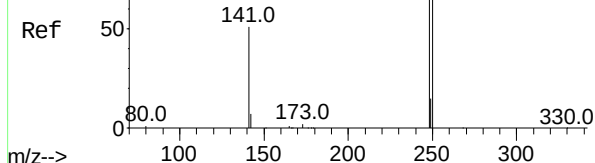





Tgt Ion:	248	Resp:	3149
Ion	Ratio	Lower	Upper
248	100		
250	97.0	77.4	116.0
141	53.6	41.4	62.0

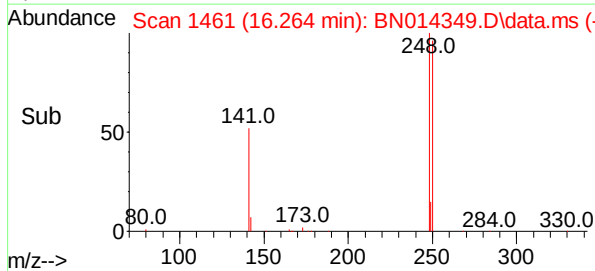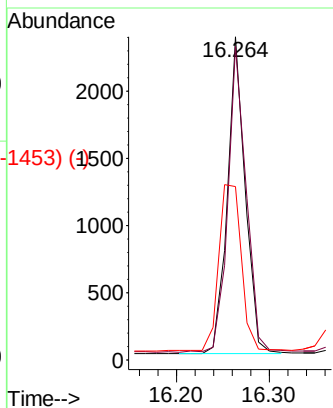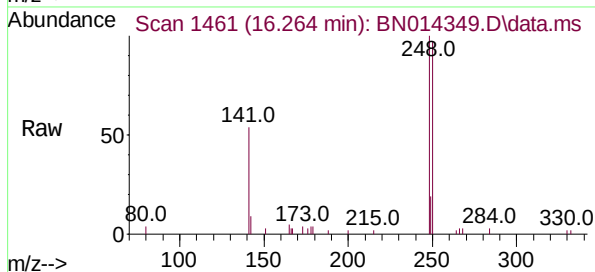

Abundance Scan 1470 (16.373 min): BN014350.D\data.ms (-1429) (-)

Hexachlorobenzene
Concen: 0.22 ng
RT: 16.373 min Scan# 1470
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21


Tgt Ion:	284	Resp:	4404
Ion	Ratio	Lower	Upper
284	100		
142	34.3	26.5	39.7
249	29.8	24.0	36.0

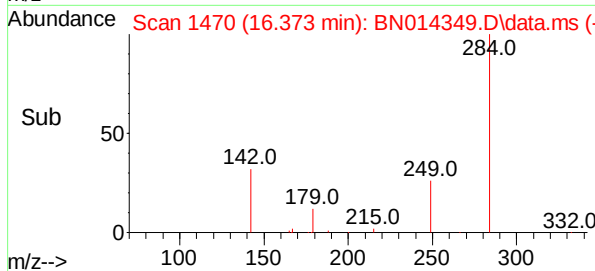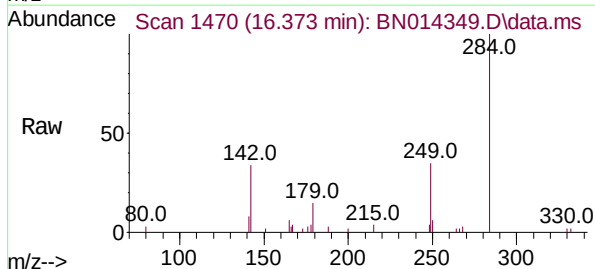



Abundance Scan 1483 (16.532 min): BN014350.D\data.ms (-1429) (-)

Atrazine
Concen: 0.18 ng
RT: 16.532 min Scan# 1483
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

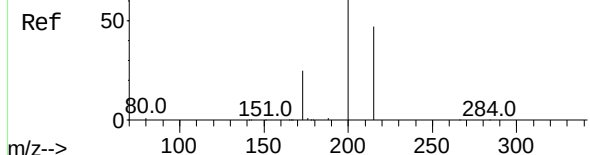

Tgt Ion:	200	Resp:	1729
Ion Ratio	Lower	Upper	
200	100		
173	26.9	21.0	31.6
215	49.2	38.7	58.1

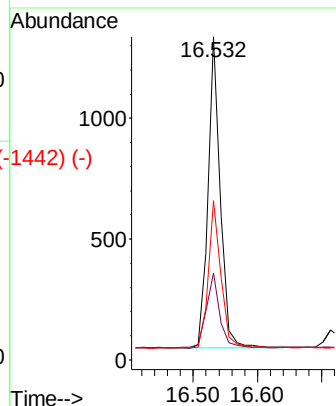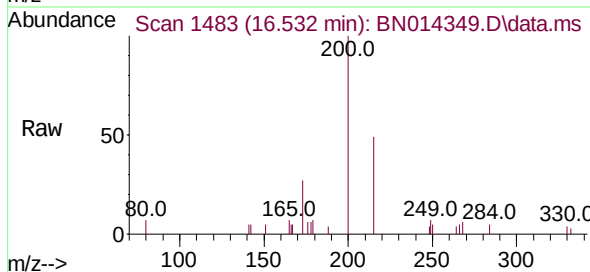




Abundance Scan 1483 (16.532 min): BN014349.D\data.ms (-1442) (-)

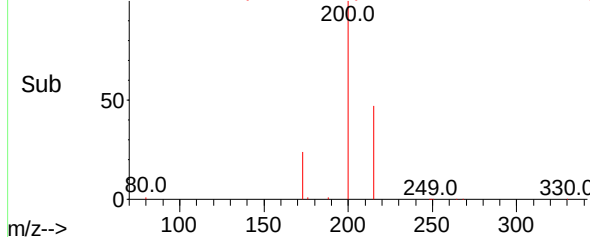


Abundance Scan 1498 (16.714 min): BN014350.D\data.ms (-1424) (-)

Pentachlorophenol
Concen: 0.13 ng
RT: 16.714 min Scan# 1498
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21


Tgt Ion:	266	Resp:	699
Ion Ratio	Lower	Upper	
266	100		
264	62.2	50.6	76.0
268	64.4	51.4	77.0

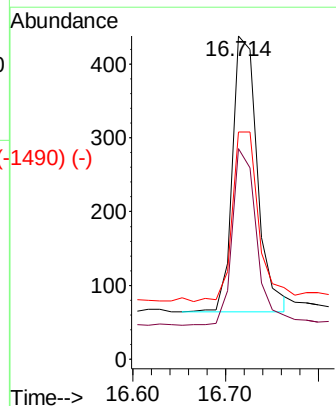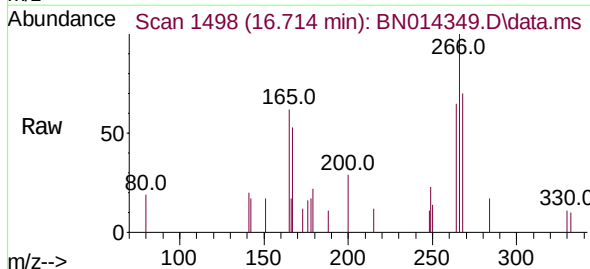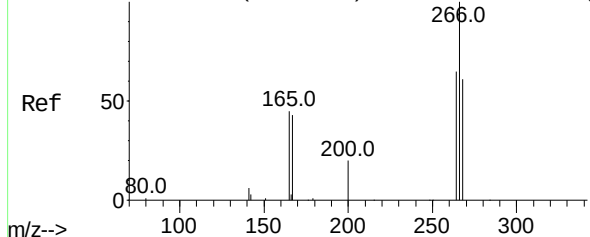

Abundance Scan 1498 (16.714 min): BN014349.D\data.ms (-1490) (-)

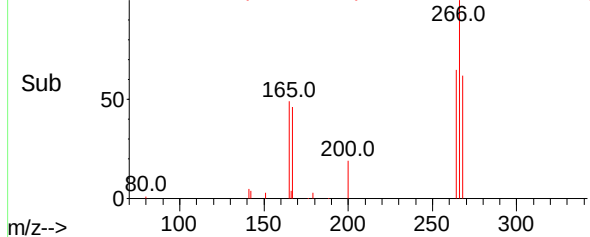




Abundance Scan 1530 (17.104 min): BN014350.D\data.ms (-1525) (-)




Phenanthrene
Concen: 0.19 ng
RT: 17.104 min Scan# 1530
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Tgt Ion:	178	Resp:	15933
Ion Ratio	Lower	Upper	
178	100		
176	19.1	15.2	22.8
179	15.4	12.2	18.4


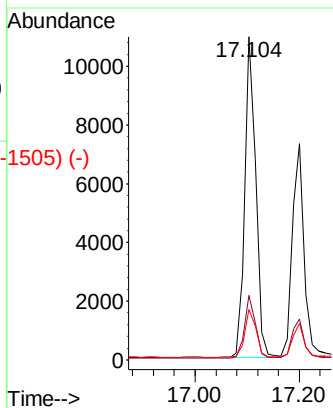
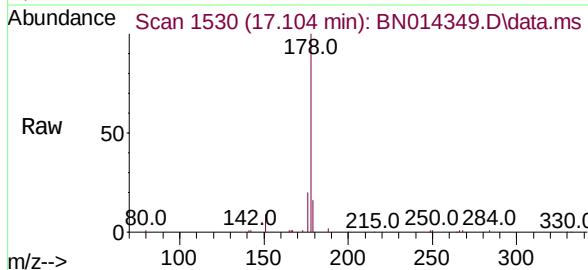


Abundance Scan 1538 (17.201 min): BN014350.D\data.ms (-1526) (-)




Anthracene
Concen: 0.18 ng
RT: 17.201 min Scan# 1538
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21

Tgt Ion:	178	Resp:	11774
Ion Ratio	Lower	Upper	
178	100		
176	18.1	15.0	22.4
179	15.4	12.2	18.2






Abundance Scan 1825 (19.101 min): BN014350.D\data.ms (-1827) (-)




Fluoranthene-d10
Concen: 0.18 ng
RT: 19.101 min Scan# 1825
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Tgt Ion:	212	Resp:	14686
Ion Ratio	Lower	Upper	
212	100		
106	12.0	9.7	14.5
104	6.8	5.4	8.0



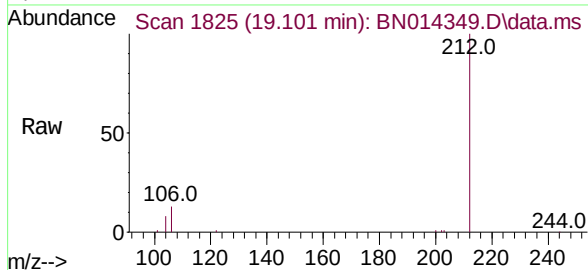


Abundance Scan 1831 (19.131 min): BN014350.D\data.ms (-1823) (-)



Fluoranthene
Concen: 0.17 ng
RT: 19.131 min Scan# 1831
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21


Tgt Ion:	202	Resp:	16030
Ion Ratio	Lower	Upper	
202	100		
101	10.4	8.2	12.4
203	17.1	13.8	20.6






Abundance Scan 2125 (21.258 min): BN014350.D\data.ms (-2129) (-)

Chrysene-d12
Concen: 0.40 ng
RT: 21.258 min Scan# 2125
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

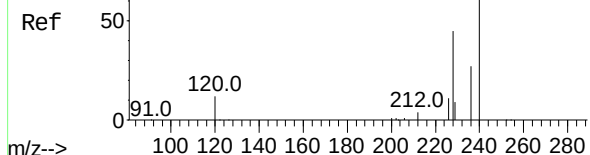


Tgt Ion:	240	Resp:	26881
Ion Ratio	Lower	Upper	
240	100		
120	13.7	10.7	16.1
236	27.0	21.5	32.3

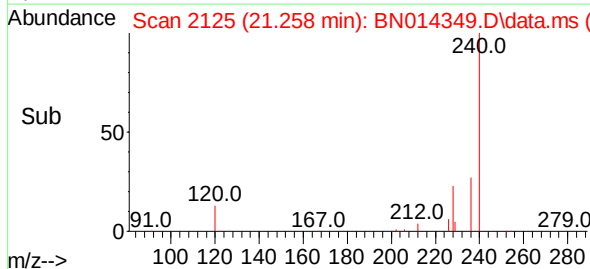

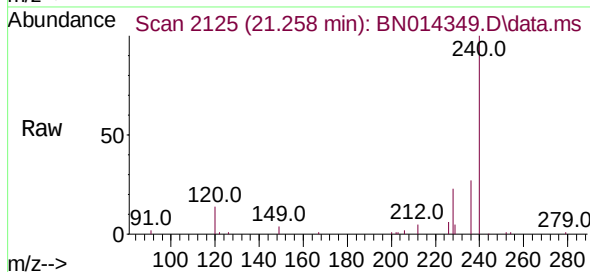


Abundance Scan 1905 (19.498 min): BN014350.D\data.ms (-1896) (-)

Pyrene
Concen: 0.21 ng
RT: 19.498 min Scan# 1905
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21

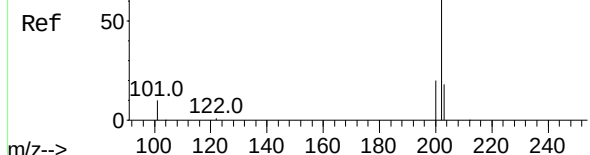


Tgt Ion:	202	Resp:	15908
Ion Ratio	Lower	Upper	
202	100		
200	20.6	16.6	24.8
203	17.5	14.1	21.1

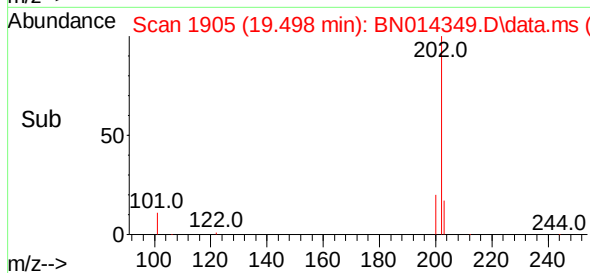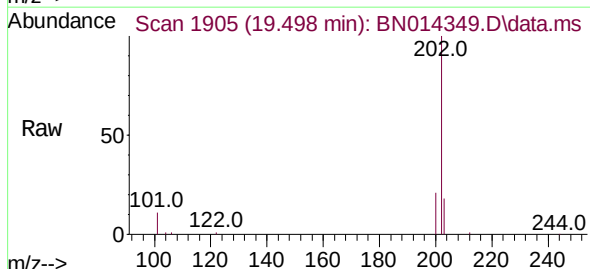



Abundance Scan 1947 (19.707 min): BN014350.D\data.ms (-1934) (-)

Terphenyl-d14
Concen: 0.20 ng
RT: 19.707 min Scan# 1947
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

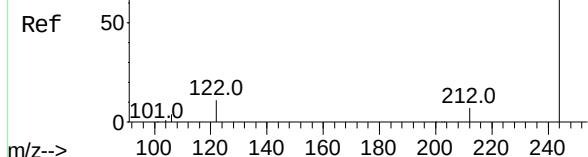

Tgt Ion	Ratio	Lower	Upper
244	100		
212	8.4	6.2	9.4
122	12.3	9.3	13.9

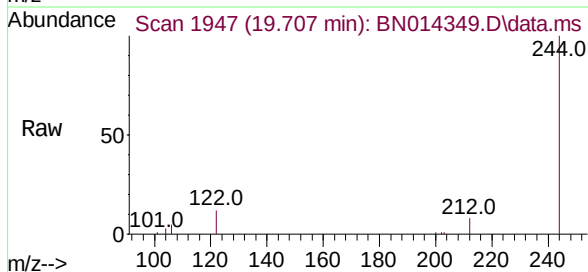




Abundance Scan 1947 (19.707 min): BN014349.D\data.ms (-1917) (-)

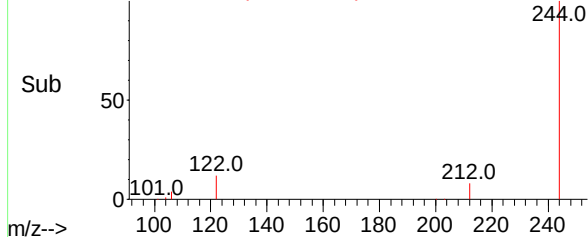


Abundance Scan 2124 (21.247 min): BN014350.D\data.ms (-2132) (-)

Benzo(a)anthracene
Concen: 0.18 ng
RT: 21.247 min Scan# 2124
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21


Tgt Ion	Ratio	Lower	Upper
228	100		
226	26.9	21.3	31.9
229	19.9	15.7	23.5

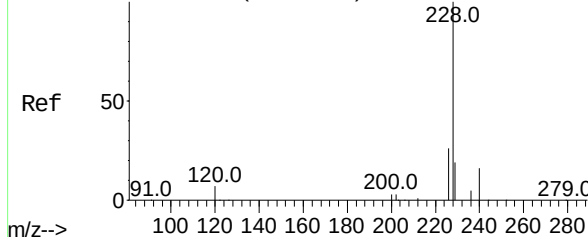

Abundance Scan 2124 (21.247 min): BN014349.D\data.ms (-2105) (-)





Abundance Scan 2129 (21.300 min): BN014350.D\data.ms (-2129) (-)

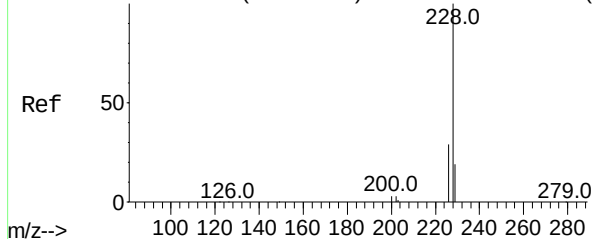


Chrysene
Concen: 0.19 ng
RT: 21.300 min Scan# 2129
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	228	Resp:	16535
Ion Ratio	Lower	Upper	
228	100		
226	29.6	23.1	34.7
229	19.9	15.7	23.5

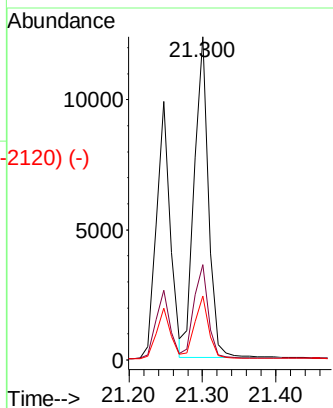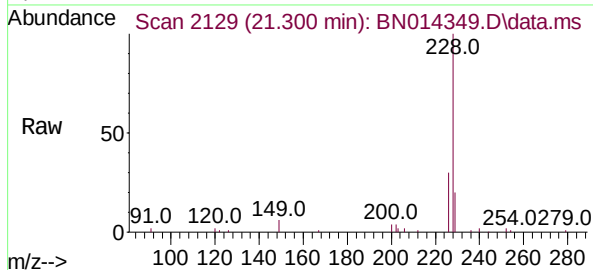

Abundance Scan 2129 (21.300 min): BN014349.D\data.ms (-2120) (-)


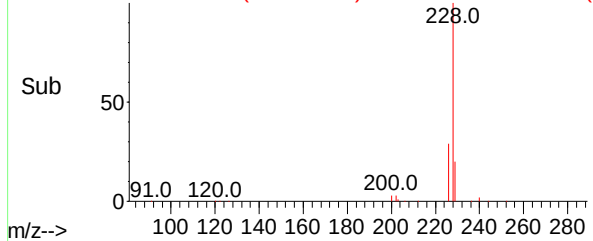


Abundance Scan 2118 (21.184 min): BN014350.D\data.ms (-2118) (-)

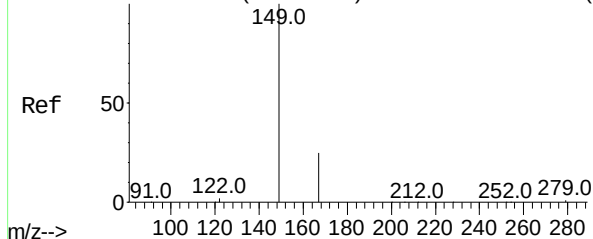


Bis(2-ethylhexyl)phthalate
Concen: 0.24 ng
RT: 21.183 min Scan# 2118
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21


Tgt Ion:	149	Resp:	4924
Ion Ratio	Lower	Upper	
149	100		
167	25.8	21.3	31.9
279	4.6	3.1	4.7

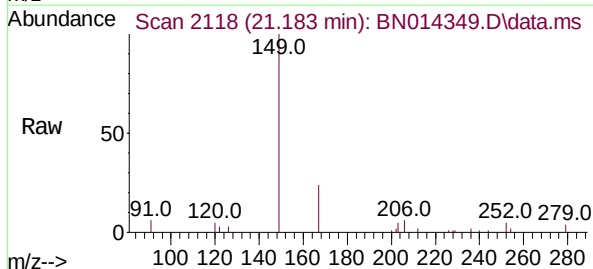

Abundance Scan 2118 (21.183 min): BN014349.D\data.ms (-2109) (-)

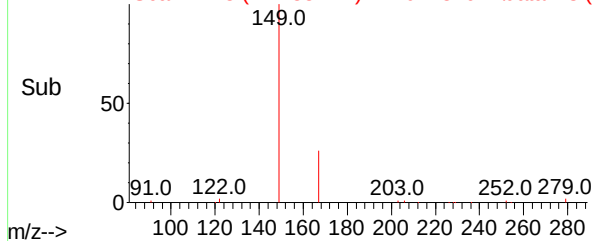


Abundance Scan 3203 (25.725 min): BN014350.D\data.ms (-3175) (-)





Indeno(1,2,3-cd)pyrene
Concen: 0.20 ng
RT: 25.722 min Scan# 3202
Delta R.T. -0.004 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

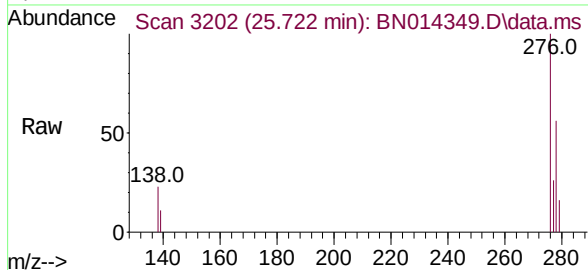


Tgt Ion	Ratio	Lower	Upper
276	100		
138	22.7	18.9	28.3
277	24.8	19.8	29.8





Abundance Scan 2550 (23.490 min): BN014350.D\data.ms (-2536) (-)




Perylene-d12
Concen: 0.40 ng
RT: 23.486 min Scan# 2549
Delta R.T. -0.003 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21



Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.9	19.8	29.6
265	42.0	34.4	51.6

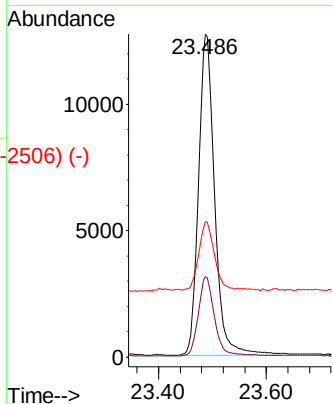




Abundance Scan 2354 (22.819 min): BN014350.D\data.ms (-2354) (-)




Benzo(b)fluoranthene
Concen: 0.16 ng
RT: 22.863 min Scan# 2367
Delta R.T. 0.044 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21

Tgt Ion:	252	Resp:	18365
Ion Ratio	Lower	Upper	
252	100		
253	26.6	19.0	28.6
125	14.1	9.7	14.5

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2



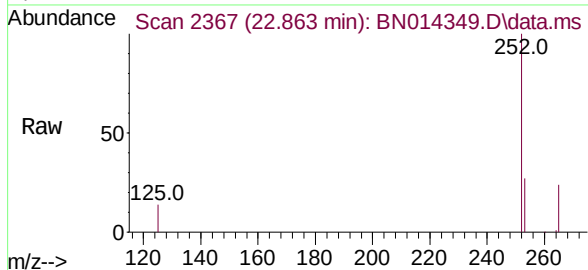


Abundance Scan 2367 (22.864 min): BN014350.D\data.ms (-2367) (-)



Benzo(k)fluoranthene
Concen: 0.17 ng
RT: 22.863 min Scan# 2367
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21


Tgt Ion:	252	Resp:	18365
Ion Ratio	Lower	Upper	
252	100		
253	26.6	19.3	28.9
125	14.1	9.4	14.2





Abundance Scan 2521 (23.391 min): BN014350.D\data.ms (-2509) (-)

Benzo(a)pyrene
Concen: 0.18 ng
RT: 23.394 min Scan# 2522
Delta R.T. 0.003 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

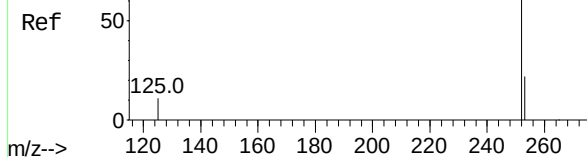

Tgt Ion:	252	Resp:	15604
Ion	Ratio	Lower	Upper
252	100		
253	30.5	20.7	31.1
125	34.2	11.8	17.6#

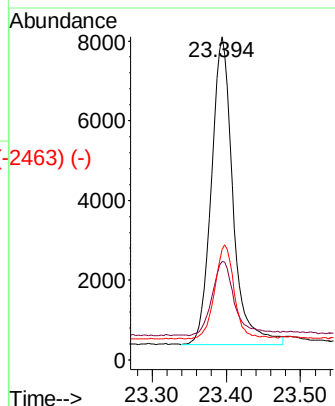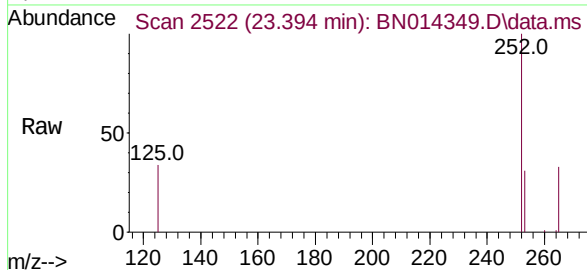




Abundance Scan 2522 (23.394 min): BN014349.D\data.ms (-2463) (-)

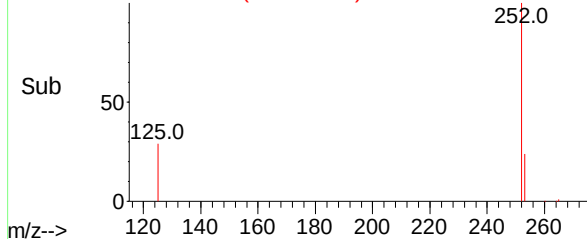


Abundance Scan 3207 (25.739 min): BN014350.D\data.ms (-3146) (-)

Dibenzo(a,h)anthracene
Concen: 0.17 ng
RT: 25.739 min Scan# 3207
Delta R.T. -0.000 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21


Tgt Ion:	278	Resp:	16702
Ion	Ratio	Lower	Upper
278	100		
139	17.2	13.3	19.9
279	27.4	20.2	30.2

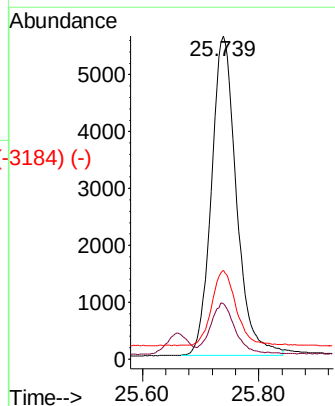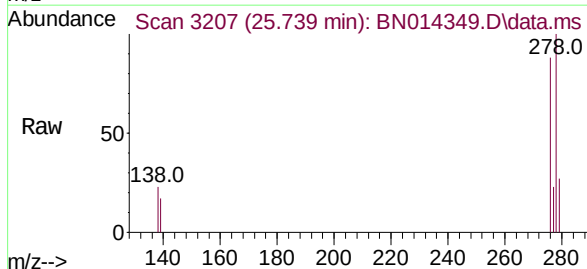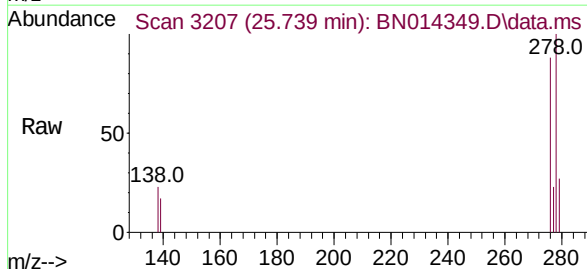

Abundance Scan 3207 (25.739 min): BN014349.D\data.ms (-3184) (-)

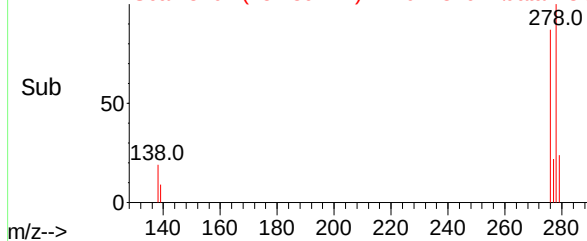


Abundance Scan 3403 (26.410 min): BN014350.D\data.ms (-3343) (-)



Benzo(g,h,i)perylene
Concen: 0.16 ng
RT: 26.406 min Scan# 3402
Delta R.T. -0.004 min
Lab File: BN014349.D
Acq: 21 Apr 2021 10:21

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Abundance Scan 3402 (26.406 min): BN014349.D\data.ms

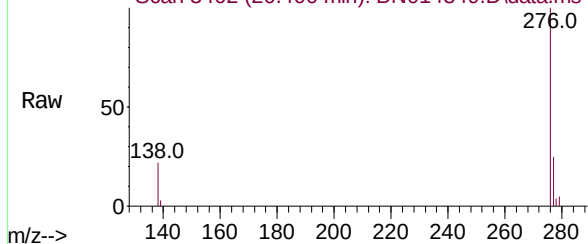

Tgt Ion	Ratio	Lower	Upper
276	100		
277	24.6	19.1	28.7
138	21.8	16.7	25.1

Abundance Scan 3402 (26.406 min): BN014349.D\data.ms (-3345) (-)

