

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042221\
 Data File : BN014354.D
 Acq On : 21 Apr 2021 13:21
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Apr 21 13:51:14 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 21 12:48:18 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.692	152	8350	0.40	ng	0.00
7) Naphthalene-d8	10.467	136	27311	0.40	ng	0.00
13) Acenaphthene-d10	14.321	164	14360	0.40	ng	0.00
19) Phenanthrene-d10	17.067	188	28867	0.40	ng	0.00
29) Chrysene-d12	21.261	240	32782	0.40	ng	0.00
36) Perylene-d12	23.493	264	24477	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.292	112	81088	4.39	ng	0.00
5) Phenol-d6	6.863	99	106762	4.59	ng	0.00
8) Nitrobenzene-d5	8.832	82	114355	6.72	ng	0.00
11) 2-Methylnaphthalene-d10	12.057	152	208681	4.97	ng	0.00
14) 2,4,6-Tribromophenol	15.818	330	28651	5.51	ng	0.00
15) 2-Fluorobiphenyl	12.938	172	273781	4.85	ng	0.00
27) Fluoranthene-d10	19.104	212	425678	5.34	ng	0.00
31) Terphenyl-d14	19.710	244	335016	4.88	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.247	88	43768	4.13	ng	99
3) n-Nitrosodimethylamine	3.561	42	31261	5.32	ng	# 95
6) bis(2-Chloroethyl)ether	7.120	93	95475	4.54	ng	98
9) Naphthalene	10.518	128	329163	4.79	ng	99
10) Hexachlorobutadiene	10.809	225	68681	5.02	ng	# 99
12) 2-Methylnaphthalene	12.133	142	222140	4.96	ng	99
16) Acenaphthylene	14.042	152	326622	5.97	ng	100
17) Acenaphthene	14.384	154	209812	5.15	ng	97
18) Fluorene	15.374	166	265590	5.35	ng	99
20) 4,6-Dinitro-2-methylph...	15.450	198	20788	6.94	ng	# 49
21) 4-Bromophenyl-phenylether	16.264	248	82936	5.42	ng	99
22) Hexachlorobenzene	16.374	284	108520	5.53	ng	99
23) Atrazine	16.532	200	57850	6.08	ng	99
24) Pentachlorophenol	16.715	266	26292	4.94	ng	99
25) Phenanthrene	17.104	178	415366	5.13	ng	100
26) Anthracene	17.201	178	368142	5.69	ng	100
28) Fluoranthene	19.134	202	482878	5.41	ng	100
30) Pyrene	19.496	202	475783	5.11	ng	100
32) Benzo(a)anthracene	21.250	228	477424	5.43	ng	99
33) Chrysene	21.303	228	497344	4.74	ng	99
34) Bis(2-ethylhexyl)phtha...	21.186	149	154289	6.27	ng	99
35) Indeno(1,2,3-cd)pyrene	25.724	276	544280	4.27	ng	100
37) Benzo(b)fluoranthene	22.822	252	479478	4.50	ng	# 95
38) Benzo(k)fluoranthene	22.870	252	486694	4.73	ng	# 95
39) Benzo(a)pyrene	23.393	252	421214	5.37	ng	# 91
40) Dibenzo(a,h)anthracene	25.741	278	456812	4.91	ng	97
41) Benzo(g,h,i)perylene	26.412	276	466704	4.74	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042221\
Data File : BN014354.D
Acq On : 21 Apr 2021 13:21
Operator : CG/JU
Sample : SSTDIC5.0
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Quant Time: Apr 21 13:51:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 21 12:48:18 2021
Response via : Initial Calibration







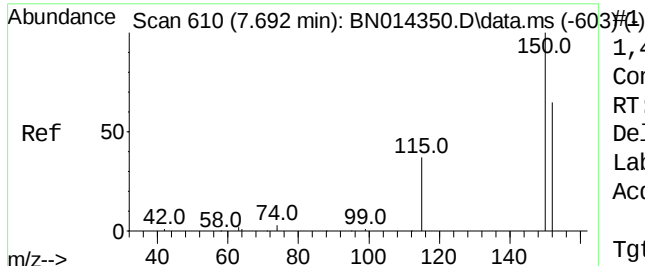

1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.692 min Scan# 610
 Delta R.T. 0.000 min
 Lab File: BN014354.D
 Acq: 21 Apr 2021 13:21




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:	152	Resp:	8350
Ion	Ratio	Lower	Upper
152	100		
150	154.9	123.4	185.2
115	60.0	47.5	71.3

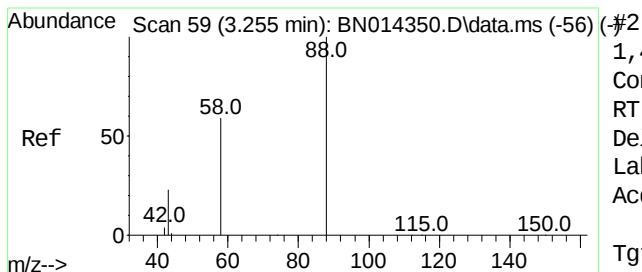

1,4-Dioxane
 Concen: 4.13 ng
 RT: 3.247 min Scan# 58
 Delta R.T. -0.008 min
 Lab File: BN014354.D
 Acq: 21 Apr 2021 13:21

Tgt Ion:	88	Resp:	43768
Ion	Ratio	Lower	Upper
88	100		
58	64.1	52.2	78.2
43	25.0	20.6	30.8









n-Nitrosodimethylamine
Concen: 5.32 ng
RT: 3.561 min Scan# 97
Delta R.T. -0.040 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 42 Resp: 31261
Ion Ratio Lower Upper
42 100
74 140.8 108.0 162.0
44 14.0 0.0 0.0#



2-Fluorophenol
Concen: 4.39 ng
RT: 5.292 min Scan# 312
Delta R.T. -0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

Tgt Ion: 112 Resp: 81088
Ion Ratio Lower Upper
112 100
64 53.9 43.0 64.6
63 29.1 23.4 35.0







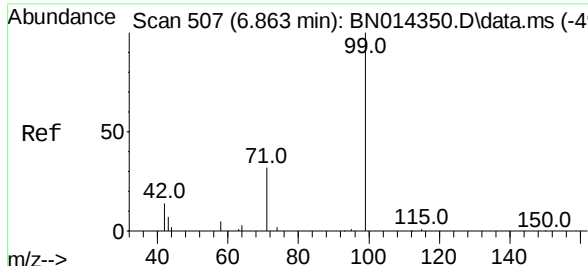

Phenol-d6
 Concen: 4.59 ng
 RT: 6.863 min Scan# 507
 Delta R.T. -0.000 min
 Lab File: BN014354.D
 Acq: 21 Apr 2021 13:21




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion:	99	Resp:	106762
Ion	Ratio	Lower	Upper
99	100		
42	19.2	16.0	24.0
71	34.5	27.8	41.8



bis(2-Chloroethyl)ether
 Concen: 4.54 ng
 RT: 7.120 min Scan# 539
 Delta R.T. -0.000 min
 Lab File: BN014354.D
 Acq: 21 Apr 2021 13:21


Tgt Ion:	93	Resp:	95475
Ion	Ratio	Lower	Upper
93	100		
63	72.7	59.4	89.2
95	32.9	27.0	40.4






Abundance Scan 857 (10.467 min): BN014350.D\data.ms (-857) (-)

Naphthalene-d8
Concen: 0.40 ng
RT: 10.467 min Scan# 857
Delta R.T. -0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0






Tgt Ion:	136	Resp:	27311
Ion	Ratio	Lower	Upper
136	100		
137	11.1	9.0	13.6
54	5.5	4.4	6.6
68	5.1	3.9	5.9



Abundance Scan 728 (8.832 min): BN014350.D\data.ms (-725) (-)

Nitrobenzene-d5
Concen: 6.72 ng
RT: 8.832 min Scan# 728
Delta R.T. -0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21


Tgt Ion:	82	Resp:	114355
Ion	Ratio	Lower	Upper
82	100		
128	41.4	30.3	45.5
54	41.9	35.8	53.8






Abundance Scan 861 (10.518 min): BN014350.D\data.ms (-855) (-)

Naphthalene
Concen: 4.79 ng
RT: 10.518 min Scan# 861
Delta R.T. -0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Tgt Ion:	128	Resp:	329163
Ion	Ratio	Lower	Upper
128	100		
129	11.0	9.0	13.6
127	12.6	10.3	15.5






Abundance Scan 884 (10.809 min): BN014350.D\data.ms (-876) (-)


Hexachlorobutadiene
Concen: 5.02 ng
RT: 10.809 min Scan# 884
Delta R.T. -0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21



Tgt Ion:	225	Resp:	68681
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.8	50.6	75.8





Abundance Scan 1063 (12.058 min): BN014350.D\data.ms (-1051) (-)




2-Methylnaphthalene-d10
Concen: 4.97 ng
RT: 12.057 min Scan# 1063
Delta R.T. -0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 208681
Ion Ratio Lower Upper
152 100
151 20.1 16.3 24.5



Abundance Scan 1063 (12.057 min): BN014354.D\data.ms (-1018) (-)





Abundance Scan 1080 (12.133 min): BN014350.D\data.ms (-1071) (-)




2-Methylnaphthalene
Concen: 4.96 ng
RT: 12.133 min Scan# 1080
Delta R.T. -0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

Tgt Ion:142 Resp: 222140
Ion Ratio Lower Upper
142 100
141 87.9 70.6 105.8
115 35.4 29.0 43.6




Abundance Scan 1080 (12.133 min): BN014354.D\data.ms (-1058) (-)






Abundance Scan 1307 (14.321 min): BN014350.D\data.ms (-1299) (-)

Acenaphthene-d10
Concen: 0.40 ng
RT: 14.321 min Scan# 1307
Delta R.T. -0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Tgt Ion:	164	Resp:	14360
Ion Ratio	Lower	Upper	
164	100		
162	101.9	81.0	121.6
160	50.5	40.7	61.1






Abundance Scan 1425 (15.818 min): BN014350.D\data.ms (-1419) (-)

2,4,6-Tribromophenol
Concen: 5.51 ng
RT: 15.818 min Scan# 1425
Delta R.T. -0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21




Tgt Ion:	330	Resp:	28651
Ion Ratio	Lower	Upper	
330	100		
332	0.0	0.0	0.0
141	33.0	26.2	39.2






Abundance Scan 1198 (12.938 min): BN014350.D\data.ms (-1195) (-)

2-Fluorobiphenyl
Concen: 4.85 ng
RT: 12.938 min Scan# 1198
Delta R.T. -0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Tgt Ion:	172	Resp:	273781
Ion Ratio	Lower	Upper	
172	100		
171	34.8	28.2	42.2
170	24.1	19.6	29.4







Abundance Scan 1285 (14.042 min): BN014350.D\data.ms (-1276) (-)

Acenaphthylene
Concen: 5.97 ng
RT: 14.042 min Scan# 1285
Delta R.T. -0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21



Tgt Ion:	152	Resp:	326622
Ion Ratio	Lower	Upper	
152	100		
151	19.3	15.6	23.4
153	13.0	10.5	15.7









Acenaphthene
Concen: 5.15 ng
RT: 14.384 min Scan# 1312
Delta R.T. -0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:	154	Resp:	209812
Ion Ratio	Lower	Upper	
154	100		
153	109.5	89.2	133.8
152	56.8	49.0	73.4



Fluorene
Concen: 5.35 ng
RT: 15.374 min Scan# 1390
Delta R.T. -0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21


Tgt Ion:	166	Resp:	265590
Ion Ratio	Lower	Upper	
166	100		
165	97.4	78.6	118.0
167	13.5	10.9	16.3





Abundance Scan 1527 (17.067 min): BN014350.D\data.ms (-1511) (-)

Phenanthrene-d10
Concen: 0.40 ng
RT: 17.067 min Scan# 1527
Delta R.T. 0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

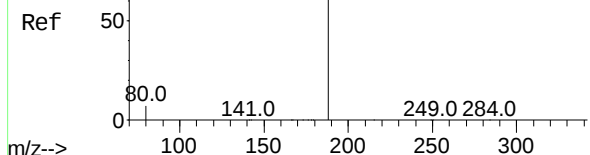

Tgt Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	7.7	6.2	9.4






Abundance Scan 1527 (17.067 min): BN014354.D\data.ms (-1511) (-)




Abundance Scan 1396 (15.450 min): BN014350.D\data.ms (-1320) (-)

4,6-Dinitro-2-methylphenol
Concen: 6.94 ng
RT: 15.450 min Scan# 1396
Delta R.T. -0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

Tgt Ion	Ratio	Lower	Upper
198	100		
51	20.2	60.0	90.0#
105	23.7	31.5	47.3#




Abundance Scan 1396 (15.450 min): BN014354.D\data.ms (-1388) (-)






Abundance Scan 1461 (16.264 min): BN014350.D\data.ms (-1427) (-)

4-Bromophenyl-phenylether
Concen: 5.42 ng
RT: 16.264 min Scan# 1461
Delta R.T. 0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Tgt Ion:	248	Resp:	82936
Ion Ratio	Lower	Upper	
248	100		
250	96.7	77.4	116.0
141	49.9	41.4	62.0






Abundance Scan 1470 (16.374 min): BN014350.D\data.ms (-1429) (-)

Hexachlorobenzene
Concen: 5.53 ng
RT: 16.374 min Scan# 1470
Delta R.T. 0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21




Tgt Ion:	284	Resp:	108520
Ion Ratio	Lower	Upper	
284	100		
142	33.0	26.5	39.7
249	29.4	24.0	36.0





Abundance Scan 1483 (16.532 min): BN014350.D\data.ms (-1429) (-)

Atrazine
Concen: 6.08 ng
RT: 16.532 min Scan# 1483
Delta R.T. 0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0



Tgt Ion:	200	Resp:	57850
Ion Ratio	Lower	Upper	
200	100		
173	26.8	21.0	31.6
215	47.2	38.7	58.1




Abundance Scan 1483 (16.532 min): BN014354.D\data.ms (-1442) (-)





Abundance Scan 1498 (16.714 min): BN014350.D\data.ms (-1424) (-)


Pentachlorophenol
Concen: 4.94 ng
RT: 16.715 min Scan# 1498
Delta R.T. 0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

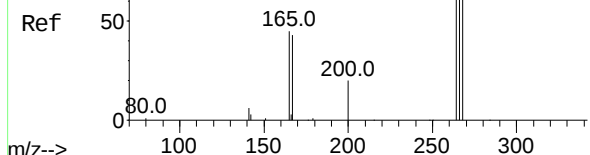


Tgt Ion:	266	Resp:	26292
Ion Ratio	Lower	Upper	
266	100		
264	62.3	50.6	76.0
268	64.2	51.4	77.0



Abundance Scan 1498 (16.715 min): BN014354.D\data.ms (-1490) (-)





Abundance Scan 1530 (17.104 min): BN014350.D\data.ms (-1525) (-)




Phenanthrene
Concen: 5.13 ng
RT: 17.104 min Scan# 1530
Delta R.T. 0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	178	Resp:	415366
Ion	Ratio	Lower	Upper
178	100		
176	19.0	15.2	22.8
179	15.3	12.2	18.4



Abundance Scan 1530 (17.104 min): BN014354.D\data.ms (-1505) (-)





Abundance Scan 1538 (17.201 min): BN014350.D\data.ms (-1525) (-)




Anthracene
Concen: 5.69 ng
RT: 17.201 min Scan# 1538
Delta R.T. 0.000 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

Tgt Ion:	178	Resp:	368142
Ion	Ratio	Lower	Upper
178	100		
176	18.5	15.0	22.4
179	15.3	12.2	18.2




Abundance Scan 1538 (17.201 min): BN014354.D\data.ms (-1530) (-)






Abundance Scan 1825 (19.101 min): BN014350.D\data.ms (-1827) (-)

Fluoranthene-d10
Concen: 5.34 ng
RT: 19.104 min Scan# 1824
Delta R.T. 0.003 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0







Tgt Ion:	212	Resp:	425678
Ion Ratio	Lower	Upper	
212	100		
106	11.9	9.7	14.5
104	6.7	5.4	8.0



Abundance Scan 1831 (19.131 min): BN014350.D\data.ms (-1829) (-)

Fluoranthene
Concen: 5.41 ng
RT: 19.134 min Scan# 1830
Delta R.T. 0.003 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

Tgt Ion:	202	Resp:	482878
Ion Ratio	Lower	Upper	
202	100		
101	10.2	8.2	12.4
203	17.4	13.8	20.6



Abundance Scan 2125 (21.258 min): BN014350.D\data.ms (-2129) (-)

Chrysene-d12

Concen: 0.40 ng

RT: 21.261 min Scan# 2124

Delta R.T. 0.003 min

Lab File: BN014354.D


Acq: 21 Apr 2021 13:21

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0






Tgt Ion:240 Resp: 32782

Ion Ratio Lower Upper

240 100

120 12.4 10.7 16.1

236 27.2 21.5 32.3



Abundance Scan 1905 (19.498 min): BN014350.D\data.ms (-1896) (-)

Pyrene

Concen: 5.11 ng

RT: 19.496 min Scan# 1903

Delta R.T. -0.002 min

Lab File: BN014354.D

Acq: 21 Apr 2021 13:21





Tgt Ion:202 Resp: 475783

Ion Ratio Lower Upper

202 100

200 20.6 16.6 24.8


203 17.5 14.1 21.1






Abundance Scan 1947 (19.707 min): BN014350.D\data.ms (-1934) (-)

Terphenyl-d14
Concen: 4.88 ng
RT: 19.710 min Scan# 1946
Delta R.T. 0.003 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.4	6.2	9.4
122	10.2	9.3	13.9






Abundance Scan 2124 (21.247 min): BN014350.D\data.ms (-2132) (-)


Benzo(a)anthracene
Concen: 5.43 ng
RT: 21.250 min Scan# 2123
Delta R.T. 0.003 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21



Tgt Ion	Ratio	Lower	Upper
228	100		
226	26.2	21.3	31.9
229	19.8	15.7	23.5




Abundance Scan 2129 (21.300 min): BN014350.D\data.ms (-2129) (-)

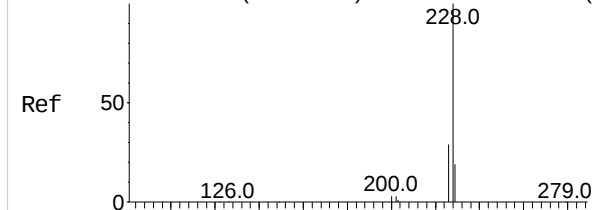


Chrysene
Concen: 4.74 ng
RT: 21.303 min Scan# 2128
Delta R.T. 0.003 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Abundance Scan 2128 (21.303 min): BN014354.D\data.ms




Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.6	23.1	34.7
229	19.9	15.7	23.5



Abundance Scan 2128 (21.303 min): BN014354.D\data.ms (-2118) (-)




Abundance Scan 2118 (21.184 min): BN014350.D\data.ms (-2118) (-)




Bis(2-ethylhexyl)phthalate
Concen: 6.27 ng
RT: 21.186 min Scan# 2117
Delta R.T. 0.003 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21


Abundance Scan 2117 (21.186 min): BN014354.D\data.ms



Tgt Ion	Ratio	Lower	Upper
149	100		
167	26.3	21.3	31.9
279	3.7	3.1	4.7




Abundance Scan 2117 (21.186 min): BN014354.D\data.ms (-2107) (-)






Abundance Scan 3203 (25.725 min): BN014350.D\data.ms (-3175) (-)

Indeno(1,2,3-cd)pyrene
Concen: 4.27 ng
RT: 25.724 min Scan# 3201
Delta R.T. -0.001 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Tgt Ion:	276	Resp:	544280
Ion Ratio	Lower	Upper	
276	100		
138	23.3	18.9	28.3
277	24.9	19.8	29.8






Abundance Scan 2550 (23.490 min): BN014350.D\data.ms (-2536) (-)


Perylene-d12
Concen: 0.40 ng
RT: 23.493 min Scan# 2549
Delta R.T. 0.003 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21



Tgt Ion:	264	Resp:	24477
Ion Ratio	Lower	Upper	
264	100		
260	24.4	19.8	29.6
265	43.4	34.4	51.6





Abundance Scan 2354 (22.819 min): BN014350.D\data.ms (-2354) (-)




Benzo(b)fluoranthene
Concen: 4.50 ng
RT: 22.822 min Scan# 2353
Delta R.T. 0.003 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

Tgt Ion:	252	Resp:	479478
Ion	Ratio	Lower	Upper
252	100		
253	21.9	19.0	28.6
125	9.4	9.7	14.5#


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0



Abundance Scan 2353 (22.822 min): BN014354.D\data.ms (-2294) (-)





Abundance Scan 2367 (22.864 min): BN014350.D\data.ms (-2367) (-)




Benzo(k)fluoranthene
Concen: 4.73 ng
RT: 22.870 min Scan# 2367
Delta R.T. 0.006 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

Tgt Ion:	252	Resp:	486694
Ion	Ratio	Lower	Upper
252	100		
253	22.0	19.3	28.9
125	9.1	9.4	14.2#




Abundance Scan 2367 (22.870 min): BN014354.D\data.ms (-2278) (-)





Abundance Scan 2521 (23.391 min): BN014350.D\data.ms (-2509) (-)

Benzo(a)pyrene
Concen: 5.37 ng
RT: 23.393 min Scan# 2520
Delta R.T. 0.003 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0



Tgt Ion:	252	Resp:	421214
Ion Ratio	Lower	Upper	
252	100		
253	21.9	20.7	31.1
125	10.6	11.8	17.6#





Abundance Scan 2520 (23.393 min): BN014354.D\data.ms (-2461) (-)




Abundance Scan 3207 (25.739 min): BN014350.D\data.ms (-3186) (-)

Dibenzo(a,h)anthracene
Concen: 4.91 ng
RT: 25.741 min Scan# 3206
Delta R.T. 0.003 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21


Tgt Ion:	278	Resp:	456812
Ion Ratio	Lower	Upper	
278	100		
139	15.2	13.3	19.9
279	23.5	20.2	30.2



Abundance Scan 3206 (25.741 min): BN014354.D\data.ms (-3182) (-)




Abundance Scan 3403 (26.410 min): BN014350.D\data.ms (-3343) (-)




Benzo(g,h,i)perylene
Concen: 4.74 ng
RT: 26.412 min Scan# 3402
Delta R.T. 0.003 min
Lab File: BN014354.D
Acq: 21 Apr 2021 13:21

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Abundance Scan 3402 (26.412 min): BN014354.D\data.ms



Tgt Ion:	276	Resp:	466704
Ion	Ratio	Lower	Upper
276	100		
277	23.7	19.1	28.7
138	19.6	16.7	25.1



Abundance Scan 3402 (26.412 min): BN014354.D\data.ms (-3343) (-)

