
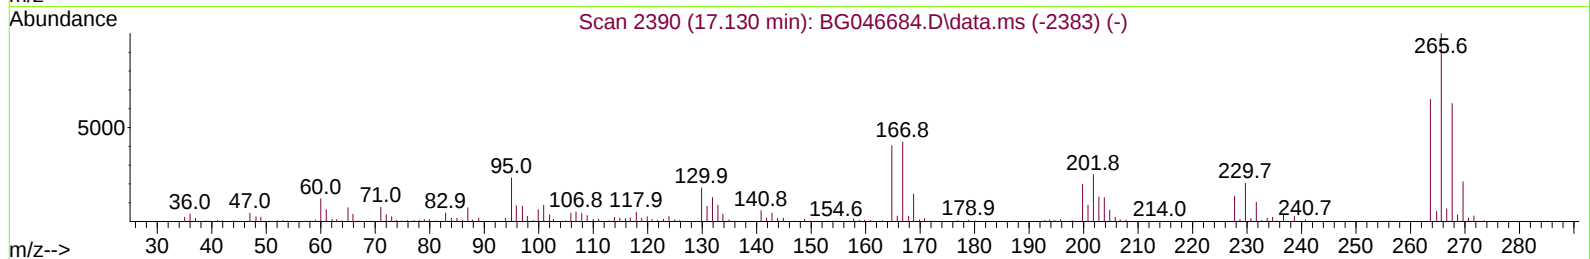
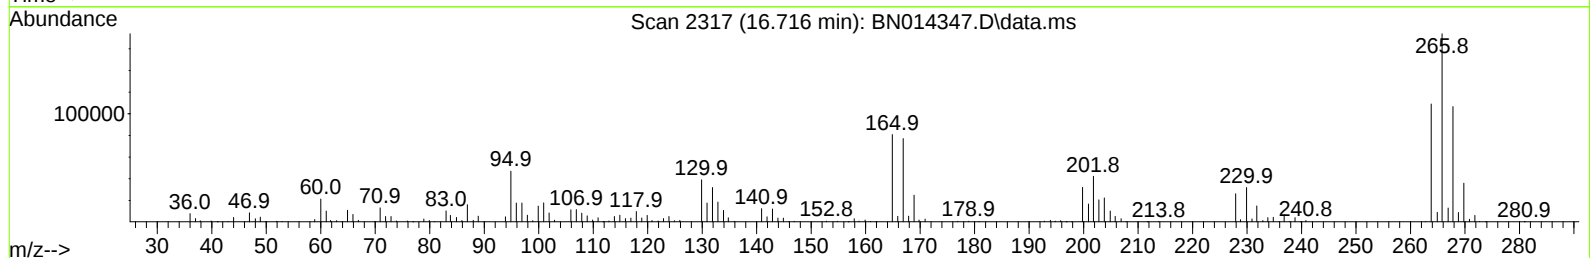


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042221\
 Data File : BN014347.D
 Acq On : 21 Apr 2021 09:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 05:56:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 09 09:55:03 2021
 Response via : Initial Calibration

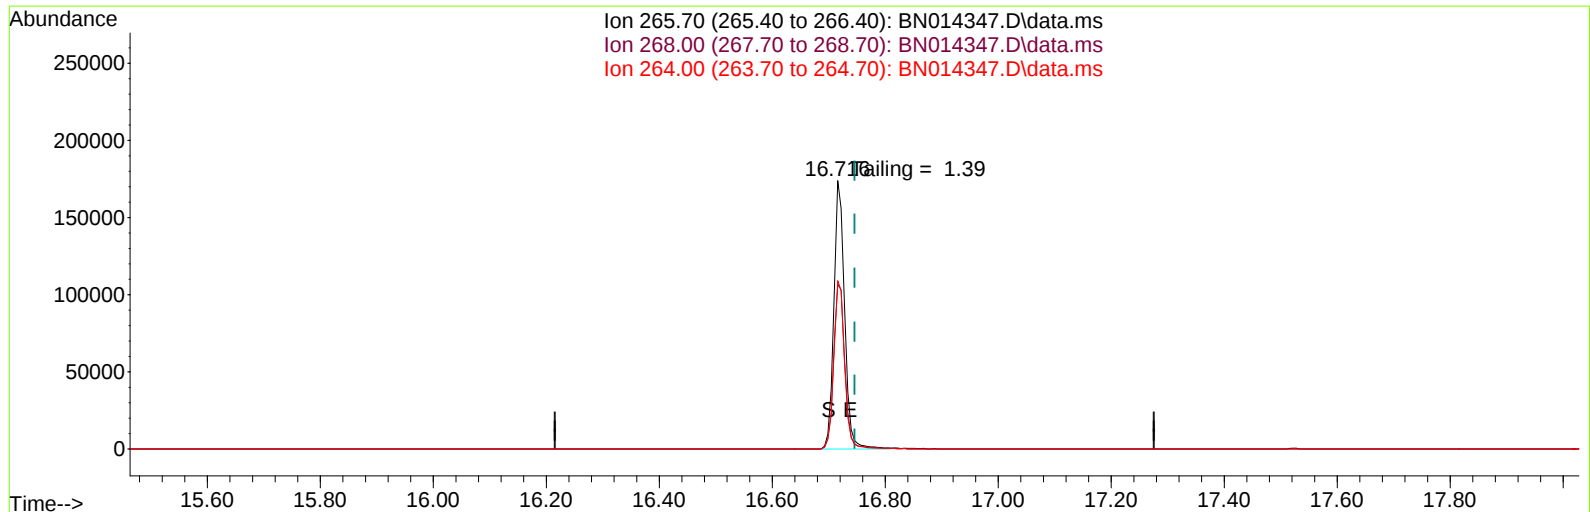

TIC: BN014347.D\data.ms

(70) Pentachlorophenol (C)




16.716min (-0.029) 21884.93 ng

response 229798

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.33
264.00	61.60	62.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042221\
Data File : BN014347.D
Acq On : 21 Apr 2021 09:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 05:56:32 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

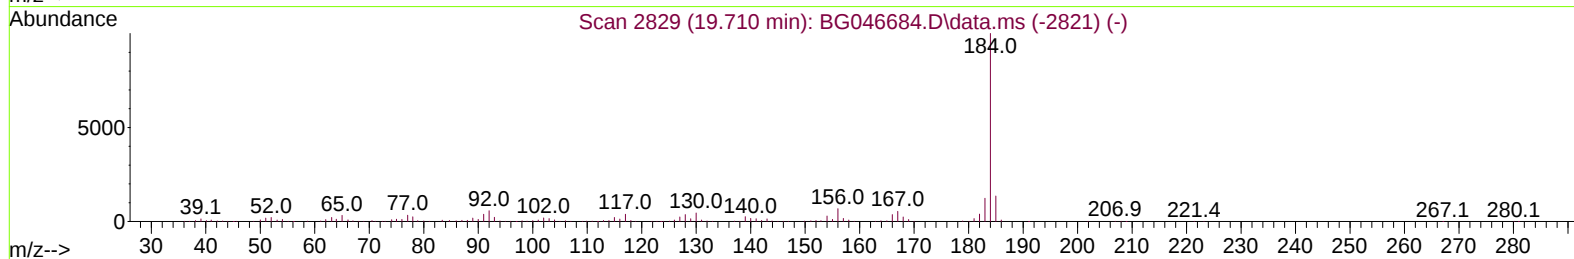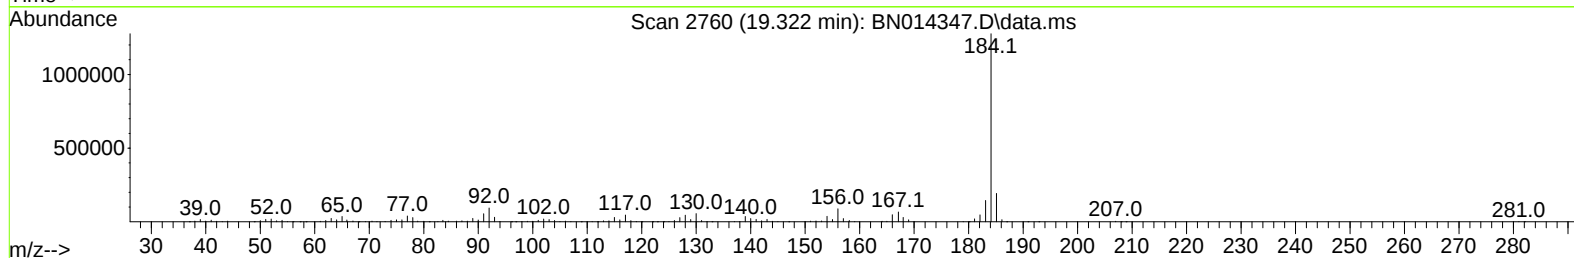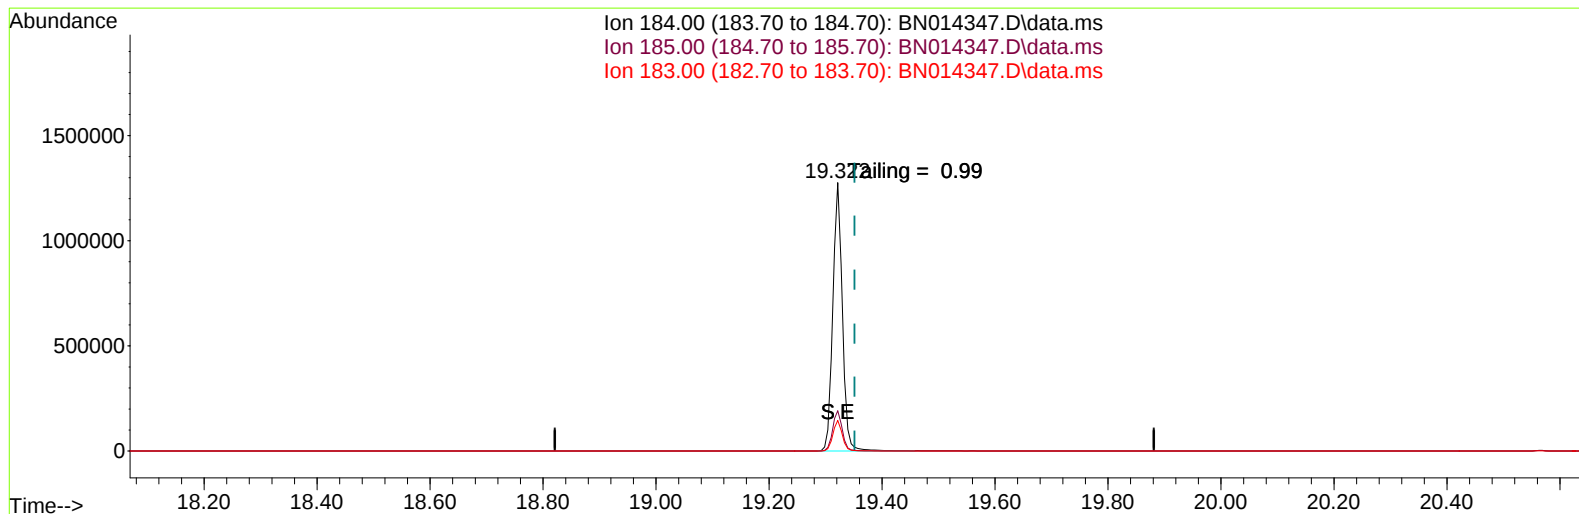

TIC: BN014347.D\data.ms

(77) Benzidine

19.322min (-0.029) 0.00 ng

response 1505166

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.07
183.00	13.20	11.38
0.00	0.00	0.00