


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042221\
 Data File : BN014362.D
 Acq On : 21 Apr 2021 19:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 21 13:57:02 2021

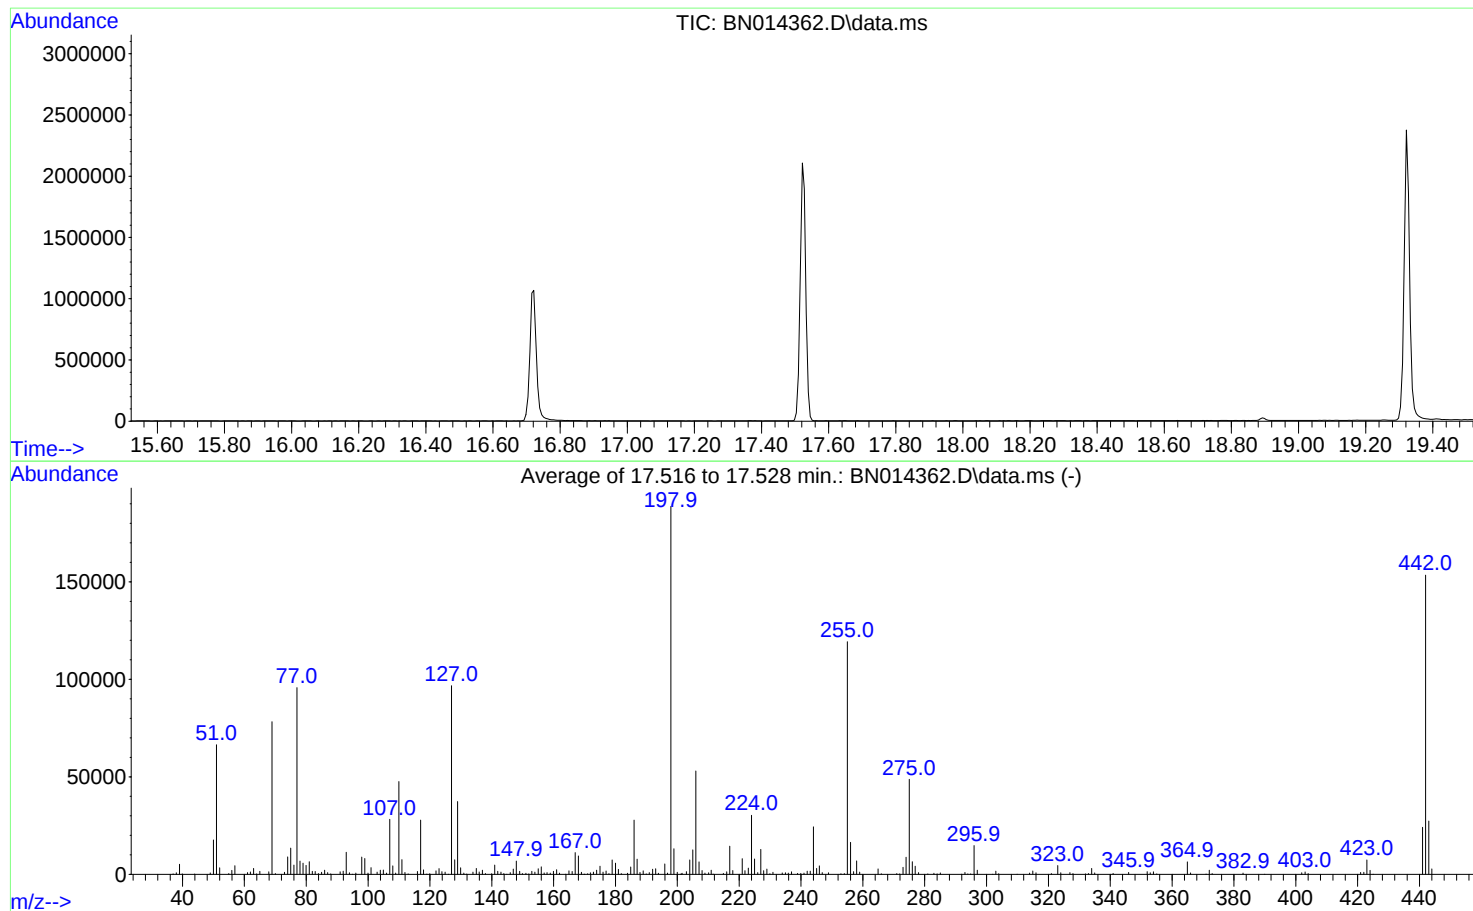




AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	66443	PASS
68	69	0.00	2	1.7	1300	PASS
69	198	0.00	100	41.5	78299	PASS
70	69	0.00	2	0.6	436	PASS
127	198	10	80	51.3	96699	PASS
197	198	0.00	2	0.4	677	PASS
198	198	100	100	100.0	188629	PASS
199	198	5	9	7.0	13154	PASS
275	198	10	60	25.8	48709	PASS
365	198	1	100	3.4	6428	PASS
441	198	0.01	100	12.8	24120	PASS
442	442	50	100	100.0	153451	PASS
443	442	15	24	17.8	27319	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042221\
Data File : BN014362.D
Acq On : 21 Apr 2021 19:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 22 03:15:49 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

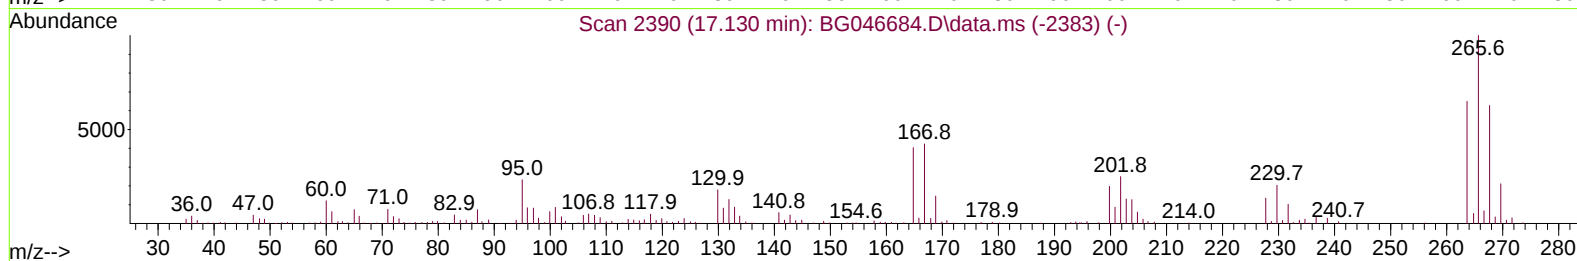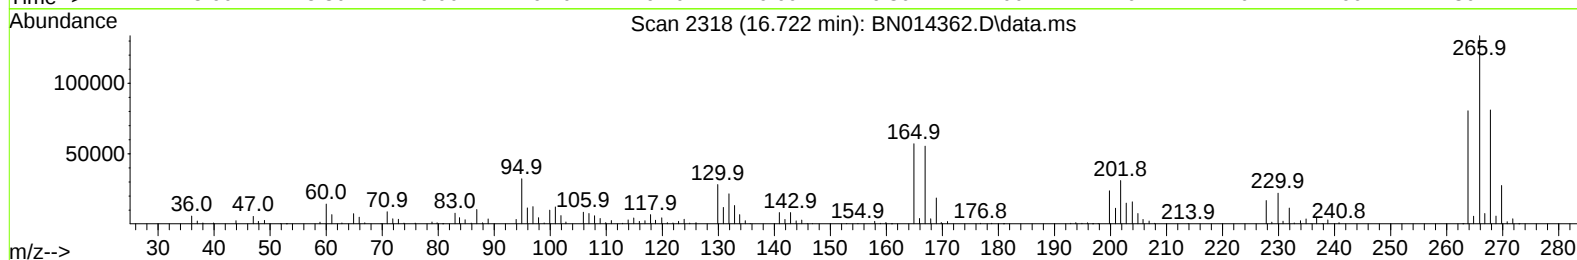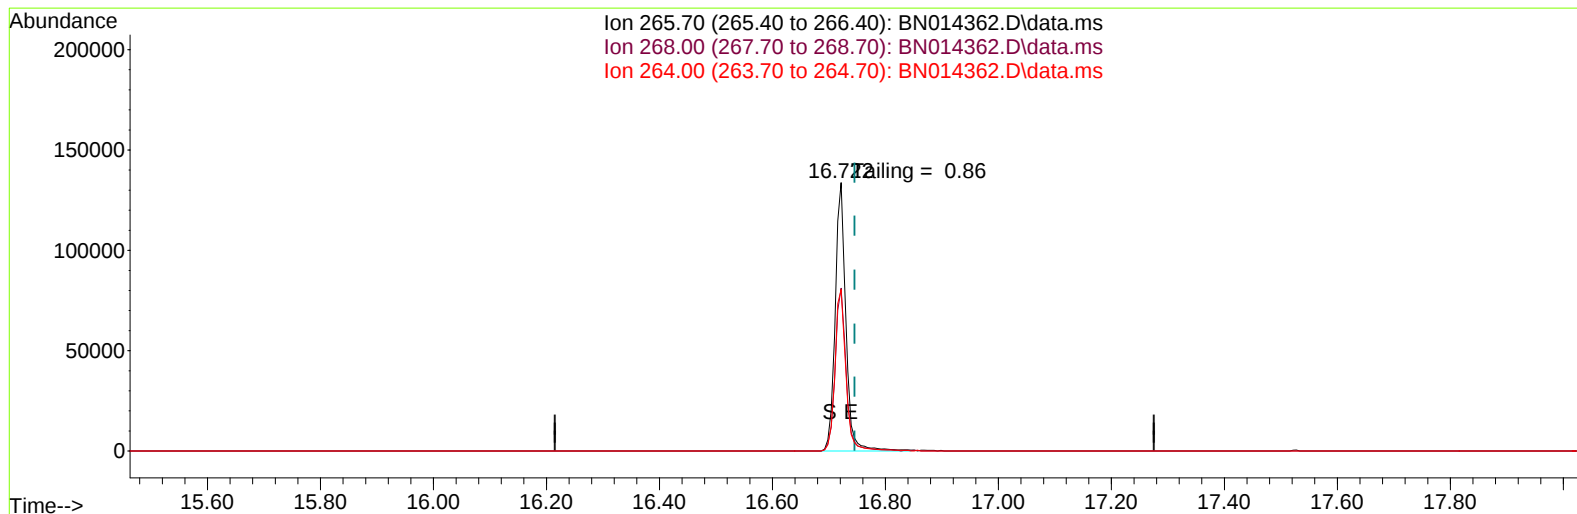

TIC: BN014362.D\data.ms

(70) Pentachlorophenol (C)

16.722min (-0.024) 17593.46 ng




response 175900

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.64
264.00	61.60	60.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042221\
Data File : BN014362.D
Acq On : 21 Apr 2021 19:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 22 03:15:49 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

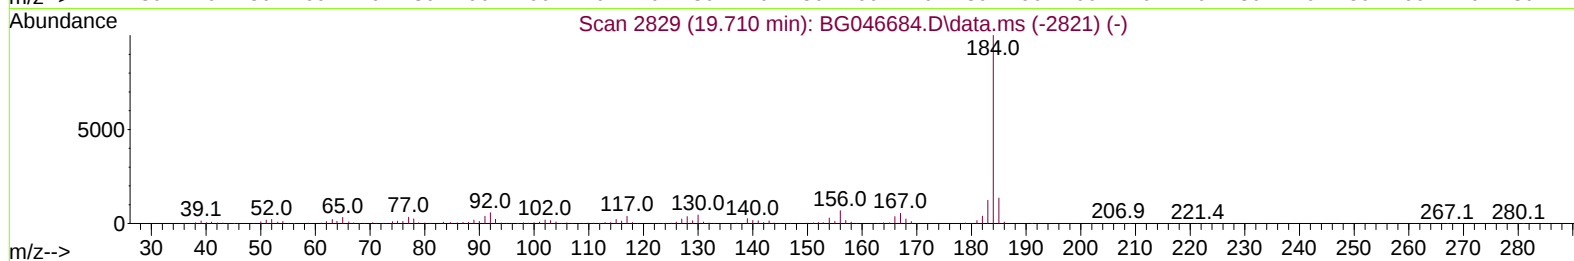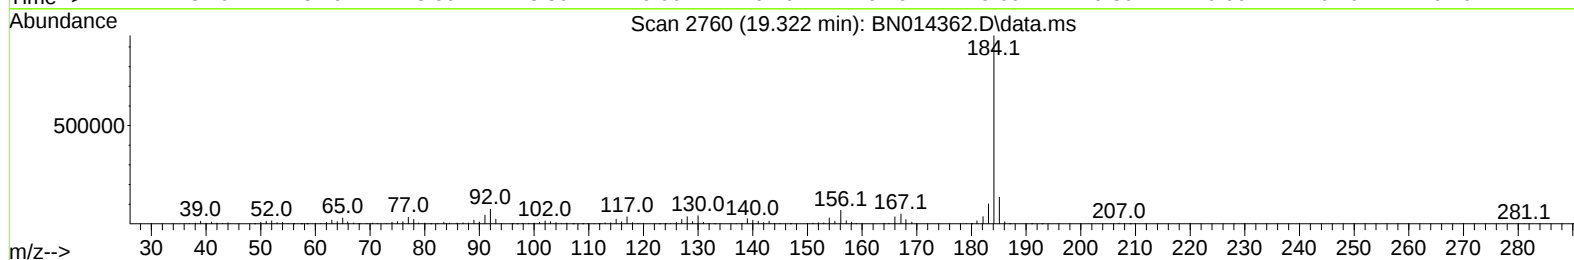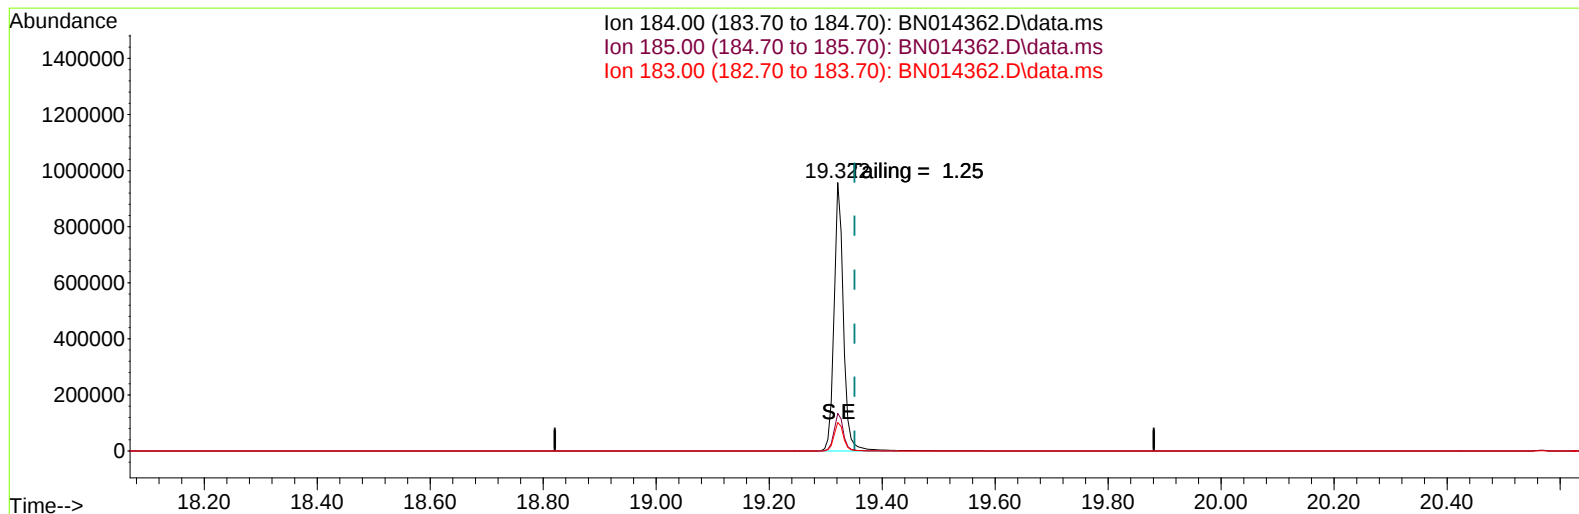

TIC: BN014362.D\data.ms

(77) Benzidine

19.322min (-0.029) 0.00 ng

response 1109038

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.06
183.00	13.20	10.60
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
4/22/2021	BNA_N	<u>BN014362.D</u>
Compound Name	Response	Retention Time
DDT	646289	20.569
DDD	2122	20.122
DDE	448	19.616
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2570	648859	0.40

Instrument :
BNA_N
ClientSampleId :
DFTPP