

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
 Data File : BN025091.D
 Acq On : 23 Apr 2023 00:40
 Operator : CG/JU
 Sample : 02399-01DL 20X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COML8DL

Quant Time: Apr 23 01:56:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 23 01:54:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	279290	20.000	ng/ul	0.00
20) Naphthalene-d8	10.728	136	1286428	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.563	164	829394	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.310	188	1895010	20.000	ng/ul	0.00
79) Chrysene-d12	21.504	240	1956909	20.000	ng/ul	0.00
88) Perylene-d12	23.945	264	2239536	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	1761	0.240	ng/uL	0.00
4) Pyridine-d5	3.722	84	304	0.014	ng/ul	0.00
7) Phenol-d5	7.081	99	7173	0.263	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.246	67	29736	1.633	ng/ul	0.00
11) 2-Chlorophenol-d4	7.446	132	21451	1.072	ng/ul	0.00
15) 4-Methylphenol-d8	8.628	113	14346	0.664	ng/ul	0.00
21) Nitrobenzene-d5	9.087	128	14448	1.387	ng/ul	0.00
24) 2-Nitrophenol-d4	9.816	143	13347	1.183	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.351	165	23716	1.176	ng/ul	0.00
31) 4-Chloroaniline-d4	10.875	131	31766	1.038	ng/ul	0.00
46) Dimethylphthalate-d6	13.975	166	107202	1.667	ng/ul	0.00
49) Acenaphthylene-d8	14.257	160	97026	1.317	ng/ul	0.00
54) 4-Nitrophenol-d4	14.798	143	476	0.036	ng/ul	0.04
60) Fluorene-d10	15.557	176	94602	1.743	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200	5736	0.465	ng/ul	0.00
73) Anthracene-d10	17.410	188	147999	1.663	ng/ul	0.00
81) Pyrene-d10	19.704	212	186509	1.641	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.786	264	186677	1.594	ng/ul	0.00
Target Compounds						
					Qvalue	
22) Nitrobenzene	9.128	77	870943	31.118	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025091.D
Acq On : 23 Apr 2023 00:40
Operator : CG/JU
Sample : 02399-01DL 20X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COML8DL

Quant Time: Apr 23 01:56:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 01:54:00 2023
Response via : Initial Calibration

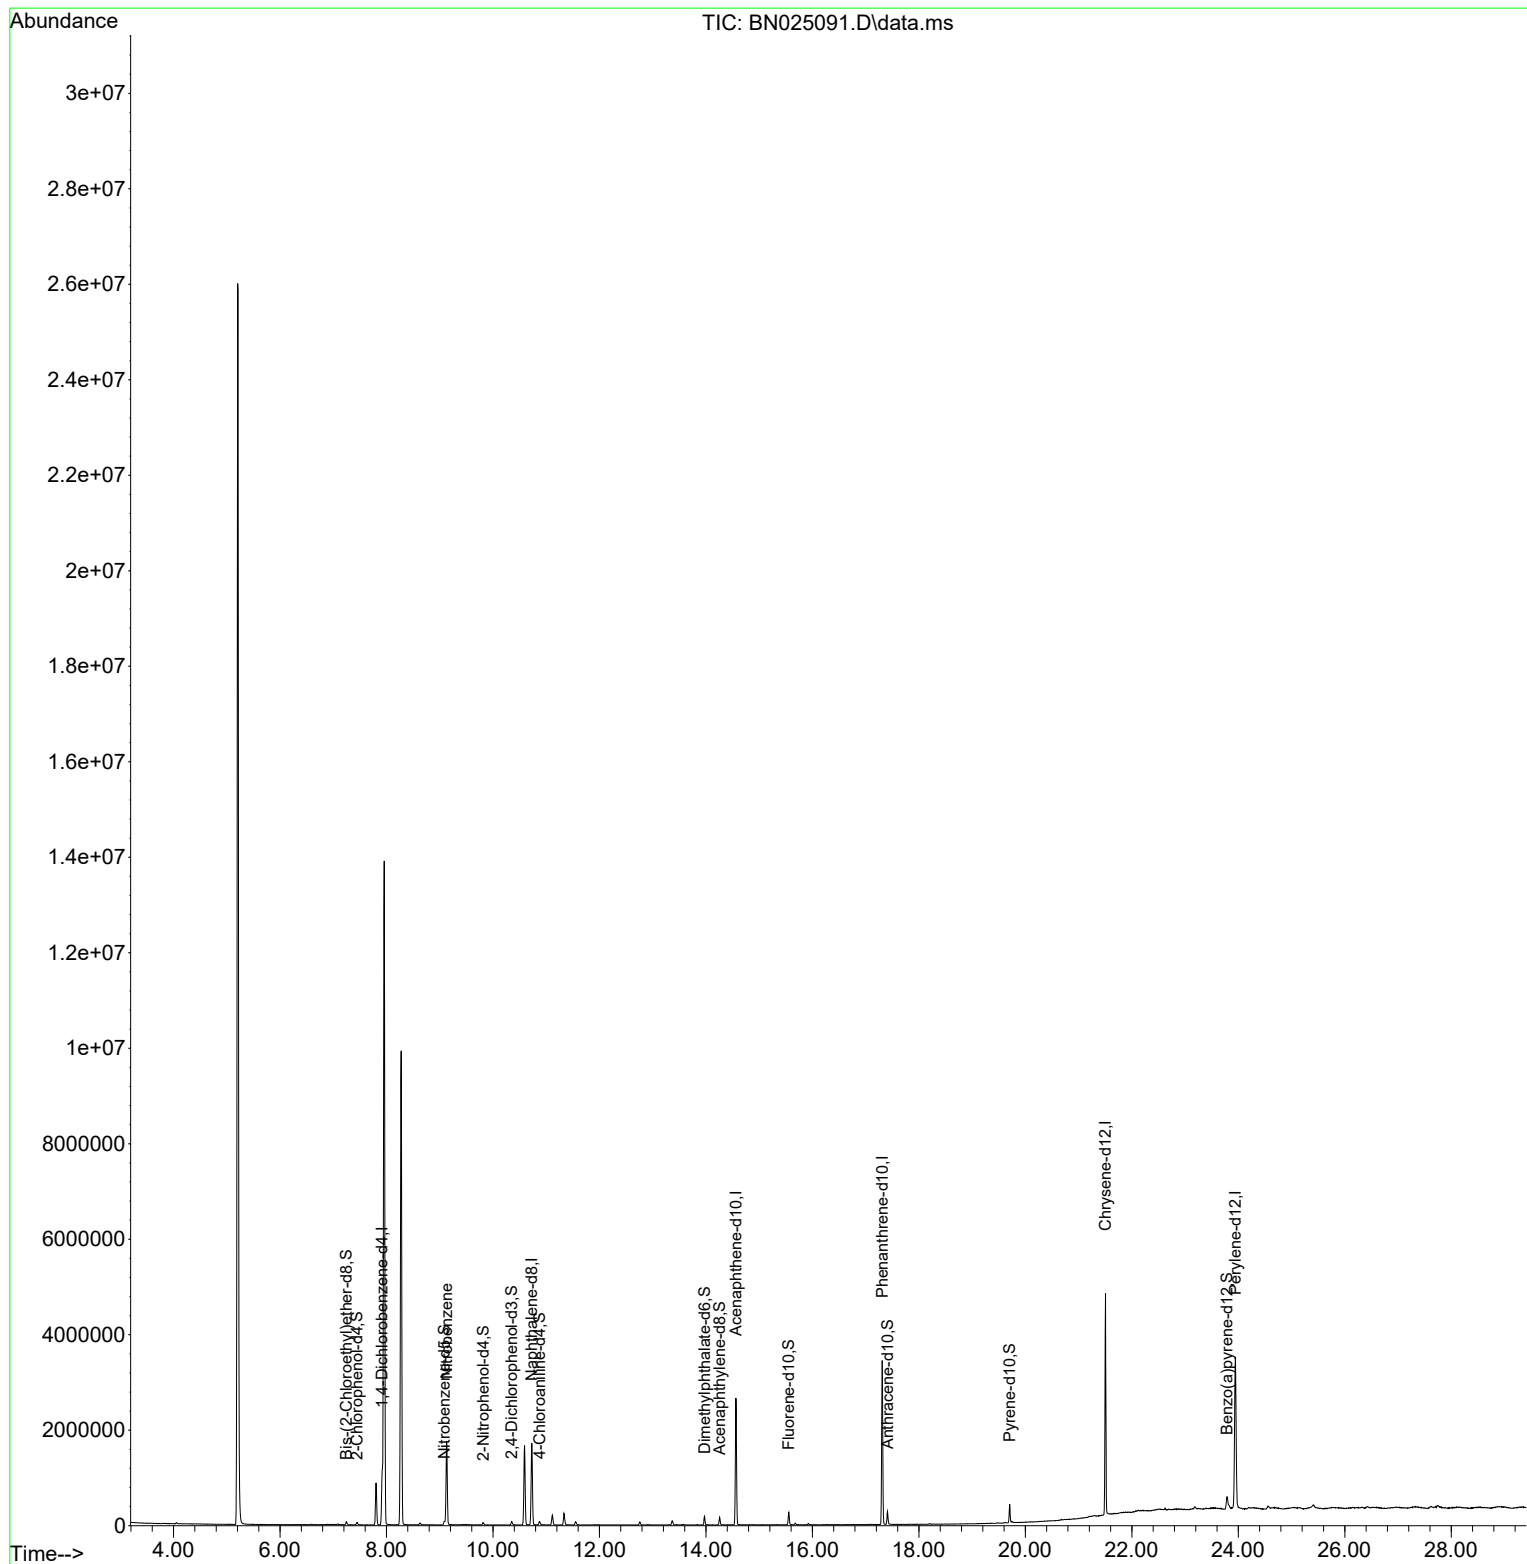

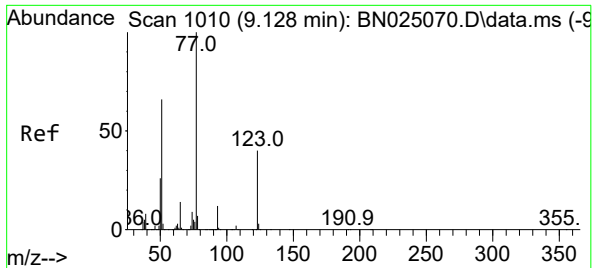

#22
 Nitrobenzene
 Concen: 31.118 ng/ul
 RT: 9.128 min Scan# 10
 Delta R.T. -0.000 min
 Lab File: BN025091.D
 Acq: 23 Apr 2023 00:40

Instrument :
 BNA_N
 ClientSampleId :
 COML8DL

Tgt Ion: 77 Resp: 870943
 Ion Ratio Lower Upper
 77 100
 123 39.9 33.5 50.3
 65 14.2 11.8 17.8

