




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
 Data File : BN025095.D
 Acq On : 23 Apr 2023 03:03
 Operator : CG/JU
 Sample : 02399-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMP3

Manual IntegrationsAPPROVED

Quant Time: Apr 23 03:36:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 23 01:54:00 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/24/2023
 Supervised By :Jagrut Upadhyay 04/24/2023

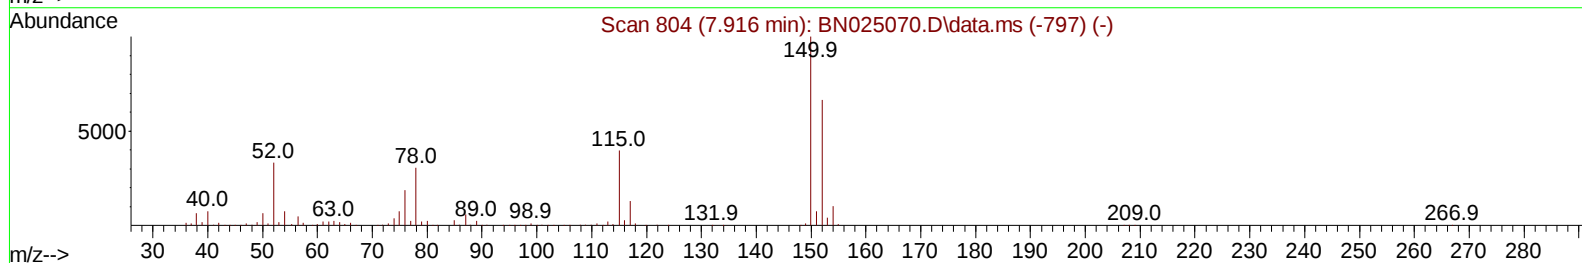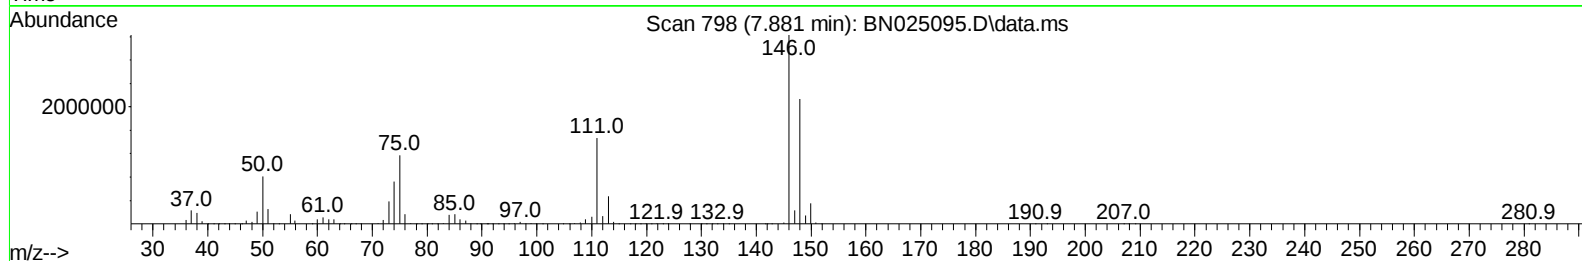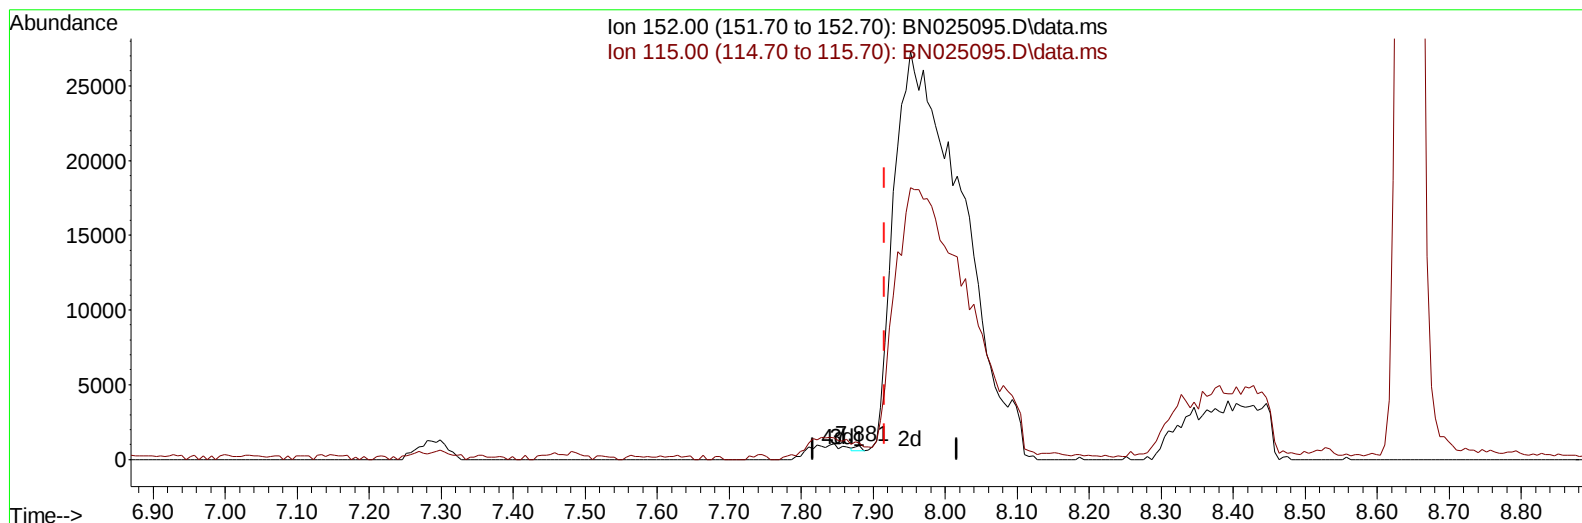

TIC: BN025095.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.881min (-0.035) 20.00 ng/u1

response 225

Ion	Exp%	Act%
152.00	100.00	100.00
115.00	63.90	118.66#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025095.D
Acq On : 23 Apr 2023 03:03
Operator : CG/JU
Sample : 02399-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMP3

Manual IntegrationsAPPROVED

Quant Time: Apr 23 03:36:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 01:54:00 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/24/2023
Supervised By :Jagrut Upadhyay 04/24/2023

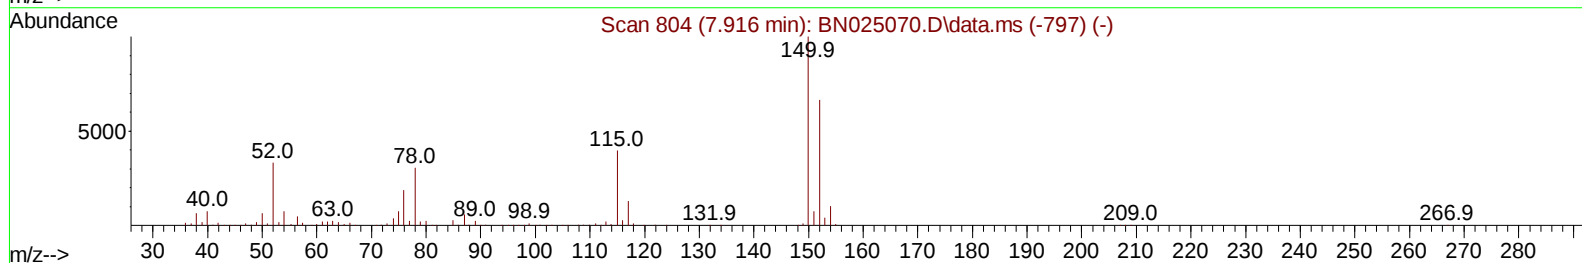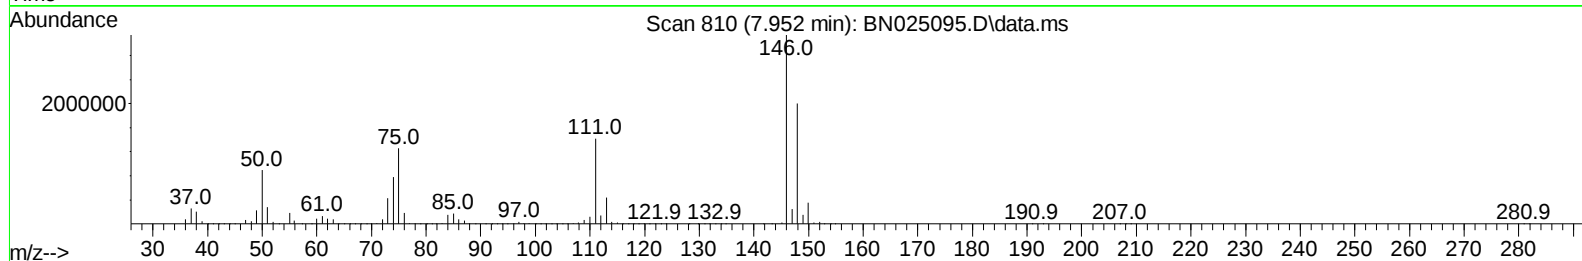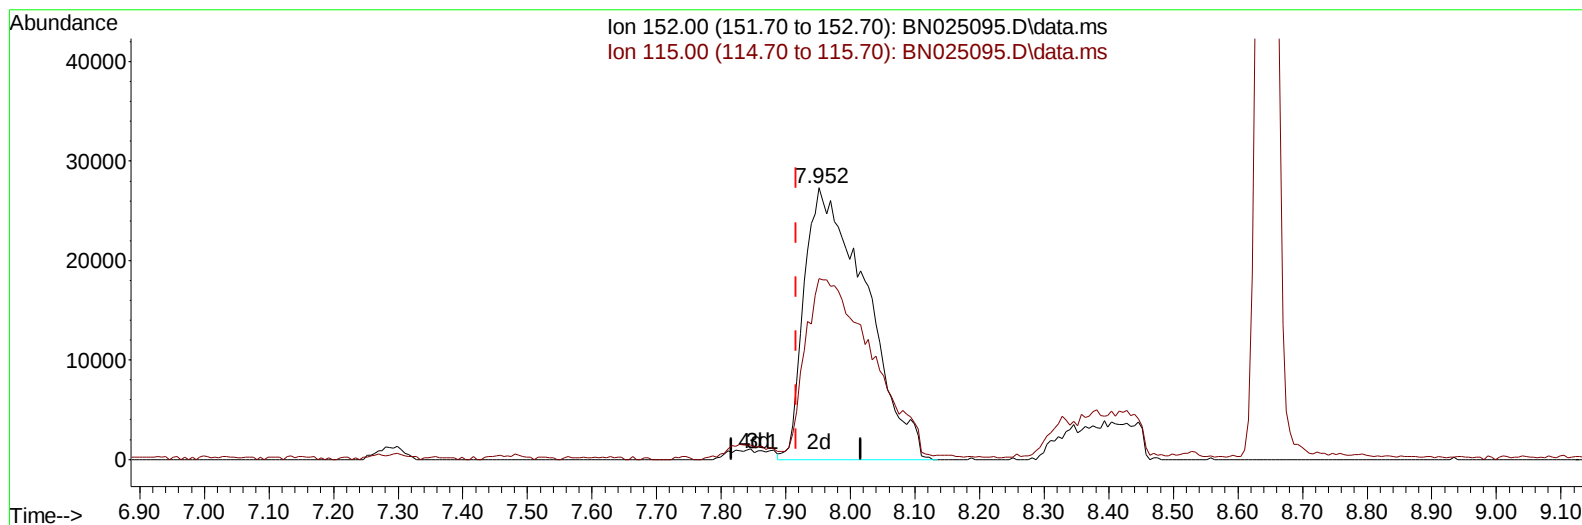

TIC: BN025095.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.952min (+ 0.036) 20.00 ng/ul m

response 181460

Ion	Exp%	Act%
152.00	100.00	100.00
115.00	63.90	66.54
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
 Data File : BN025095.D
 Acq On : 23 Apr 2023 03:03
 Operator : CG/JU
 Sample : 02399-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMP3

Manual IntegrationsAPPROVED

Quant Time: Apr 23 03:36:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 23 01:54:00 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/24/2023
 Supervised By :Jagrut Upadhyay 04/24/2023

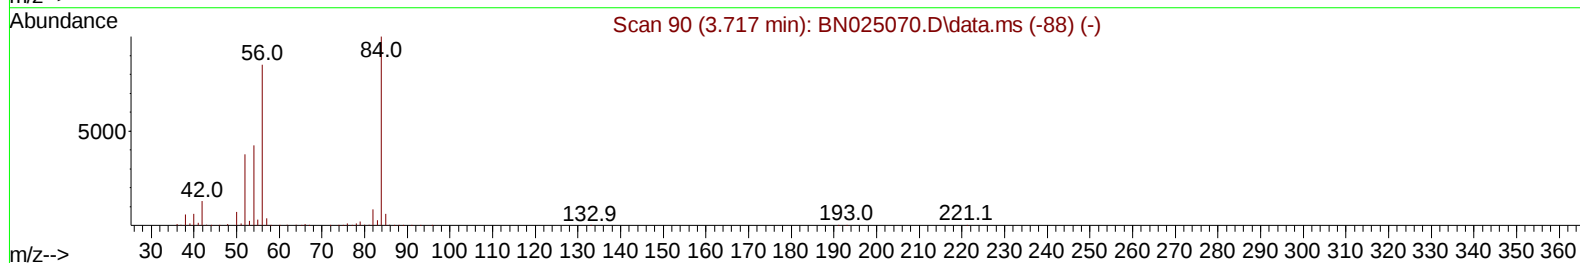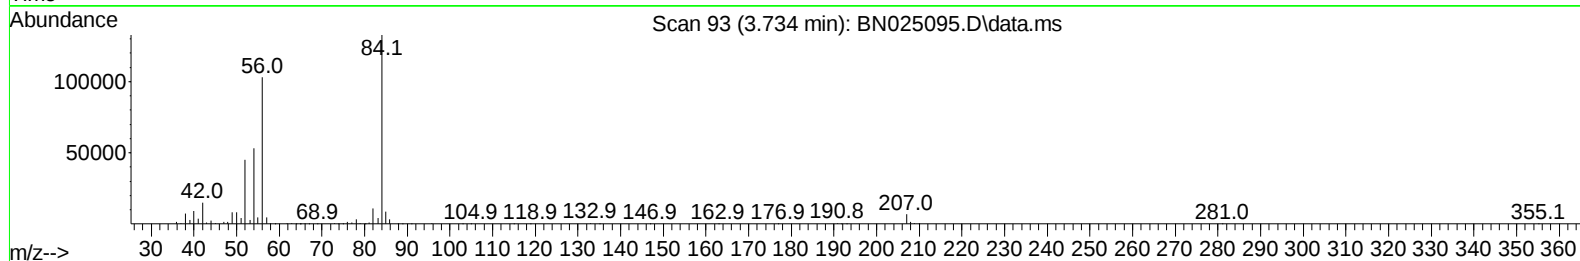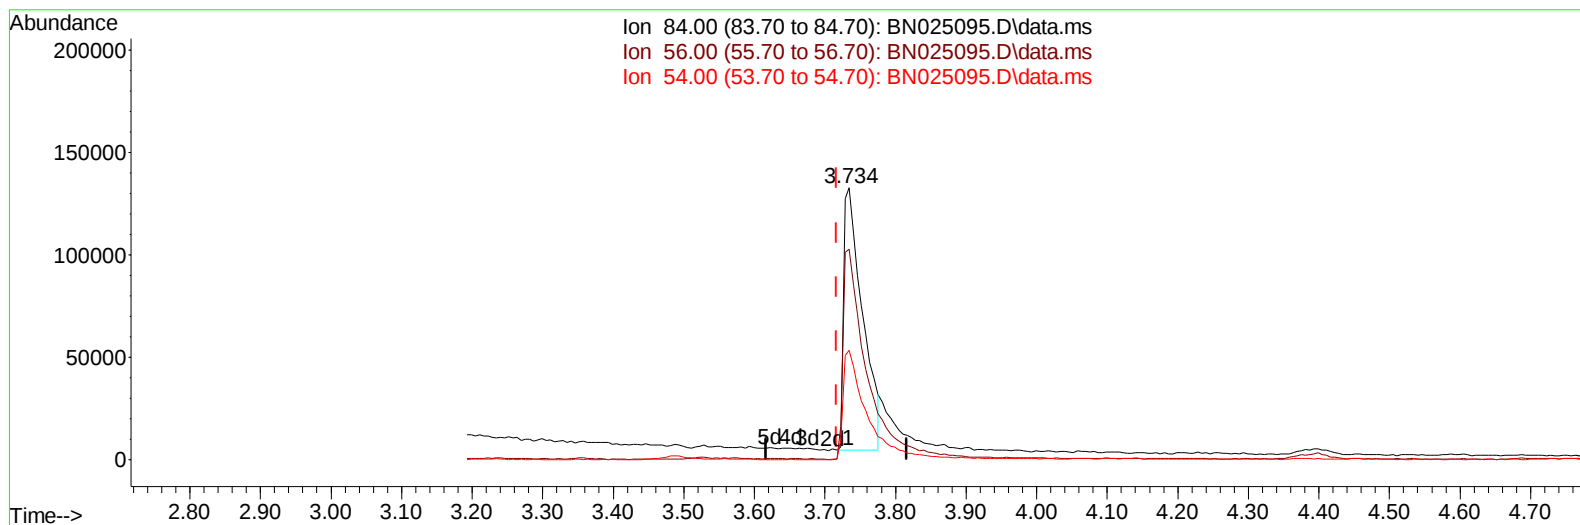

TIC: BN025095.D\data.ms

(4) Pyridine-d5 (S)

3.734min (+ 0.018) 16.70 ng/u1

response 238383

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	82.10	77.52
54.00	40.20	40.22
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
 Data File : BN025095.D
 Acq On : 23 Apr 2023 03:03
 Operator : CG/JU
 Sample : 02399-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMP3

Manual IntegrationsAPPROVED

Quant Time: Apr 23 03:36:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 23 01:54:00 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/24/2023
 Supervised By :Jagrut Upadhyay 04/24/2023

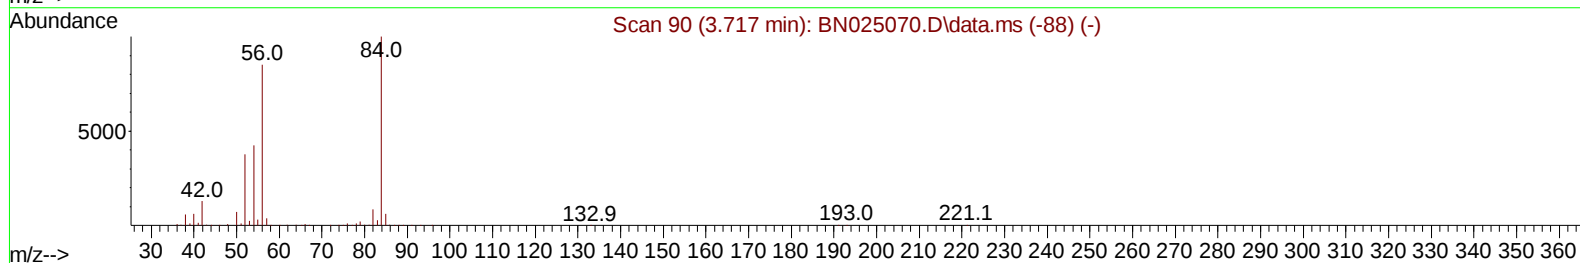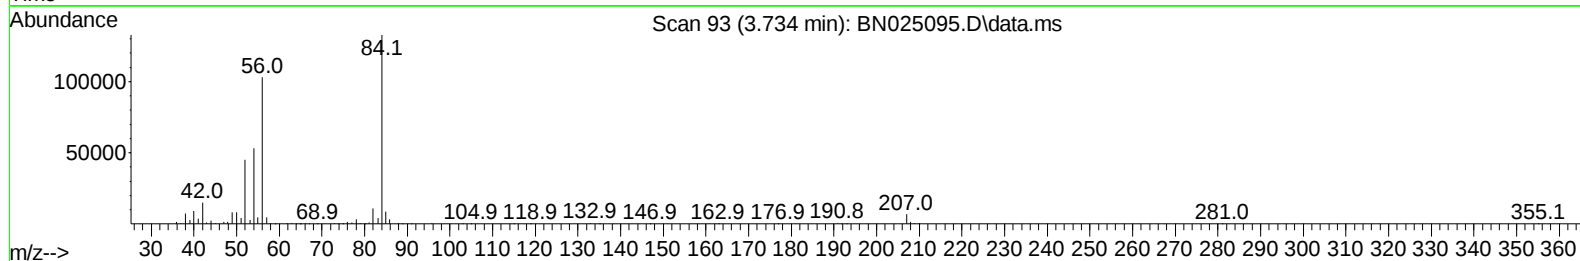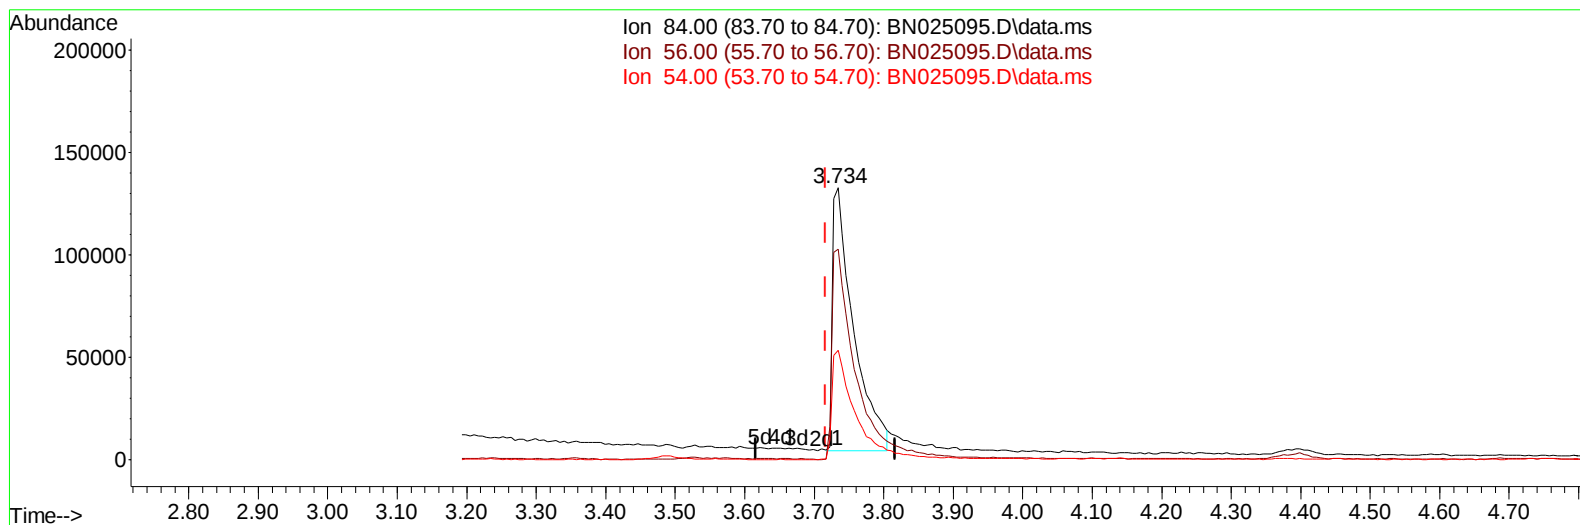

TIC: BN025095.D\data.ms

(4) Pyridine-d5 (S)

3.734min (+ 0.018) 18.80 ng/ul m

response 268383

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	82.10	77.52
54.00	40.20	40.22
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025095.D
Acq On : 23 Apr 2023 03:03
Operator : CG/JU
Sample : 02399-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMP3

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/24/2023
Supervised By :Jagrut Upadhyay 04/24/2023

Quant Time: Apr 23 03:36:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 01:54:00 2023
Response via : Initial Calibration

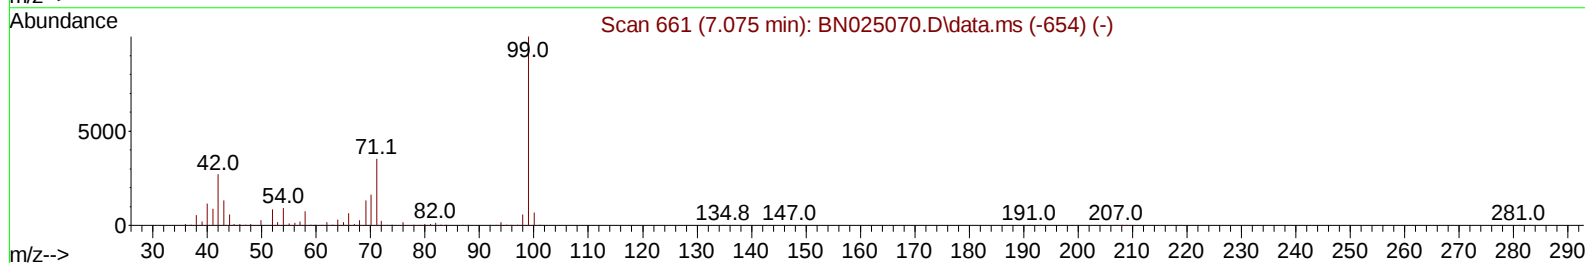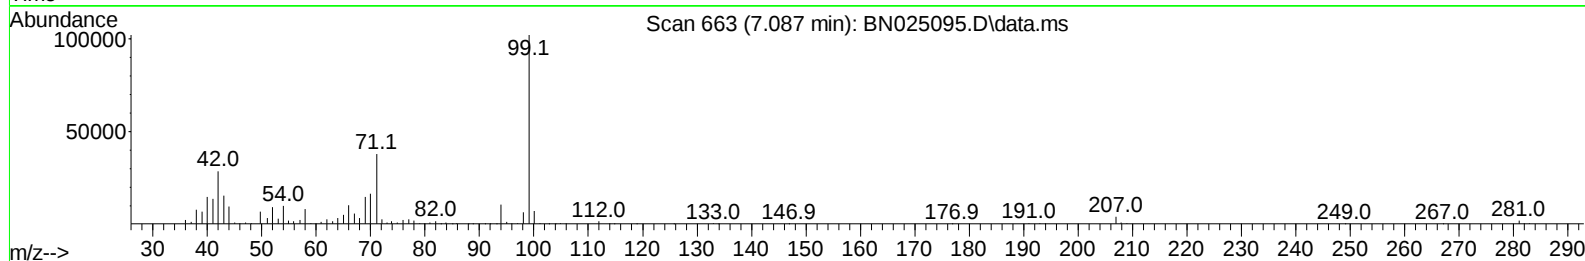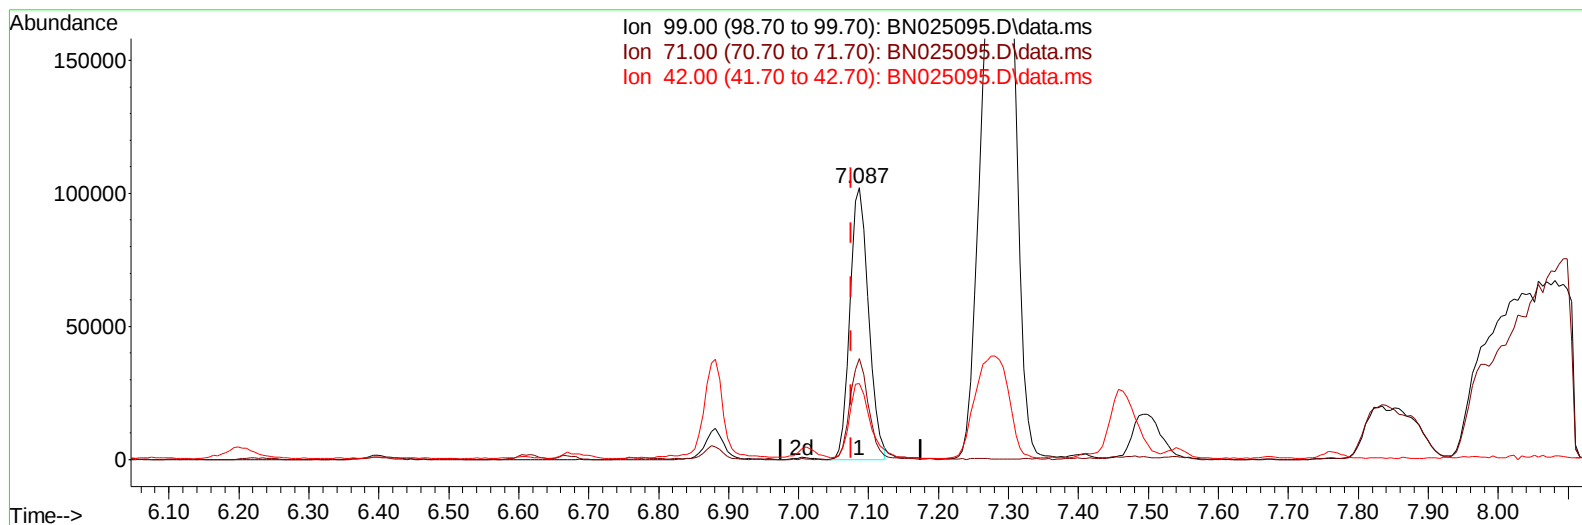

TIC: BN025095.D\data.ms

(7) Phenol-d5 (S)

7.087min (+ 0.012) 10.60 ng/u1

response 187502

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	35.10	37.11
42.00	26.10	27.93
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
 Data File : BN025095.D
 Acq On : 23 Apr 2023 03:03
 Operator : CG/JU
 Sample : 02399-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMP3

Manual IntegrationsAPPROVED

Quant Time: Apr 23 03:36:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 23 01:54:00 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/24/2023
 Supervised By :Jagrut Upadhyay 04/24/2023

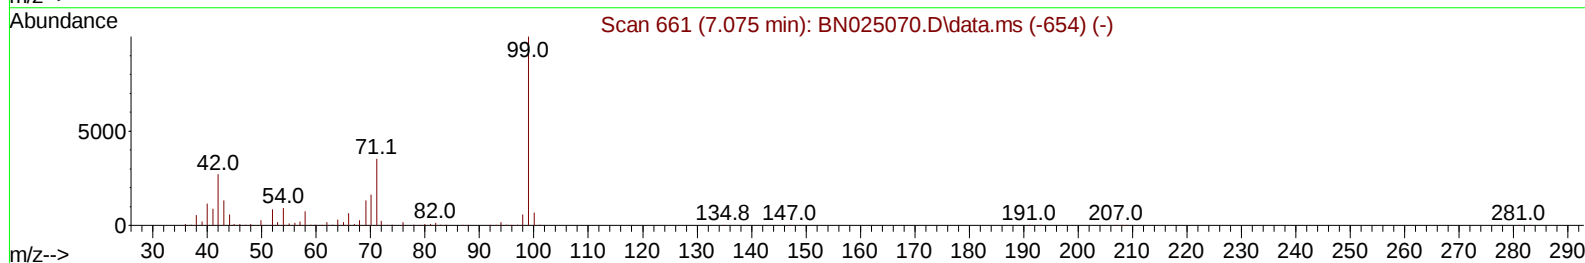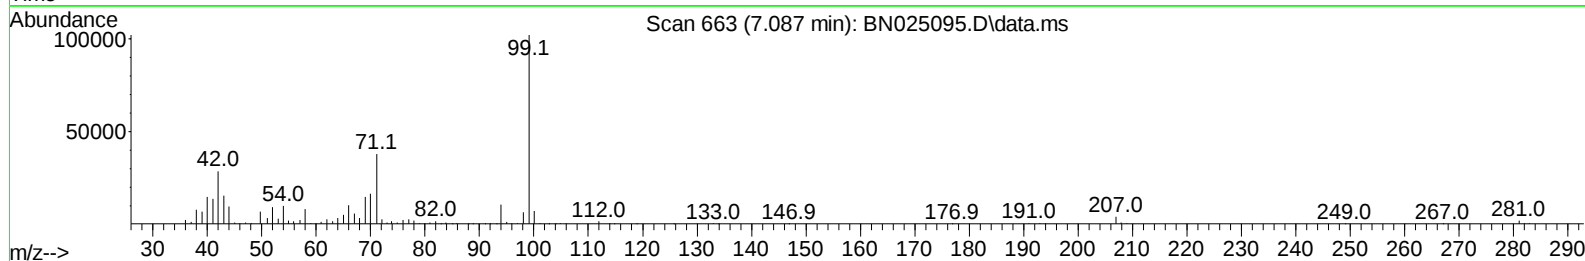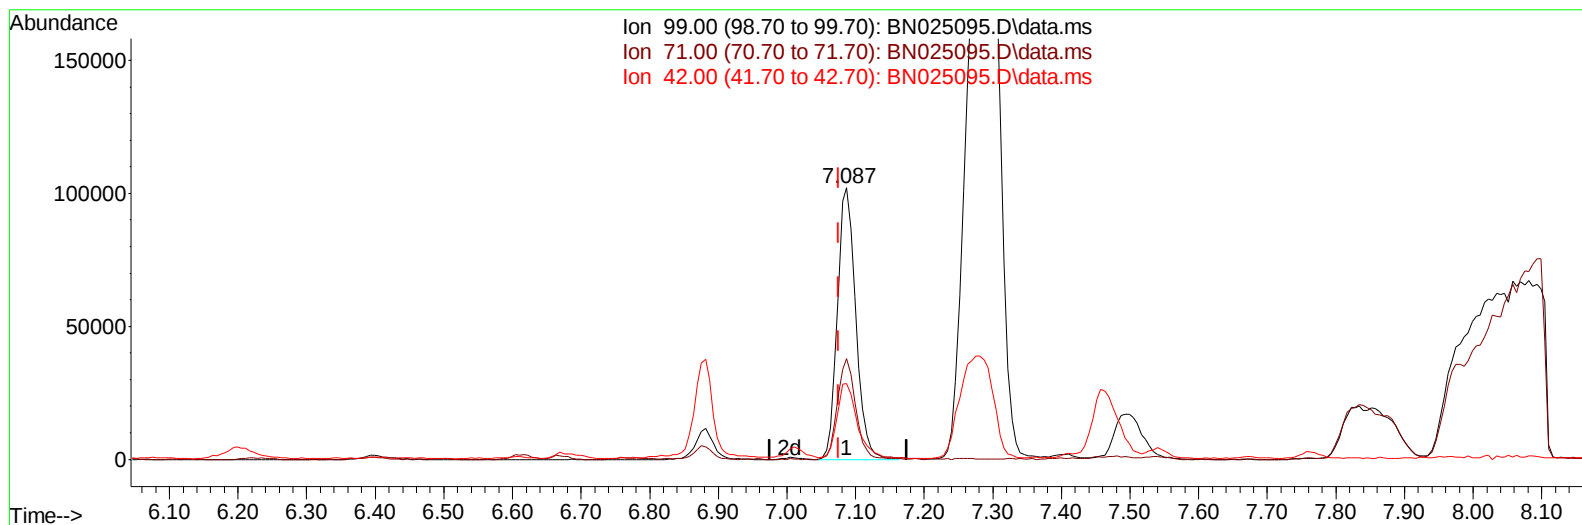

TIC: BN025095.D\data.ms

(7) Phenol-d5 (S)

7.087min (+ 0.012) 10.75 ng/ul m

response 190189

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	35.10	37.11
42.00	26.10	27.93
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
 Data File : BN025095.D
 Acq On : 23 Apr 2023 03:03
 Operator : CG/JU
 Sample : 02399-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMP3

Manual IntegrationsAPPROVED

Quant Time: Apr 23 03:36:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 23 01:54:00 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/24/2023
 Supervised By :Jagrut Upadhyay 04/24/2023

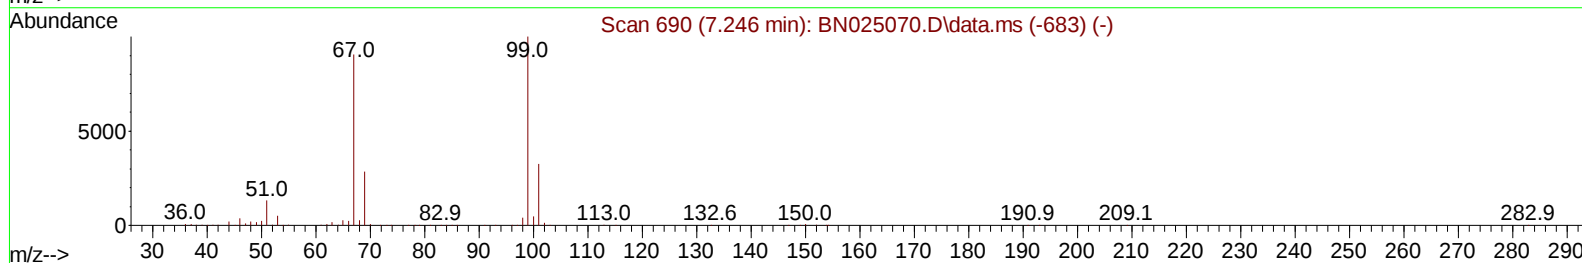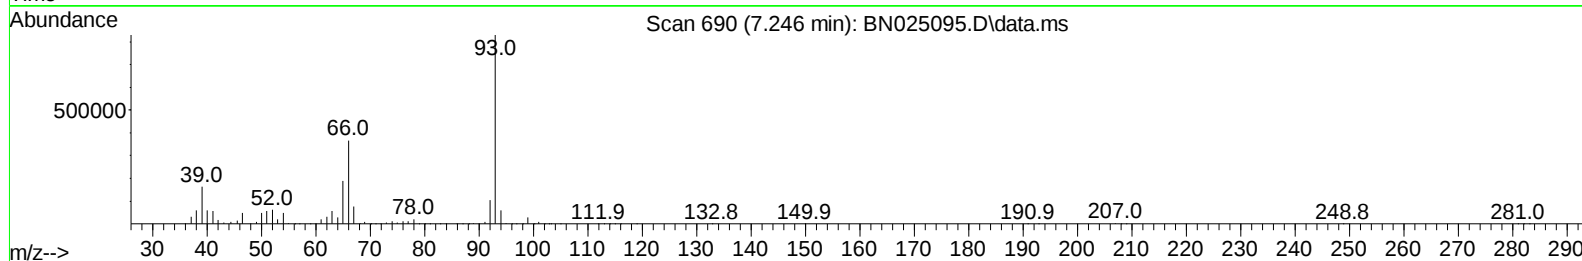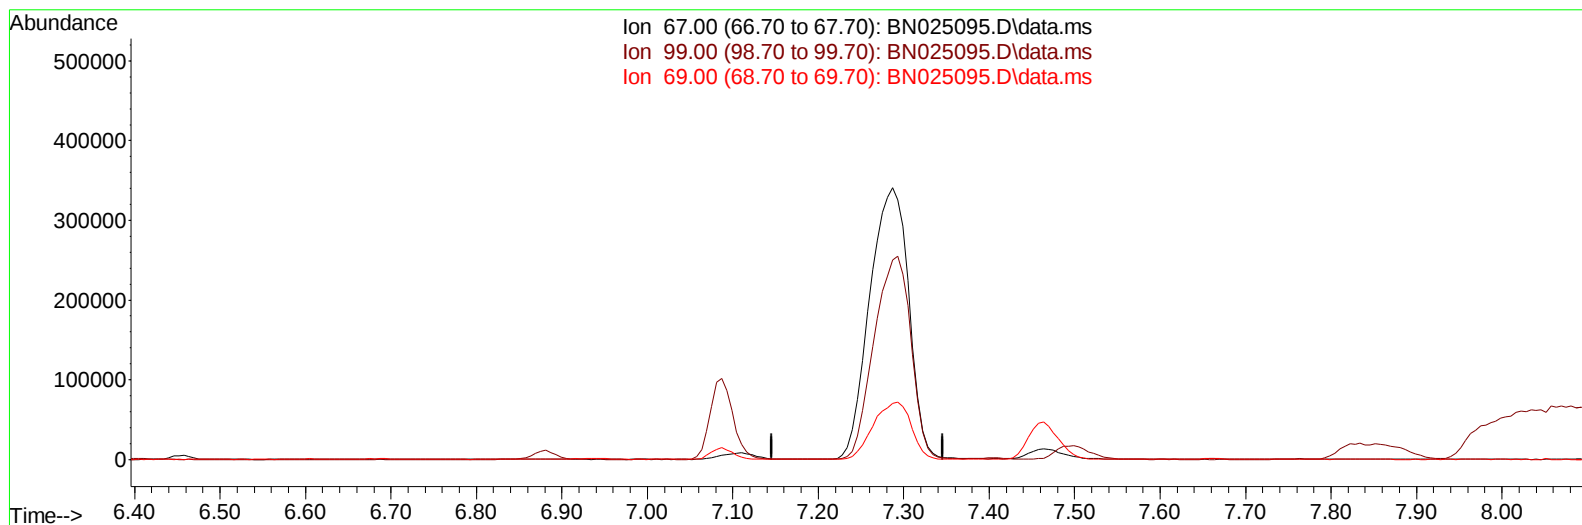

TIC: BN025095.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.246min (-7.246) 0.00 ng/u1

response 0

Ion	Exp%	Act%
67.00	100.00	0.00
99.00	108.30	0.00#
69.00	30.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025095.D
Acq On : 23 Apr 2023 03:03
Operator : CG/JU
Sample : 02399-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMP3

Manual IntegrationsAPPROVED

Quant Time: Apr 23 03:36:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 01:54:00 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/24/2023
Supervised By :Jagrut Upadhyay 04/24/2023

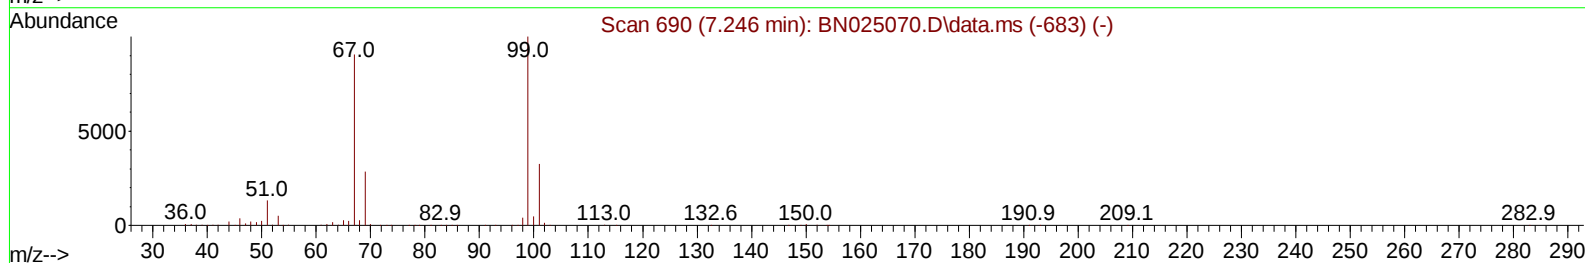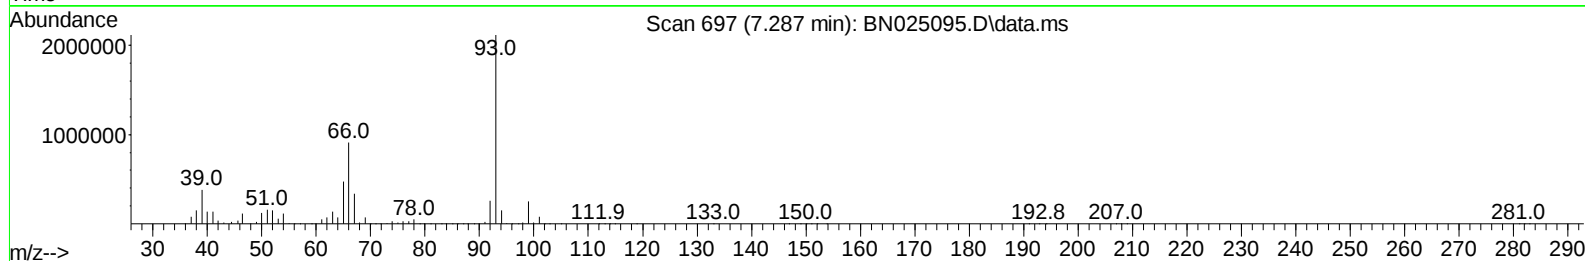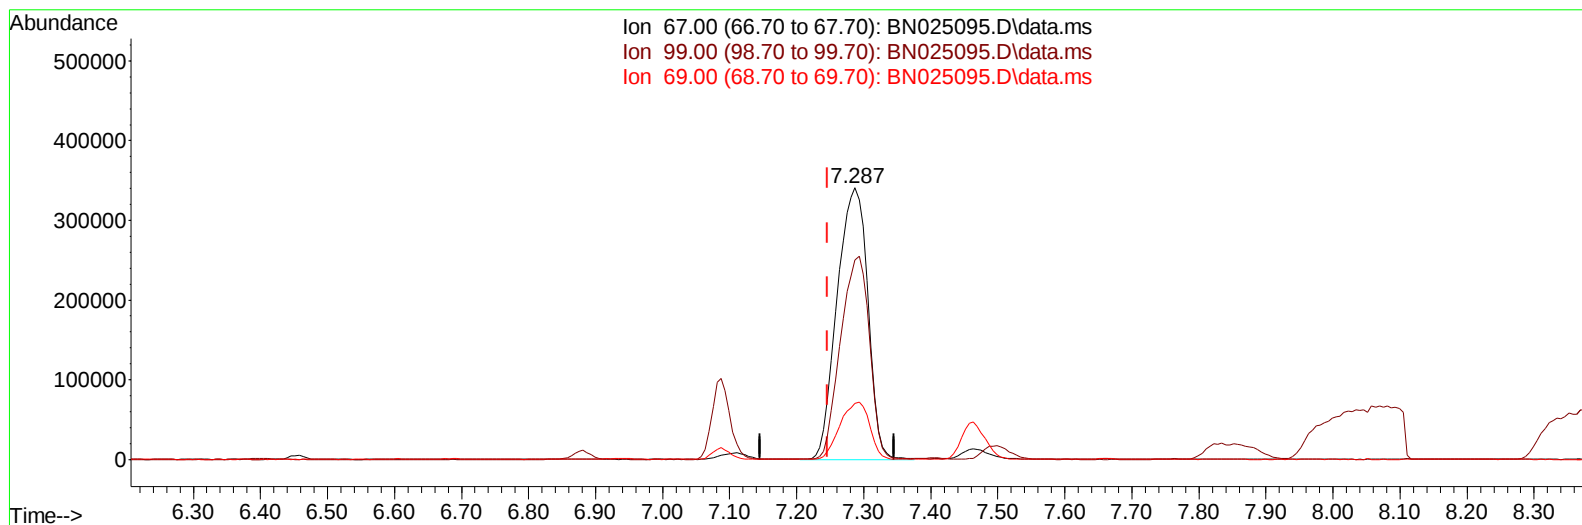

TIC: BN025095.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.287min (+ 0.041) 91.69 ng/ul m

response 1084953

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	108.30	73.36#
69.00	30.20	20.75#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025095.D
Acq On : 23 Apr 2023 03:03
Operator : CG/JU
Sample : 02399-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMP3

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/24/2023
Supervised By :Jagrut Upadhyay 04/24/2023

Quant Time: Apr 23 03:36:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 01:54:00 2023
Response via : Initial Calibration

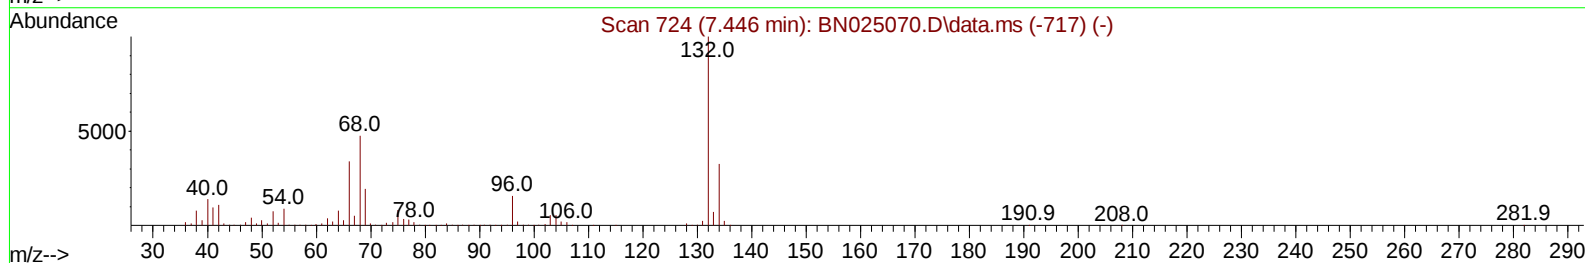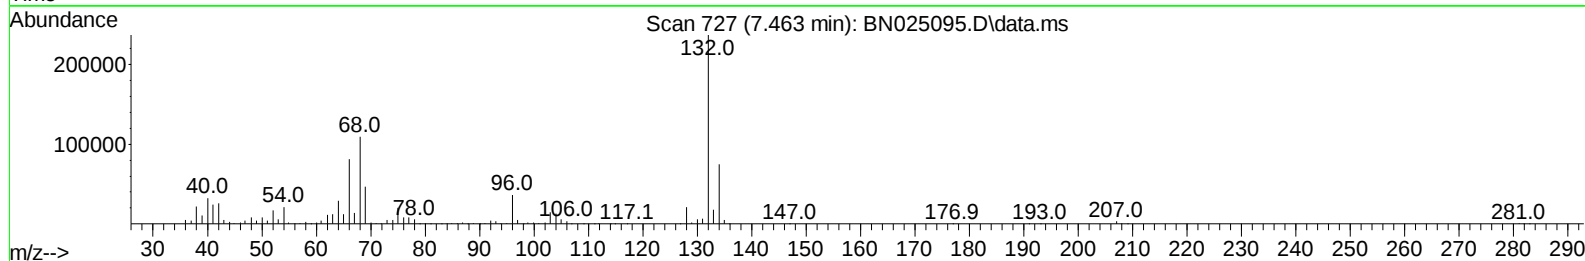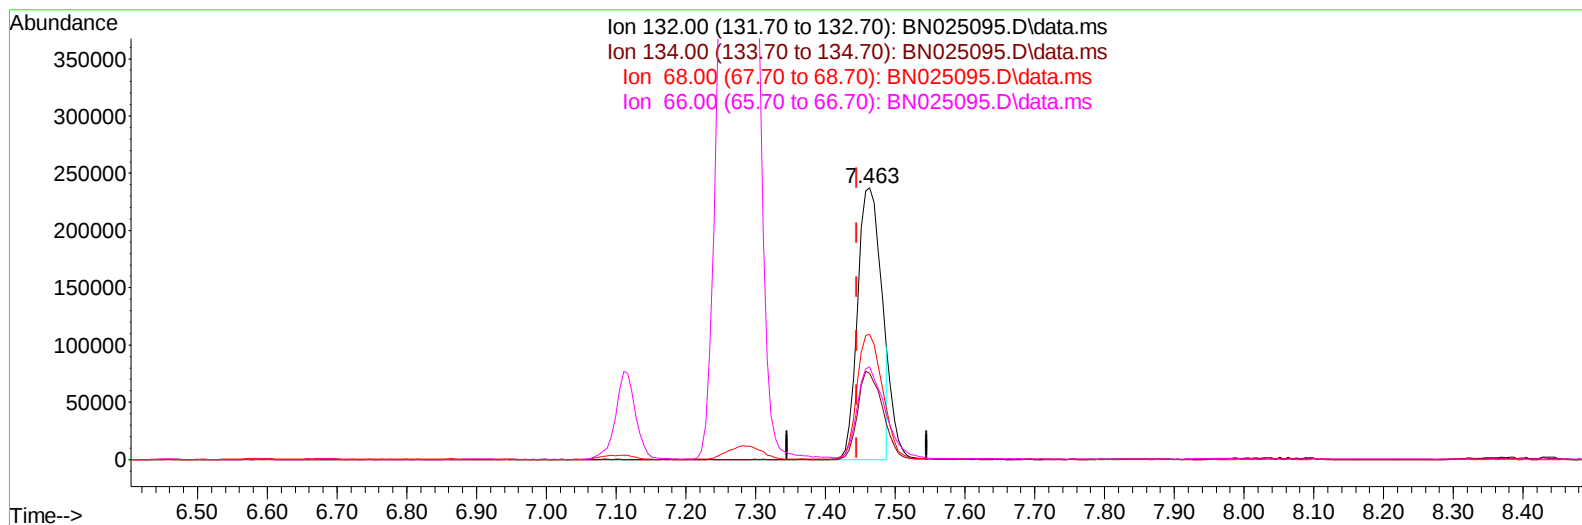

TIC: BN025095.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.463min (+ 0.018) 42.55 ng/u1

response 553138

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	32.10	31.68
68.00	46.90	46.04
66.00	32.70	34.17




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025095.D
Acq On : 23 Apr 2023 03:03
Operator : CG/JU
Sample : 02399-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMP3

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/24/2023
Supervised By :Jagrut Upadhyay 04/24/2023

Quant Time: Apr 23 03:36:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 01:54:00 2023
Response via : Initial Calibration

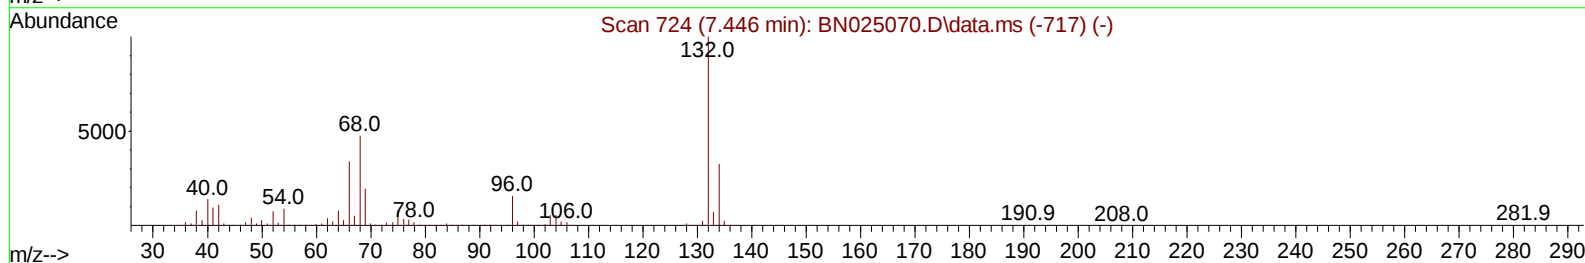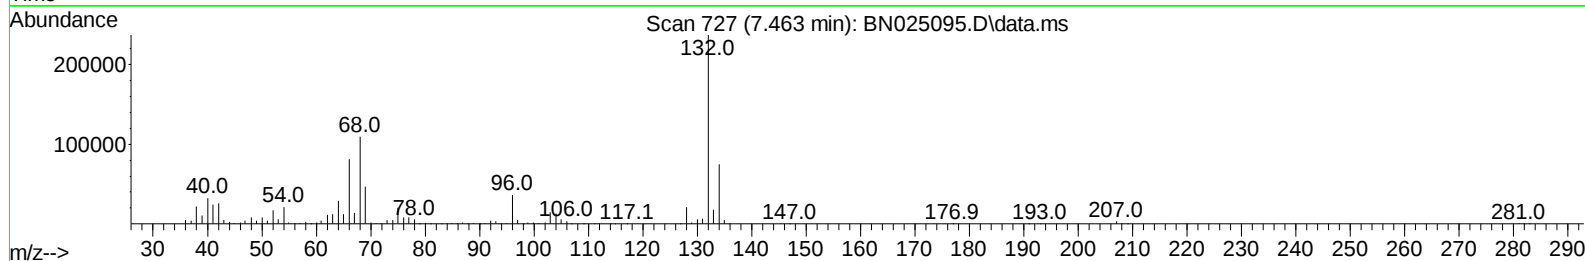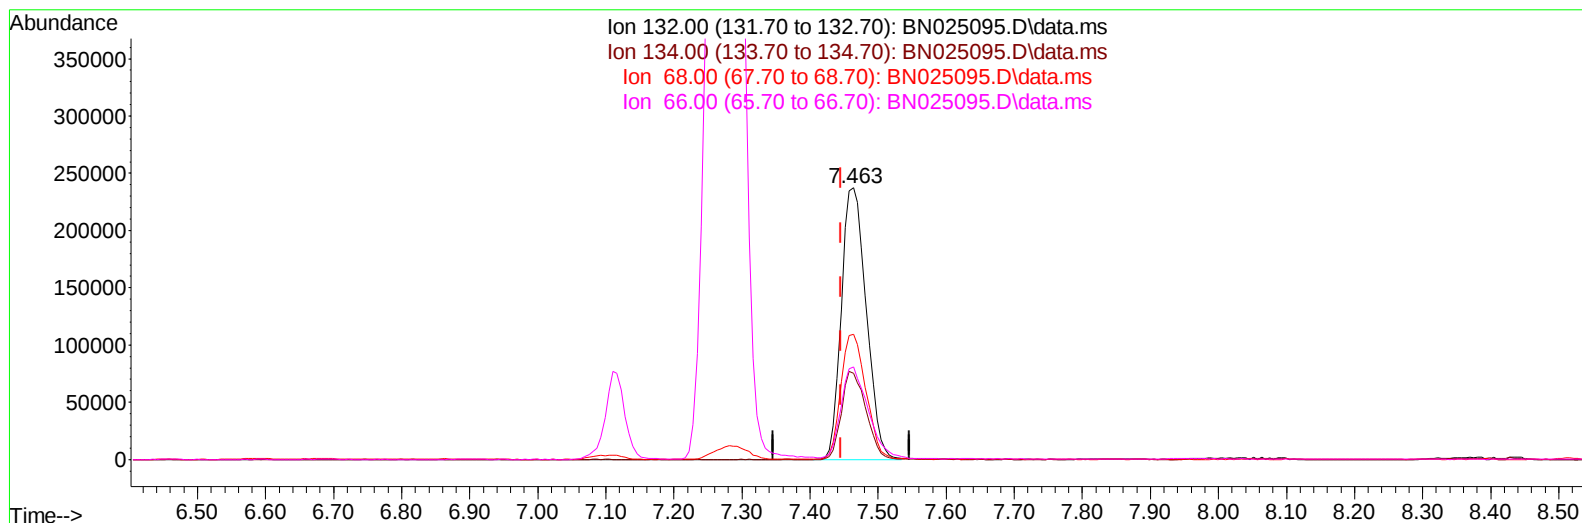

TIC: BN025095.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.463min (+ 0.018) 46.18 ng/ul m

response 600417

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	32.10	31.68
68.00	46.90	46.04
66.00	32.70	34.17




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025095.D
Acq On : 23 Apr 2023 03:03
Operator : CG/JU
Sample : 02399-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMP3

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/24/2023
Supervised By :Jagrut Upadhyay 04/24/2023

Quant Time: Apr 23 03:36:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 01:54:00 2023
Response via : Initial Calibration

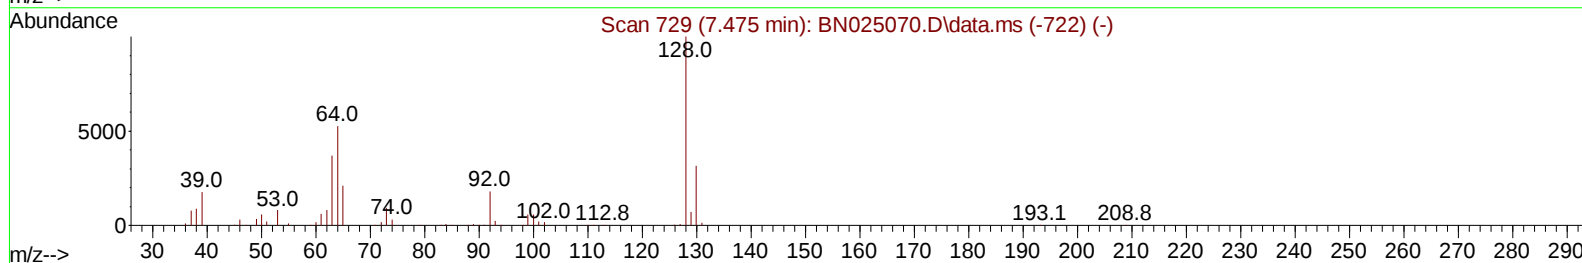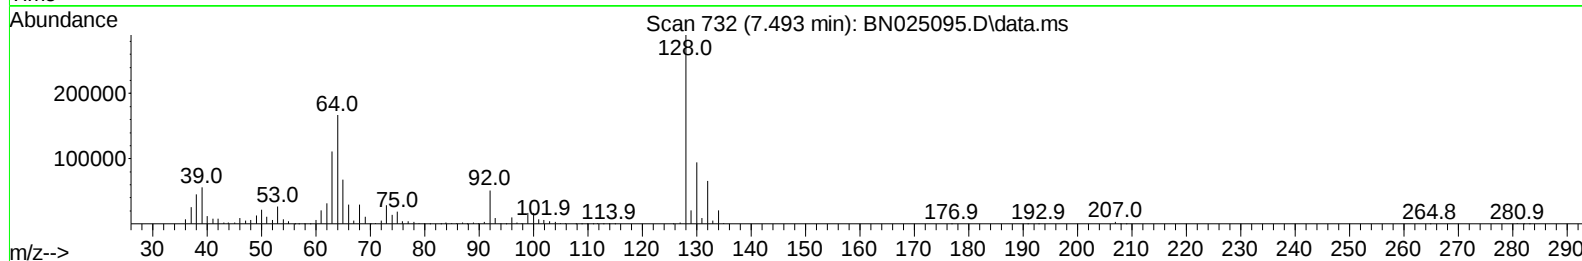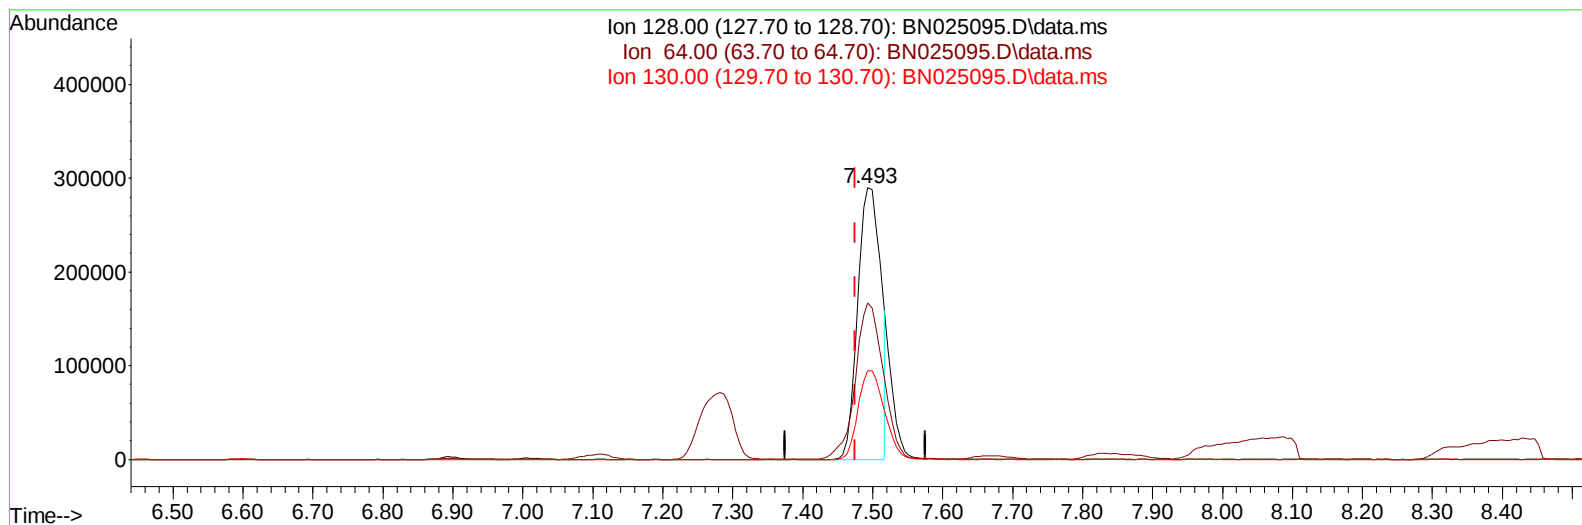

TIC: BN025095.D\data.ms

(12) 2-Chlorophenol

7.493min (+ 0.018) 48.77 ng/u1

response 662281

Ion	Exp%	Act%
128.00	100.00	100.00
64.00	56.00	57.60
130.00	33.20	32.65
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025095.D
Acq On : 23 Apr 2023 03:03
Operator : CG/JU
Sample : 02399-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMP3

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/24/2023
Supervised By :Jagrut Upadhyay 04/24/2023

Quant Time: Apr 23 03:36:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 01:54:00 2023
Response via : Initial Calibration

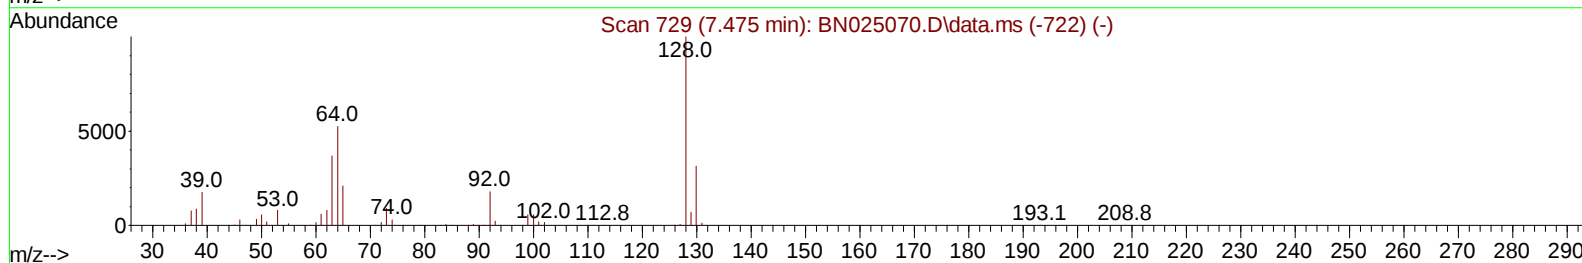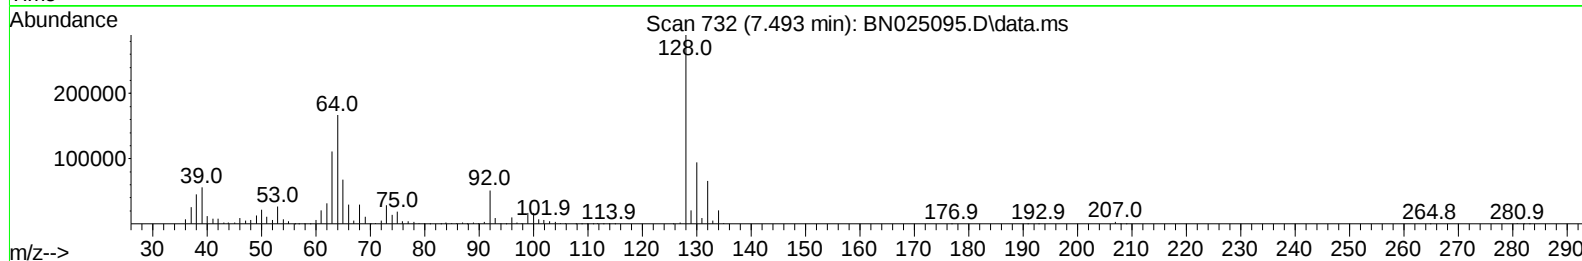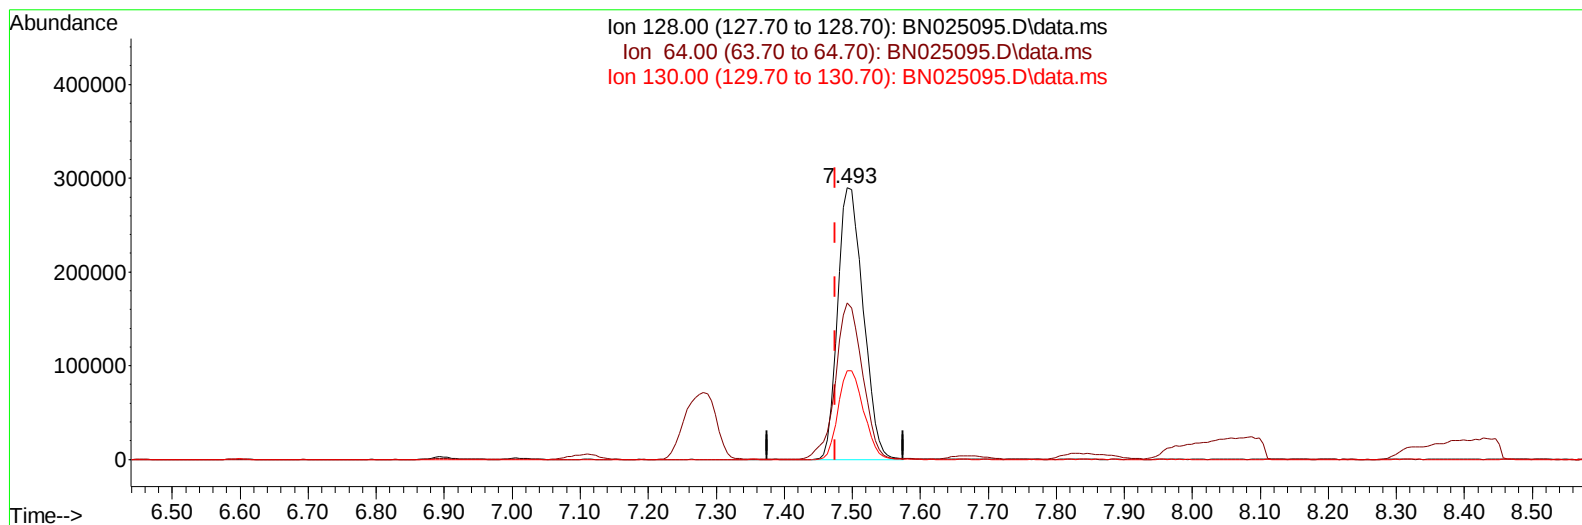

TIC: BN025095.D\data.ms

(12) 2-Chlorophenol

7.493min (+ 0.018) 55.73 ng/ul m

response 756752

Ion	Exp%	Act%
128.00	100.00	100.00
64.00	56.00	57.60
130.00	33.20	32.65
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025095.D
Acq On : 23 Apr 2023 03:03
Operator : CG/JU
Sample : 02399-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMP3

Manual IntegrationsAPPROVED

Quant Time: Apr 23 03:36:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 01:54:00 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/24/2023
Supervised By :Jagrut Upadhyay 04/24/2023

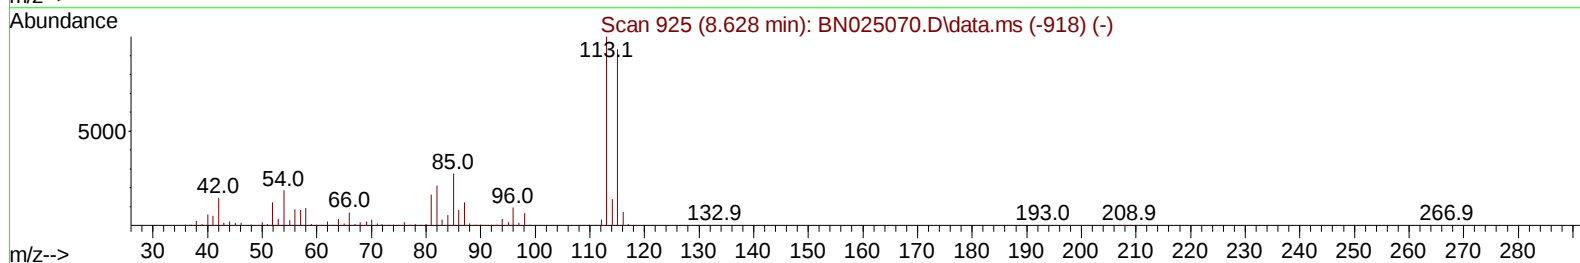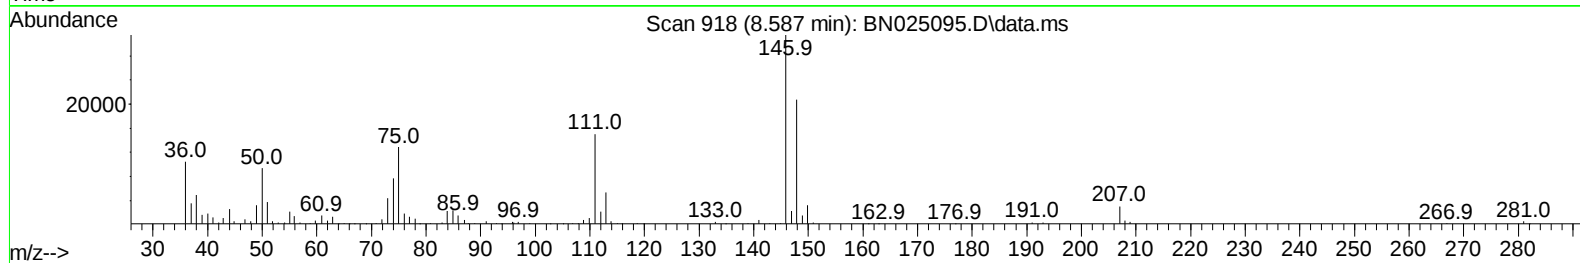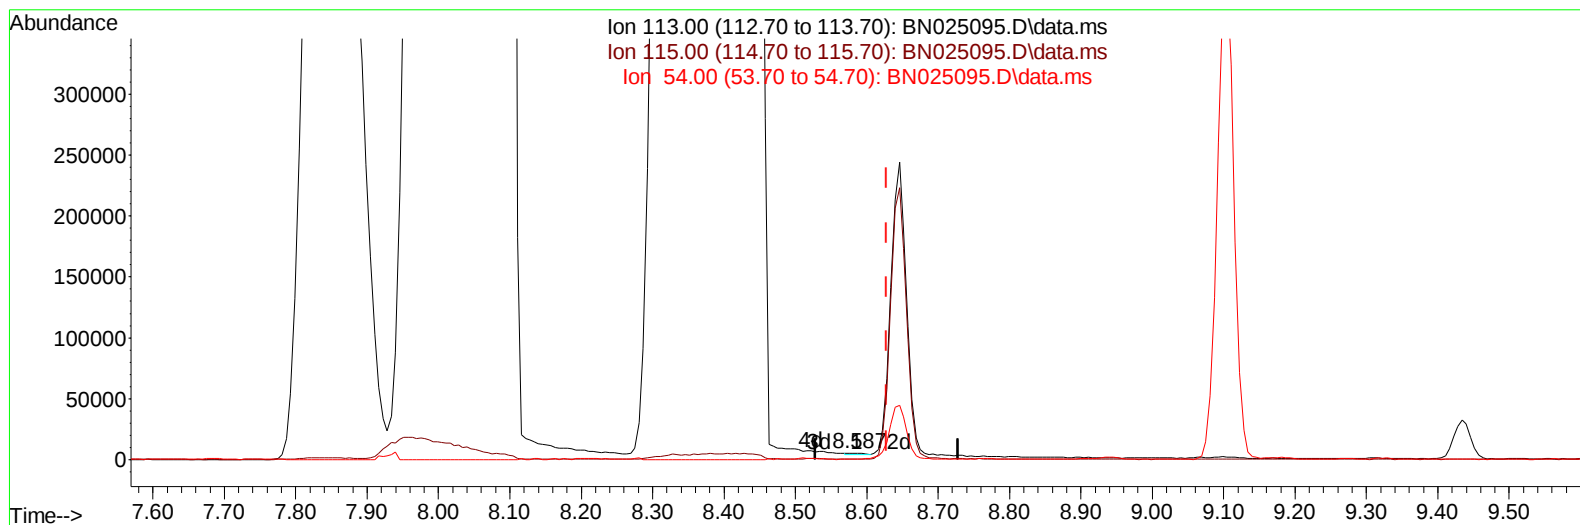

TIC: BN025095.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.587min (-0.041) 0.11 ng/u1

response 1603

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	94.90	5.74#
54.00	17.80	6.50#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025095.D
Acq On : 23 Apr 2023 03:03
Operator : CG/JU
Sample : 02399-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMP3

Manual IntegrationsAPPROVED

Quant Time: Apr 23 03:36:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 01:54:00 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/24/2023
Supervised By :Jagrut Upadhyay 04/24/2023

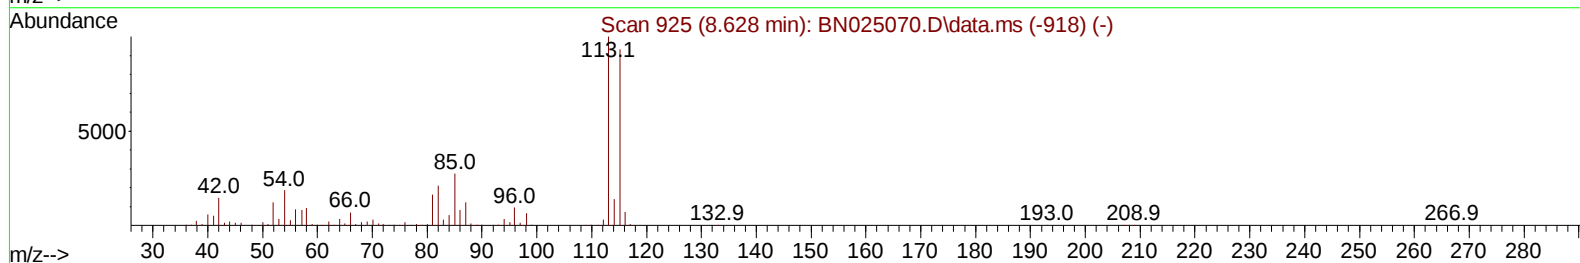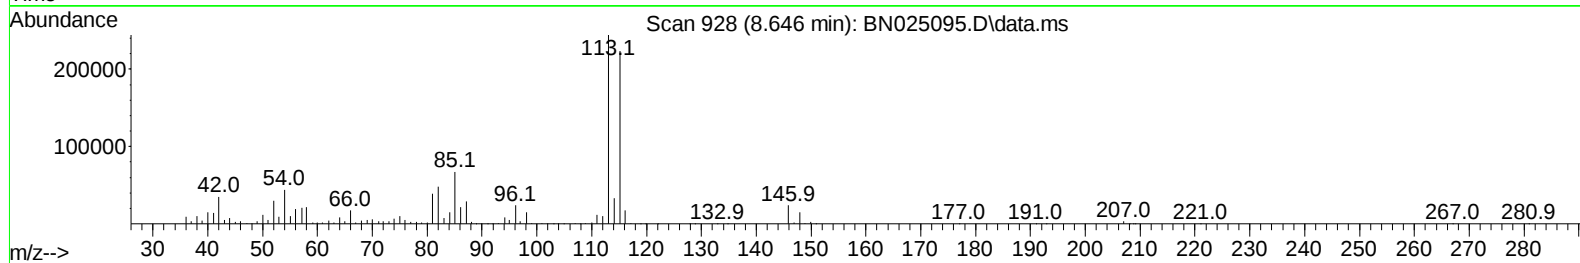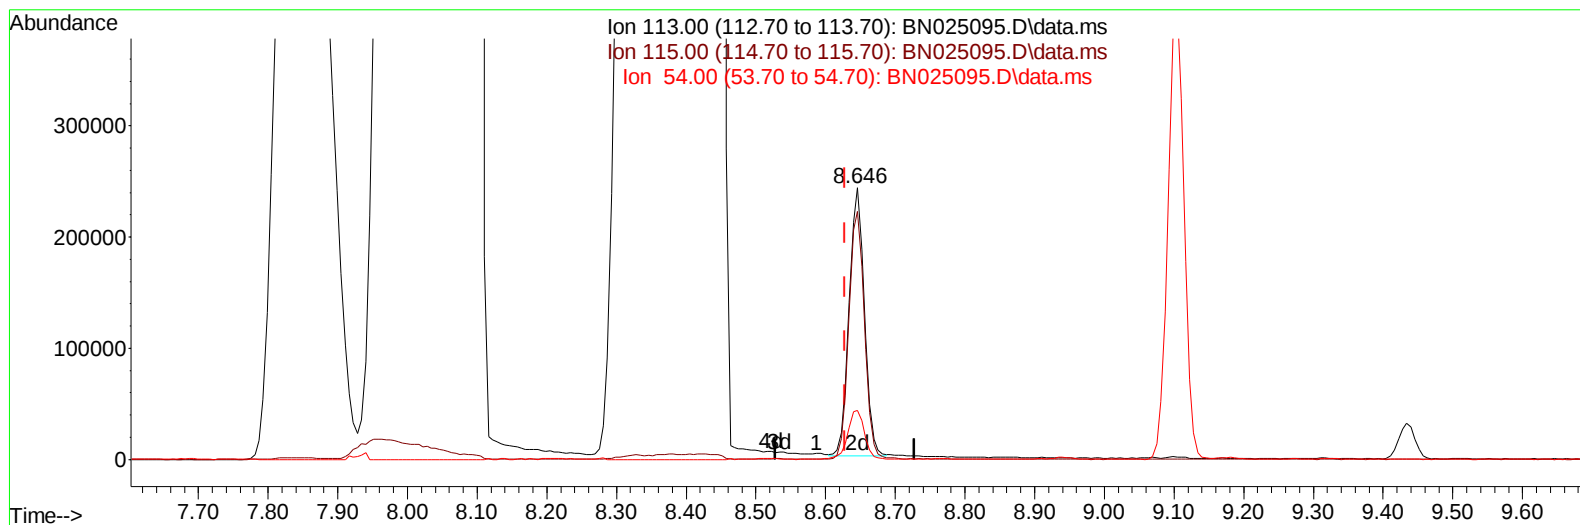

TIC: BN025095.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.646min (+ 0.018) 26.03 ng/ul m

response 365535

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	94.90	91.40
54.00	17.80	18.12
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025095.D
Acq On : 23 Apr 2023 03:03
Operator : CG/JU
Sample : 02399-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMP3

Manual IntegrationsAPPROVED

Quant Time: Apr 23 03:36:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 01:54:00 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/24/2023
Supervised By :Jagrut Upadhyay 04/24/2023

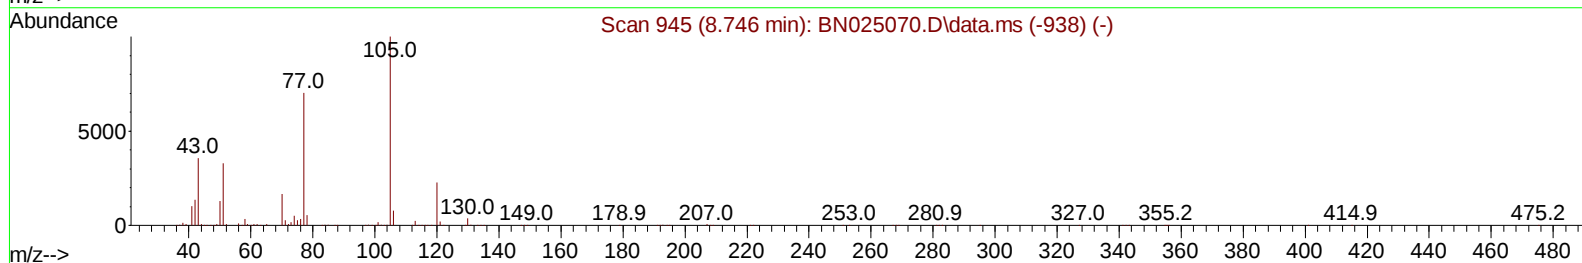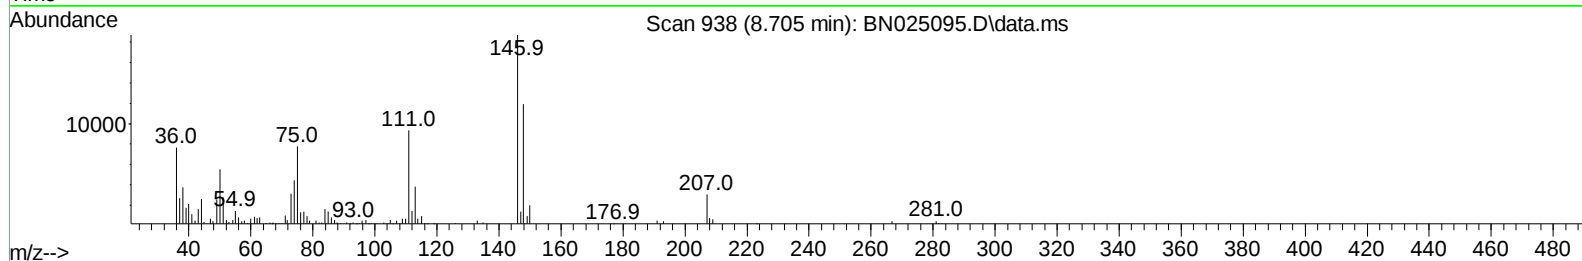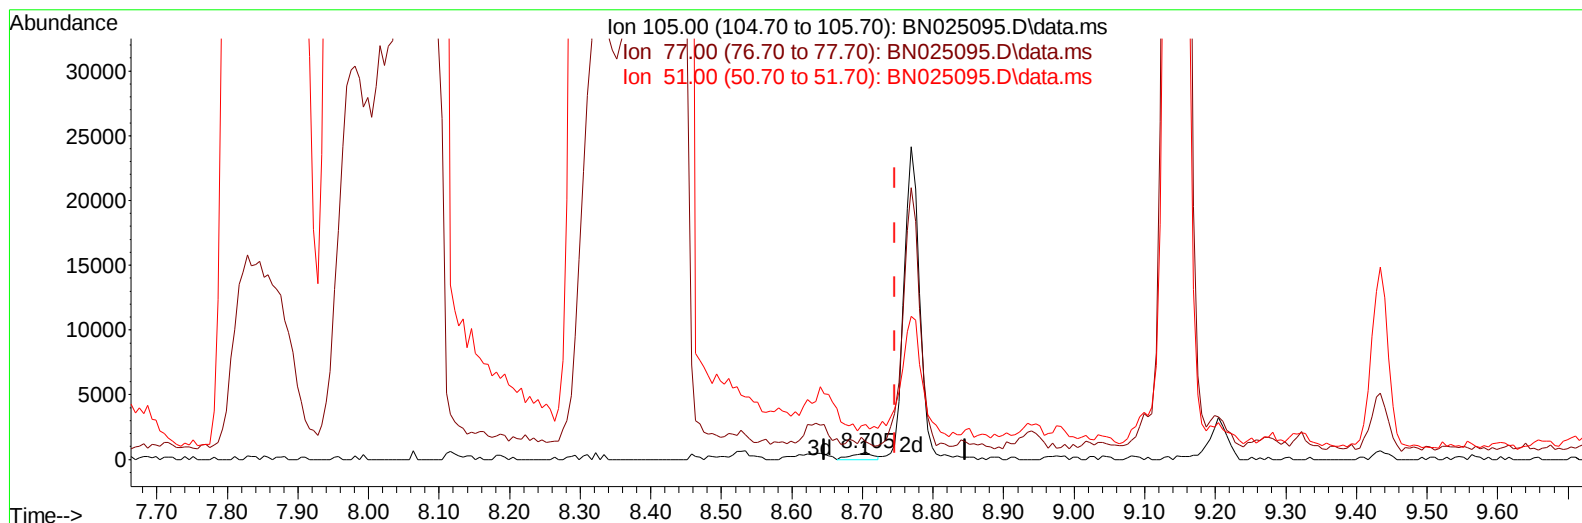

TIC: BN025095.D\data.ms

(16) Acetophenone

8.705min (-0.041) 0.05 ng/u1

response 1094

Ion	Exp%	Act%
105.00	100.00	100.00
77.00	81.00	190.85#
51.00	35.90	375.17#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025095.D
Acq On : 23 Apr 2023 03:03
Operator : CG/JU
Sample : 02399-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMP3

Manual IntegrationsAPPROVED

Quant Time: Apr 23 03:36:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 01:54:00 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/24/2023
Supervised By :Jagrut Upadhyay 04/24/2023

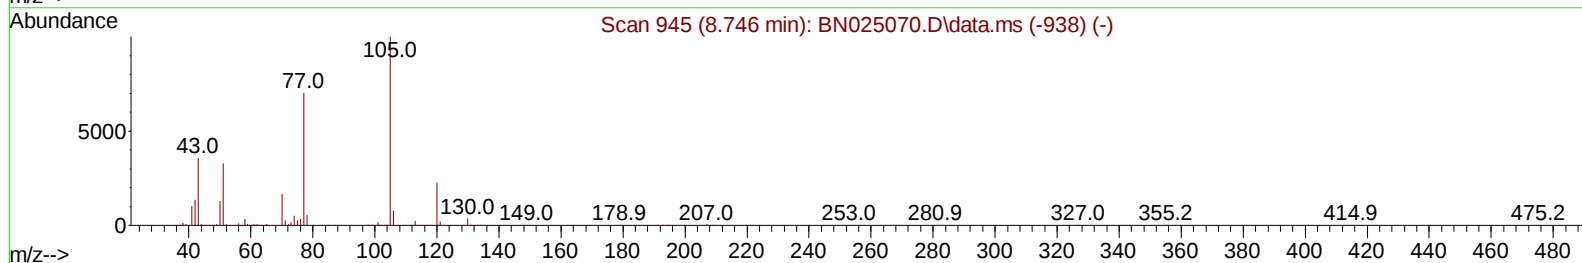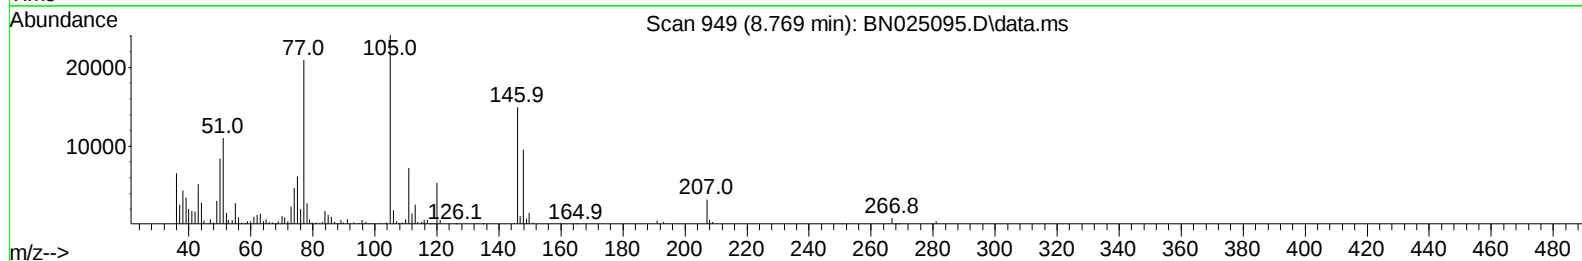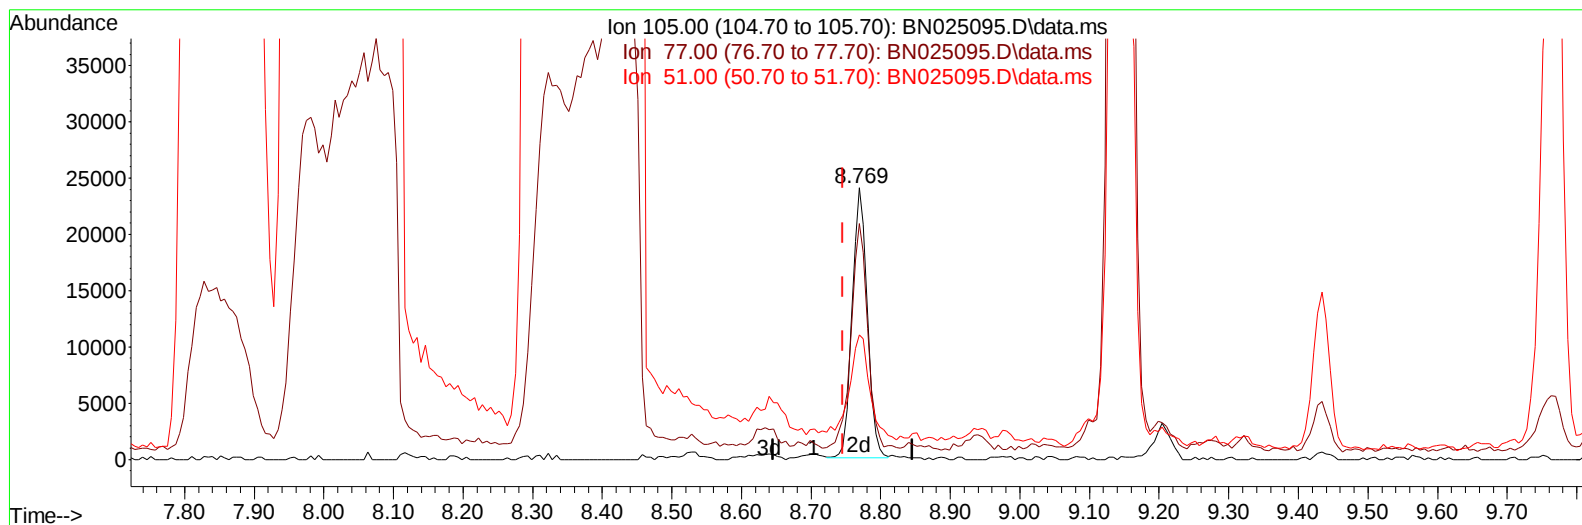

TIC: BN025095.D\data.ms

(16) Acetophenone

8.769min (+ 0.024) 1.65 ng/u1 m

response 36550

Ion	Exp%	Act%
105.00	100.00	100.00
77.00	81.00	86.90
51.00	35.90	45.86#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
 Data File : BN025095.D
 Acq On : 23 Apr 2023 03:03
 Operator : CG/JU
 Sample : 02399-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMP3

Manual IntegrationsAPPROVED

Quant Time: Apr 23 03:36:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 23 01:54:00 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/24/2023
 Supervised By :Jagrut Upadhyay 04/24/2023

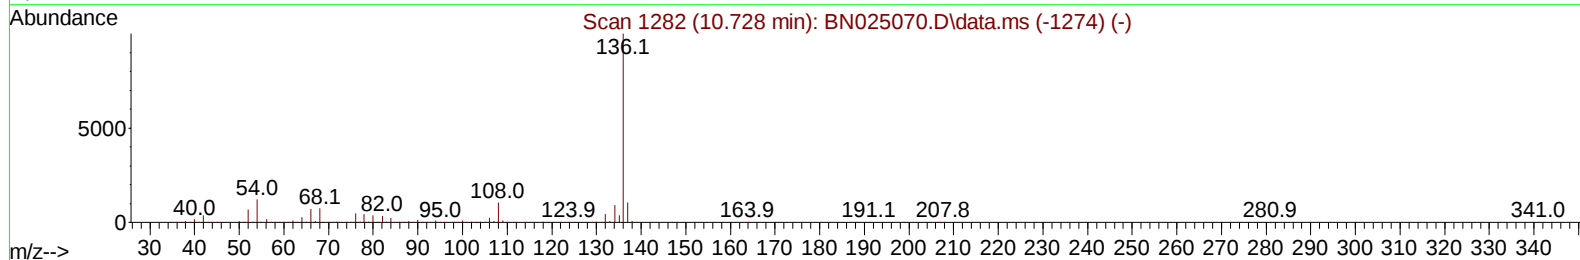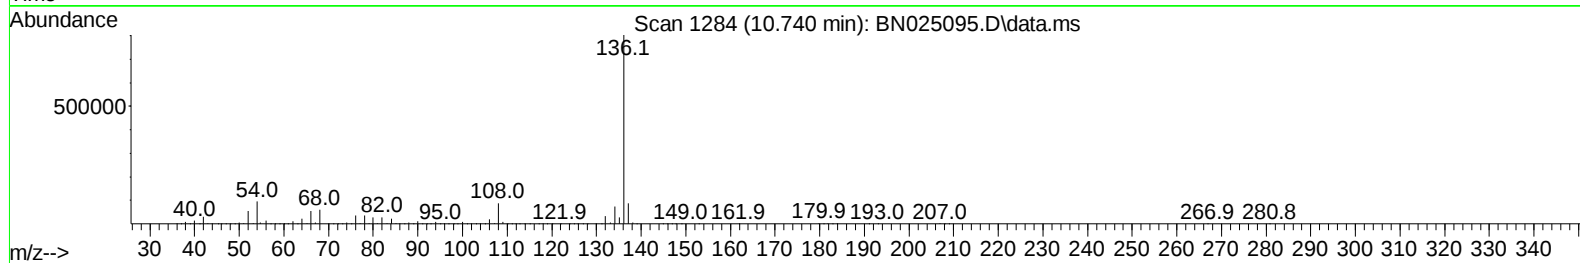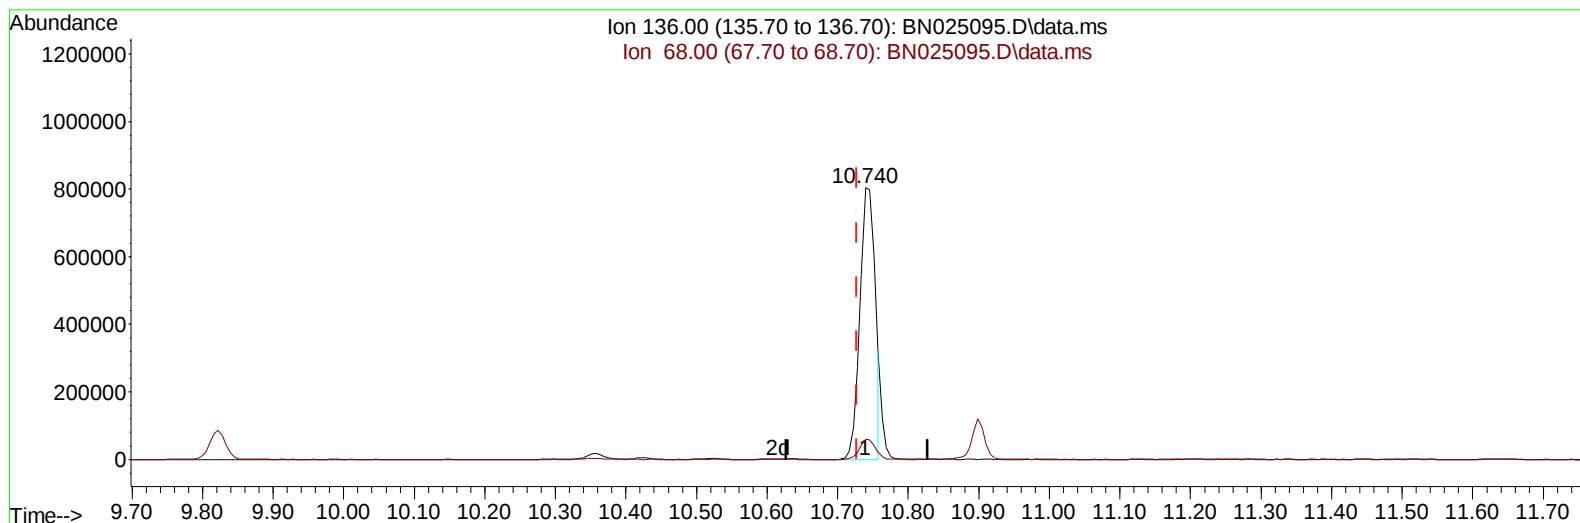

TIC: BN025095.D\data.ms

(20) Naphthalene-d8 (I)

10.740min (+ 0.012) 20.00 ng/u1

response 1226097

Ion	Exp%	Act%
136.00	100.00	100.00
68.00	7.70	7.45
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
 Data File : BN025095.D
 Acq On : 23 Apr 2023 03:03
 Operator : CG/JU
 Sample : 02399-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMP3

Manual IntegrationsAPPROVED

Quant Time: Apr 23 03:36:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 23 01:54:00 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/24/2023
 Supervised By :Jagrut Upadhyay 04/24/2023

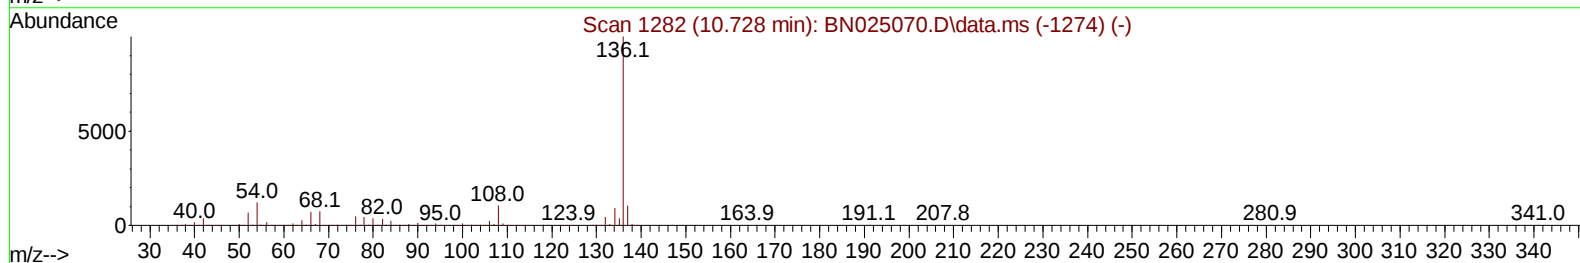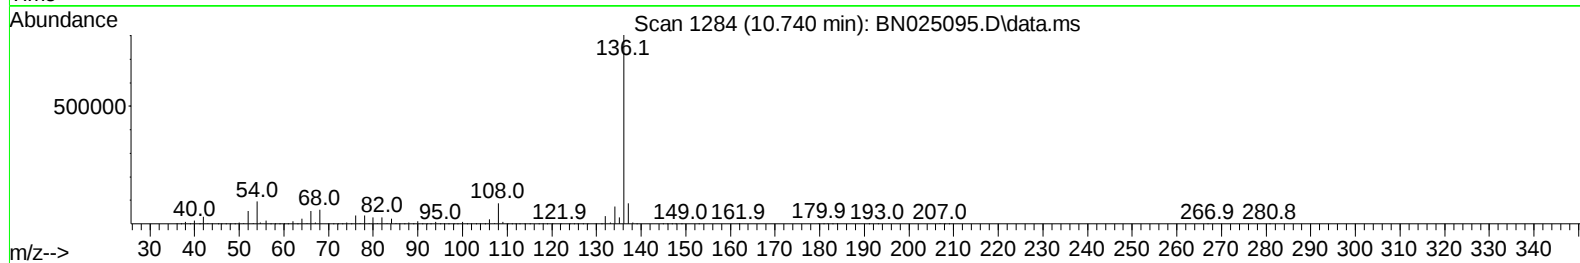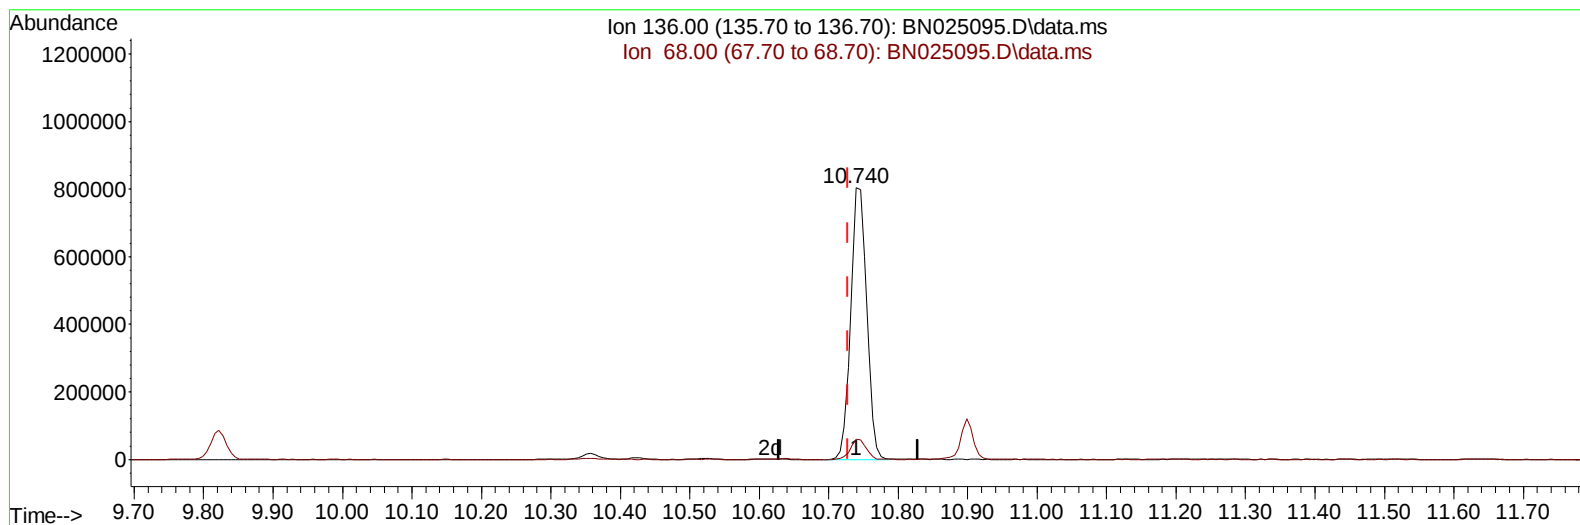

TIC: BN025095.D\data.ms

(20) Naphthalene-d8 (I)

10.740min (+ 0.012) 20.00 ng/ul m

response 1285601

Ion	Exp%	Act%
136.00	100.00	100.00
68.00	7.70	7.45
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
 Data File : BN025095.D
 Acq On : 23 Apr 2023 03:03
 Operator : CG/JU
 Sample : 02399-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMP3

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/24/2023
 Supervised By :Jagrut Upadhyay 04/24/2023

Quant Time: Apr 23 03:36:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 23 01:54:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	181460m	20.000	ng/ul	0.04
20) Naphthalene-d8	10.740	136	1285601m	20.000	ng/ul	0.01
38) Acenaphthene-d10	14.563	164	789424	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.310	188	1752066	20.000	ng/ul	0.00
79) Chrysene-d12	21.498	240	1822147	20.000	ng/ul	-0.01
88) Perylene-d12	23.927	264	2111916	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	36444	7.644	ng/uL	0.00
4) Pyridine-d5	3.734	84	268383m	18.799	ng/ul	0.02
7) Phenol-d5	7.087	99	190189m	10.750	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.287	67	1084953m	91.690	ng/ul	0.04
11) 2-Chlorophenol-d4	7.463	132	600417m	46.182	ng/ul	0.02
15) 4-Methylphenol-d8	8.646	113	365535m	26.027	ng/ul	0.02
21) Nitrobenzene-d5	9.105	128	403510	38.764	ng/ul	0.02
24) 2-Nitrophenol-d4	9.822	143	428113	37.970	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.357	165	647497	32.130	ng/ul	0.01
31) 4-Chloroaniline-d4	10.899	131	888280	29.045	ng/ul	0.03
46) Dimethylphthalate-d6	13.975	166	2329418	38.064	ng/ul	0.00
49) Acenaphthylene-d8	14.257	160	2619876	37.358	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	87950	7.011	ng/ul	0.00
60) Fluorene-d10	15.557	176	2045905	39.596	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200	358702	31.459	ng/ul	0.00
73) Anthracene-d10	17.410	188	3356912	40.795	ng/ul	0.00
81) Pyrene-d10	19.704	212	4072151	38.486	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.774	264	4399199	39.839	ng/ul	0.00
Target Compounds						
						Qvalue
8) Phenol	7.111	94	345607	18.758	ng/ul	99
12) 2-Chlorophenol	7.493	128	756752m	55.730	ng/ul	
16) Acetophenone	8.769	105	36550m	1.646	ng/ul	
22) Nitrobenzene	9.146	77	409624	14.645	ng/ul	99
32) 4-Chloroaniline	10.916	127	896967	28.972	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.757	216	94678	4.112	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025095.D
Acq On : 23 Apr 2023 03:03
Operator : CG/JU
Sample : 02399-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMP3

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/24/2023
Supervised By :Jagrut Upadhyay 04/24/2023

Quant Time: Apr 23 03:36:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 01:54:00 2023
Response via : Initial Calibration

