

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
 Data File : BN025100.D
 Acq On : 23 Apr 2023 06:02
 Operator : CG/JU
 Sample : 02399-12
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMN3

Quant Time: Apr 23 06:31:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 23 01:54:00 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	295623	20.000	ng/ul	0.00
20) Naphthalene-d8	10.728	136	1349971	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.563	164	886561	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.310	188	1964403	20.000	ng/ul	0.00
79) Chrysene-d12	21.498	240	1994413	20.000	ng/ul	-0.01
88) Perylene-d12	23.921	264	2268745	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	33077	4.258	ng/uL	0.00
4) Pyridine-d5	3.722	84	170794	7.343	ng/ul	0.00
7) Phenol-d5	7.075	99	155917	5.410	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.246	67	673529	34.939	ng/ul	0.00
11) 2-Chlorophenol-d4	7.446	132	531924	25.114	ng/ul	0.00
15) 4-Methylphenol-d8	8.628	113	335782	14.676	ng/ul	0.00
21) Nitrobenzene-d5	9.087	128	379949	34.760	ng/ul	0.00
24) 2-Nitrophenol-d4	9.810	143	401835	33.940	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.346	165	635091	30.011	ng/ul	0.00
31) 4-Chloroaniline-d4	10.869	131	979193	30.491	ng/ul	0.00
46) Dimethylphthalate-d6	13.975	166	2601113	37.847	ng/ul	0.00
49) Acenaphthylene-d8	14.257	160	2885622	36.639	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	59730	4.240	ng/ul	0.00
60) Fluorene-d10	15.557	176	2219362	38.247	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200	361791	28.300	ng/ul	0.00
73) Anthracene-d10	17.410	188	3646412	39.523	ng/ul	0.00
81) Pyrene-d10	19.704	212	4290175	37.044	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.768	264	4635815	39.080	ng/ul	-0.01
Target Compounds						
35) 4-Chloro-3-methylphenol	12.010	107	103002	4.136	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025100.D
Acq On : 23 Apr 2023 06:02
Operator : CG/JU
Sample : 02399-12
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMN3

Quant Time: Apr 23 06:31:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 01:54:00 2023
Response via : Initial Calibration

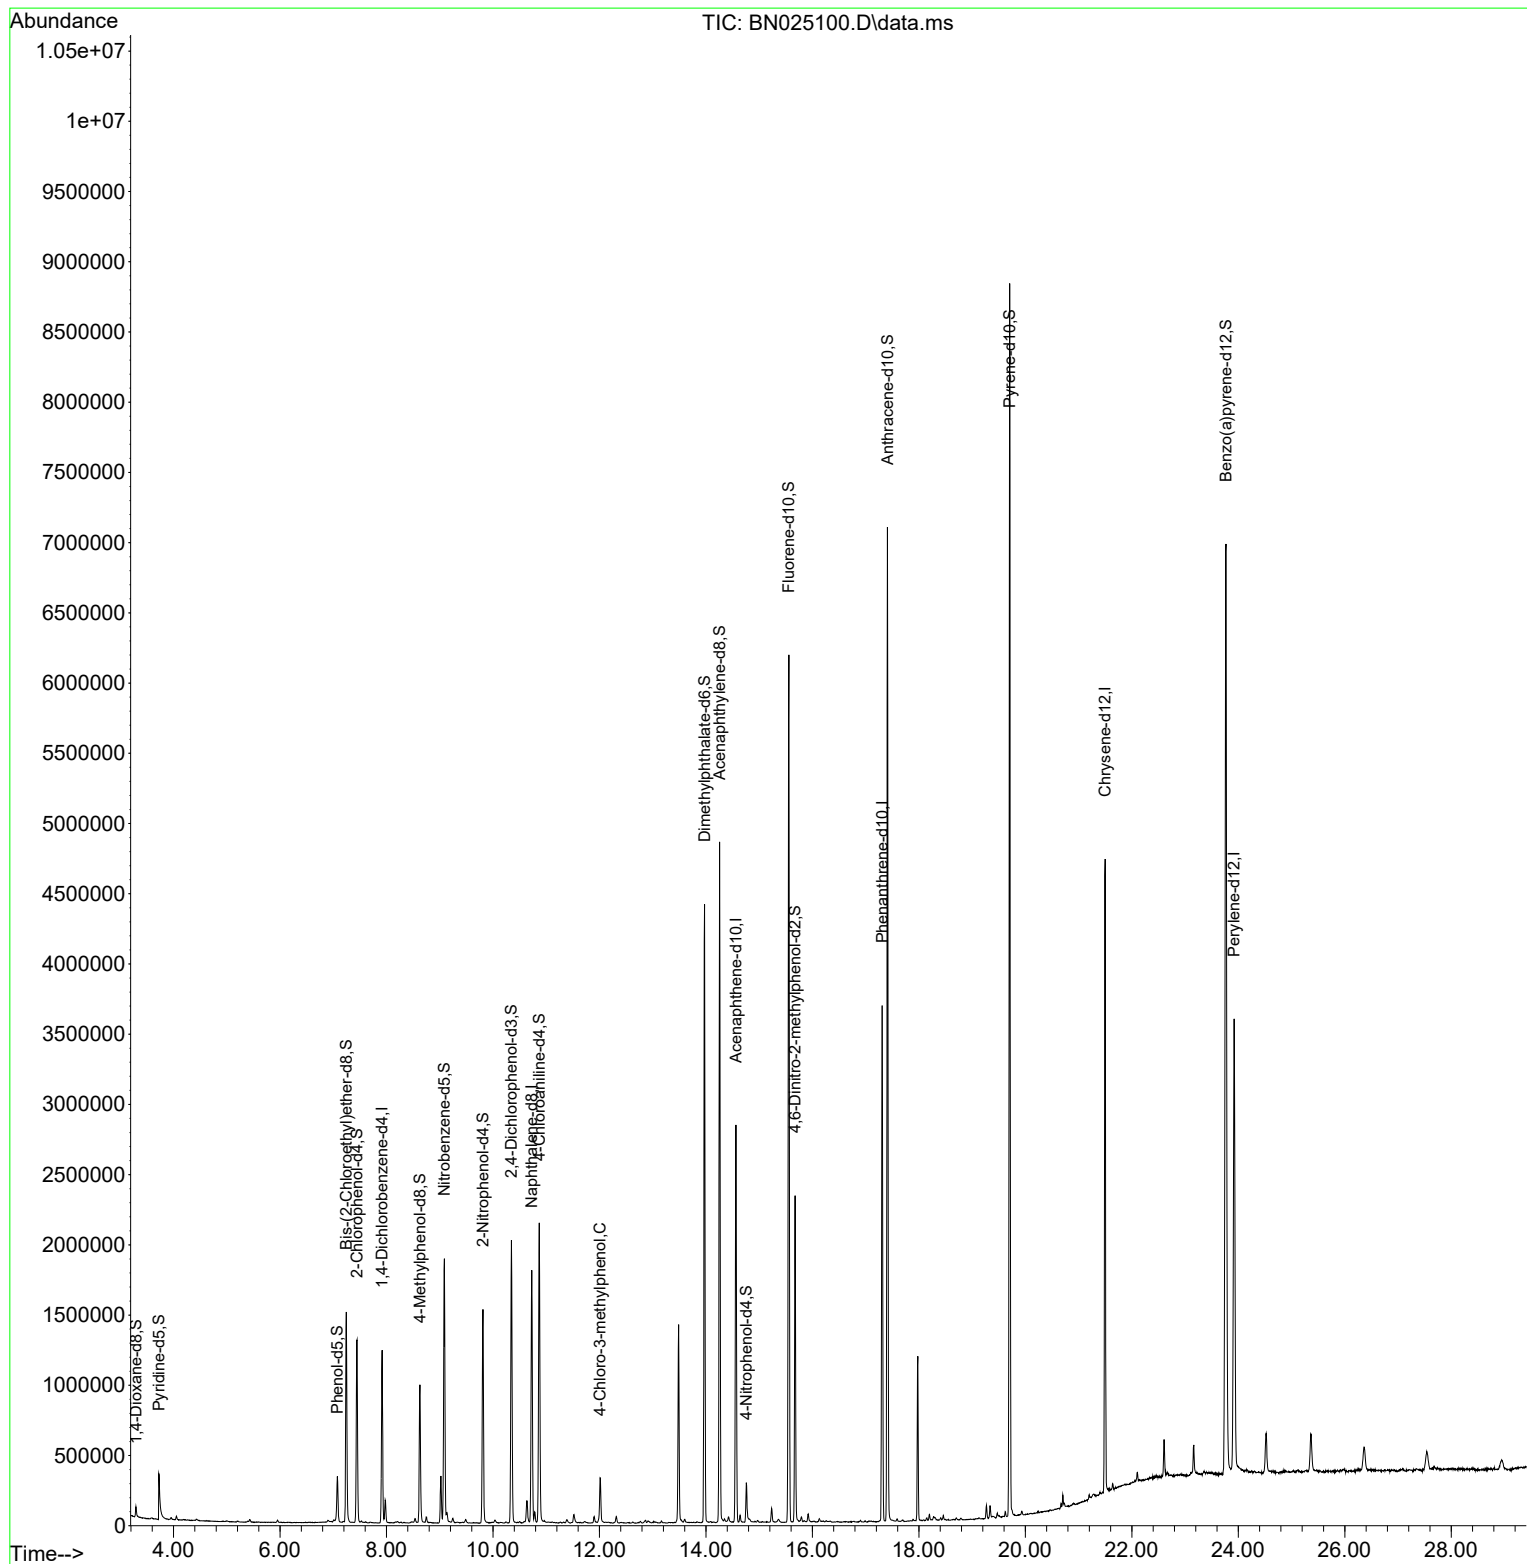

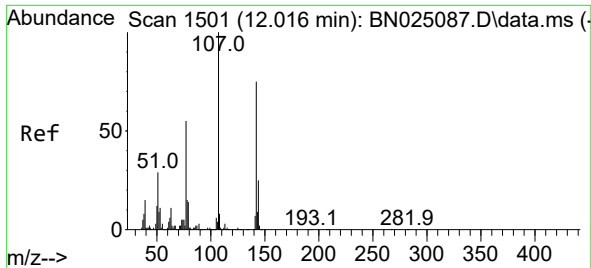

#35
 4-Chloro-3-methylphenol
 Concen: 4.136 ng/ul
 RT: 12.010 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BN025100.D
 Acq: 23 Apr 2023 06:02

Instrument :
 BNA_N
 ClientSampleId :
 COMN3

Tgt Ion:107 Resp: 103002
 Ion Ratio Lower Upper
 107 100
 144 23.7 19.6 29.4
 142 73.8 60.7 91.1

