

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
 Data File : BN025101.D
 Acq On : 23 Apr 2023 06:38
 Operator : CG/JU
 Sample : 02399-16
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMM8

Quant Time: Apr 23 07:11:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 23 01:54:00 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	233959	20.000	ng/ul	0.00
20) Naphthalene-d8	10.728	136	1036883	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.563	164	685749	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.310	188	1508198	20.000	ng/ul	0.00
79) Chrysene-d12	21.498	240	1569582	20.000	ng/ul	-0.01
88) Perylene-d12	23.933	264	1861331	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	26018	4.232	ng/uL	0.00
4) Pyridine-d5	3.728	84	138841	7.543	ng/ul	0.01
7) Phenol-d5	7.075	99	107056	4.693	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.246	67	524668	34.390	ng/ul	0.00
11) 2-Chlorophenol-d4	7.440	132	392126	23.393	ng/ul	0.00
15) 4-Methylphenol-d8	8.628	113	231568	12.788	ng/ul	0.00
21) Nitrobenzene-d5	9.087	128	288122	34.319	ng/ul	0.00
24) 2-Nitrophenol-d4	9.810	143	295625	32.509	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.345	165	474345	29.184	ng/ul	0.00
31) 4-Chloroaniline-d4	10.869	131	680135	27.573	ng/ul	0.00
46) Dimethylphthalate-d6	13.975	166	1990021	37.434	ng/ul	0.00
49) Acenaphthylene-d8	14.257	160	2144733	35.207	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	36812	3.378	ng/ul	0.00
60) Fluorene-d10	15.557	176	1720151	38.324	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.674	200	277026	28.224	ng/ul	0.00
73) Anthracene-d10	17.410	188	2827599	39.918	ng/ul	0.00
81) Pyrene-d10	19.704	212	3357664	36.840	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.780	264	3780889	38.849	ng/ul	0.00
Target Compounds						
39) 1,2,4,5-Tetrachloroben...	12.757	216	45441	2.272	ng/ul	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025101.D
Acq On : 23 Apr 2023 06:38
Operator : CG/JU
Sample : 02399-16
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMM8

Quant Time: Apr 23 07:11:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 01:54:00 2023
Response via : Initial Calibration

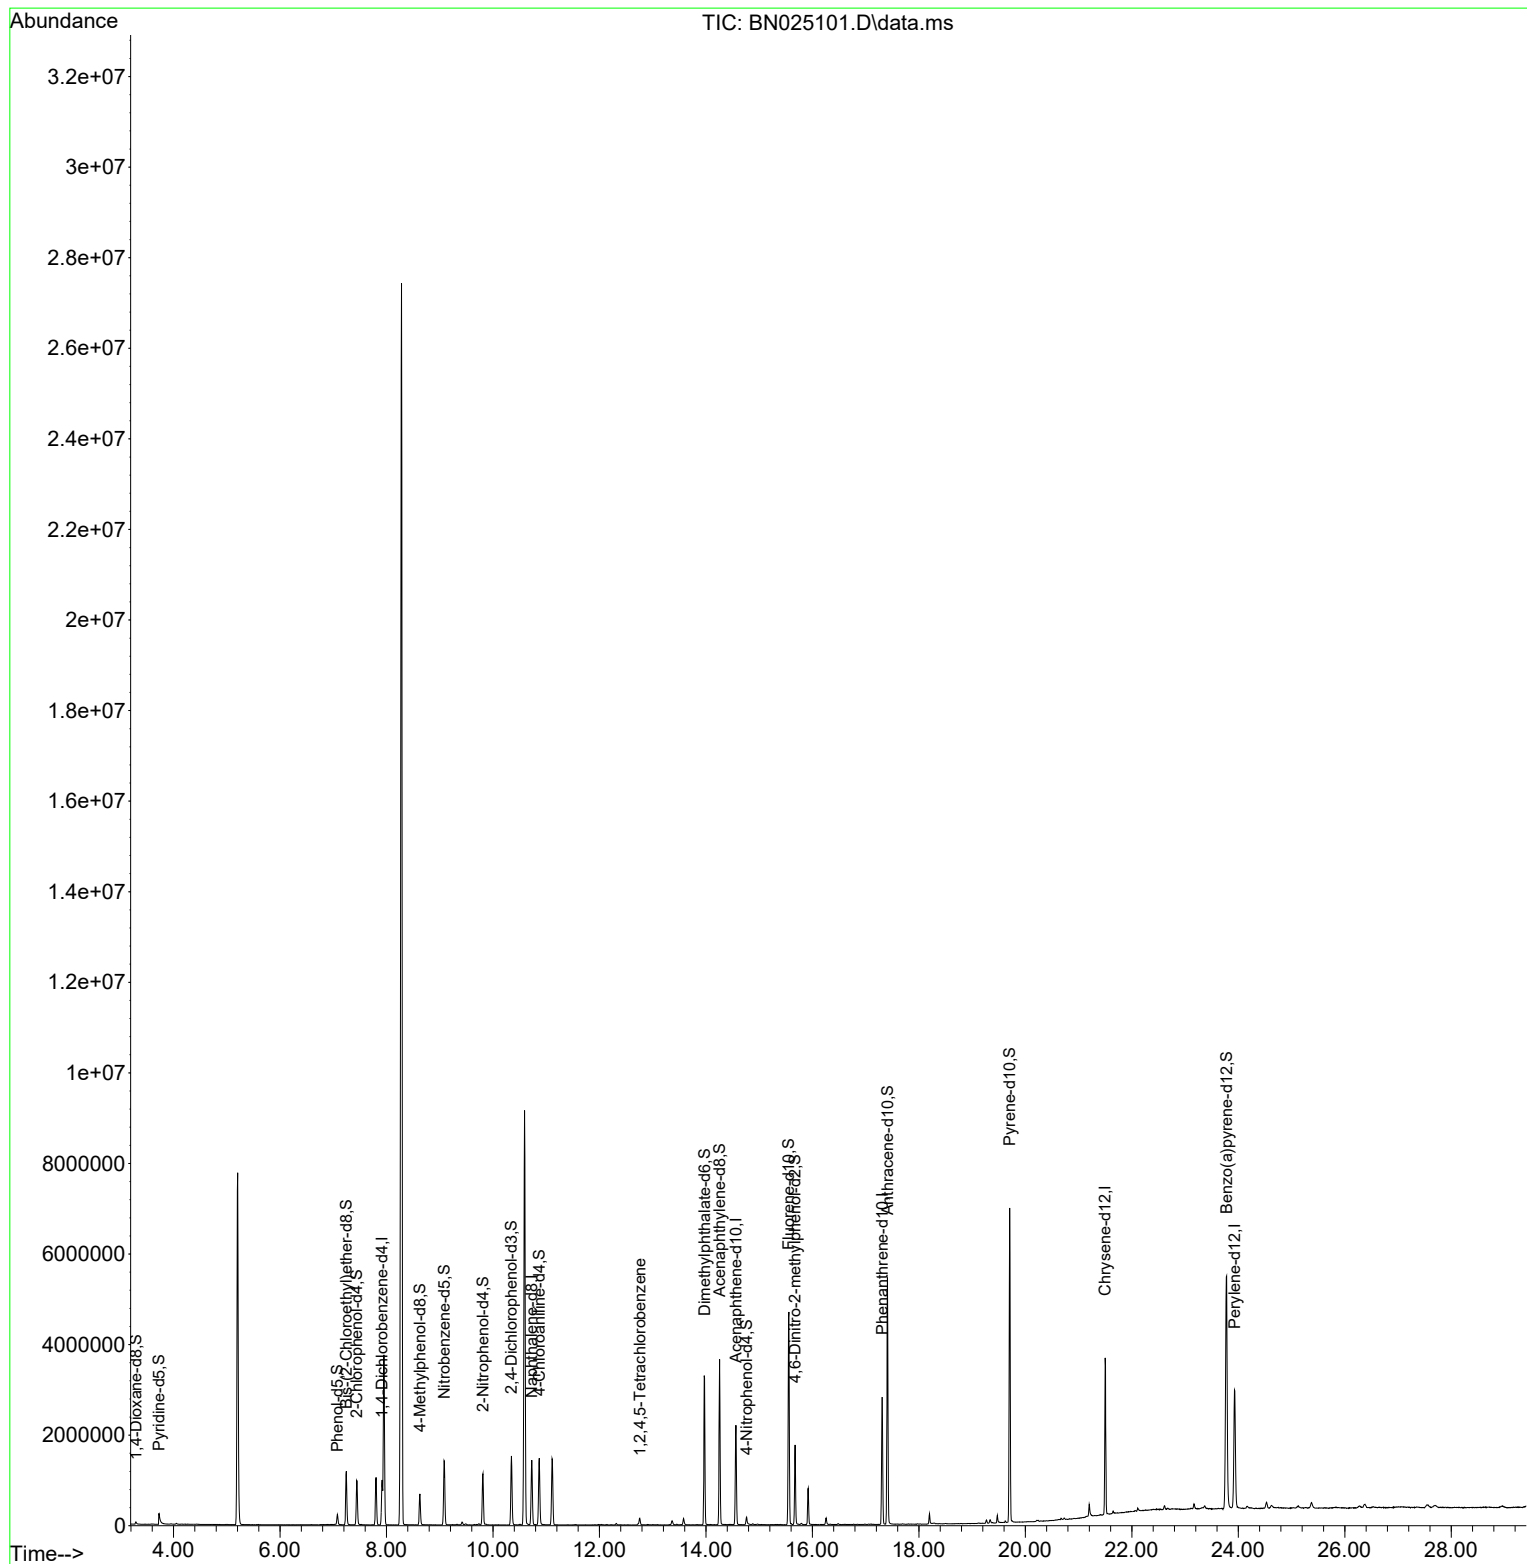

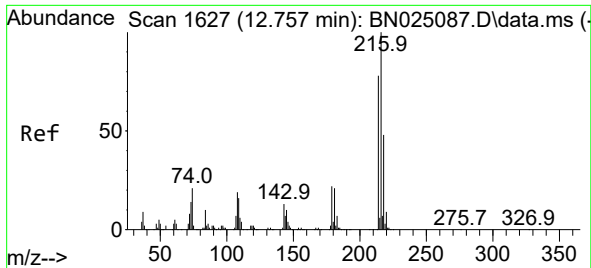

#39

1,2,4,5-Tetrachlorobenzene

Concen: 2.272 ng/ul

RT: 12.757 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN025101.D


Acq: 23 Apr 2023 06:38

Instrument :

BNA_N

ClientSampleId :

COMM8

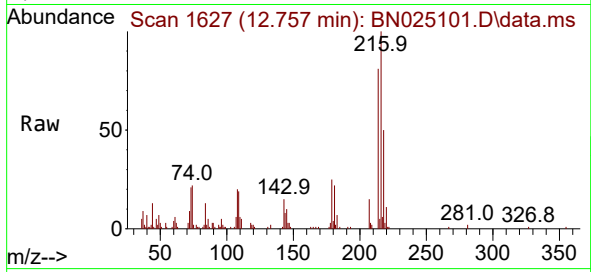

Tgt Ion:216 Resp: 45441

Ion Ratio Lower Upper

216 100

214 81.0 62.2 93.4

179 24.7 16.8 25.2

108 20.1 15.0 22.6

