

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
 Data File : BN025071.D
 Acq On : 22 Apr 2023 12:09
 Operator : CG/JU
 Sample : PB152281BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK281

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN025071.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	14	18	24	rBV	84186	117461	1.23%	0.132%
2	3.716	87	90	113	rBV	1122208	1944229	20.43%	2.181%
3	4.058	144	148	152	rVB5	16874	25458	0.27%	0.029%
4	7.075	654	661	674	rBV	1415360	2222066	23.35%	2.493%
5	7.246	683	690	701	rBV	1101226	1716965	18.04%	1.926%
6	7.352	707	708	712	rVB3	12462	14711	0.15%	0.017%
7	7.446	717	724	733	rVV	1317346	2122085	22.30%	2.381%
8	7.916	796	804	813	rBV	1098717	1767245	18.57%	1.983%
9	8.628	918	925	935	rBV	1682117	2654640	27.90%	2.979%
10	9.087	995	1003	1013	rBV	1381584	2280136	23.96%	2.558%
11	9.810	1118	1126	1138	rBV	1195673	1941439	20.40%	2.178%
12	10.346	1210	1217	1226	rBV	1611971	2622194	27.56%	2.942%
13	10.728	1275	1282	1293	rVB	1578043	2632919	27.67%	2.954%
14	10.869	1298	1306	1320	rBV	1777404	3032848	31.87%	3.403%
15	11.922	1477	1485	1489	rBV7	6495	15759	0.17%	0.018%
16	12.316	1547	1552	1558	rBV5	27355	57183	0.60%	0.064%
17	13.545	1757	1761	1765	rVB3	9244	11402	0.12%	0.013%
18	13.975	1827	1834	1845	rBV	3191538	4347287	45.68%	4.878%
19	14.257	1874	1882	1891	rBV	3364493	4801559	50.46%	5.387%
20	14.404	1904	1907	1909	rBV4	9998	11823	0.12%	0.013%
21	14.563	1926	1934	1943	rBV	2511280	3632444	38.17%	4.076%
22	14.757	1960	1967	1981	rBV	1679280	2492893	26.20%	2.797%
23	14.975	2001	2004	2008	rVB6	7383	11392	0.12%	0.013%
24	15.345	2062	2067	2071	rVV5	9104	18880	0.20%	0.021%
25	15.381	2071	2073	2079	rVB5	6294	10161	0.11%	0.011%
26	15.557	2096	2103	2113	rVB	4340262	6036124	63.43%	6.773%
27	15.675	2117	2123	2131	rBV	1891096	2403338	25.26%	2.697%
28	15.798	2140	2144	2149	rVB6	21860	32958	0.35%	0.037%
29	15.957	2167	2171	2176	rBV6	7966	14472	0.15%	0.016%
30	17.310	2395	2401	2410	rBV	3290339	4453650	46.80%	4.997%
31	17.410	2411	2418	2432	rVV2	4754577	6667663	70.07%	7.481%
32	18.198	2547	2552	2557	rBV5	50884	91974	0.97%	0.103%
33	19.269	2729	2734	2739	rBV5	63871	90565	0.95%	0.102%
34	19.339	2743	2746	2754	rVB2	57741	92586	0.97%	0.104%
35	19.474	2766	2769	2774	rBV4	27973	35134	0.37%	0.039%
36	19.704	2802	2808	2818	rBV	5768273	7920882	83.24%	8.887%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025071.D
Acq On : 22 Apr 2023 12:09
Operator : CG/JU
Sample : PB152281BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK281

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Title : SVOA CALIBRATION

37	21.510	3109	3115	3123	rBV	3948516	5280161	55.49%	5.924%
38	23.792	3496	3503	3519	rVB2	5064444	9516113	100.00%	10.677%
39	23.951	3522	3530	3543	rVB2	2719362	5985375	62.90%	6.716%




Sum of corrected areas: 89126174

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025071.D
Acq On : 22 Apr 2023 12:09
Operator : CG/JU
Sample : PB152281BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK281

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

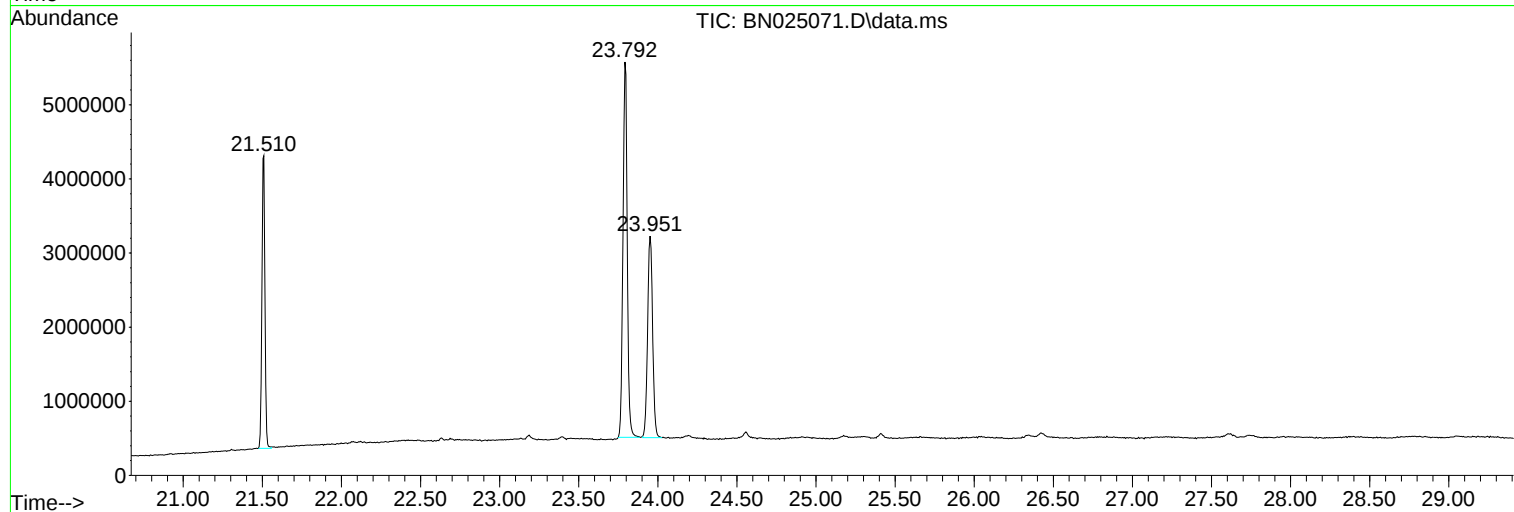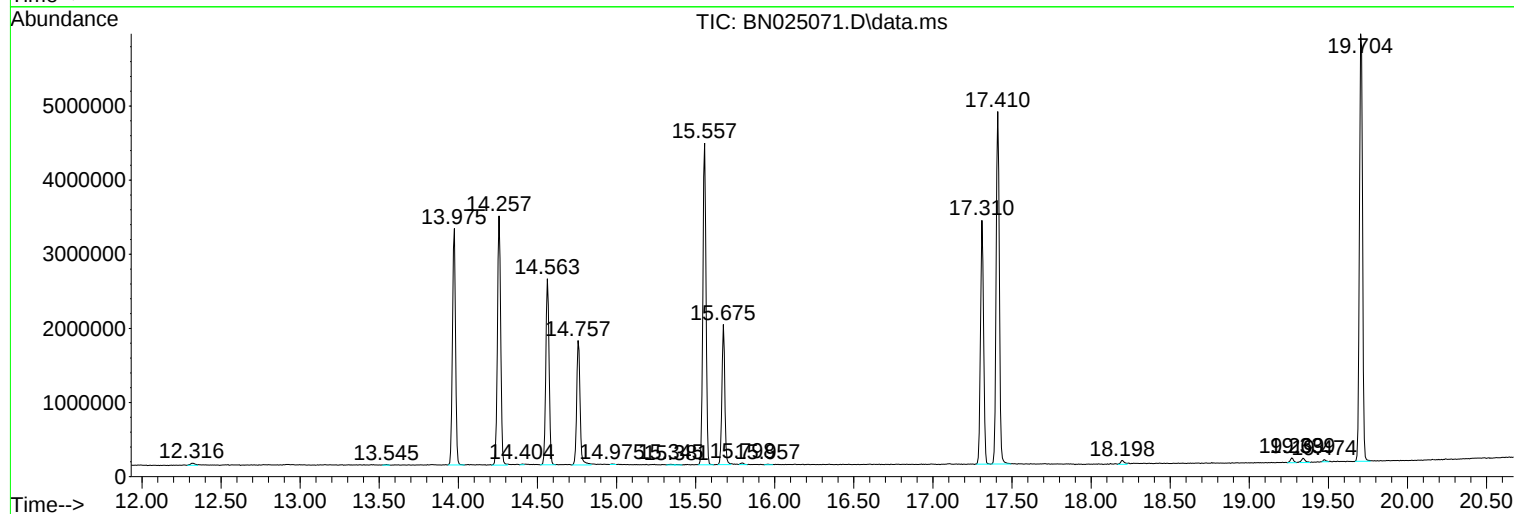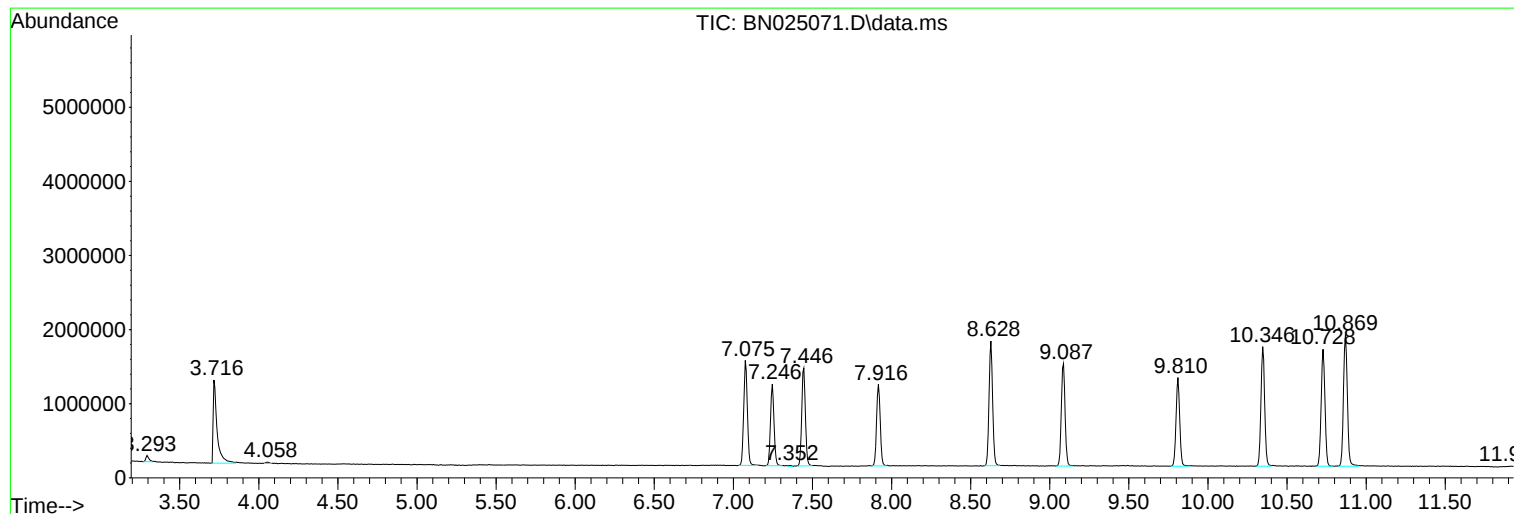

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025071.D
Acq On : 22 Apr 2023 12:09
Operator : CG/JU
Sample : PB152281BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK281

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025071.D
Acq On : 22 Apr 2023 12:09
Operator : CG/JU
Sample : PB152281BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK281

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------