

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
 Data File : BN025086.D
 Acq On : 22 Apr 2023 21:05
 Operator : CG/JU
 Sample : PB152278BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK278

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN025086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	14	18	30	rVB	62163	94393	1.18%	0.130%
2	3.716	87	90	115	rBV	867219	1544671	19.27%	2.134%
3	4.052	142	147	152	rBV2	15194	24142	0.30%	0.033%
4	7.075	654	661	679	rVB	1137910	1790075	22.33%	2.473%
5	7.246	683	690	700	rBV	911303	1418641	17.70%	1.960%
6	7.440	713	723	733	rBV	1062898	1728124	21.56%	2.387%
7	7.916	797	804	812	rBV	818781	1302807	16.25%	1.800%
8	8.628	917	925	937	rBV	1334117	2148595	26.80%	2.968%
9	9.087	993	1003	1015	rBV	1083857	1804326	22.51%	2.492%
10	9.810	1119	1126	1138	rBV	900967	1491729	18.61%	2.061%
11	10.346	1209	1217	1230	rBV	1276585	2115624	26.39%	2.922%
12	10.728	1274	1282	1292	rBV	1233721	2029063	25.31%	2.803%
13	10.869	1298	1306	1320	rBV	1417585	2462308	30.72%	3.401%
14	11.987	1490	1496	1501	rVB9	5147	12215	0.15%	0.017%
15	12.322	1547	1553	1559	rBV2	21241	36538	0.46%	0.050%
16	12.916	1649	1654	1659	rBV4	7977	13896	0.17%	0.019%
17	13.451	1740	1745	1752	rVB	22402	37566	0.47%	0.052%
18	13.828	1806	1809	1813	rBV6	5359	8756	0.11%	0.012%
19	13.969	1827	1833	1845	rBV	2590830	3629845	45.28%	5.014%
20	14.257	1875	1882	1893	rBV	2696011	3919056	48.89%	5.414%
21	14.563	1926	1934	1941	rBV	1913603	2804803	34.99%	3.874%
22	14.757	1960	1967	1983	rBV	1370804	1945714	24.27%	2.688%
23	14.969	2002	2003	2010	rVB7	5858	8224	0.10%	0.011%
24	15.551	2096	2102	2111	rBV	3506997	5085976	63.44%	7.026%
25	15.675	2117	2123	2132	rBV	1369829	1785359	22.27%	2.466%
26	15.792	2139	2143	2149	rVB3	15975	27703	0.35%	0.038%
27	17.310	2394	2401	2411	rBV	2549700	3510387	43.79%	4.849%
28	17.410	2411	2418	2431	rBV	4071802	5718993	71.34%	7.900%
29	18.198	2548	2552	2555	rBV6	10460	16334	0.20%	0.023%
30	19.269	2729	2734	2740	rBV3	50422	77694	0.97%	0.107%
31	19.339	2742	2746	2752	rBV	44089	66694	0.83%	0.092%
32	19.704	2802	2808	2814	rBV	5334740	6839951	85.32%	9.448%
33	21.504	3109	3114	3125	rBV	3300012	4188646	52.25%	5.786%
34	23.792	3495	3503	3518	rBV2	3996129	8016455	100.00%	11.074%
35	23.945	3522	3529	3541	rVB2	2391583	4687465	58.47%	6.475%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025086.D
Acq On : 22 Apr 2023 21:05
Operator : CG/JU
Sample : PB152278BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK278

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Title : SVOA CALIBRATION




Sum of corrected areas: 72392768

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025086.D
Acq On : 22 Apr 2023 21:05
Operator : CG/JU
Sample : PB152278BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK278

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

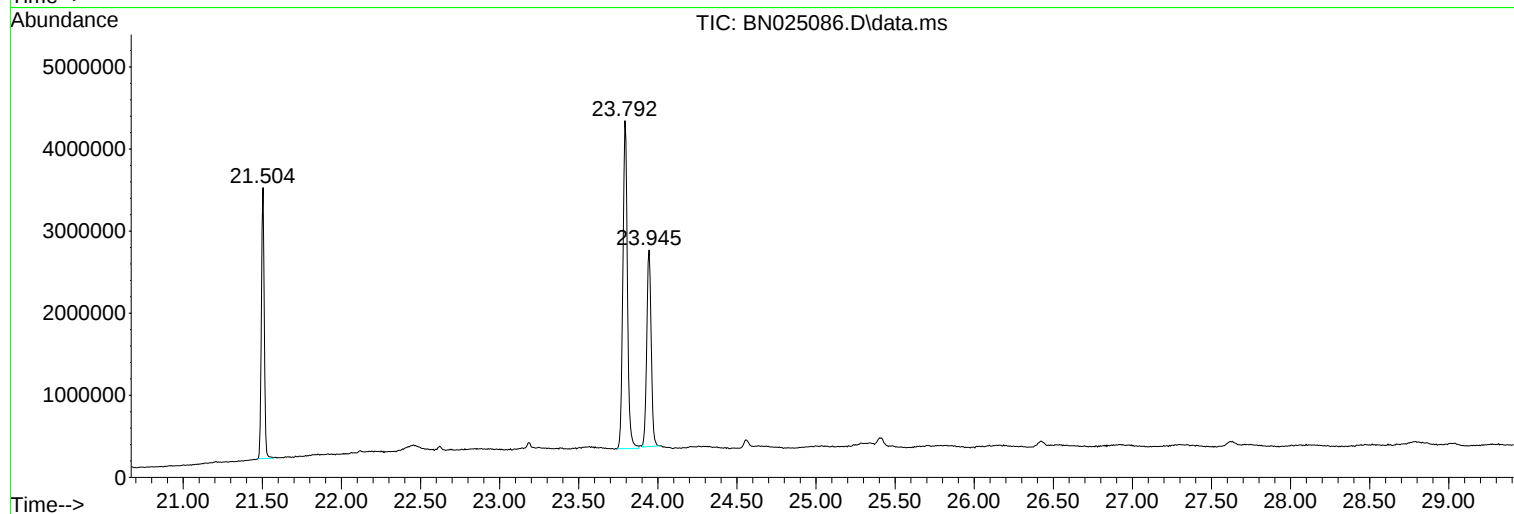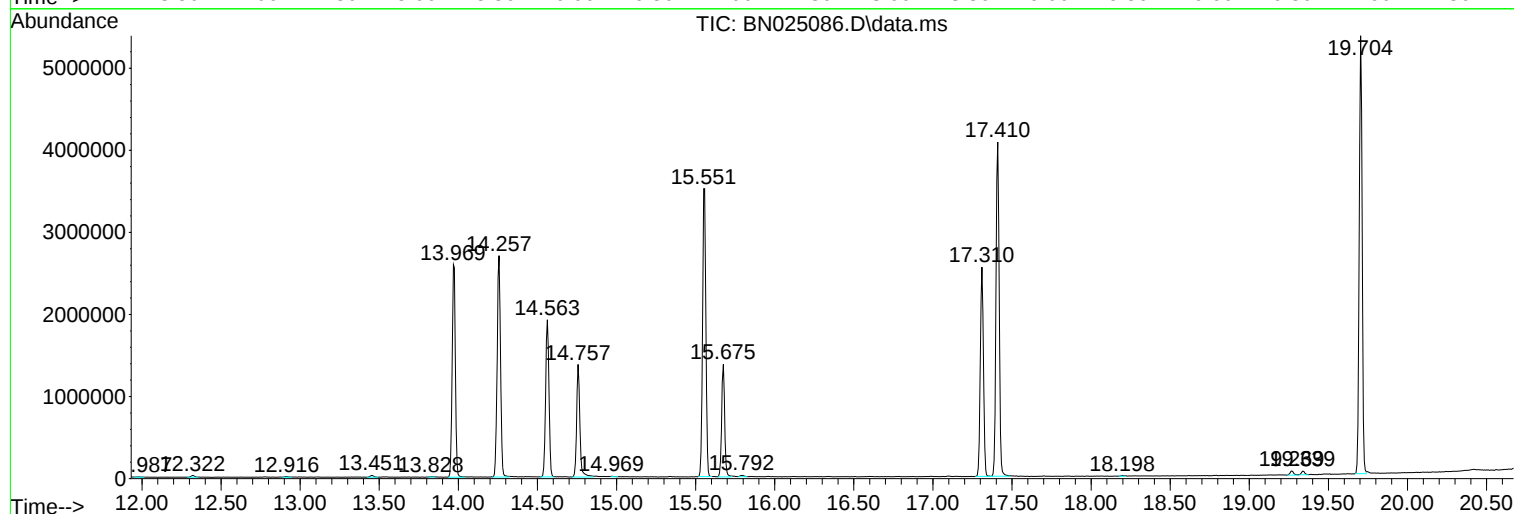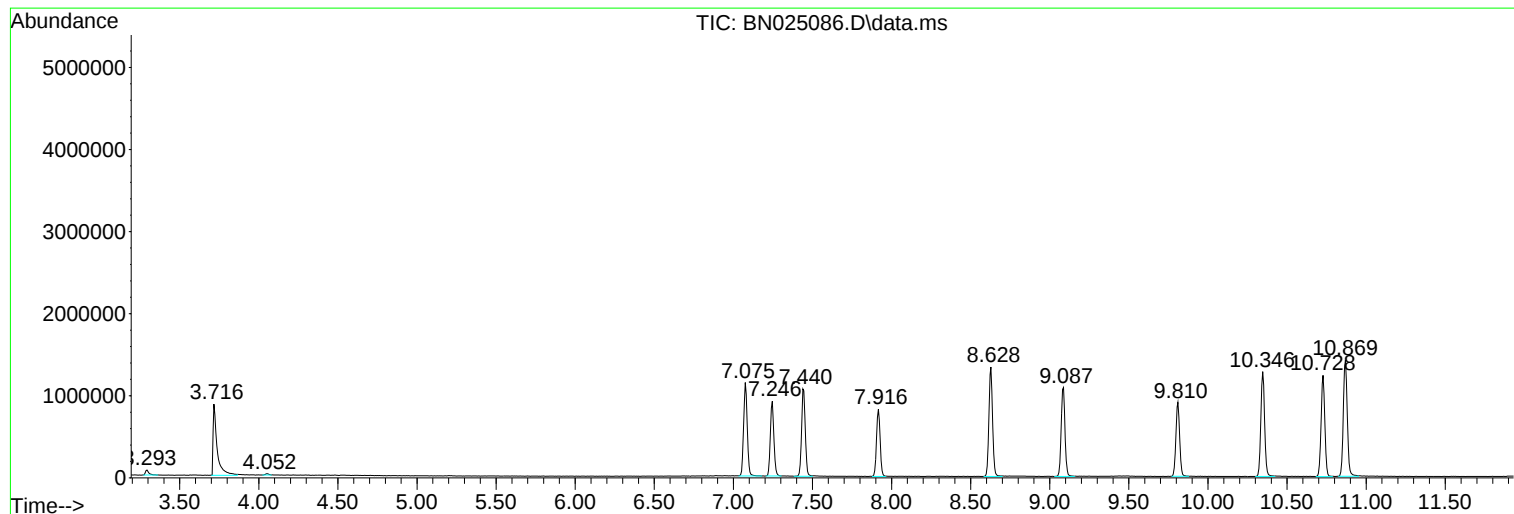

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025086.D
Acq On : 22 Apr 2023 21:05
Operator : CG/JU
Sample : PB152278BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK278

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025086.D
Acq On : 22 Apr 2023 21:05
Operator : CG/JU
Sample : PB152278BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK278

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------