

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
 Data File : BN025089.D
 Acq On : 22 Apr 2023 23:28
 Operator : CG/JU
 Sample : PB152283BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK283

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN025089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	14	18	26	rBV	78668	114292	1.18%	0.133%
2	3.717	87	90	116	rBV	1052216	1813961	18.67%	2.107%
3	4.052	143	147	151	rBV2	25951	33449	0.34%	0.039%
4	7.075	654	661	675	rBV	1396593	2157970	22.21%	2.506%
5	7.246	681	690	700	rBV	1155943	1752887	18.04%	2.036%
6	7.446	714	724	736	rBV	1330312	2146836	22.10%	2.493%
7	7.916	797	804	816	rBV	957332	1507068	15.51%	1.750%
8	8.628	918	925	937	rBV	1671910	2637561	27.15%	3.063%
9	9.087	992	1003	1015	rBV	1338570	2177953	22.42%	2.529%
10	9.810	1117	1126	1137	rBV	1160388	1861341	19.16%	2.162%
11	10.346	1209	1217	1227	rBV	1601727	2577519	26.53%	2.993%
12	10.728	1274	1282	1292	rBV	1391002	2283575	23.51%	2.652%
13	10.869	1298	1306	1319	rBV	1765405	2949363	30.36%	3.425%
14	11.904	1480	1482	1488	rVB4	5482	10406	0.11%	0.012%
15	12.322	1547	1553	1559	rBV2	25961	44447	0.46%	0.052%
16	12.916	1650	1654	1662	rBV8	6833	13039	0.13%	0.015%
17	13.451	1739	1745	1752	rBV6	7152	13874	0.14%	0.016%
18	13.828	1806	1809	1818	rVB6	5331	11961	0.12%	0.014%
19	13.975	1826	1834	1843	rBV	3274401	4429418	45.59%	5.144%
20	14.257	1875	1882	1897	rBV	3350489	4789083	49.29%	5.562%
21	14.563	1927	1934	1944	rBV	2111924	3143931	32.36%	3.651%
22	14.757	1959	1967	1984	rBV	1701718	2478625	25.51%	2.879%
23	15.340	2062	2066	2070	rBV5	5937	9975	0.10%	0.012%
24	15.557	2094	2103	2111	rBV	4408623	6123992	63.03%	7.112%
25	15.675	2116	2123	2136	rVV	1837757	2405617	24.76%	2.794%
26	15.792	2139	2143	2150	rVV2	23021	39807	0.41%	0.046%
27	17.310	2395	2401	2409	rBV	2771846	3882916	39.97%	4.509%
28	17.410	2412	2418	2435	rVB2	5200666	7092524	73.00%	8.237%
29	17.704	2463	2468	2474	rVB6	8985	15562	0.16%	0.018%
30	18.204	2548	2553	2555	rBV5	8796	13851	0.14%	0.016%
31	19.269	2730	2734	2741	rVB3	59674	83334	0.86%	0.097%
32	19.339	2741	2746	2753	rBV	57351	86986	0.90%	0.101%
33	19.704	2802	2808	2820	rBV	5996813	8133400	83.72%	9.446%
34	21.510	3109	3115	3122	rBV	3455756	4548480	46.82%	5.282%
35	23.786	3495	3502	3516	rBV	5213207	9715256	100.00%	11.283%
36	23.939	3521	3528	3538	rVB	2360631	5007902	51.55%	5.816%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025089.D
Acq On : 22 Apr 2023 23:28
Operator : CG/JU
Sample : PB152283BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK283

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Title : SVOA CALIBRATION




Sum of corrected areas: 86108161

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025089.D
Acq On : 22 Apr 2023 23:28
Operator : CG/JU
Sample : PB152283BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK283

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

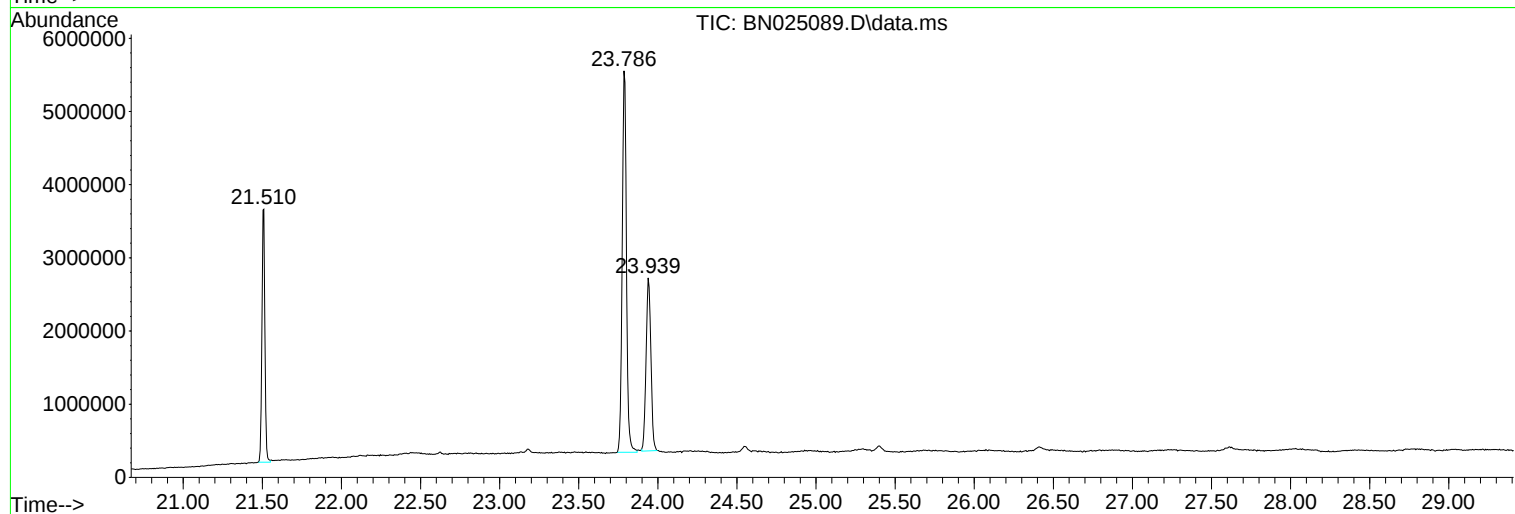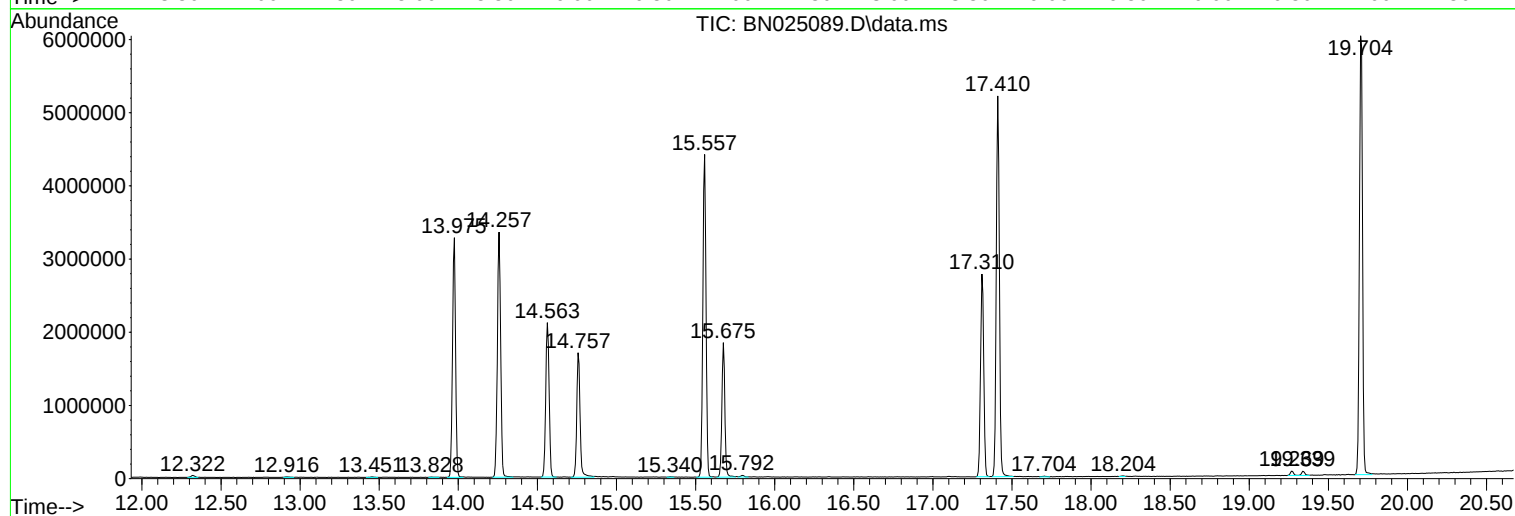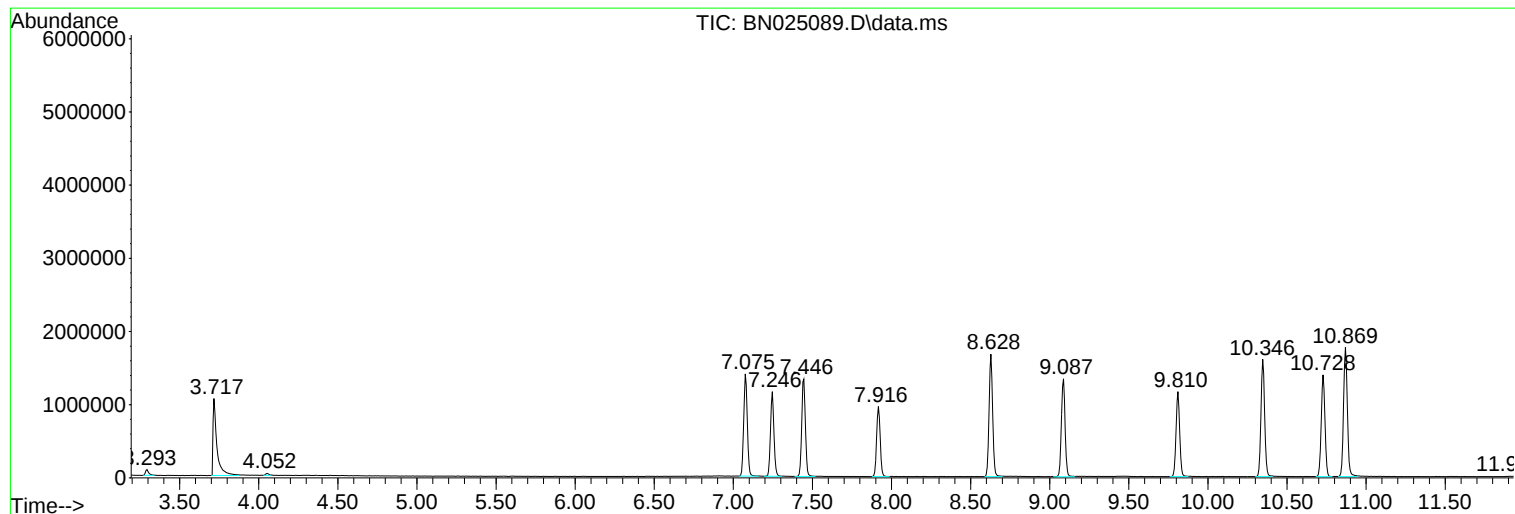

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025089.D
Acq On : 22 Apr 2023 23:28
Operator : CG/JU
Sample : PB152283BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK283

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025089.D
Acq On : 22 Apr 2023 23:28
Operator : CG/JU
Sample : PB152283BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK283

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc