

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
 Data File : BN025099.D
 Acq On : 23 Apr 2023 05:26
 Operator : CG/JU
 Sample : 02399-11
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN025099.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	15	18	28	rVB	76906	114840	0.82%	0.104%
2	3.728	90	92	108	rBV	228705	389106	2.78%	0.352%
3	3.958	128	131	137	rVB5	14486	21488	0.15%	0.019%
4	4.052	144	147	153	rVB2	23927	36586	0.26%	0.033%
5	5.205	338	343	353	rVB	36020	60549	0.43%	0.055%
6	6.905	627	632	636	rBV3	16317	32444	0.23%	0.029%
7	7.075	655	661	670	rVB	345373	532827	3.81%	0.482%
8	7.246	683	690	700	rBV	1511363	2349514	16.78%	2.125%
9	7.446	716	724	734	rBV	1317970	2130830	15.22%	1.928%
10	7.528	734	738	744	rVB4	9698	15866	0.11%	0.014%
11	7.799	778	784	790	rBV5	13056	23426	0.17%	0.021%
12	7.916	797	804	819	rBV	1238833	2051168	14.65%	1.856%
13	8.269	859	864	870	rBV2	39035	68084	0.49%	0.062%
14	8.628	916	925	935	rBV	1046872	1666062	11.90%	1.507%
15	9.087	994	1003	1015	rBV	1893124	3054901	21.82%	2.764%
16	9.310	1035	1041	1051	rBV2	18770	40536	0.29%	0.037%
17	9.810	1118	1126	1134	rBV	1538723	2460086	17.57%	2.225%
18	10.346	1209	1217	1230	rBV	2017023	3298368	23.56%	2.984%
19	10.587	1252	1258	1266	rBV	76807	131052	0.94%	0.119%
20	10.728	1274	1282	1290	rBV	1834601	3031868	21.65%	2.743%
21	10.869	1298	1306	1318	rBV	1631807	2781313	19.86%	2.516%
22	11.116	1341	1348	1353	rVB2	41482	69836	0.50%	0.063%
23	11.516	1412	1416	1421	rBV6	9324	18524	0.13%	0.017%
24	12.316	1546	1552	1559	rVB	38598	63868	0.46%	0.058%
25	12.728	1617	1622	1625	rBV4	17166	28114	0.20%	0.025%
26	12.757	1625	1627	1635	rVB8	10689	18303	0.13%	0.017%
27	12.916	1649	1654	1659	rBV4	7451	15119	0.11%	0.014%
28	12.993	1663	1667	1676	rBV9	8474	17926	0.13%	0.016%
29	13.363	1724	1730	1739	rBV3	50431	83170	0.59%	0.075%
30	13.451	1739	1745	1751	rVV	40914	67459	0.48%	0.061%
31	13.975	1827	1834	1842	rBV	4621412	6188362	44.20%	5.598%
32	14.257	1875	1882	1894	rBV	4785578	6917462	49.41%	6.258%
33	14.434	1907	1912	1918	rBV	34316	52490	0.37%	0.047%
34	14.563	1927	1934	1943	rBV	2986024	4257388	30.41%	3.851%
35	14.757	1962	1967	1982	rBV	322502	579856	4.14%	0.525%
36	14.881	1983	1988	1993	rVB	46290	67690	0.48%	0.061%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
 Data File : BN025099.D
 Acq On : 23 Apr 2023 05:26
 Operator : CG/JU
 Sample : 02399-11
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

37	14.969	1999	2003	2008	rVB7	12564	19108	0.14%	0.017%
38	15.557	2093	2103	2117	rBV	6284648	8893997	63.52%	8.046%
39	15.675	2117	2123	2133	rBV	2671313	3427659	24.48%	3.101%
40	15.792	2140	2143	2151	rVB3	32631	49126	0.35%	0.044%
41	16.339	2232	2236	2242	rVB8	10958	18021	0.13%	0.016%
42	16.710	2295	2299	2305	rBV2	32102	40837	0.29%	0.037%
43	16.769	2305	2309	2314	rVV8	19062	26752	0.19%	0.024%
44	17.098	2361	2365	2369	rBV4	9035	14833	0.11%	0.013%
45	17.310	2394	2401	2410	rBV	3785996	5243784	37.45%	4.744%
46	17.410	2411	2418	2434	rVV2	7399646	10263941	73.31%	9.285%
47	17.692	2462	2466	2474	rVB6	10564	21470	0.15%	0.019%
48	18.198	2547	2552	2558	rBV	61269	89935	0.64%	0.081%
49	19.269	2729	2734	2740	rBV	98144	147310	1.05%	0.133%
50	19.339	2741	2746	2751	rVV	96794	149809	1.07%	0.136%
51	19.475	2765	2769	2775	rBV2	70244	96213	0.69%	0.087%
52	19.622	2791	2794	2799	rVB	45701	57191	0.41%	0.052%
53	19.704	2802	2808	2814	rBV	9096625	12259774	87.56%	11.091%
54	20.669	2969	2972	2976	rBV3	51619	70457	0.50%	0.064%
55	21.504	3108	3114	3120	rBV	4562835	6110257	43.64%	5.528%
56	23.792	3494	3503	3516	rBV2	7202216	14001411	100.00%	12.666%
57	23.945	3521	3529	3542	rVB2	3112361	6803466	48.59%	6.155%




Sum of corrected areas: 110541832

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025099.D
Acq On : 23 Apr 2023 05:26
Operator : CG/JU
Sample : 02399-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

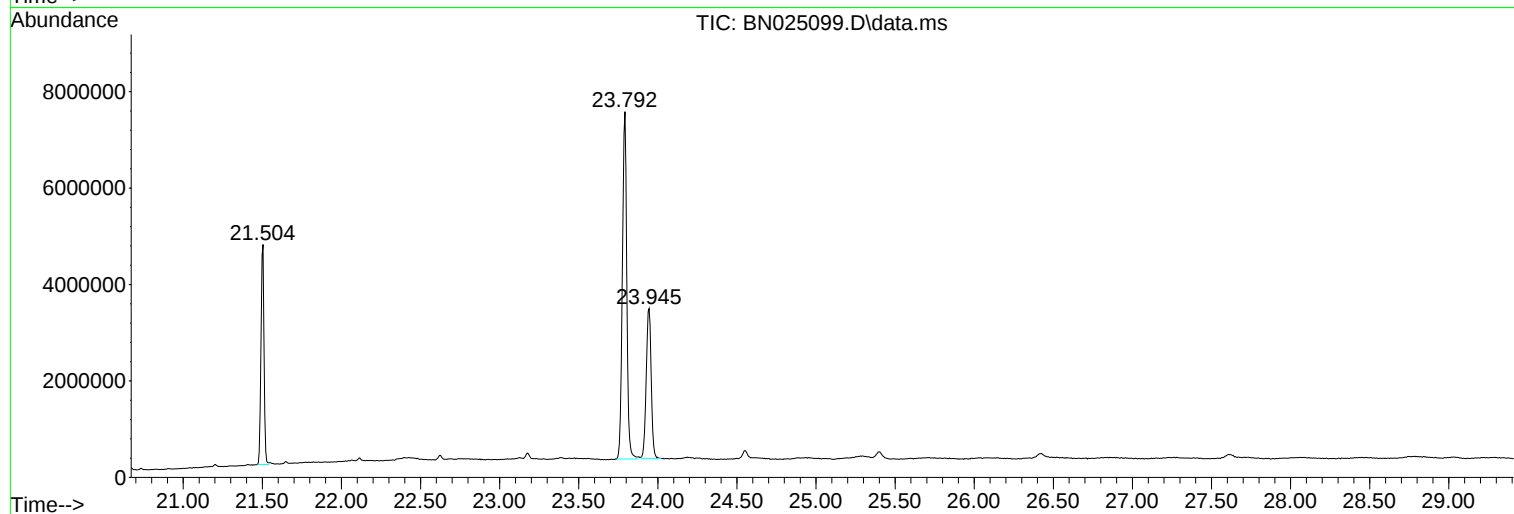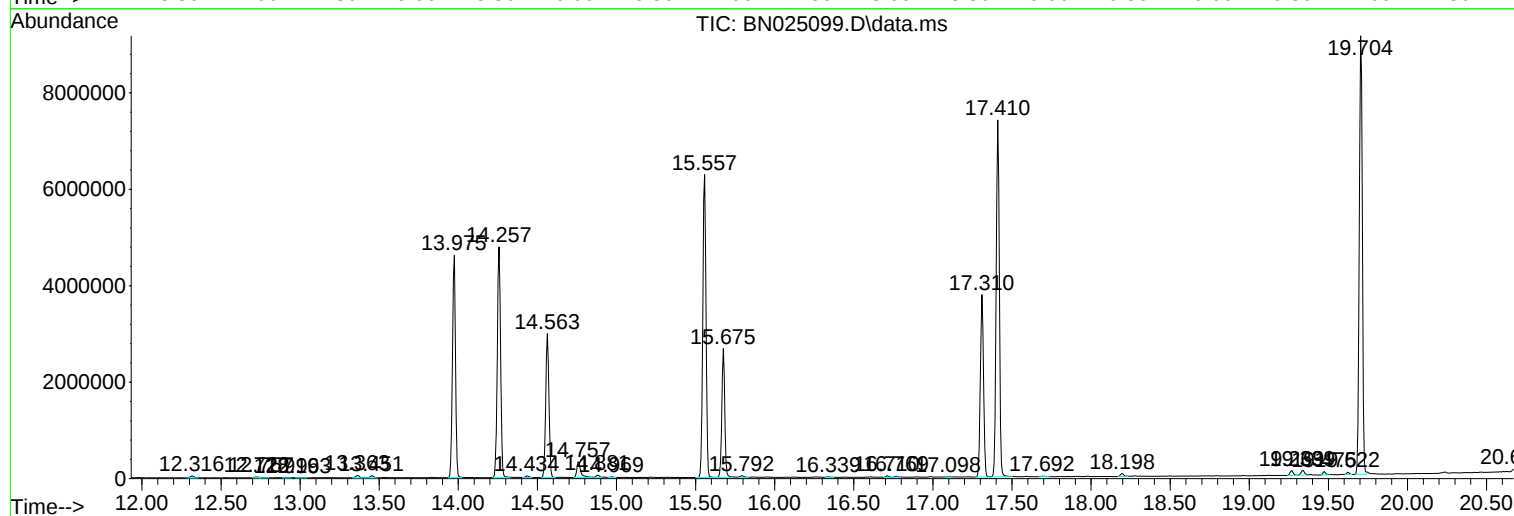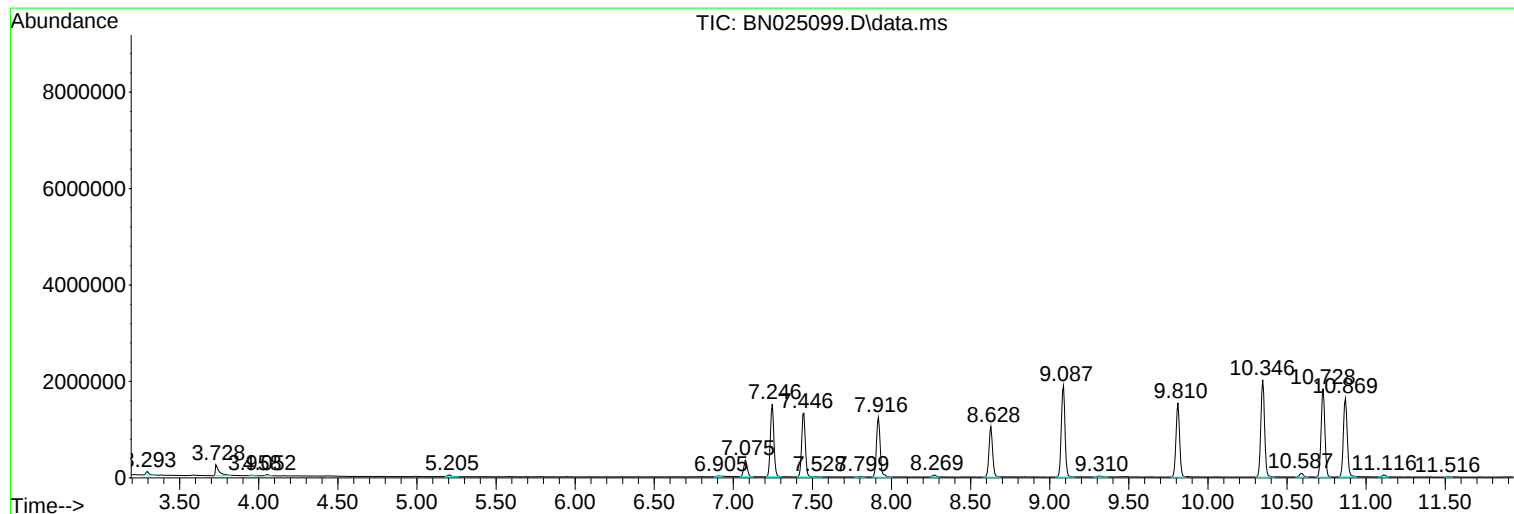

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025099.D
Acq On : 23 Apr 2023 05:26
Operator : CG/JU
Sample : 02399-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042223\
Data File : BN025099.D
Acq On : 23 Apr 2023 05:26
Operator : CG/JU
Sample : 02399-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc