

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031116.D
 Acq On : 22 Apr 2024 10:56
 Operator : MA/JU
 Sample : PB160379BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK379

Quant Time: Apr 22 23:25:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 22:56:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	116493	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.410	136	538939	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.275	164	373217	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.028	188	844268	20.000	ng/ul	0.00
79) Chrysene-d12	21.263	240	950457	20.000	ng/ul	0.00
88) Perylene-d12	24.168	264	1170689	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	14273	5.724	ng/uL	0.00
4) Pyridine-d5	3.552	84	178733	24.890	ng/ul	0.00
7) Phenol-d5	6.805	99	318538	32.415	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	196511	34.371	ng/ul	0.00
11) 2-Chlorophenol-d4	7.164	132	255862	33.440	ng/ul	0.00
15) 4-Methylphenol-d8	8.334	113	266063	32.194	ng/ul	0.00
21) Nitrobenzene-d5	8.787	128	131977	34.083	ng/ul	0.00
24) 2-Nitrophenol-d4	9.505	143	135805	33.740	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.034	165	256896	32.364	ng/ul	0.00
31) 4-Chloroaniline-d4	10.552	131	316757	25.536	ng/ul	-0.01
46) Dimethylphthalate-d6	13.693	166	882098	33.964	ng/ul	0.00
49) Acenaphthylene-d8	13.969	160	1017362	34.568	ng/ul	0.00
54) 4-Nitrophenol-d4	14.493	143	148925	27.473	ng/ul	0.00
60) Fluorene-d10	15.275	176	805611	35.633	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.398	200	99800	23.430	ng/ul	0.00
73) Anthracene-d10	17.128	188	1335934	36.507	ng/ul	0.00
81) Pyrene-d10	19.428	212	1672714	35.814	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.968	264	1978732	35.643	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.334	70	6495	1.018 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031116.D
Acq On : 22 Apr 2024 10:56
Operator : MA/JU
Sample : PB160379BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK379


Quant Time: Apr 22 23:25:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 22:56:25 2024
Response via : Initial Calibration

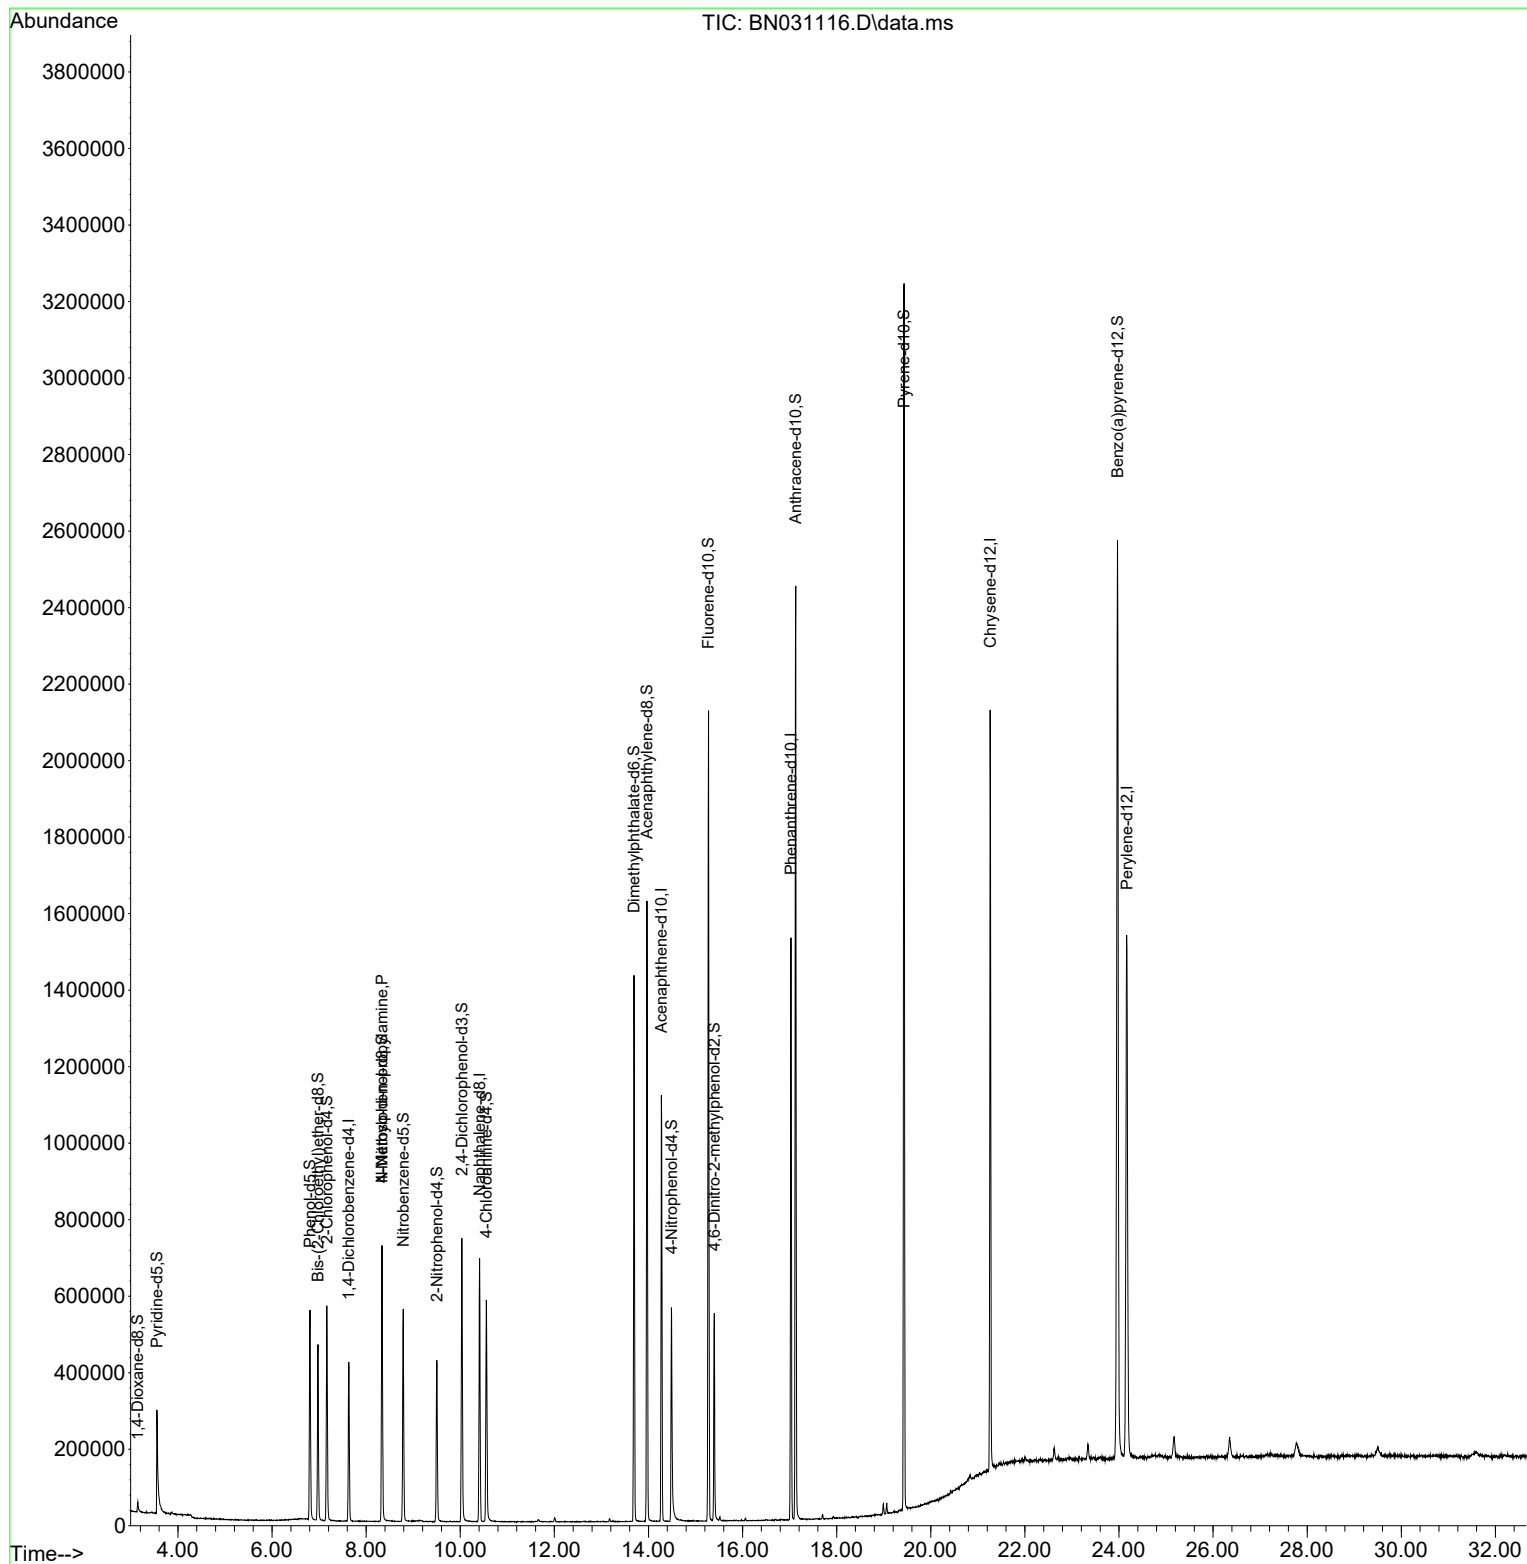

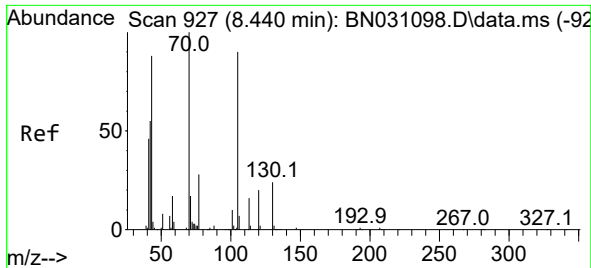

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.018 ng/ul
 RT: 8.334 min Scan# 909
 Delta R.T. -0.106 min
 Lab File: BN031116.D
 Acq: 22 Apr 2024 10:56

Instrument :
 BNA_N
 ClientSampleId :
 SBLK379

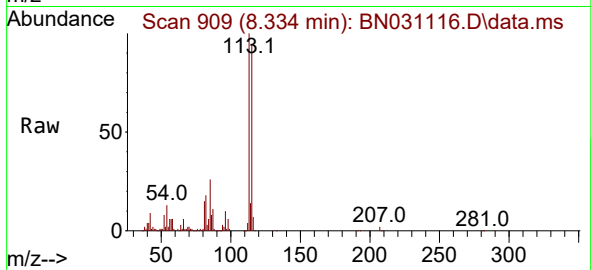

Tgt Ion: 70 Resp: 6495

Ion	Ratio	Lower	Upper
70	100		
42	353.8	45.0	67.6#
101	0.0	8.1	12.1#
130	0.0	19.2	28.8#

