

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031149.D
 Acq On : 23 Apr 2024 10:17
 Operator : MA/JU
 Sample : PB160417BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK417

Quant Time: Apr 23 22:40:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 22:56:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	117086	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.410	136	542410	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.275	164	369171	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.028	188	856488	20.000	ng/ul	0.00
79) Chrysene-d12	21.263	240	1003776	20.000	ng/ul	0.00
88) Perylene-d12	24.163	264	1200711	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	19014	7.587	ng/uL	0.00
4) Pyridine-d5	3.546	84	273974	37.960	ng/ul	0.00
7) Phenol-d5	6.805	99	379213	38.394	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.969	67	222524	38.723	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.163	132	306173	39.812	ng/ul	0.00
15) 4-Methylphenol-d8	8.334	113	311718	37.527	ng/ul	0.00
21) Nitrobenzene-d5	8.787	128	158438	40.655	ng/ul	0.00
24) 2-Nitrophenol-d4	9.499	143	170986	42.208	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.034	165	302714	37.892	ng/ul	0.00
31) 4-Chloroaniline-d4	10.552	131	450443	36.081	ng/ul	-0.01
46) Dimethylphthalate-d6	13.693	166	1005577	39.143	ng/ul	0.00
49) Acenaphthylene-d8	13.969	160	1170921	40.222	ng/ul	0.00
54) 4-Nitrophenol-d4	14.487	143	193790	36.142	ng/ul	0.00
60) Fluorene-d10	15.275	176	917565	41.029	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.398	200	133825	30.970	ng/ul	0.00
73) Anthracene-d10	17.128	188	1560517	42.036	ng/ul	0.00
81) Pyrene-d10	19.427	212	1970622	39.952	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.968	264	2399539	42.143	ng/ul	0.00


Target Compounds					Qvalue	
17) N-Nitroso-di-n-propyla...	8.334	70	7565	1.179	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031149.D
Acq On : 23 Apr 2024 10:17
Operator : MA/JU
Sample : PB160417BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK417


Quant Time: Apr 23 22:40:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 22:56:25 2024
Response via : Initial Calibration

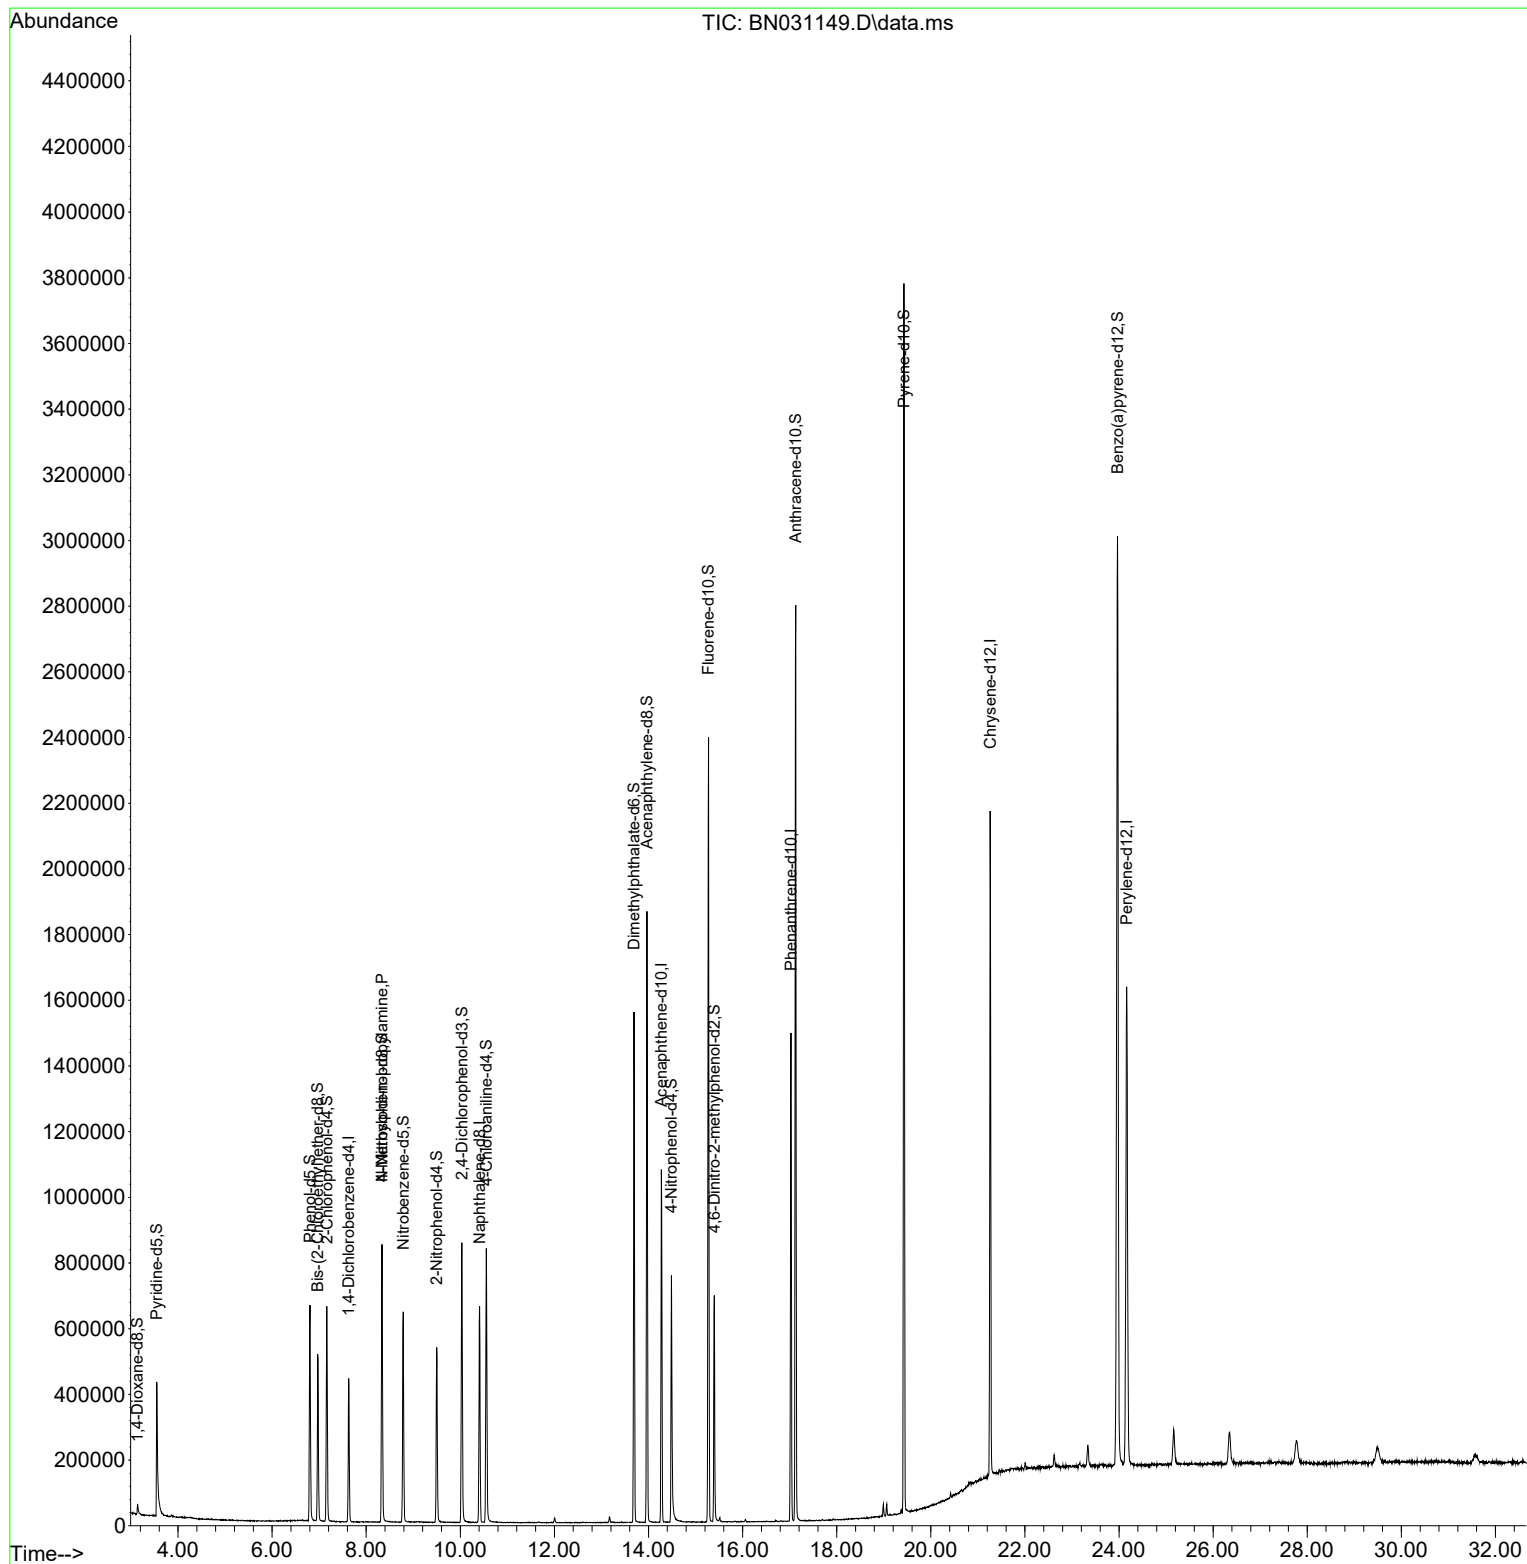

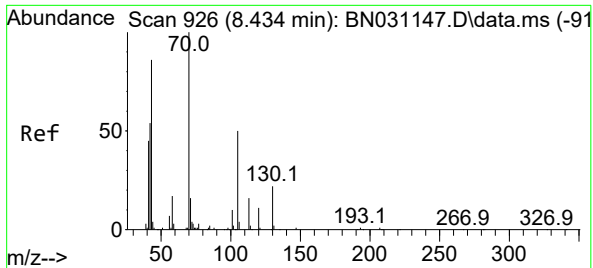

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.179 ng/ul
 RT: 8.334 min Scan# 909
 Delta R.T. -0.106 min
 Lab File: BN031149.D
 Acq: 23 Apr 2024 10:17

Instrument :
 BNA_N
 ClientSampleId :
 SBLK417

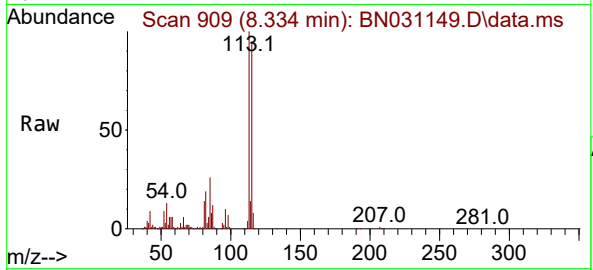

Tgt Ion: 70 Resp: 7565

Ion	Ratio	Lower	Upper
70	100		
42	380.2	45.0	67.6#
101	0.0	8.1	12.1#
130	0.0	19.2	28.8#

