

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031118.D
 Acq On : 22 Apr 2024 12:14
 Operator : MA/JU
 Sample : P2170-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EZZZ7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/24/2024

Quant Time: Apr 22 23:41:50 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 22:56:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	101838	20.000	ng/u1	0.00
20) Naphthalene-d8	10.410	136	472882	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.274	164	317046	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.027	188	742610	20.000	ng/u1	0.00
79) Chrysene-d12	21.268	240	876809	20.000	ng/u1	0.00
88) Perylene-d12	24.168	264	1097027	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	6311	2.895	ng/uL	0.00
4) Pyridine-d5	3.557	84	62418	9.943	ng/u1	0.00
7) Phenol-d5	6.804	99	169271	19.704	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	110390	22.086	ng/u1	0.00
11) 2-Chlorophenol-d4	7.163	132	139671	20.881	ng/u1	0.00
15) 4-Methylphenol-d8	8.339	113	90485	12.524	ng/u1	0.00
21) Nitrobenzene-d5	8.787	128	71933	21.172	ng/u1	0.00
24) 2-Nitrophenol-d4	9.504	143	68882	19.504	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.034	165	146005	20.963	ng/u1	0.00
31) 4-Chloroaniline-d4	10.557	131	166537	15.301	ng/u1	0.00
46) Dimethylphthalate-d6	13.692	166	530284	24.036	ng/u1	0.00
49) Acenaphthylene-d8	13.969	160	593593	23.743	ng/u1	0.00
54) 4-Nitrophenol-d4	14.492	143	70918	15.401	ng/u1	0.00
60) Fluorene-d10	15.274	176	503160	26.198	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.398	200	41200	10.997	ng/u1	0.00
73) Anthracene-d10	17.127	188	831034	25.819	ng/u1	0.00
81) Pyrene-d10	19.427	212	1189359	27.604	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.968	264	1441440	27.708	ng/u1	0.00
Target Compounds					Qvalue	
8) Phenol	6.834	94	14984	1.692	ng/u1	97
16) Acetophenone	8.451	105	81366	7.269	ng/u1	99
72) Phenanthrene	17.068	178	46438	1.182	ng/u1	99
80) Fluoranthene	19.092	202	144174	2.827	ng/u1	96
82) Pyrene	19.457	202	142189	2.654	ng/u1	97
85) Benzo(a)anthracene	21.245	228	75008m	1.260	ng/u1	
87) Chrysene	21.309	228	95037	1.682	ng/u1	96
90) Benzo(b)fluoranthene	23.245	252	120898	1.959	ng/u1#	92
93) Benzo(a)pyrene	24.027	252	80094	1.301	ng/u1	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031118.D
Acq On : 22 Apr 2024 12:14
Operator : MA/JU
Sample : P2170-03
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
EZZZ7

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/24/2024


Quant Time: Apr 22 23:41:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 22:56:25 2024
Response via : Initial Calibration

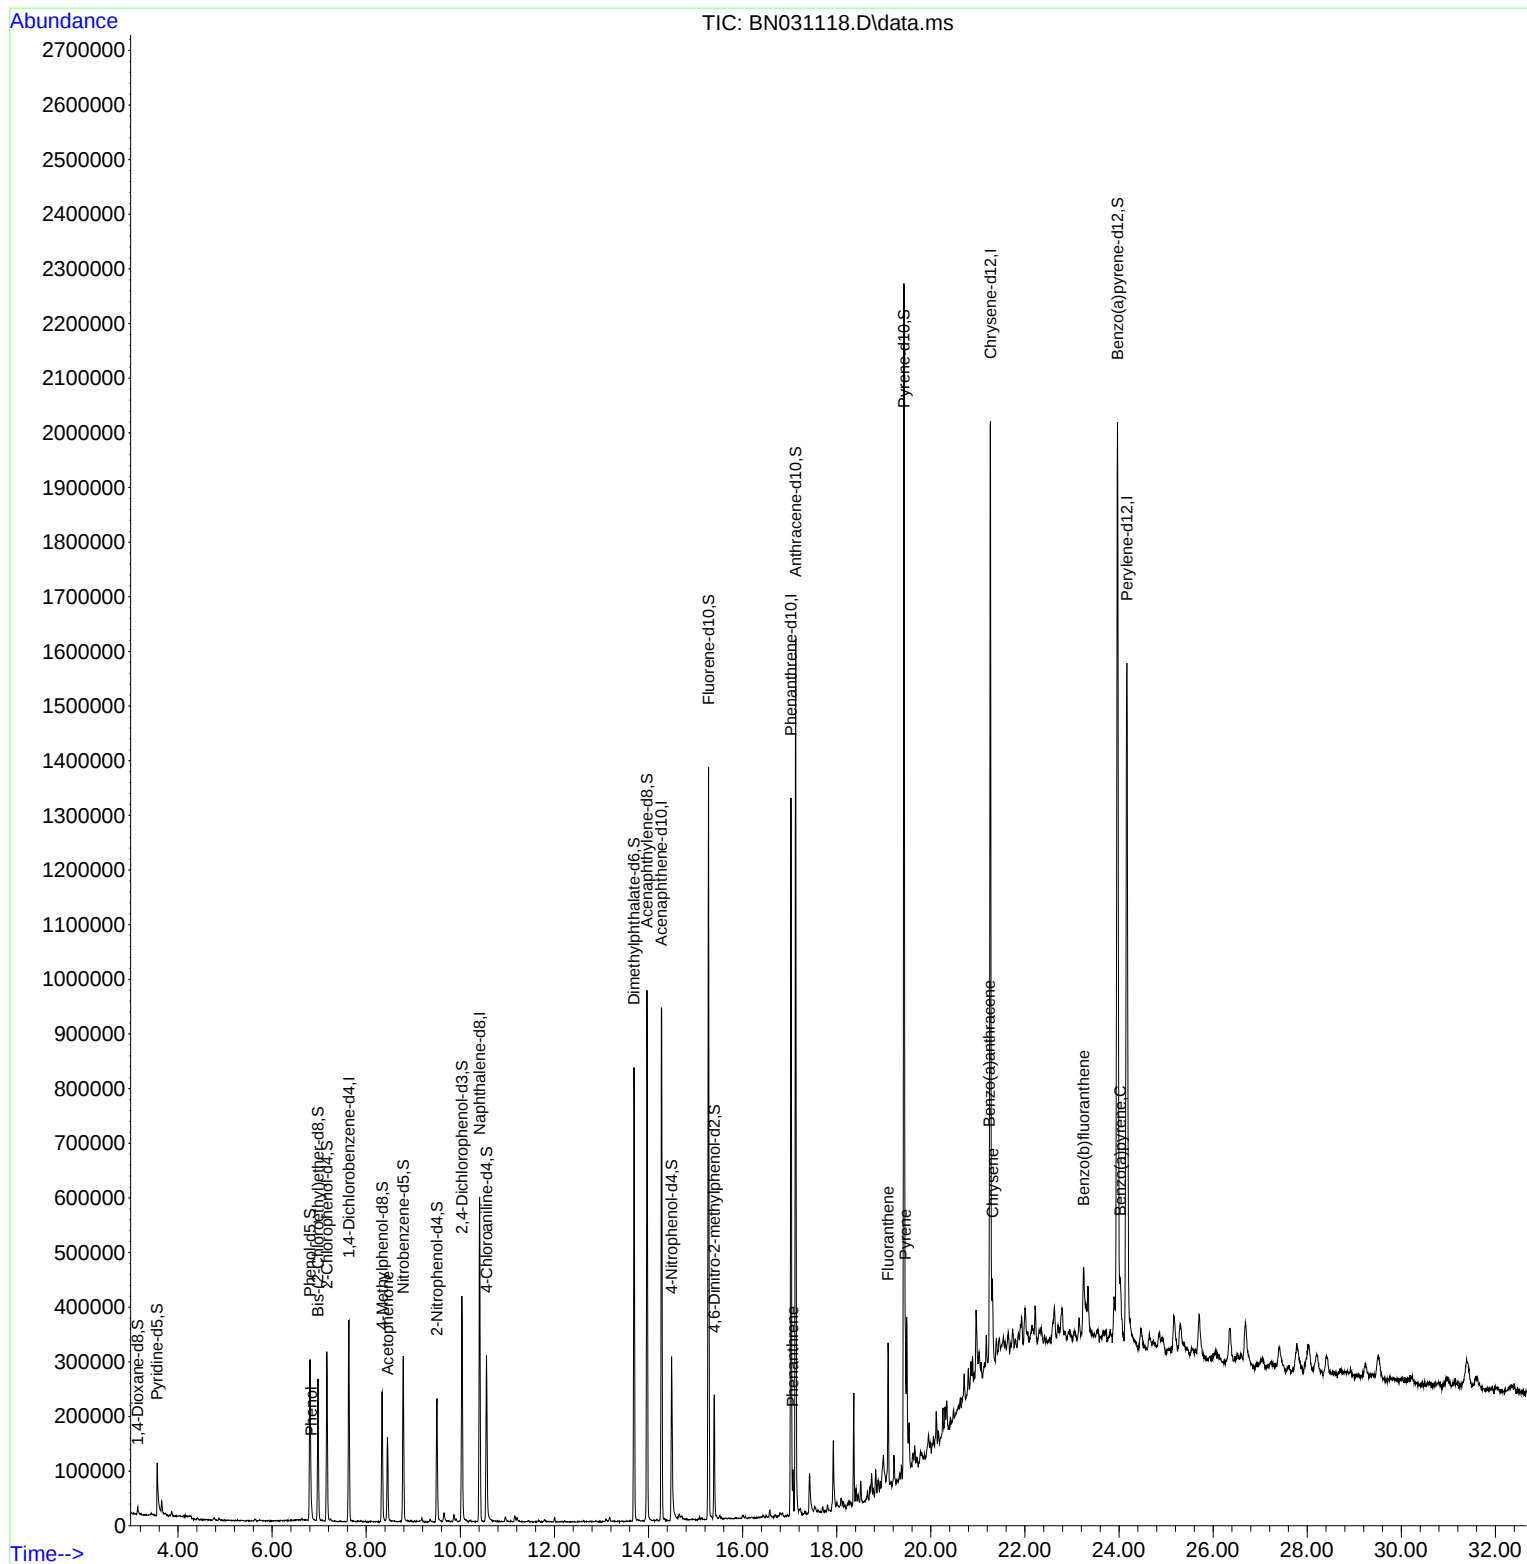

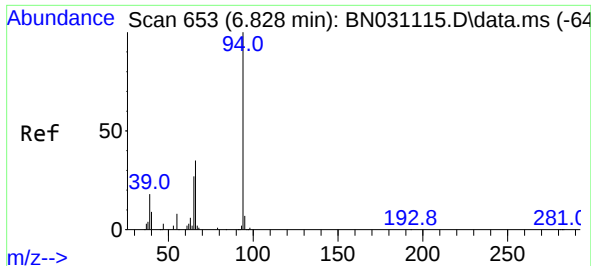

#8
Phenol
Concen: 1.692 ng/ul
RT: 6.834 min Scan# 653
Delta R.T. -0.000 min
Lab File: BN031118.D
Acq: 22 Apr 2024 12:14




Instrument :
BNA_N
ClientSampleId :
EZZZ7

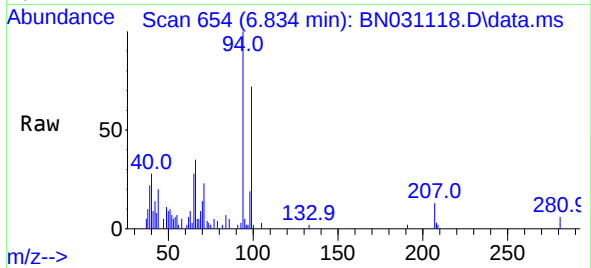

Tgt Ion: 94 Resp: 14984
Ion Ratio Lower Upper
94 100
65 28.0 22.0 33.0
66 34.9 29.8 44.6




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/24/2024

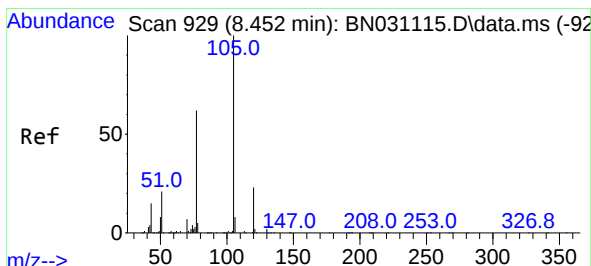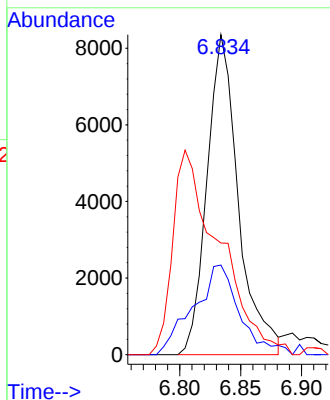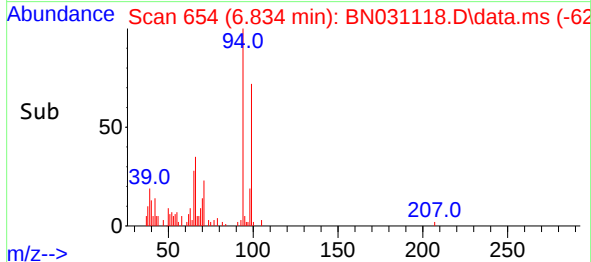

#16
Acetophenone
Concen: 7.269 ng/ul
RT: 8.451 min Scan# 929
Delta R.T. -0.006 min
Lab File: BN031118.D
Acq: 22 Apr 2024 12:14


Tgt Ion:105 Resp: 81366
Ion Ratio Lower Upper
105 100
77 75.8 60.2 90.4
51 25.5 20.6 31.0

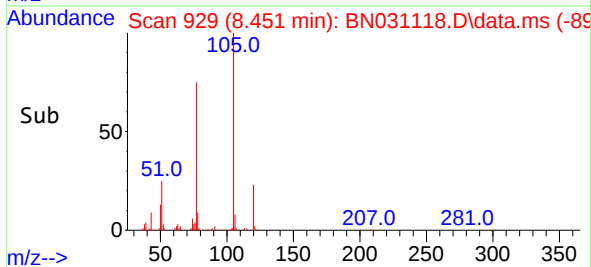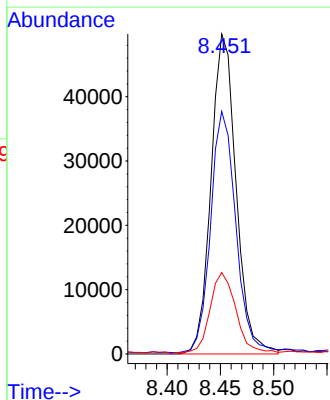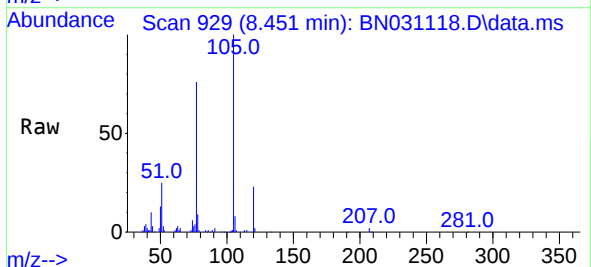

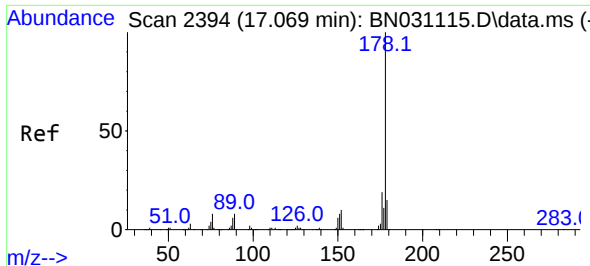

#72
Phenanthrene
Concen: 1.182 ng/ul
RT: 17.068 min Scan# 21
Delta R.T. -0.006 min
Lab File: BN031118.D
Acq: 22 Apr 2024 12:14




Instrument :
BNA_N
ClientSampleId :
EZZZ7

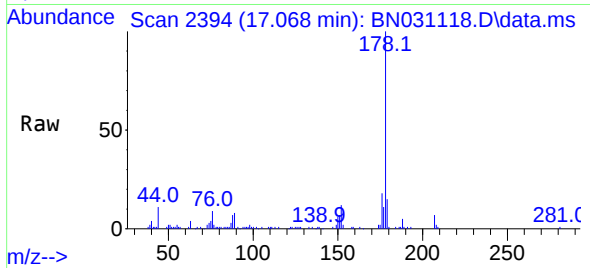


Tgt Ion:178 Resp: 46438
Ion Ratio Lower Upper
178 100
179 15.3 12.4 18.6
176 17.6 14.6 21.8

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/24/2024

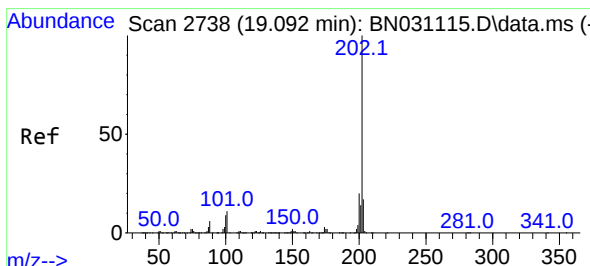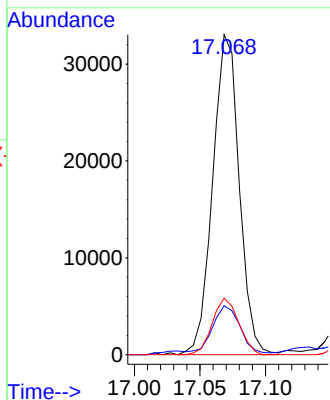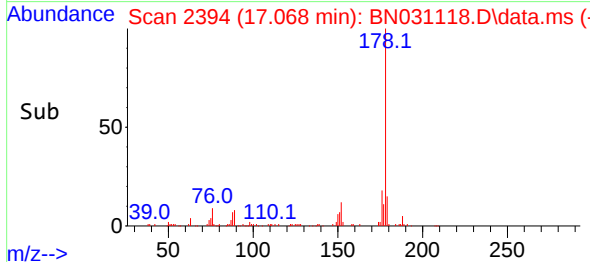


#80
Fluoranthene
Concen: 2.827 ng/ul
RT: 19.092 min Scan# 2738
Delta R.T. -0.006 min
Lab File: BN031118.D
Acq: 22 Apr 2024 12:14

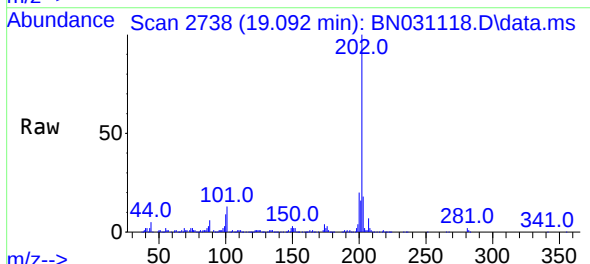


Tgt Ion:202 Resp: 144174
Ion Ratio Lower Upper
202 100
101 13.5 9.0 13.6
100 9.1 6.9 10.3

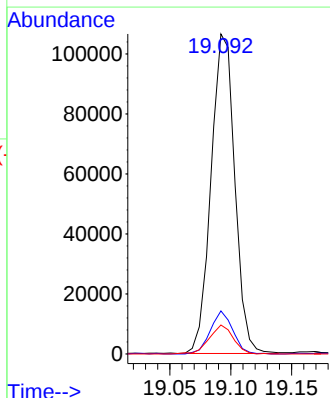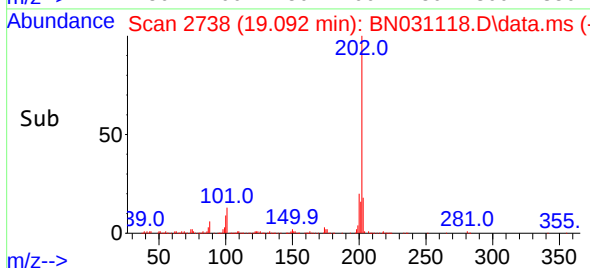

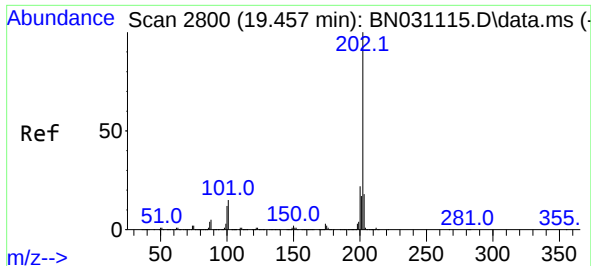

#82
Pyrene
Concen: 2.654 ng/ul
RT: 19.457 min Scan# 21
Delta R.T. -0.006 min
Lab File: BN031118.D
Acq: 22 Apr 2024 12:14




Instrument :
BNA_N
ClientSampleId :
EZZZ7

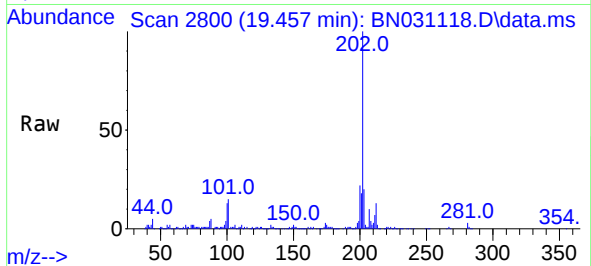


Tgt Ion:202 Resp: 142189
Ion Ratio Lower Upper
202 100
101 14.7 11.1 16.7
100 12.9 9.3 13.9

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/24/2024

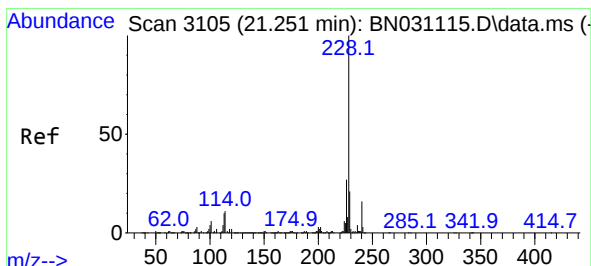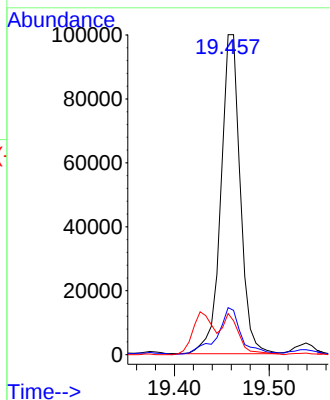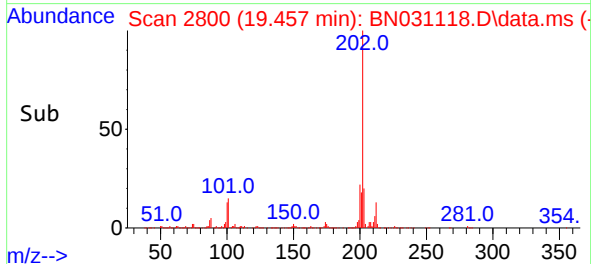


#85
Benzo(a)anthracene
Concen: 1.260 ng/ul m
RT: 21.245 min Scan# 3104
Delta R.T. -0.006 min
Lab File: BN031118.D
Acq: 22 Apr 2024 12:14

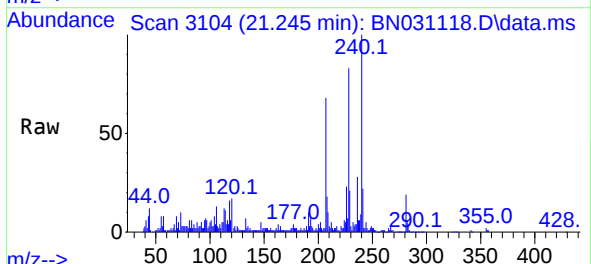


Tgt Ion:228 Resp: 75008
Ion Ratio Lower Upper
228 100
229 25.8 16.7 25.1#
226 28.1 21.2 31.8

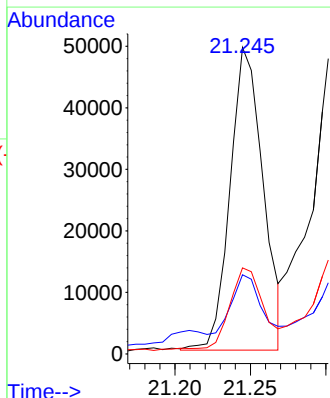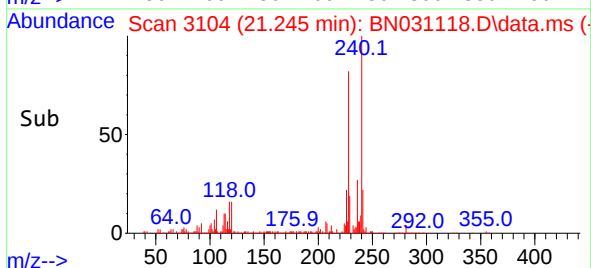

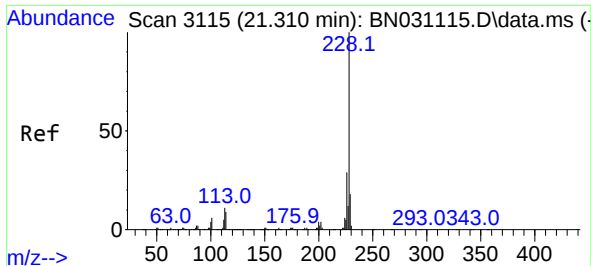

#87
Chrysene
Concen: 1.682 ng/u1
RT: 21.309 min Scan# 3115
Delta R.T. -0.000 min
Lab File: BN031118.D
Acq: 22 Apr 2024 12:14




Instrument :
BNA_N
ClientSampleId :
EZZZ7

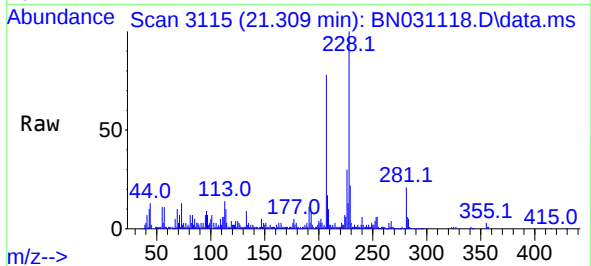


Tgt Ion:228 Resp: 9503
Ion Ratio Lower Upper
228 100
226 30.0 22.6 34.0
229 22.4 15.8 23.8

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/24/2024

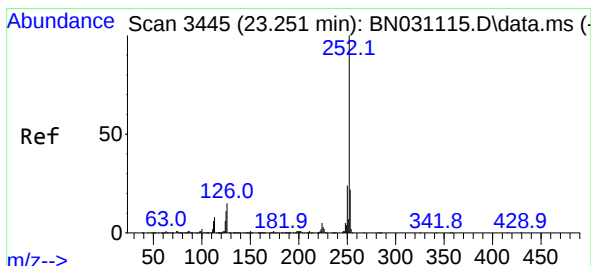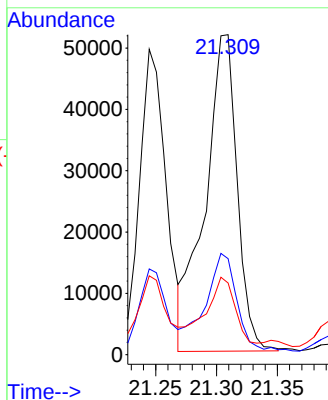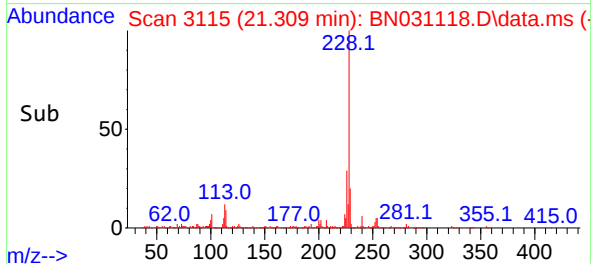


#90
Benzo(b)fluoranthene
Concen: 1.959 ng/u1
RT: 23.245 min Scan# 3444
Delta R.T. -0.012 min
Lab File: BN031118.D
Acq: 22 Apr 2024 12:14

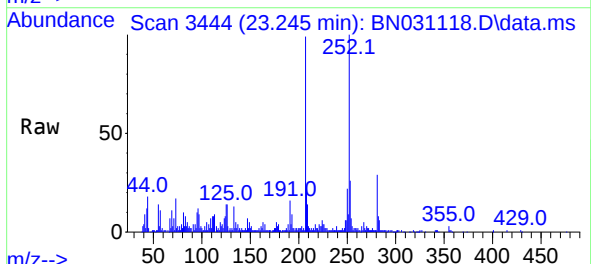


Tgt Ion:252 Resp: 120898
Ion Ratio Lower Upper
252 100
253 25.8 17.6 26.4
125 14.0 8.6 12.8

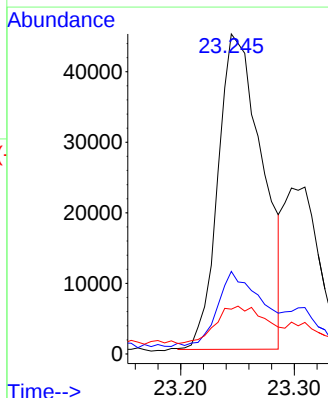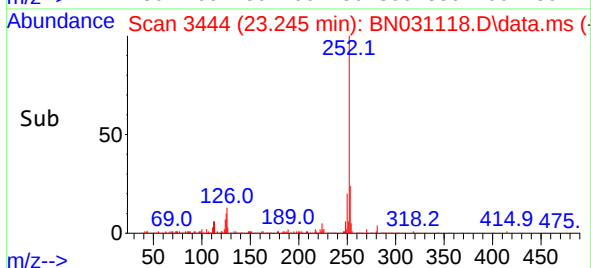

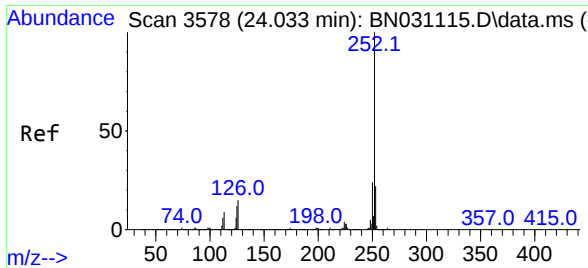

#93
 Benzo(a)pyrene
 Concen: 1.301 ng/ul
 RT: 24.027 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BN031118.D
 Acq: 22 Apr 2024 12:14

Instrument :
 BNA_N
 ClientSampleId :
 EZZZ7

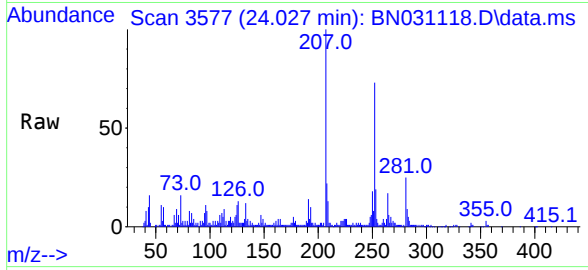

Tgt Ion:252 Resp: 80094

Ion	Ratio	Lower	Upper
252	100		
253	26.3	17.7	26.5
125	14.8	9.9	14.9

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/24/2024

