

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031151.D
 Acq On : 23 Apr 2024 12:18
 Operator : MA/JU
 Sample : P2077-09DL 5X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AL3DL

Quant Time: Apr 23 23:00:19 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 22:56:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	98858	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.410	136	465228	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.275	164	321255	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.028	188	765958	20.000	ng/u1	0.00
79) Chrysene-d12	21.263	240	840282	20.000	ng/u1	0.00
88) Perylene-d12	24.163	264	954634	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.152	96	1392	0.658	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	6.811	99	8523	1.022	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	31029	6.395	ng/u1	0.00
11) 2-Chlorophenol-d4	7.163	132	28262	4.353	ng/u1	0.00
15) 4-Methylphenol-d8	8.340	113	16717	2.384	ng/u1	0.00
21) Nitrobenzene-d5	8.787	128	19451	5.819	ng/u1	0.00
24) 2-Nitrophenol-d4	9.505	143	16785	4.831	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.034	165	33809	4.934	ng/u1	0.00
31) 4-Chloroaniline-d4	10.557	131	49464	4.619	ng/u1	0.00
46) Dimethylphthalate-d6	13.693	166	161806	7.238	ng/u1	0.00
49) Acenaphthylene-d8	13.969	160	168088	6.635	ng/u1	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	
60) Fluorene-d10	15.275	176	154525	7.940	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.398	200	10532	2.725	ng/u1	0.00
73) Anthracene-d10	17.128	188	265982	8.012	ng/u1	0.00
81) Pyrene-d10	19.428	212	344331	8.339	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.957	264	367417	8.116	ng/u1	-0.02
Target Compounds						
59) Diethylphthalate	15.110	149	1112963	46.925	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031151.D
Acq On : 23 Apr 2024 12:18
Operator : MA/JU
Sample : P2077-09DL 5X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COAL3DL


Quant Time: Apr 23 23:00:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 22:56:25 2024
Response via : Initial Calibration

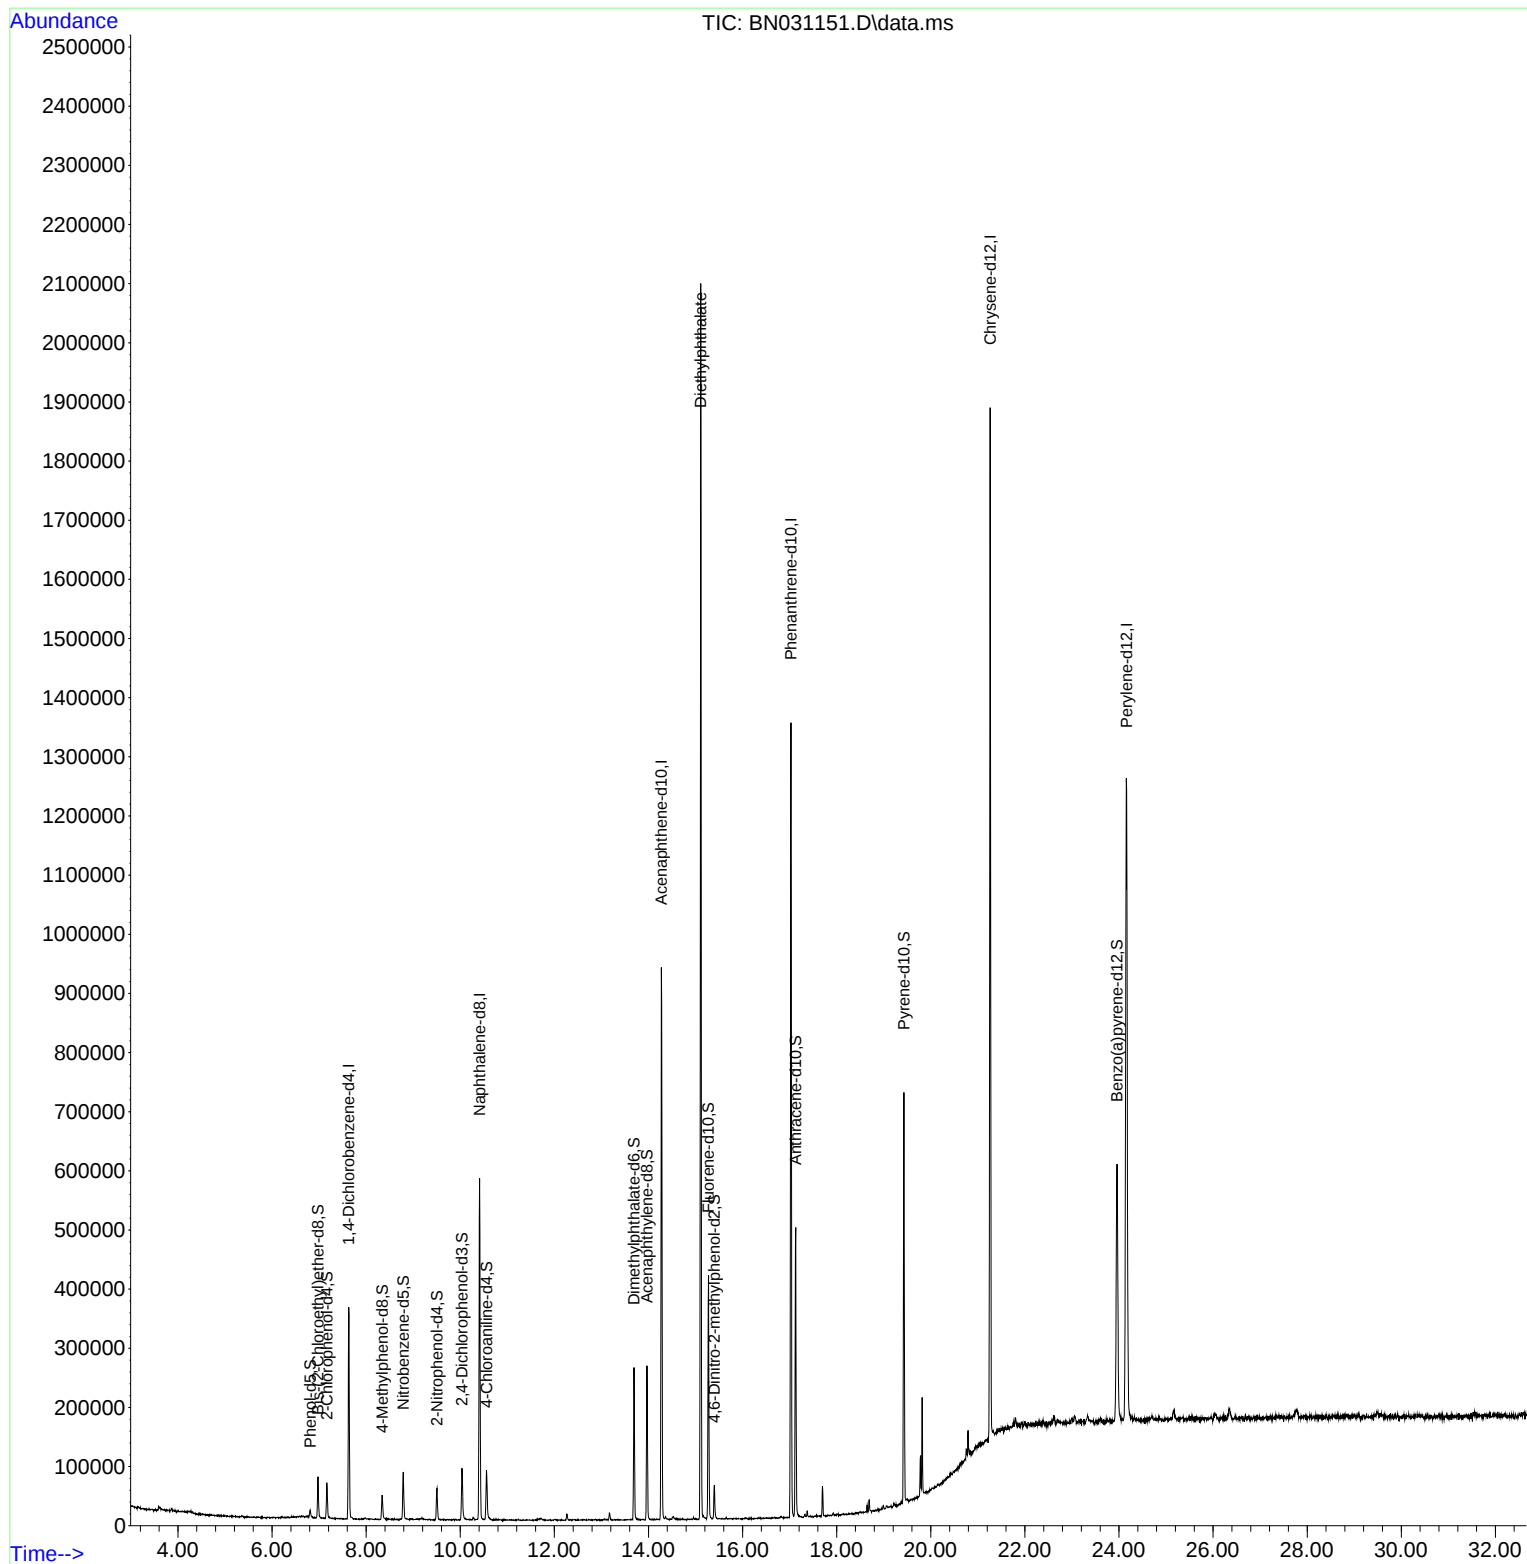

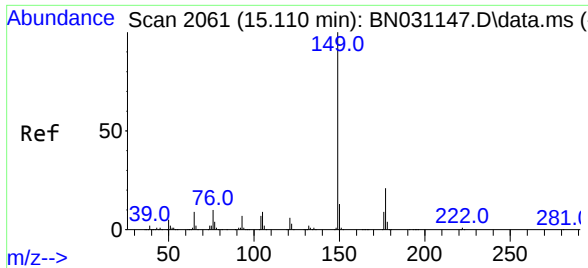

#59
 Diethylphthalate
 Concen: 46.925 ng/ul
 RT: 15.110 min Scan# 20
 Delta R.T. -0.006 min
 Lab File: BN031151.D
 Acq: 23 Apr 2024 12:18

Instrument :
 BNA_N
 ClientSampleId :
 C0AL3DL

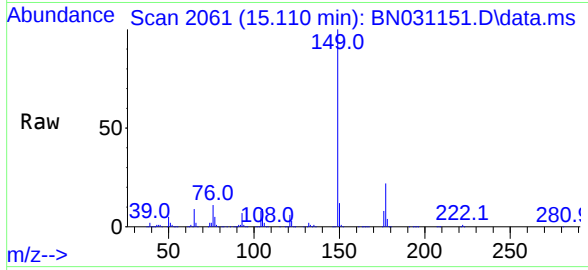

Tgt Ion:149 Resp: 1112963

Ion	Ratio	Lower	Upper
149	100		
177	21.7	16.8	25.2
150	12.4	10.1	15.1

