

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031182.D
 Acq On : 24 Apr 2024 10:07
 Operator : MA/JU
 Sample : P2141-03
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSR6

Quant Time: Apr 24 11:25:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 22:56:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	124395	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.404	136	576116	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.275	164	393650	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.028	188	894713	20.000	ng/u1	0.00
79) Chrysene-d12	21.263	240	1001874	20.000	ng/u1	0.00
88) Perylene-d12	24.162	264	1086417	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	9767	3.668	ng/uL	0.00
4) Pyridine-d5	3.558	84	87846	11.456	ng/u1	0.00
7) Phenol-d5	6.805	99	80760	7.696	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.969	67	237623	38.921	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.163	132	247785	30.327	ng/u1	0.00
15) 4-Methylphenol-d8	8.334	113	161974	18.354	ng/u1	0.00
21) Nitrobenzene-d5	8.781	128	170878	41.281	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.498	143	169413	39.373	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.028	165	298001	35.120	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.551	131	386967	29.183	ng/u1	-0.01
46) Dimethylphthalate-d6	13.692	166	1131100	41.291	ng/u1	0.00
49) Acenaphthylene-d8	13.969	160	1268851	40.876	ng/u1	0.00
54) 4-Nitrophenol-d4	14.492	143	34571	6.047	ng/u1	0.00
60) Fluorene-d10	15.275	176	1004837	42.137	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.398	200	134055	29.698	ng/u1	0.00
73) Anthracene-d10	17.127	188	1731213	44.642	ng/u1	0.00
81) Pyrene-d10	19.427	212	2219725	45.087	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.968	264	2455452	47.661	ng/u1	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.181	88	2873	1.018	ng/uL#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031182.D
Acq On : 24 Apr 2024 10:07
Operator : MA/JU
Sample : P2141-03
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSR6


Quant Time: Apr 24 11:25:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 22:56:25 2024
Response via : Initial Calibration

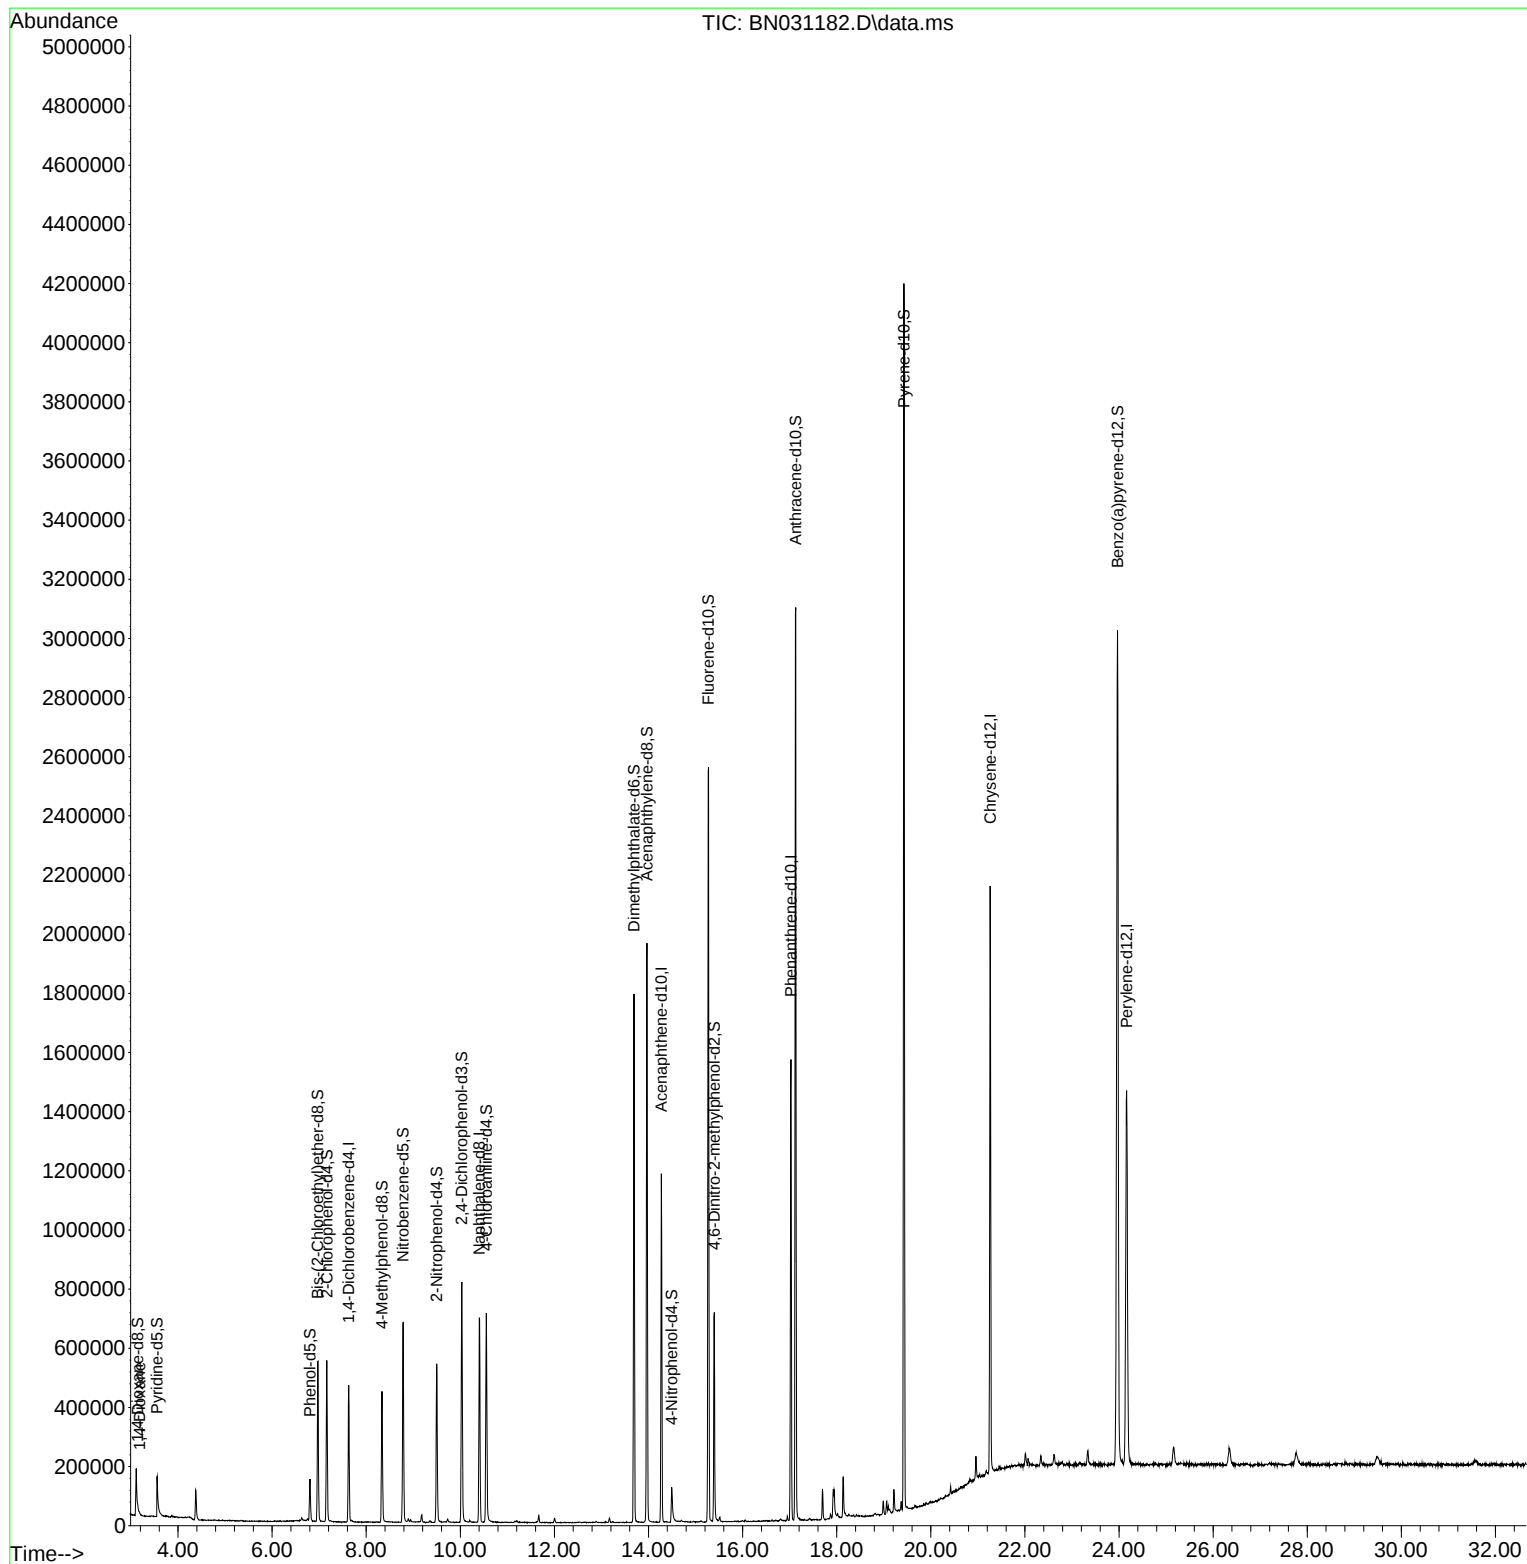

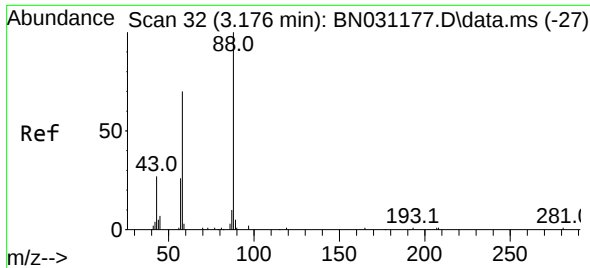

#2
 1,4-Dioxane
 Concen: 1.018 ng/uL
 RT: 3.181 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: BN031182.D
 Acq: 24 Apr 2024 10:07

Instrument :
 BNA_N
 ClientSampleId :
 YCSR6

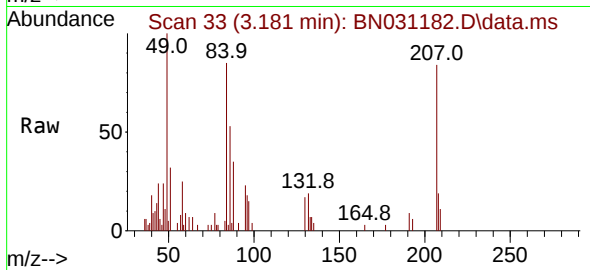

Tgt Ion: 88 Resp: 2873
 Ion Ratio Lower Upper
 88 100
 43 40.5 22.2 33.2#
 58 70.8 50.2 75.2

