

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031117.D
 Acq On : 22 Apr 2024 11:35
 Operator : MA/JU
 Sample : P2170-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EZZZ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031117.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	24	27	36	rVB2	13801	21629	0.79%	0.169%
2	3.652	110	113	121	rBV3	14066	21647	0.79%	0.170%
3	3.723	123	125	127	rBV3	4018	3338	0.12%	0.026%
4	4.405	239	241	247	rVB5	2089	3231	0.12%	0.025%
5	4.511	256	259	262	rBV5	1895	2794	0.10%	0.022%
6	4.764	300	302	310	rVB6	3367	6201	0.23%	0.049%
7	6.822	650	652	656	rVB5	1937	3038	0.11%	0.024%
8	6.975	672	678	686	rBV	184227	288365	10.55%	2.260%
9	7.169	706	711	712	rBV5	2655	3310	0.12%	0.026%
10	7.246	719	724	729	rBV5	3022	4928	0.18%	0.039%
11	7.628	782	789	797	rBV	386373	618814	22.64%	4.849%
12	8.340	907	910	915	rVV7	2160	3669	0.13%	0.029%
13	8.458	925	930	935	rBV4	5207	8535	0.31%	0.067%
14	8.787	979	986	994	rBV	177504	291289	10.66%	2.283%
15	8.946	1009	1013	1020	rVB8	2455	6046	0.22%	0.047%
16	9.181	1049	1053	1058	rVB2	7797	11234	0.41%	0.088%
17	9.363	1079	1084	1088	rBV5	8137	13597	0.50%	0.107%
18	9.505	1096	1108	1117	rBV	106878	186141	6.81%	1.459%
19	9.910	1173	1177	1185	rBV4	3695	8049	0.29%	0.063%
20	10.410	1252	1262	1274	rBV	606893	1005885	36.81%	7.882%
21	10.569	1287	1289	1297	rVB8	3921	6513	0.24%	0.051%
22	10.969	1356	1357	1360	rVV3	3036	2931	0.11%	0.023%
23	11.163	1385	1390	1398	rBV3	9671	21086	0.77%	0.165%
24	11.657	1466	1474	1475	rBV5	4007	6893	0.25%	0.054%
25	11.834	1501	1504	1508	rVB4	2599	3461	0.13%	0.027%
26	11.922	1515	1519	1523	rBV5	2318	3778	0.14%	0.030%
27	13.099	1715	1719	1725	rVB4	6073	7883	0.29%	0.062%
28	13.175	1727	1732	1739	rVV7	7172	10711	0.39%	0.084%
29	13.693	1813	1820	1829	rBV	603933	815892	29.86%	6.394%
30	14.175	1900	1902	1909	rVB4	3469	5138	0.19%	0.040%
31	14.275	1913	1919	1932	rBV	999562	1468777	53.75%	11.510%
32	14.481	1950	1954	1956	rBV3	10495	13688	0.50%	0.107%
33	14.504	1956	1958	1965	rVB7	13029	18625	0.68%	0.146%
34	15.140	2063	2066	2070	rVB5	2520	2748	0.10%	0.022%
35	15.275	2083	2089	2097	rVB	61578	89900	3.29%	0.704%
36	15.398	2104	2110	2118	rBV	133489	192128	7.03%	1.506%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031117.D
 Acq On : 22 Apr 2024 11:35
 Operator : MA/JU
 Sample : P2170-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EZZZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

37	15.998	2208	2212	2214	rBV4	2788	4116	0.15%	0.032%
38	16.434	2283	2286	2291	rBV4	4576	7294	0.27%	0.057%
39	16.798	2345	2348	2349	rBV3	3303	3234	0.12%	0.025%
40	16.822	2349	2352	2361	rVB8	3442	9369	0.34%	0.073%
41	16.951	2371	2374	2377	rBV4	2632	3508	0.13%	0.027%
42	17.028	2381	2387	2396	rVV	1402517	1932593	70.72%	15.144%
43	17.122	2400	2403	2407	rVB3	6299	8582	0.31%	0.067%
44	17.228	2414	2421	2425	rBV8	11885	19418	0.71%	0.152%
45	17.704	2498	2502	2504	rBV4	3882	5091	0.19%	0.040%
46	17.798	2515	2518	2525	rVB8	7917	12338	0.45%	0.097%
47	17.928	2535	2540	2547	rBV	87238	122656	4.49%	0.961%
48	18.010	2550	2554	2556	rVB5	4957	6389	0.23%	0.050%
49	18.363	2610	2614	2620	rVB7	5502	9110	0.33%	0.071%
50	19.075	2731	2735	2736	rBV4	11687	14963	0.55%	0.117%
51	19.092	2736	2738	2744	rVB5	10200	15591	0.57%	0.122%
52	19.216	2755	2759	2766	rBV2	41423	61426	2.25%	0.481%
53	19.486	2802	2805	2808	rBV5	8612	12000	0.44%	0.094%
54	20.957	3052	3055	3062	rBV	79395	108618	3.97%	0.851%
55	21.263	3102	3107	3118	rBV	1714348	2490236	91.13%	19.514%
56	24.163	3592	3600	3612	rVB2	1128925	2732701	100.00%	21.414%


Sum of corrected areas: 12761125

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031117.D
Acq On : 22 Apr 2024 11:35
Operator : MA/JU
Sample : P2170-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EZZZ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

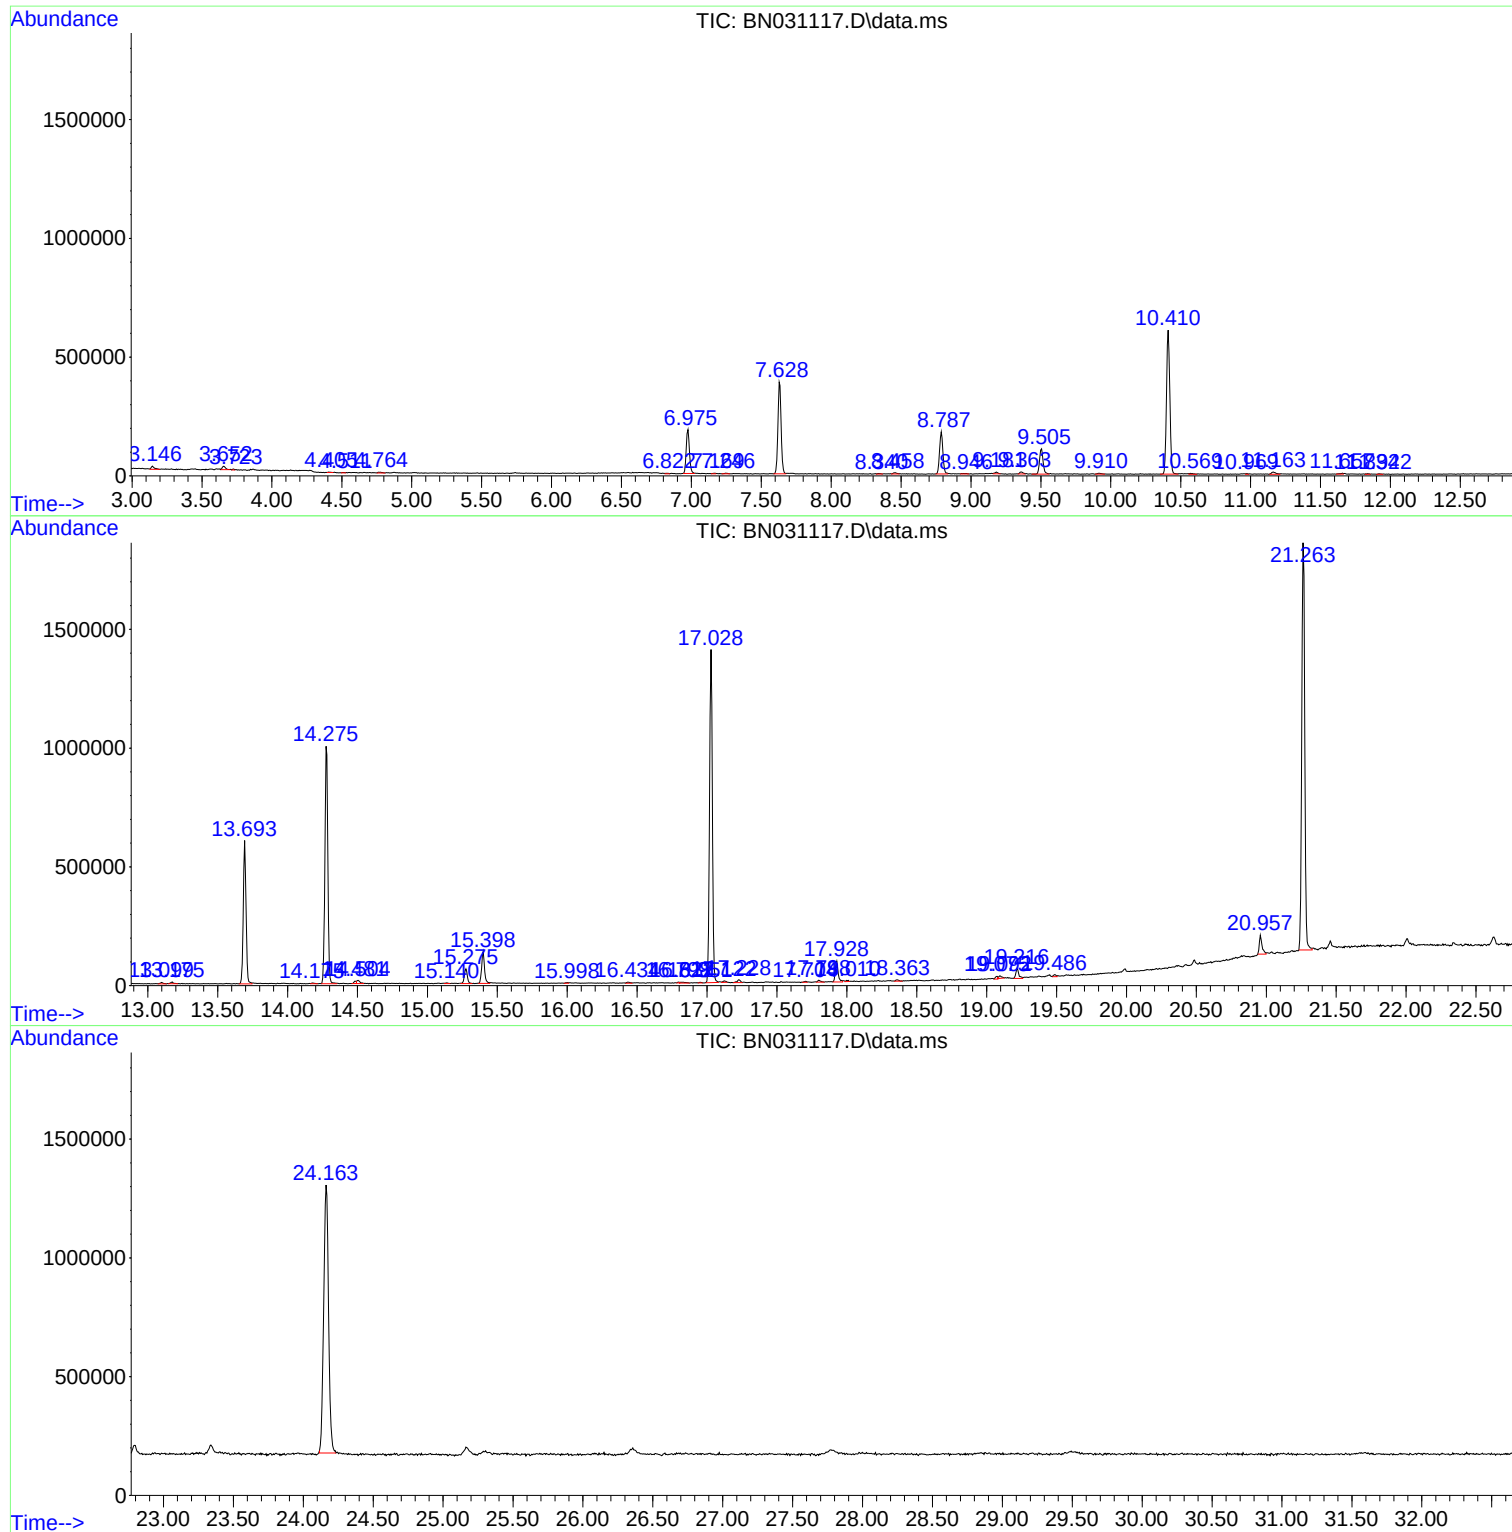

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031117.D
Acq On : 22 Apr 2024 11:35
Operator : MA/JU
Sample : P2170-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EZZZ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031117.D
Acq On : 22 Apr 2024 11:35
Operator : MA/JU
Sample : P2170-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EZZZ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------