

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031119.D
 Acq On : 22 Apr 2024 12:54
 Operator : MA/JU
 Sample : P2170-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EZZZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031119.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	24	27	31	rVB3	9946	12218	0.39%	0.093%
2	3.434	72	76	77	rBV3	4618	6434	0.20%	0.049%
3	3.599	101	104	110	rBV5	5413	10313	0.33%	0.079%
4	3.652	110	113	118	rBV2	12347	19282	0.61%	0.147%
5	3.864	144	149	156	rBV5	6974	12297	0.39%	0.094%
6	6.499	592	597	599	rBV5	2452	3166	0.10%	0.024%
7	6.975	671	678	688	rBV	149317	238473	7.57%	1.820%
8	7.246	720	724	727	rBV5	2320	3391	0.11%	0.026%
9	7.628	783	789	798	rBV	388090	638041	20.26%	4.868%
10	8.163	875	880	882	rBV5	2109	4080	0.13%	0.031%
11	8.458	925	930	932	rBV5	3520	4712	0.15%	0.036%
12	8.787	980	986	994	rBV	134416	227936	7.24%	1.739%
13	8.899	1001	1005	1010	rVV7	1973	3291	0.10%	0.025%
14	8.946	1010	1013	1019	rVB6	3433	5770	0.18%	0.044%
15	9.181	1050	1053	1061	rVB4	4993	8540	0.27%	0.065%
16	9.358	1079	1083	1090	rVB5	7567	13073	0.42%	0.100%
17	9.505	1102	1108	1116	rBV	86238	146147	4.64%	1.115%
18	9.681	1134	1138	1144	rVB6	1986	3301	0.10%	0.025%
19	9.910	1173	1177	1180	rBV4	4364	5509	0.17%	0.042%
20	10.410	1254	1262	1271	rBV	611872	1012278	32.14%	7.724%
21	10.569	1285	1289	1295	rBV9	3116	5424	0.17%	0.041%
22	11.163	1384	1390	1396	rBV3	10628	21491	0.68%	0.164%
23	11.446	1432	1438	1442	rVB7	1619	3546	0.11%	0.027%
24	11.834	1501	1504	1510	rBV8	2457	3902	0.12%	0.030%
25	12.216	1563	1569	1574	rBV6	3914	9143	0.29%	0.070%
26	13.028	1701	1707	1708	rBV6	1822	3488	0.11%	0.027%
27	13.099	1712	1719	1724	rVV6	5096	10149	0.32%	0.077%
28	13.175	1726	1732	1736	rVB6	8807	14121	0.45%	0.108%
29	13.693	1811	1820	1825	rBV	456200	640307	20.33%	4.886%
30	13.740	1825	1828	1835	rVB	70716	100822	3.20%	0.769%
31	13.934	1856	1861	1862	rBV5	2352	3162	0.10%	0.024%
32	14.181	1897	1903	1910	rBV5	6443	10757	0.34%	0.082%
33	14.281	1913	1920	1929	rBV	968610	1452265	46.10%	11.081%
34	14.487	1950	1955	1956	rBV4	10089	13351	0.42%	0.102%
35	14.504	1956	1958	1964	rVB7	12744	15701	0.50%	0.120%
36	14.798	2006	2008	2015	rVB7	2092	4089	0.13%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031119.D
 Acq On : 22 Apr 2024 12:54
 Operator : MA/JU
 Sample : P2170-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EZZZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

37	15.081	2051	2056	2059	rBV3	3089	5075	0.16%	0.039%
38	15.134	2062	2065	2070	rVV3	3006	4550	0.14%	0.035%
39	15.275	2083	2089	2094	rBV	45183	66244	2.10%	0.505%
40	15.398	2105	2110	2120	rBV	102483	155383	4.93%	1.186%
41	15.540	2132	2134	2138	rVB6	2973	4313	0.14%	0.033%
42	16.004	2208	2213	2215	rBV5	7117	11955	0.38%	0.091%
43	16.792	2345	2347	2351	rVV4	4297	7330	0.23%	0.056%
44	16.839	2353	2355	2358	rVB4	3112	4117	0.13%	0.031%
45	17.028	2380	2387	2395	rBV	1382960	1895826	60.19%	14.466%
46	17.128	2401	2404	2408	rVB3	7439	9415	0.30%	0.072%
47	17.228	2416	2421	2426	rBV8	8645	13057	0.41%	0.100%
48	17.316	2433	2436	2440	rBV6	3703	5296	0.17%	0.040%
49	17.534	2469	2473	2476	rVV4	5720	7995	0.25%	0.061%
50	17.704	2499	2502	2505	rBV5	6440	7875	0.25%	0.060%
51	17.804	2516	2519	2523	rBV5	3571	5873	0.19%	0.045%
52	17.928	2535	2540	2546	rBV	105885	143688	4.56%	1.096%
53	17.998	2550	2552	2557	rVB6	4562	6810	0.22%	0.052%
54	18.228	2588	2591	2596	rBV6	5869	8394	0.27%	0.064%
55	18.363	2610	2614	2617	rBV6	6600	9778	0.31%	0.075%
56	19.222	2755	2760	2767	rBV2	74040	120242	3.82%	0.917%
57	19.492	2802	2806	2815	rBV	54694	81924	2.60%	0.625%
58	20.963	3053	3056	3064	rBV2	75198	112124	3.56%	0.856%
59	21.269	3102	3108	3116	rBV	1761074	2578348	81.85%	19.674%
60	24.169	3592	3601	3615	rVB	1238384	3149993	100.00%	24.036%


Sum of corrected areas: 13105575

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031119.D
Acq On : 22 Apr 2024 12:54
Operator : MA/JU
Sample : P2170-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EZZZ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

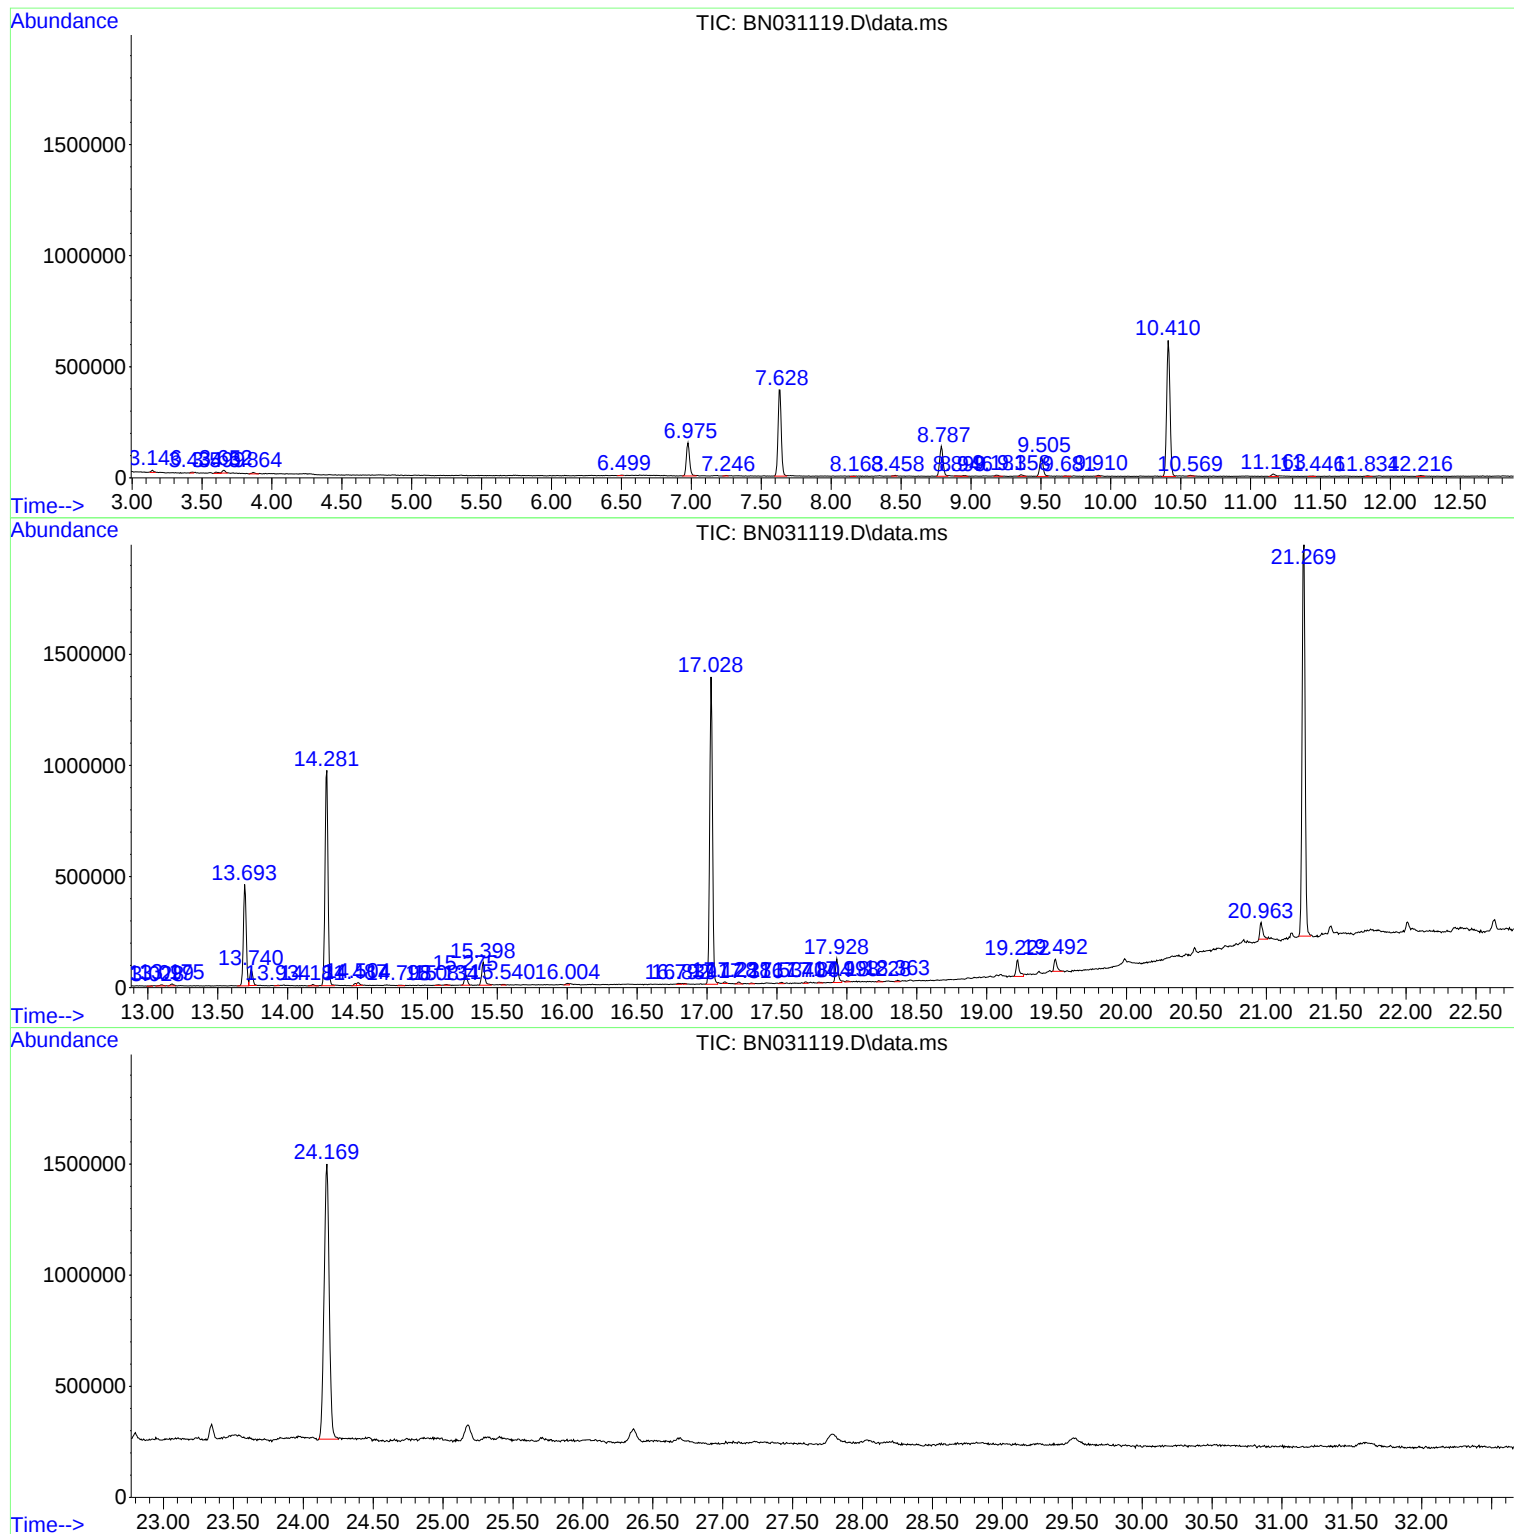

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031119.D
Acq On : 22 Apr 2024 12:54
Operator : MA/JU
Sample : P2170-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EZZZ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031119.D
Acq On : 22 Apr 2024 12:54
Operator : MA/JU
Sample : P2170-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EZZZ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc