

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031133.D
 Acq On : 22 Apr 2024 22:52
 Operator : MA/JU
 Sample : PB160417BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK417

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031133.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	23	27	35	rVB	23067	39147	0.76%	0.108%
2	3.552	94	96	121	rBV	305235	558375	10.85%	1.538%
3	6.805	643	649	658	rBV	481153	780757	15.17%	2.151%
4	6.975	672	678	687	rVB	388607	605841	11.78%	1.669%
5	7.163	704	710	721	rBV	496291	789967	15.35%	2.176%
6	7.634	784	790	797	rBV	321712	515320	10.02%	1.420%
7	8.340	901	910	924	rBV	625379	1037338	20.16%	2.857%
8	8.787	979	986	997	rBV	483941	785547	15.27%	2.164%
9	9.504	1101	1108	1123	rBV	390214	662170	12.87%	1.824%
10	10.034	1191	1198	1213	rBV	630754	1082046	21.03%	2.981%
11	10.410	1255	1262	1271	rBV	493325	826115	16.06%	2.276%
12	10.557	1279	1287	1296	rBV	631084	1070296	20.80%	2.948%
13	12.010	1528	1534	1538	rBV3	10839	16226	0.32%	0.045%
14	13.175	1727	1732	1739	rBV2	15156	26297	0.51%	0.072%
15	13.692	1811	1820	1831	rBV	1126901	1590999	30.92%	4.383%
16	13.969	1860	1867	1880	rBV	1372068	2026951	39.40%	5.583%
17	14.281	1913	1920	1928	rVB	808653	1185301	23.04%	3.265%
18	14.492	1949	1956	1977	rBV	501548	908935	17.67%	2.504%
19	15.275	2081	2089	2100	rBV	1827561	2544191	49.45%	7.008%
20	15.398	2102	2110	2121	rBV	514310	721576	14.02%	1.988%
21	15.510	2126	2129	2134	rVB4	8016	12683	0.25%	0.035%
22	16.057	2219	2222	2229	rVB7	5751	9275	0.18%	0.026%
23	17.028	2381	2387	2397	rBV	1109558	1551101	30.15%	4.273%
24	17.128	2398	2404	2422	rVB2	2130683	3027342	58.84%	8.339%
25	18.992	2717	2721	2725	rVB4	31250	39412	0.77%	0.109%
26	19.063	2729	2733	2738	rVB	26605	34801	0.68%	0.096%
27	19.433	2789	2796	2802	rBV	2918959	3911581	76.02%	10.775%
28	21.263	3102	3107	3116	rBV	1451642	2176101	42.29%	5.994%
29	23.968	3558	3567	3579	rVB	2177732	5145142	100.00%	14.173%
30	24.168	3593	3601	3611	rVB	1094130	2621943	50.96%	7.222%




Sum of corrected areas: 36302776

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031133.D
Acq On : 22 Apr 2024 22:52
Operator : MA/JU
Sample : PB160417BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK417

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

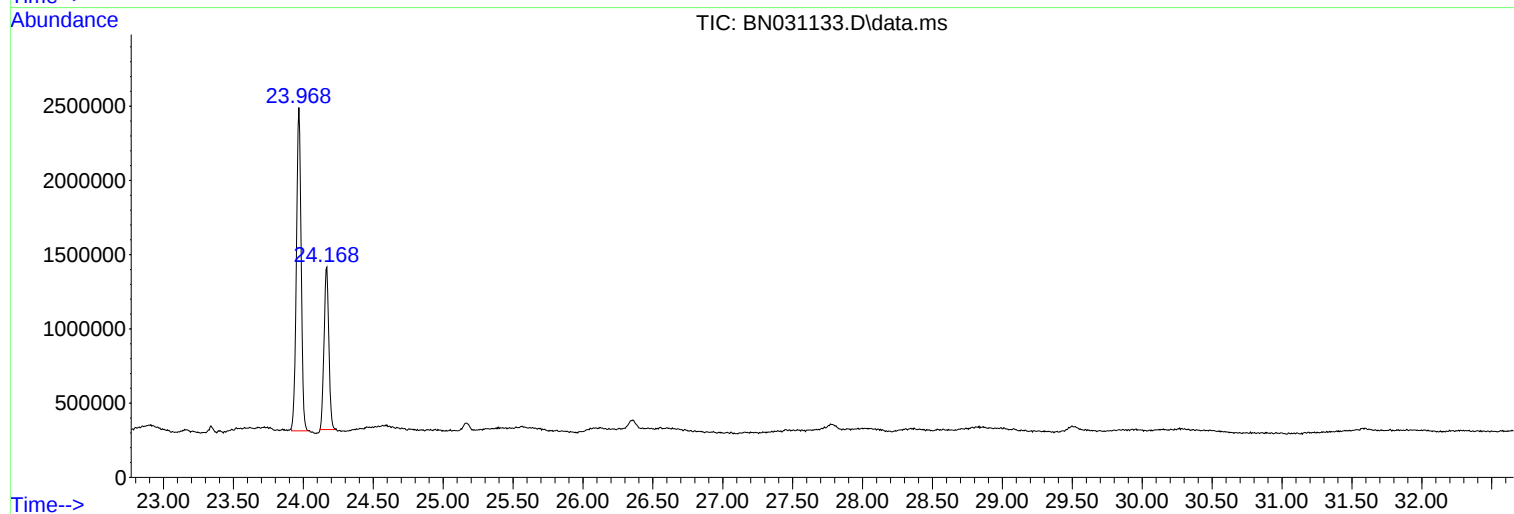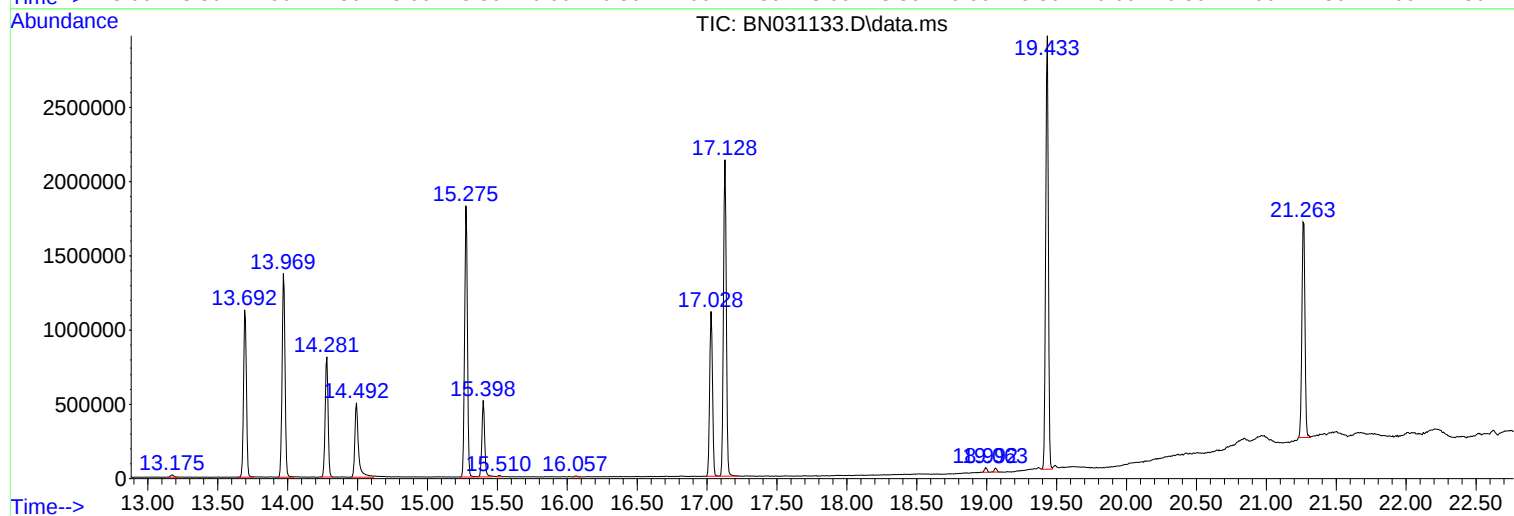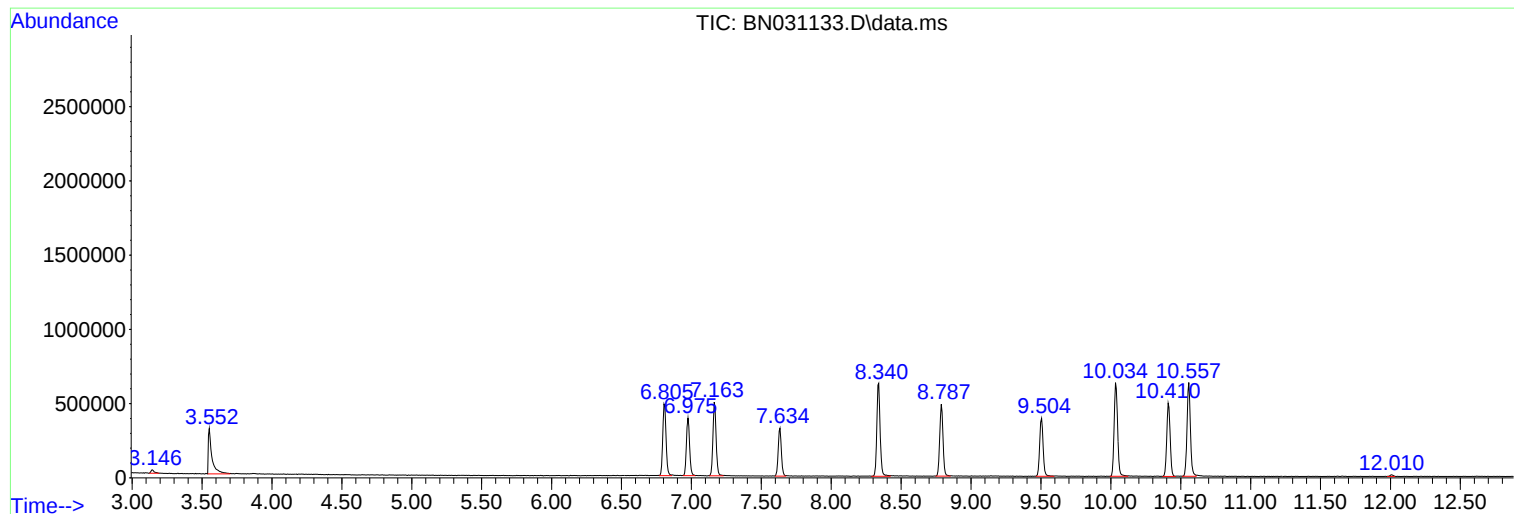

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031133.D
Acq On : 22 Apr 2024 22:52
Operator : MA/JU
Sample : PB160417BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK417

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031133.D
Acq On : 22 Apr 2024 22:52
Operator : MA/JU
Sample : PB160417BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK417

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc