

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031139.D
 Acq On : 23 Apr 2024 02:50
 Operator : MA/JU
 Sample : P2202-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COAN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031139.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.111	18	21	23	rBV3	5866	7737	0.12%	0.018%
2	3.140	23	26	32	rVB	15237	24263	0.38%	0.058%
3	6.805	643	649	660	rVB	216109	348737	5.53%	0.832%
4	6.975	671	678	688	rBV	454938	726531	11.51%	1.734%
5	7.163	703	710	718	rBV	565471	886538	14.05%	2.116%
6	7.628	782	789	798	rBV	390105	625168	9.91%	1.492%
7	8.334	902	909	918	rBV	549465	903528	14.32%	2.157%
8	8.787	979	986	998	rBV	592193	966623	15.32%	2.307%
9	8.893	1000	1004	1012	rVV9	8499	21522	0.34%	0.051%
10	8.952	1012	1014	1022	rVB9	4300	8840	0.14%	0.021%
11	9.181	1046	1053	1061	rVB2	16395	27172	0.43%	0.065%
12	9.504	1100	1108	1118	rBV	473985	807025	12.79%	1.926%
13	9.910	1173	1177	1186	rVB2	8464	13015	0.21%	0.031%
14	10.034	1191	1198	1215	rBV	779737	1300233	20.61%	3.104%
15	10.410	1254	1262	1271	rBV	628439	1027930	16.29%	2.454%
16	10.557	1282	1287	1297	rVB	18612	36948	0.59%	0.088%
17	11.669	1471	1476	1481	rBV2	9270	13924	0.22%	0.033%
18	12.004	1526	1533	1539	rBV3	13043	23642	0.37%	0.056%
19	13.169	1725	1731	1737	rVB4	12947	22622	0.36%	0.054%
20	13.693	1814	1820	1828	rBV	1490945	1995302	31.62%	4.763%
21	13.969	1860	1867	1879	rBV	1646159	2471837	39.17%	5.900%
22	14.275	1913	1919	1930	rBV	1027694	1510431	23.94%	3.605%
23	14.492	1951	1956	1976	rBV	219227	421312	6.68%	1.006%
24	14.710	1989	1993	1996	rVB6	3660	6893	0.11%	0.016%
25	15.275	2082	2089	2097	rBV	2238480	3205292	50.80%	7.651%
26	15.398	2104	2110	2124	rBV	679604	934906	14.82%	2.232%
27	15.516	2126	2130	2135	rVB4	12133	19039	0.30%	0.045%
28	16.057	2218	2222	2230	rBV5	8357	14031	0.22%	0.033%
29	17.028	2381	2387	2397	rBV	1381173	1956591	31.01%	4.670%
30	17.128	2398	2404	2416	rVV	2845891	3955126	62.68%	9.440%
31	17.228	2418	2421	2426	rVB7	12069	19025	0.30%	0.045%
32	17.698	2498	2501	2505	rBV6	5342	9379	0.15%	0.022%
33	17.928	2535	2540	2546	rBV	84700	119641	1.90%	0.286%
34	18.992	2717	2721	2726	rBV2	40343	51794	0.82%	0.124%
35	19.063	2729	2733	2737	rBV	42976	59432	0.94%	0.142%
36	19.216	2755	2759	2765	rBV2	88828	131227	2.08%	0.313%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031139.D
Acq On : 23 Apr 2024 02:50
Operator : MA/JU
Sample : P2202-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION

37	19.369	2783	2785	2790	rBV6	12990	14032	0.22%	0.033%
38	19.433	2790	2796	2802	rBV2	3529140	5015941	79.49%	11.972%
39	19.486	2802	2805	2813	rVB2	21162	40459	0.64%	0.097%
40	21.263	3102	3107	3115	rBV2	1844490	2655632	42.09%	6.339%
41	23.968	3558	3567	3584	rVB2	2518217	6310117	100.00%	15.062%
42	24.163	3592	3600	3613	rVB	1285091	3186089	50.49%	7.605%




Sum of corrected areas: 41895526

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031139.D
Acq On : 23 Apr 2024 02:50
Operator : MA/JU
Sample : P2202-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COAN6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

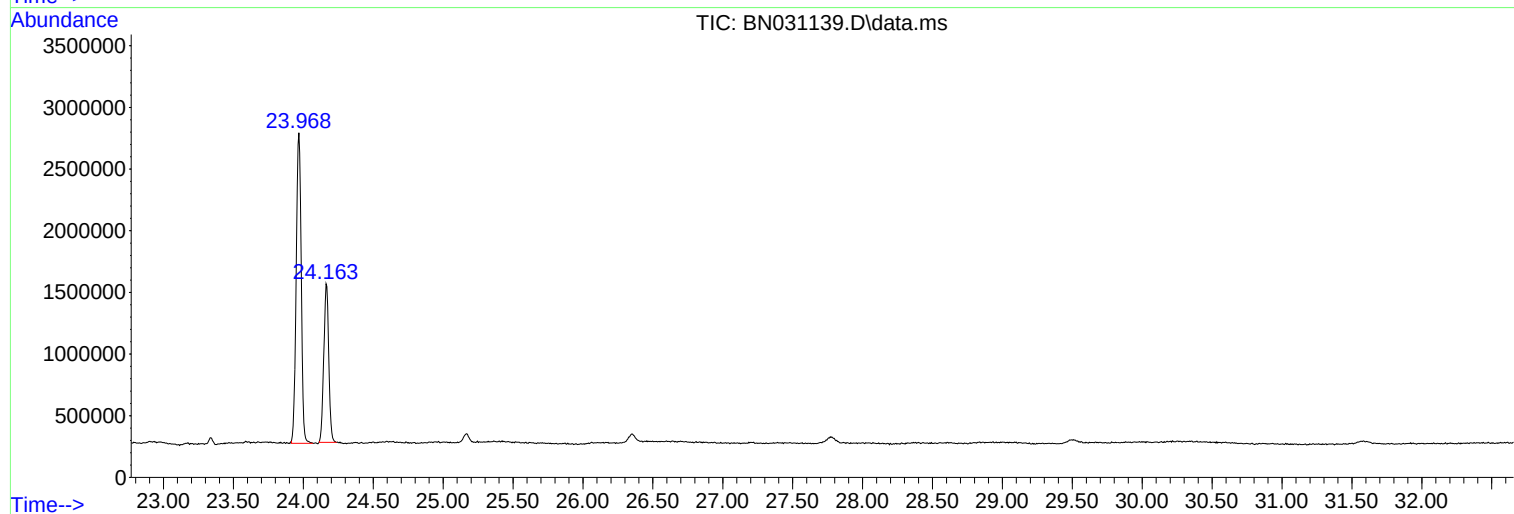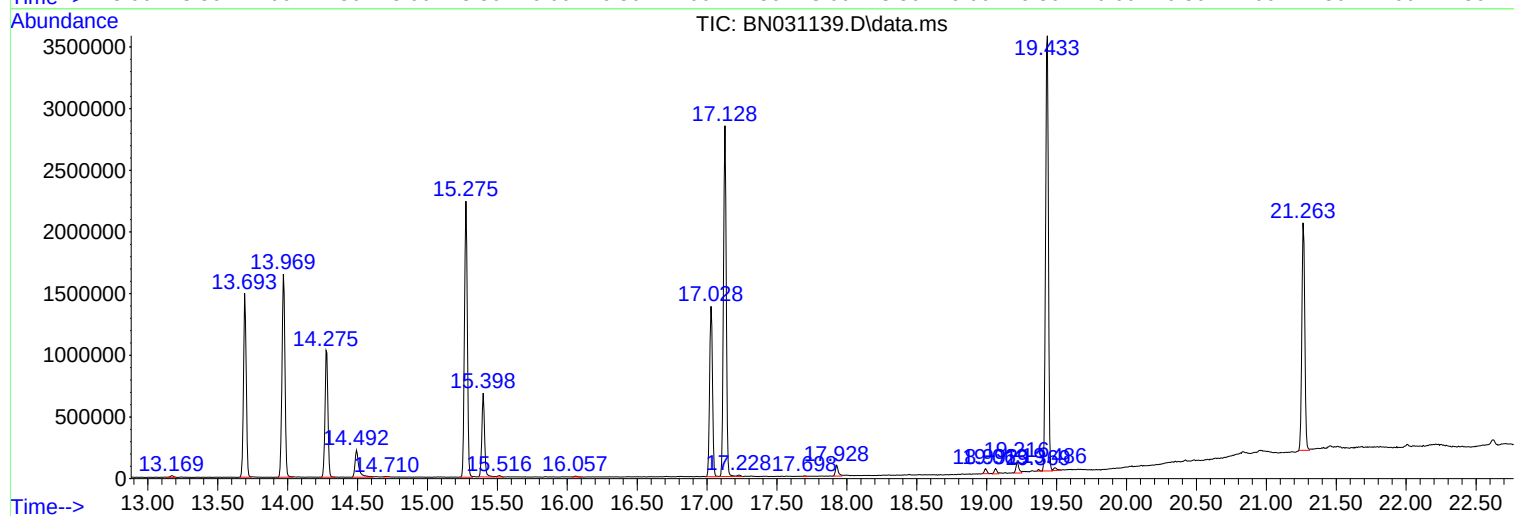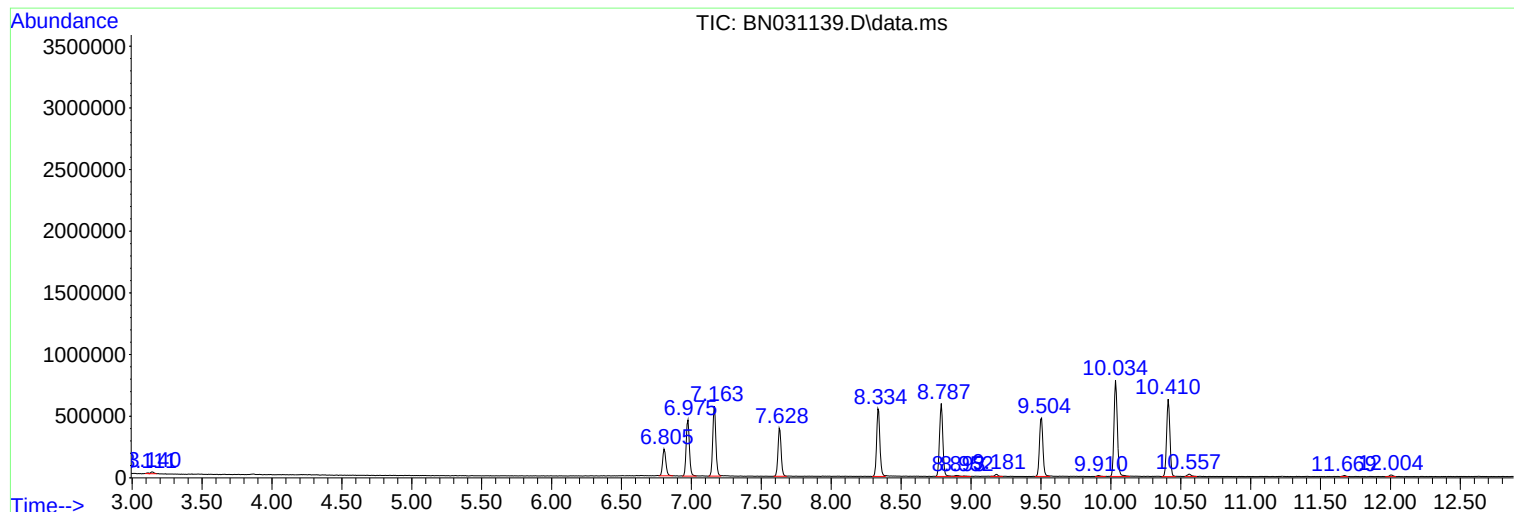

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031139.D
Acq On : 23 Apr 2024 02:50
Operator : MA/JU
Sample : P2202-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031139.D
Acq On : 23 Apr 2024 02:50
Operator : MA/JU
Sample : P2202-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------