

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031142.D
 Acq On : 23 Apr 2024 04:48
 Operator : MA/JU
 Sample : P2142-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031142.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.111	18	21	23	rBV3	10470	11812	0.13%	0.021%
2	3.146	24	27	33	rVB	20976	30075	0.33%	0.053%
3	3.564	96	98	106	rBV	51585	89831	1.00%	0.158%
4	4.381	232	237	248	rVB2	22367	42617	0.47%	0.075%
5	4.976	332	338	344	rBV	16278	28895	0.32%	0.051%
6	6.805	642	649	660	rBV	183331	298054	3.31%	0.525%
7	6.975	672	678	689	rBV	581563	934816	10.37%	1.646%
8	7.164	703	710	722	rBV	614341	976327	10.84%	1.720%
9	7.628	781	789	796	rBV	554727	892950	9.91%	1.573%
10	7.693	796	800	806	rVB	51172	81198	0.90%	0.143%
11	7.981	844	849	853	rVB5	6544	11949	0.13%	0.021%
12	8.334	903	909	921	rBV	520631	845405	9.38%	1.489%
13	8.787	979	986	996	rBV	755221	1227158	13.62%	2.161%
14	9.499	1099	1107	1122	rBV	600535	1020997	11.33%	1.798%
15	9.905	1173	1176	1182	rBV3	5287	9615	0.11%	0.017%
16	10.034	1190	1198	1214	rBV	947624	1543844	17.13%	2.719%
17	10.411	1253	1262	1273	rBV	856336	1391909	15.45%	2.452%
18	10.558	1279	1287	1303	rBV	498296	883026	9.80%	1.555%
19	12.005	1526	1533	1541	rBV	19580	30601	0.34%	0.054%
20	13.169	1725	1731	1736	rBV4	17497	28197	0.31%	0.050%
21	13.693	1812	1820	1832	rBV	1868021	2559931	28.41%	4.509%
22	13.969	1860	1867	1878	rBV	2208784	3193883	35.45%	5.625%
23	14.275	1913	1919	1928	rBV	1318697	1992051	22.11%	3.509%
24	14.493	1950	1956	1968	rBV	220529	386382	4.29%	0.681%
25	14.704	1987	1992	1998	rVB10	4529	9240	0.10%	0.016%
26	14.869	2015	2020	2024	rVB	9815	15068	0.17%	0.027%
27	15.275	2082	2089	2100	rBV	2931746	4144051	45.99%	7.299%
28	15.398	2103	2110	2122	rVV	1058443	1456014	16.16%	2.564%
29	15.510	2125	2129	2139	rVB4	19866	36536	0.41%	0.064%
30	15.734	2164	2167	2172	rBV2	10809	13504	0.15%	0.024%
31	15.998	2209	2212	2219	rVV5	7955	13187	0.15%	0.023%
32	16.063	2219	2223	2227	rVB3	11401	17457	0.19%	0.031%
33	16.434	2284	2286	2293	rVB7	7351	10285	0.11%	0.018%
34	16.569	2303	2309	2314	rBV9	4808	9676	0.11%	0.017%
35	16.793	2343	2347	2349	rBV3	8557	10201	0.11%	0.018%
36	16.840	2351	2355	2359	rVB	20987	28649	0.32%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031142.D
 Acq On : 23 Apr 2024 04:48
 Operator : MA/JU
 Sample : P2142-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

37	17.028	2381	2387	2396	rBV	1946289	2605357	28.92%	4.589%
38	17.128	2397	2404	2417	rVB	3834195	5415692	60.11%	9.539%
39	17.528	2469	2472	2476	rVB4	9411	13119	0.15%	0.023%
40	17.645	2488	2492	2497	rBV8	9498	17122	0.19%	0.030%
41	17.698	2497	2501	2509	rVB10	14571	22284	0.25%	0.039%
42	17.810	2515	2520	2521	rBV5	10439	15276	0.17%	0.027%
43	17.928	2535	2540	2547	rBV4	64090	96827	1.07%	0.171%
44	18.010	2552	2554	2559	rVB6	8723	13439	0.15%	0.024%
45	18.222	2587	2590	2594	rBV4	7646	9952	0.11%	0.018%
46	18.263	2594	2597	2601	rBV4	7912	11733	0.13%	0.021%
47	18.416	2620	2623	2628	rVB6	9773	13839	0.15%	0.024%
48	18.687	2665	2669	2672	rBV5	13252	18605	0.21%	0.033%
49	18.992	2716	2721	2725	rBV2	55837	78722	0.87%	0.139%
50	19.063	2729	2733	2737	rBV	59219	80317	0.89%	0.141%
51	19.216	2755	2759	2768	rBV4	42432	65705	0.73%	0.116%
52	19.298	2770	2773	2777	rBV5	13760	24630	0.27%	0.043%
53	19.369	2782	2785	2788	rVB4	15391	17064	0.19%	0.030%
54	19.434	2789	2796	2802	rBV	5031578	6969390	77.35%	12.275%
55	19.486	2803	2805	2809	rVB2	16953	20261	0.22%	0.036%
56	21.263	3101	3107	3115	rBV2	2493674	3598931	39.94%	6.339%
57	23.975	3557	3568	3582	rVB2	3590007	9010278	100.00%	15.870%
58	24.163	3591	3600	3614	rVB	1803218	4382923	48.64%	7.720%




Sum of corrected areas: 56776857

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031142.D
Acq On : 23 Apr 2024 04:48
Operator : MA/JU
Sample : P2142-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

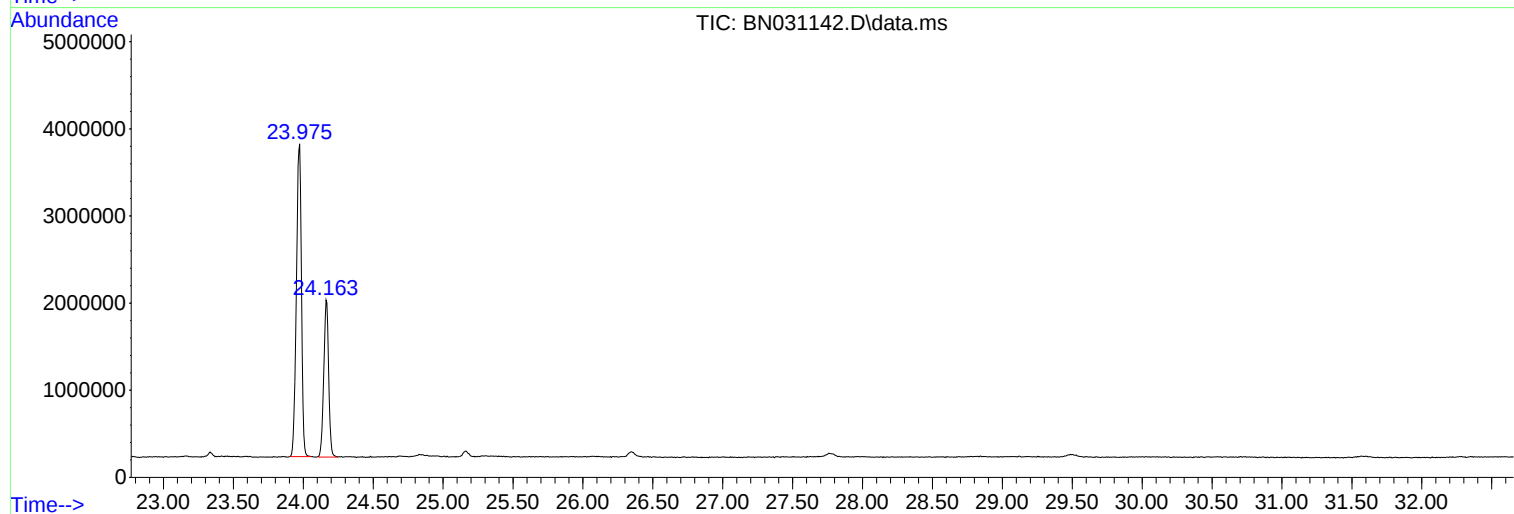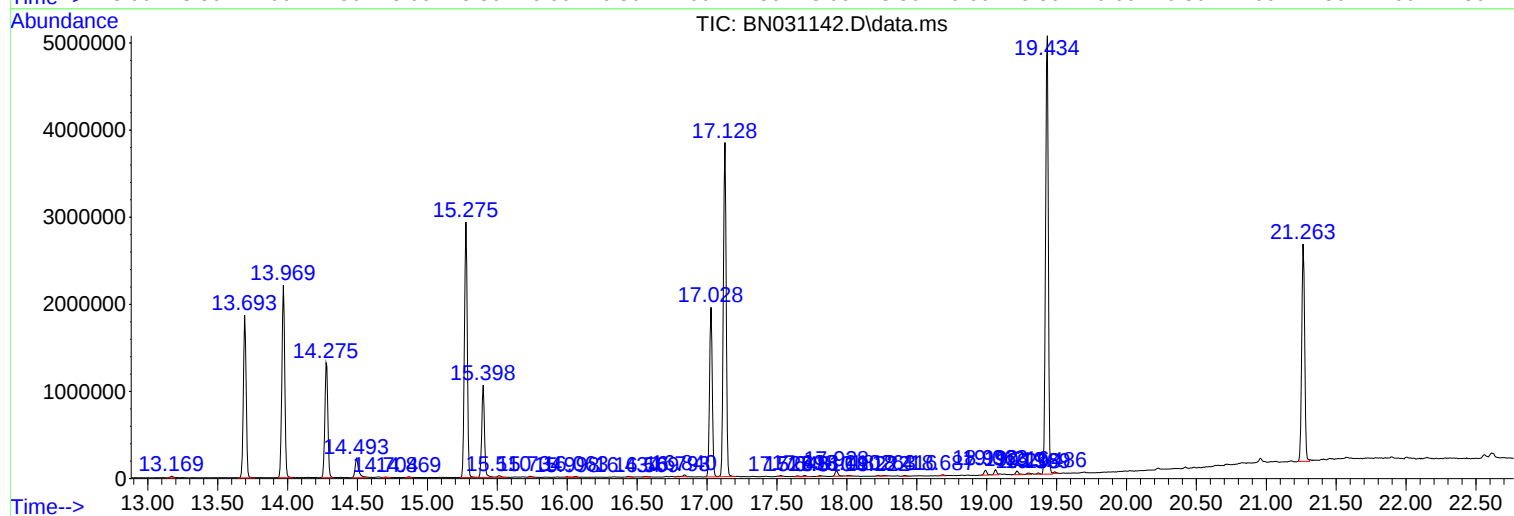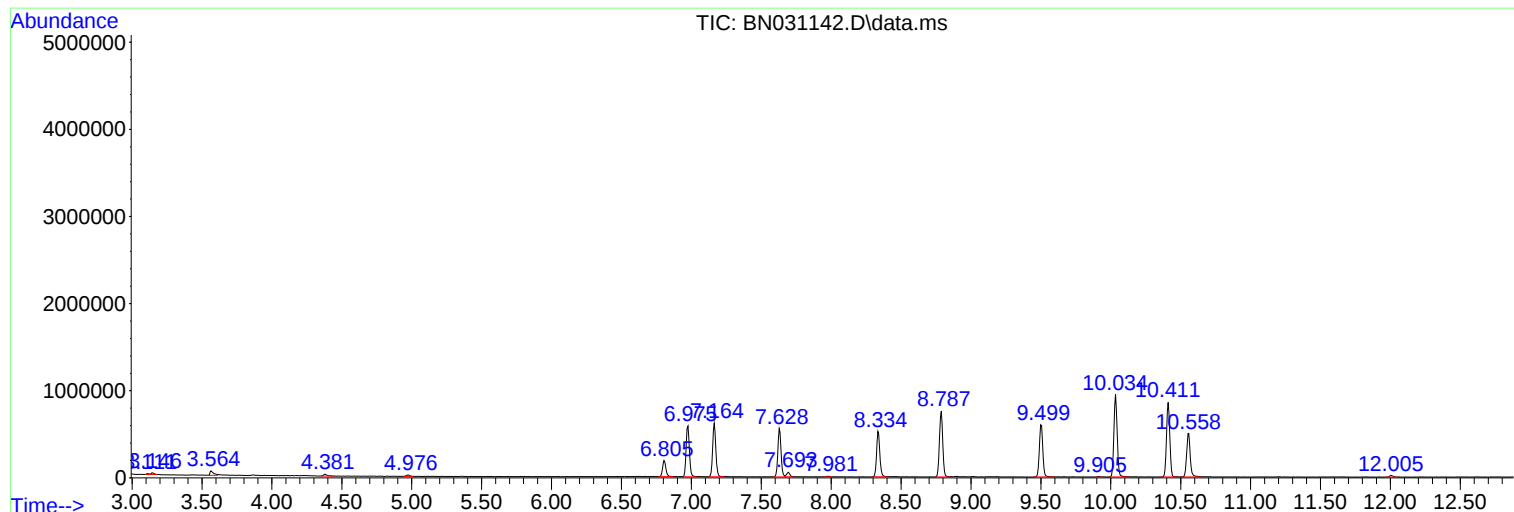

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031142.D
Acq On : 23 Apr 2024 04:48
Operator : MA/JU
Sample : P2142-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031142.D
Acq On : 23 Apr 2024 04:48
Operator : MA/JU
Sample : P2142-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc