

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031143.D
 Acq On : 23 Apr 2024 05:27
 Operator : MA/JU
 Sample : P2142-04
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031143.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.111	17	21	40	rVB2	120817	233745	3.59%	0.518%
2	3.558	95	97	113	rBV	107955	210398	3.23%	0.466%
3	3.864	147	149	154	rBV5	6485	6978	0.11%	0.015%
4	4.381	232	237	246	rVB	41874	69954	1.08%	0.155%
5	4.970	334	337	342	rBV4	9196	13111	0.20%	0.029%
6	5.699	457	461	467	rVB	19638	31087	0.48%	0.069%
7	6.805	642	649	659	rBV	148009	231706	3.56%	0.514%
8	6.975	671	678	690	rVB	490685	787465	12.11%	1.746%
9	7.164	702	710	721	rBV	512085	808637	12.43%	1.793%
10	7.628	782	789	796	rBV	447566	710567	10.92%	1.575%
11	7.693	796	800	810	rVB	39295	62676	0.96%	0.139%
12	8.334	902	909	919	rBV	423289	692273	10.64%	1.535%
13	8.787	979	986	995	rBV	633882	1026349	15.78%	2.275%
14	9.499	1099	1107	1120	rBV	506846	852415	13.10%	1.890%
15	10.034	1190	1198	1213	rBV	776942	1300244	19.99%	2.883%
16	10.410	1254	1262	1270	rBV	696640	1144658	17.60%	2.538%
17	10.552	1279	1286	1299	rBV	663311	1182072	18.17%	2.621%
18	12.004	1526	1533	1538	rBV	14727	27764	0.43%	0.062%
19	13.169	1725	1731	1736	rBV4	14514	24846	0.38%	0.055%
20	13.246	1739	1744	1753	rVB4	3549	8422	0.13%	0.019%
21	13.693	1814	1820	1829	rBV	1516331	2099330	32.27%	4.654%
22	13.969	1860	1867	1880	rBV	1830548	2686748	41.30%	5.957%
23	14.275	1913	1919	1929	rBV	1125125	1654146	25.43%	3.667%
24	14.493	1951	1956	1972	rBV	129379	258019	3.97%	0.572%
25	14.698	1987	1991	1996	rVB8	7172	11259	0.17%	0.025%
26	14.869	2015	2020	2022	rBV3	5691	7834	0.12%	0.017%
27	15.275	2082	2089	2102	rBV	2336604	3353532	51.55%	7.435%
28	15.398	2104	2110	2121	rBV	722141	1000044	15.37%	2.217%
29	15.516	2125	2130	2134	rVB2	10849	16196	0.25%	0.036%
30	15.645	2147	2152	2157	rVB5	12705	16298	0.25%	0.036%
31	15.740	2165	2168	2175	rVB7	5361	9677	0.15%	0.021%
32	16.057	2220	2222	2227	rVB4	8962	11991	0.18%	0.027%
33	16.434	2284	2286	2293	rVB5	6250	8560	0.13%	0.019%
34	16.563	2304	2308	2315	rVB10	3628	7732	0.12%	0.017%
35	16.792	2343	2347	2349	rBV5	5357	7103	0.11%	0.016%
36	16.957	2370	2375	2379	rVB4	12663	15429	0.24%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031143.D
 Acq On : 23 Apr 2024 05:27
 Operator : MA/JU
 Sample : P2142-04
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

37	17.028	2381	2387	2393	rVV	1525844	2145942	32.99%	4.758%
38	17.128	2397	2404	2417	rVV	2813133	3954545	60.79%	8.767%
39	17.487	2462	2465	2469	rVV4	5808	8033	0.12%	0.018%
40	17.645	2487	2492	2497	rBV	44678	59834	0.92%	0.133%
41	17.698	2499	2501	2506	rVB6	5195	7370	0.11%	0.016%
42	17.798	2513	2518	2527	rBV7	25250	42459	0.65%	0.094%
43	17.928	2533	2540	2546	rBV2	37157	57951	0.89%	0.128%
44	18.010	2550	2554	2561	rVB5	7590	14145	0.22%	0.031%
45	18.992	2717	2721	2725	rBV2	44129	54348	0.84%	0.120%
46	19.063	2729	2733	2737	rBV	39906	55580	0.85%	0.123%
47	19.222	2756	2760	2766	rBV8	20466	32388	0.50%	0.072%
48	19.369	2782	2785	2789	rBV6	10738	13508	0.21%	0.030%
49	19.428	2789	2795	2802	rBV	3723325	5171882	79.51%	11.466%
50	21.263	3101	3107	3116	rBV	2010319	2915659	44.82%	6.464%
51	23.969	3557	3567	3579	rBV2	2698213	6504772	100.00%	14.421%
52	24.163	3592	3600	3613	rVB	1432775	3477533	53.46%	7.710%




Sum of corrected areas: 45105214

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031143.D
Acq On : 23 Apr 2024 05:27
Operator : MA/JU
Sample : P2142-04
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

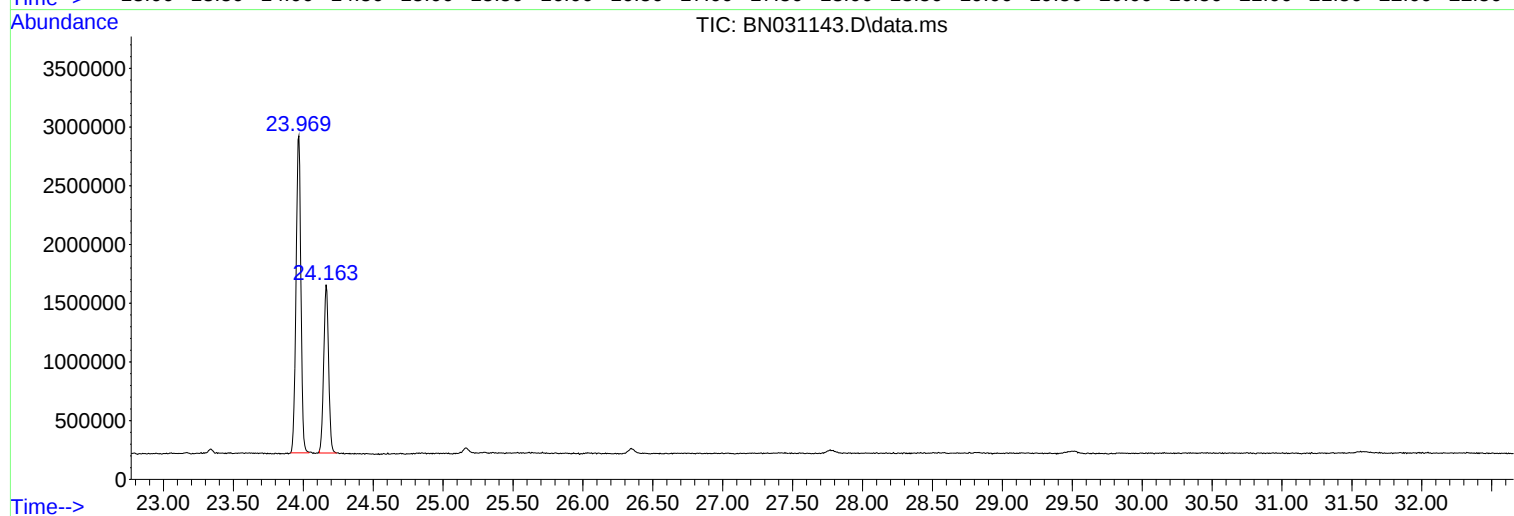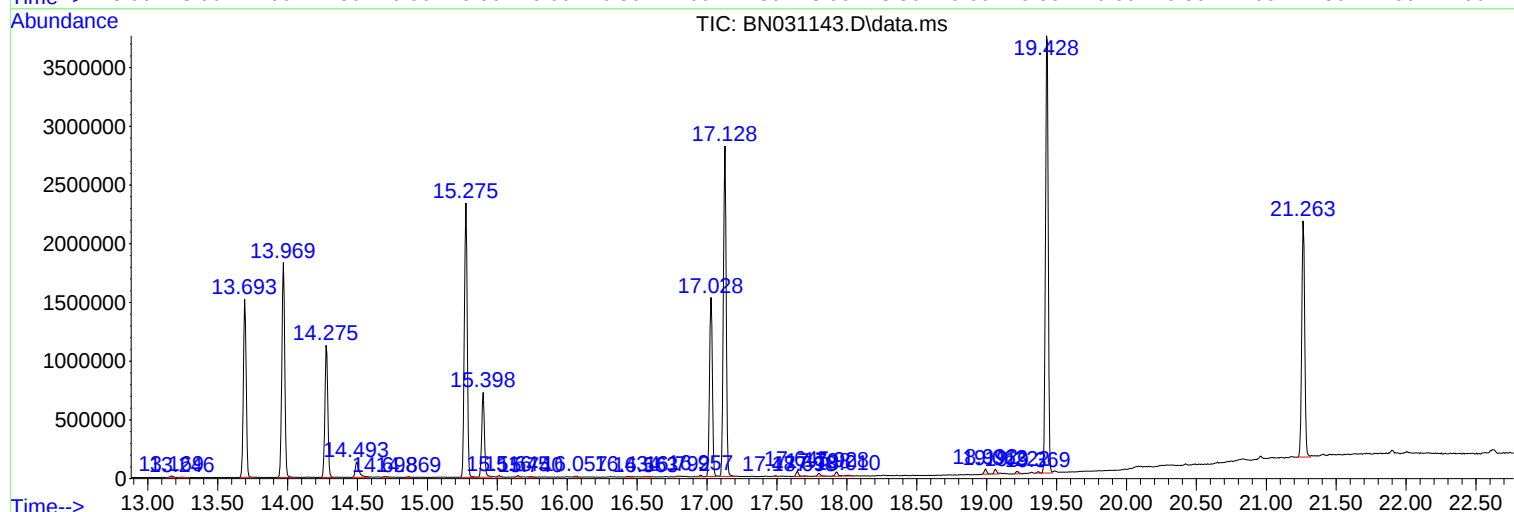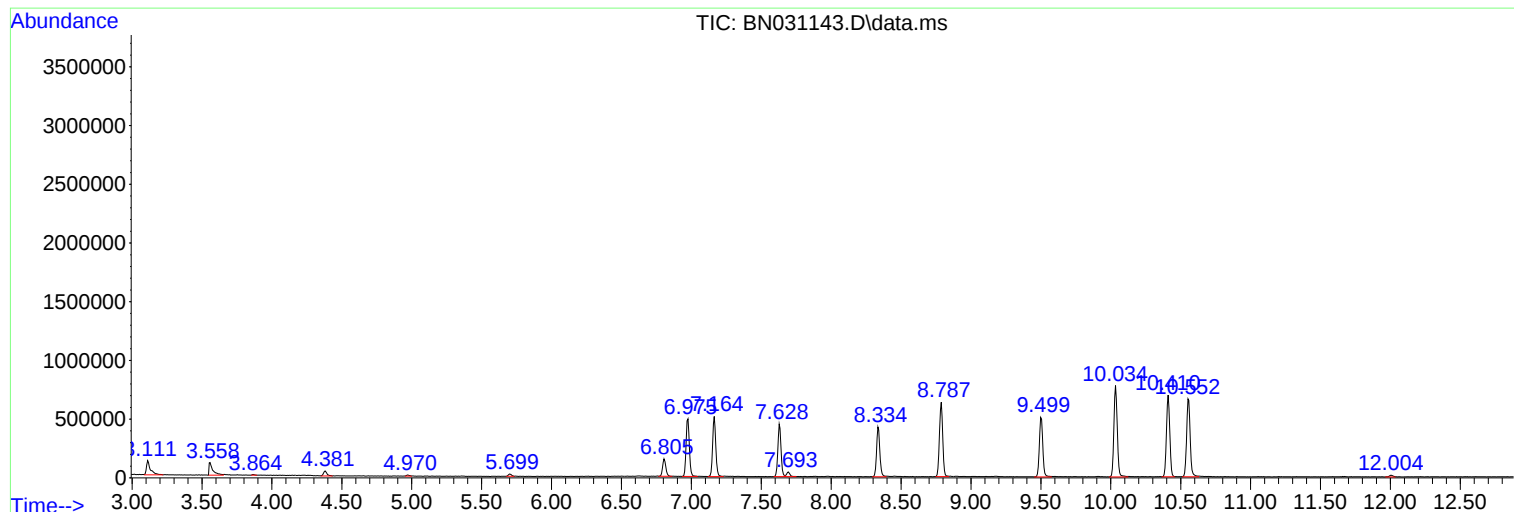

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031143.D
Acq On : 23 Apr 2024 05:27
Operator : MA/JU
Sample : P2142-04
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031143.D
Acq On : 23 Apr 2024 05:27
Operator : MA/JU
Sample : P2142-04
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------