

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031148.D
 Acq On : 23 Apr 2024 09:37
 Operator : MA/JU
 Sample : PB160361BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK361

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031148.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	23	26	34	rBV	27787	40085	0.76%	0.102%
2	3.546	92	95	112	rBV	292907	526632	9.97%	1.336%
3	6.799	642	648	659	rBV	546893	863696	16.35%	2.190%
4	6.969	671	677	687	rBV	431470	675213	12.79%	1.712%
5	7.158	701	709	719	rBV	559647	880092	16.66%	2.232%
6	7.622	782	788	800	rBV	385088	628834	11.91%	1.595%
7	8.328	901	908	923	rBV	682003	1120207	21.21%	2.841%
8	8.781	977	985	994	rBV	540468	873682	16.54%	2.216%
9	9.499	1100	1107	1117	rBV	429741	715624	13.55%	1.815%
10	10.028	1190	1197	1210	rBV	696781	1168436	22.12%	2.963%
11	10.405	1254	1261	1270	rVB	595566	982405	18.60%	2.491%
12	10.552	1278	1286	1300	rBV	393411	689378	13.05%	1.748%
13	12.005	1528	1533	1539	rBV3	11624	18300	0.35%	0.046%
14	13.169	1727	1731	1737	rVB3	9387	15507	0.29%	0.039%
15	13.693	1810	1820	1827	rBV	1295654	1750001	33.14%	4.438%
16	13.969	1859	1867	1879	rBV	1483130	2213003	41.90%	5.612%
17	14.275	1913	1919	1928	rBV	1001628	1401012	26.53%	3.553%
18	14.487	1949	1955	1979	rBV	550436	997052	18.88%	2.529%
19	15.275	2080	2089	2100	rBV	1938066	2800826	53.03%	7.103%
20	15.398	2103	2110	2121	rVV	565732	764969	14.48%	1.940%
21	15.510	2125	2129	2133	rVB4	8629	12482	0.24%	0.032%
22	16.063	2218	2223	2227	rVB8	7865	11535	0.22%	0.029%
23	17.028	2381	2387	2397	rBV	1342061	1821515	34.49%	4.619%
24	17.128	2397	2404	2420	rVV	2321478	3254728	61.63%	8.254%
25	17.698	2498	2501	2506	rVB5	7036	7369	0.14%	0.019%
26	18.992	2717	2721	2727	rVB3	32649	41104	0.78%	0.104%
27	19.063	2729	2733	2737	rBV	28003	35238	0.67%	0.089%
28	19.122	2741	2743	2746	rBV4	4120	5371	0.10%	0.014%
29	19.434	2789	2796	2803	rBV	3036778	4254458	80.56%	10.789%
30	21.263	3102	3107	3119	rBV2	1779160	2587671	49.00%	6.562%
31	23.969	3558	3567	3583	rVB2	2214400	5281213	100.00%	13.393%
32	24.163	3592	3600	3617	rVB	1252039	2993901	56.69%	7.593%




Sum of corrected areas: 39431539

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031148.D
Acq On : 23 Apr 2024 09:37
Operator : MA/JU
Sample : PB160361BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK361

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

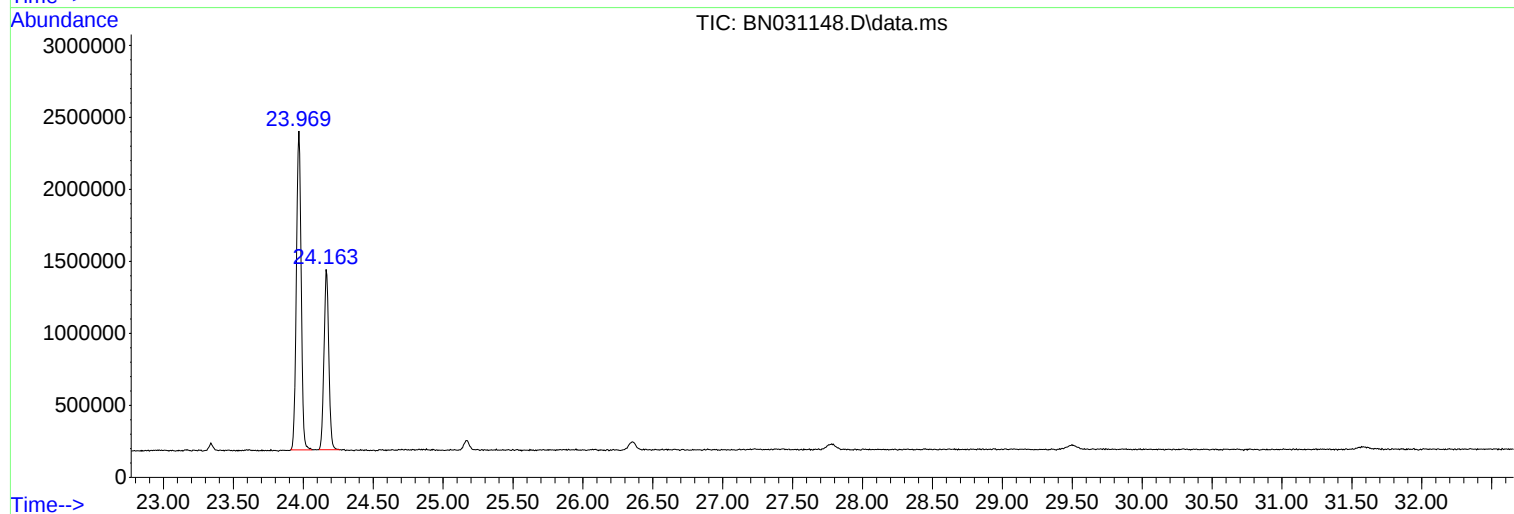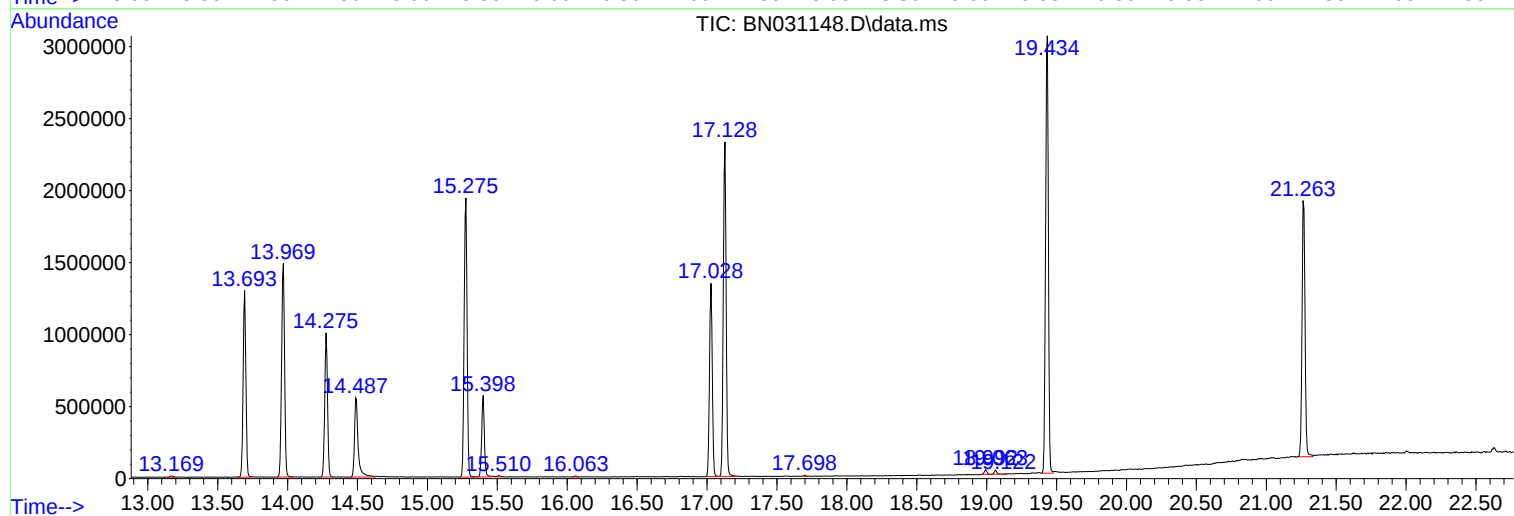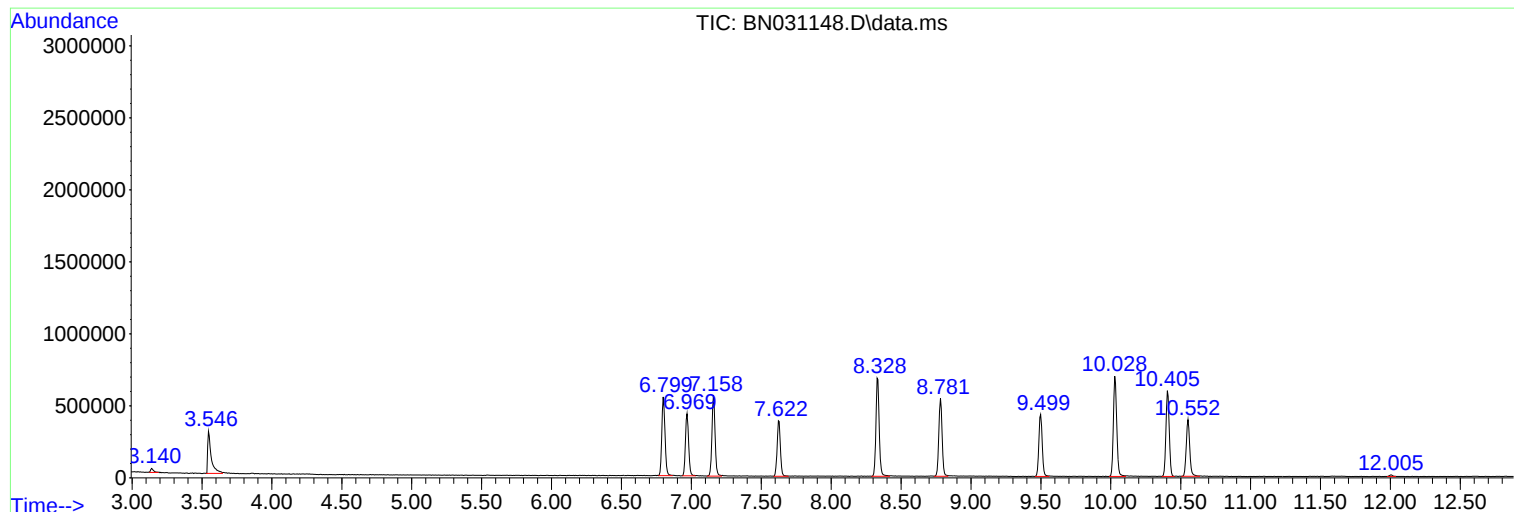

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031148.D
Acq On : 23 Apr 2024 09:37
Operator : MA/JU
Sample : PB160361BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK361

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031148.D
Acq On : 23 Apr 2024 09:37
Operator : MA/JU
Sample : PB160361BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK361

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc