

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031151.D
 Acq On : 23 Apr 2024 12:18
 Operator : MA/JU
 Sample : P2077-09DL 5X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AL3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031151.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	24	26	27	rBV2	4435	4096	0.15%	0.023%
2	3.587	100	102	106	rBV4	7427	10257	0.39%	0.057%
3	3.858	146	148	152	rVB4	4130	5265	0.20%	0.029%
4	4.693	286	290	293	rBV6	2382	3605	0.14%	0.020%
5	6.628	617	619	623	rBV4	2614	3461	0.13%	0.019%
6	6.811	645	650	658	rVB2	12751	22764	0.86%	0.127%
7	6.975	671	678	688	rBV	70238	113677	4.27%	0.633%
8	7.163	704	710	718	rBV	61006	99571	3.74%	0.554%
9	7.628	783	789	797	rBV	358363	577369	21.70%	3.214%
10	7.975	845	848	854	rVB7	2474	3896	0.15%	0.022%
11	8.340	904	910	920	rBV	41345	76944	2.89%	0.428%
12	8.787	980	986	996	rBV	79806	132149	4.97%	0.736%
13	9.181	1050	1053	1057	rVB5	2521	2763	0.10%	0.015%
14	9.352	1077	1082	1084	rVB5	2077	3729	0.14%	0.021%
15	9.505	1101	1108	1114	rBV	54171	94578	3.56%	0.526%
16	9.857	1165	1168	1171	rVB3	2404	2907	0.11%	0.016%
17	10.034	1192	1198	1209	rBV	87121	160392	6.03%	0.893%
18	10.275	1235	1239	1244	rVB5	4367	7165	0.27%	0.040%
19	10.410	1255	1262	1271	rBV	576783	936278	35.19%	5.212%
20	10.557	1281	1287	1297	rBV	83243	154853	5.82%	0.862%
21	11.204	1394	1397	1401	rBV5	1565	3153	0.12%	0.018%
22	11.669	1472	1476	1477	rBV4	2149	2688	0.10%	0.015%
23	11.710	1480	1483	1490	rVB7	3010	5991	0.23%	0.033%
24	12.010	1529	1534	1535	rBV4	2272	3894	0.15%	0.022%
25	12.263	1573	1577	1584	rVB2	10778	16375	0.62%	0.091%
26	13.069	1712	1714	1719	rVB4	2646	3950	0.15%	0.022%
27	13.169	1726	1731	1736	rBV3	12204	20225	0.76%	0.113%
28	13.693	1815	1820	1828	rBV	257407	351083	13.20%	1.954%
29	13.969	1861	1867	1875	rBV	260875	386560	14.53%	2.152%
30	14.275	1913	1919	1928	rBV	933558	1387993	52.17%	7.727%
31	14.357	1931	1933	1938	rVB5	4087	5429	0.20%	0.030%
32	14.522	1956	1961	1962	rBV4	4824	7382	0.28%	0.041%
33	14.957	2031	2035	2040	rBV4	4133	4493	0.17%	0.025%
34	15.110	2055	2061	2069	rBV	2088505	2660319	100.00%	14.809%
35	15.275	2082	2089	2098	rBV	412081	583382	21.93%	3.248%
36	15.398	2105	2110	2118	rBV	55771	82401	3.10%	0.459%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031151.D
 Acq On : 23 Apr 2024 12:18
 Operator : MA/JU
 Sample : P2077-09DL 5X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AL3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

37	15.651	2149	2153	2155	rBV4	3050	3336	0.13%	0.019%
38	16.816	2347	2351	2354	rBV3	3136	3896	0.15%	0.022%
39	17.028	2381	2387	2397	rBV	1343890	1852376	69.63%	10.312%
40	17.128	2397	2404	2414	rVV	488705	692247	26.02%	3.854%
41	17.328	2434	2438	2441	rVB6	4400	5603	0.21%	0.031%
42	17.375	2442	2446	2451	rVB2	9604	11146	0.42%	0.062%
43	17.698	2497	2501	2505	rBV4	51344	64455	2.42%	0.359%
44	17.922	2536	2539	2543	rBV5	3685	5447	0.20%	0.030%
45	18.004	2551	2553	2558	rVB6	3310	5518	0.21%	0.031%
46	18.481	2631	2634	2637	rBV5	3246	5305	0.20%	0.030%
47	18.645	2659	2662	2665	rVB3	12274	12687	0.48%	0.071%
48	18.692	2665	2670	2673	rBV2	21229	28194	1.06%	0.157%
49	18.992	2718	2721	2724	rVB4	5947	7861	0.30%	0.044%
50	19.216	2757	2759	2764	rVB6	5356	5954	0.22%	0.033%
51	19.428	2790	2795	2802	rBV	694781	925649	34.79%	5.153%
52	19.780	2851	2855	2858	rBV	67219	76366	2.87%	0.425%
53	19.816	2858	2861	2868	rVB	162672	175296	6.59%	0.976%
54	20.792	3024	3027	3032	rBV3	42077	46007	1.73%	0.256%
55	21.263	3101	3107	3117	rBV	1741221	2429930	91.34%	13.527%
56	23.957	3558	3565	3578	rVB2	429772	1013369	38.09%	5.641%
57	24.157	3591	3599	3614	rVB2	1083296	2651997	99.69%	14.763%


Sum of corrected areas: 17963676

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031151.D
Acq On : 23 Apr 2024 12:18
Operator : MA/JU
Sample : P2077-09DL 5X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL3DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

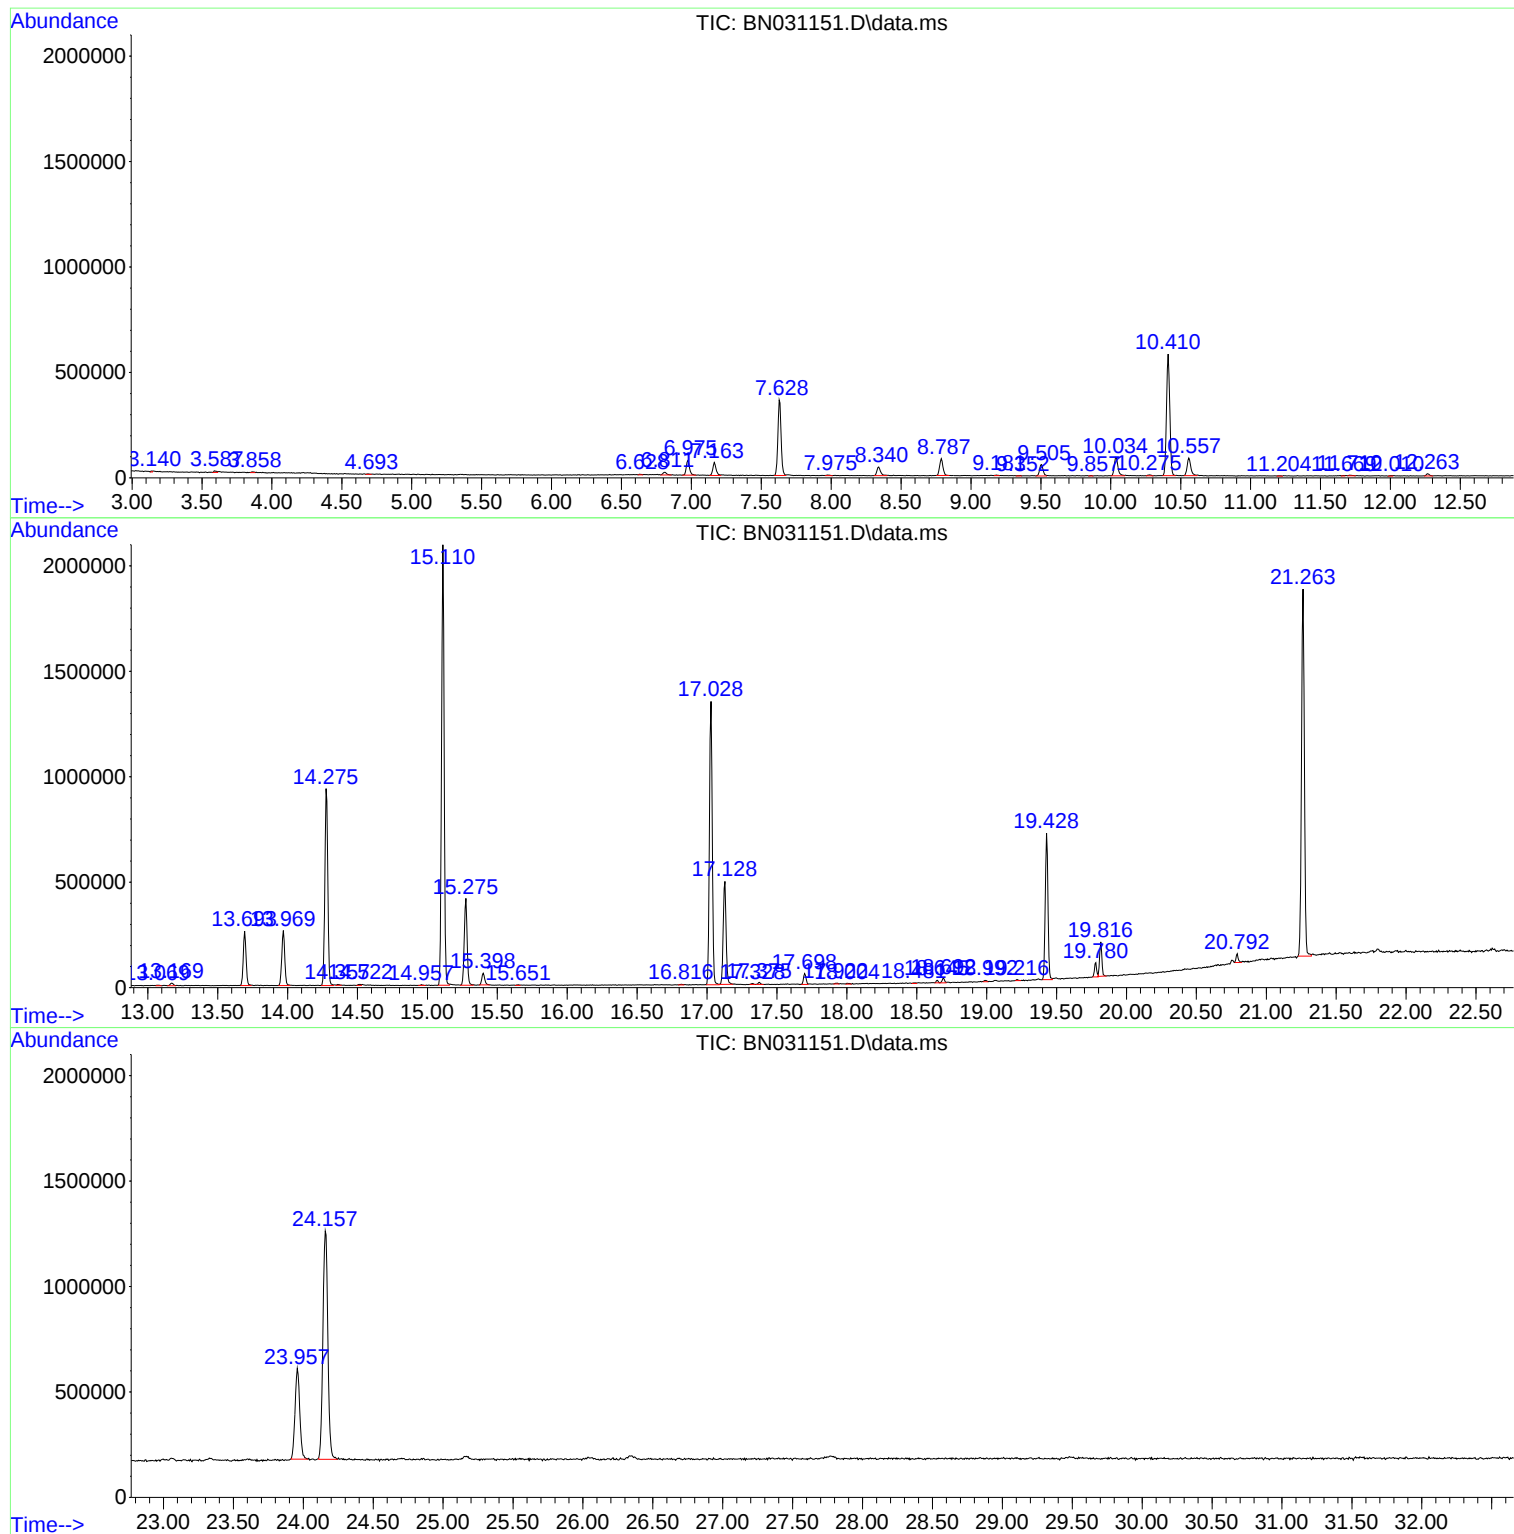

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031151.D
Acq On : 23 Apr 2024 12:18
Operator : MA/JU
Sample : P2077-09DL 5X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL3DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031151.D
Acq On : 23 Apr 2024 12:18
Operator : MA/JU
Sample : P2077-09DL 5X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL3DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc