

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031155.D
 Acq On : 23 Apr 2024 14:58
 Operator : MA/JU
 Sample : P2164-02
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0SA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031155.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	23	27	32	rBV	19311	28872	0.62%	0.064%
2	3.422	70	74	84	rBV	16749	32454	0.69%	0.072%
3	3.552	94	96	112	rBV	278515	487066	10.39%	1.085%
4	3.864	147	149	154	rVB5	6622	8700	0.19%	0.019%
5	5.734	464	467	471	rBV4	5087	8264	0.18%	0.018%
6	6.634	617	620	625	rVB7	3929	6976	0.15%	0.016%
7	6.805	643	649	664	rBV	507363	812125	17.33%	1.809%
8	6.975	672	678	692	rVB	410567	641303	13.69%	1.428%
9	7.163	703	710	721	rBV	507274	796704	17.00%	1.775%
10	7.628	781	789	797	rBV	555317	905587	19.32%	2.017%
11	7.705	799	802	809	rVB8	4599	9806	0.21%	0.022%
12	8.334	902	909	921	rBV	670372	1070104	22.84%	2.384%
13	8.787	979	986	1002	rBV	516485	833212	17.78%	1.856%
14	8.946	1009	1013	1019	rVB7	4494	7172	0.15%	0.016%
15	9.181	1048	1053	1056	rVB4	6400	8415	0.18%	0.019%
16	9.357	1077	1083	1091	rVB3	18463	31249	0.67%	0.070%
17	9.504	1100	1108	1117	rBV	408052	677628	14.46%	1.509%
18	9.916	1175	1178	1184	rVB7	3706	5745	0.12%	0.013%
19	10.034	1190	1198	1215	rBV	688937	1148169	24.50%	2.557%
20	10.199	1224	1226	1235	rVB8	3693	7527	0.16%	0.017%
21	10.410	1254	1262	1272	rBV	897752	1461284	31.18%	3.255%
22	10.551	1278	1286	1302	rBV	612681	1081076	23.07%	2.408%
23	10.969	1352	1357	1362	rVB8	4761	7987	0.17%	0.018%
24	11.157	1384	1389	1396	rBV2	19657	34383	0.73%	0.077%
25	11.916	1514	1518	1524	rBV3	4653	6983	0.15%	0.016%
26	12.004	1529	1533	1539	rVB	12200	18976	0.40%	0.042%
27	13.098	1713	1719	1724	rBV7	4903	8398	0.18%	0.019%
28	13.175	1724	1732	1740	rVV3	14594	27490	0.59%	0.061%
29	13.692	1814	1820	1827	rBV	1307063	1805555	38.53%	4.022%
30	13.969	1857	1867	1879	rBV	1584650	2272567	48.50%	5.062%
31	14.187	1900	1904	1910	rVB5	8327	14578	0.31%	0.032%
32	14.275	1913	1919	1931	rBV	1434994	2126441	45.38%	4.737%
33	14.492	1949	1956	1973	rBV	570829	1004268	21.43%	2.237%
34	14.669	1983	1986	1988	rBV4	4061	5590	0.12%	0.012%
35	14.704	1988	1992	1998	rVB8	7626	15619	0.33%	0.035%
36	15.086	2051	2057	2059	rBV5	4482	7381	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031155.D
 Acq On : 23 Apr 2024 14:58
 Operator : MA/JU
 Sample : P2164-02
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0SA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

37	15.134	2062	2065	2070	rVB5	4690	6593	0.14%	0.015%
38	15.275	2082	2089	2098	rBV	2068588	2900641	61.90%	6.461%
39	15.398	2104	2110	2123	rBV	478681	664817	14.19%	1.481%
40	15.516	2126	2130	2137	rVB6	11341	18317	0.39%	0.041%
41	15.645	2149	2152	2157	rVB5	3832	4946	0.11%	0.011%
42	15.998	2210	2212	2218	rVB7	5439	7070	0.15%	0.016%
43	16.063	2219	2223	2228	rVB5	7452	9737	0.21%	0.022%
44	16.433	2284	2286	2289	rBV4	4604	4944	0.11%	0.011%
45	16.951	2372	2374	2379	rVB6	4135	5620	0.12%	0.013%
46	17.028	2379	2387	2393	rBV	1998737	2734536	58.35%	6.091%
47	17.128	2398	2404	2414	rVV	2347652	3315543	70.75%	7.385%
48	17.228	2417	2421	2426	rVB7	13014	19476	0.42%	0.043%
49	17.322	2433	2437	2441	rBV3	7823	10234	0.22%	0.023%
50	17.704	2499	2502	2507	rBV3	12746	16662	0.36%	0.037%
51	17.869	2526	2530	2534	rBV5	9220	13329	0.28%	0.030%
52	17.928	2535	2540	2550	rBV	175379	246103	5.25%	0.548%
53	18.222	2588	2590	2594	rVB5	5287	5850	0.12%	0.013%
54	18.357	2611	2613	2618	rVB5	7509	9676	0.21%	0.022%
55	18.398	2618	2620	2626	rBV7	4646	10008	0.21%	0.022%
56	18.869	2696	2700	2702	rBV5	10140	14803	0.32%	0.033%
57	18.992	2716	2721	2725	rBV	34993	50453	1.08%	0.112%
58	19.063	2729	2733	2736	rBV	37100	52727	1.13%	0.117%
59	19.092	2736	2738	2742	rVB2	30197	38070	0.81%	0.085%
60	19.216	2755	2759	2767	rBV	85669	119203	2.54%	0.266%
61	19.369	2782	2785	2789	rBV6	12970	18764	0.40%	0.042%
62	19.427	2789	2795	2803	rVV	3045732	4240069	90.48%	9.445%
63	19.486	2803	2805	2812	rVB3	35838	45390	0.97%	0.101%
64	19.780	2852	2855	2858	rBV3	20334	24727	0.53%	0.055%
65	19.816	2858	2861	2865	rVB2	22780	24422	0.52%	0.054%
66	19.986	2887	2890	2894	rVB2	36188	40935	0.87%	0.091%
67	20.480	2971	2974	2978	rBV	59966	69172	1.48%	0.154%
68	20.957	3051	3055	3062	rBV	222377	357405	7.63%	0.796%
69	21.263	3101	3107	3118	rBV	2374096	3525633	75.24%	7.853%
70	21.457	3136	3140	3144	rBV	69031	94447	2.02%	0.210%
71	22.004	3230	3233	3241	rVB2	66974	110986	2.37%	0.247%
72	23.333	3456	3459	3466	rVB3	69326	126979	2.71%	0.283%
73	23.962	3557	3566	3583	rVB2	1942283	4686142	100.00%	10.438%
74	24.162	3591	3600	3616	rVB3	1505682	3824244	81.61%	8.518%

Sum of corrected areas: 44894327




Instrument :
BNA_N
ClientSampleId :
C0SA0

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031155.D
Acq On : 23 Apr 2024 14:58
Operator : MA/JU
Sample : P2164-02
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0SA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

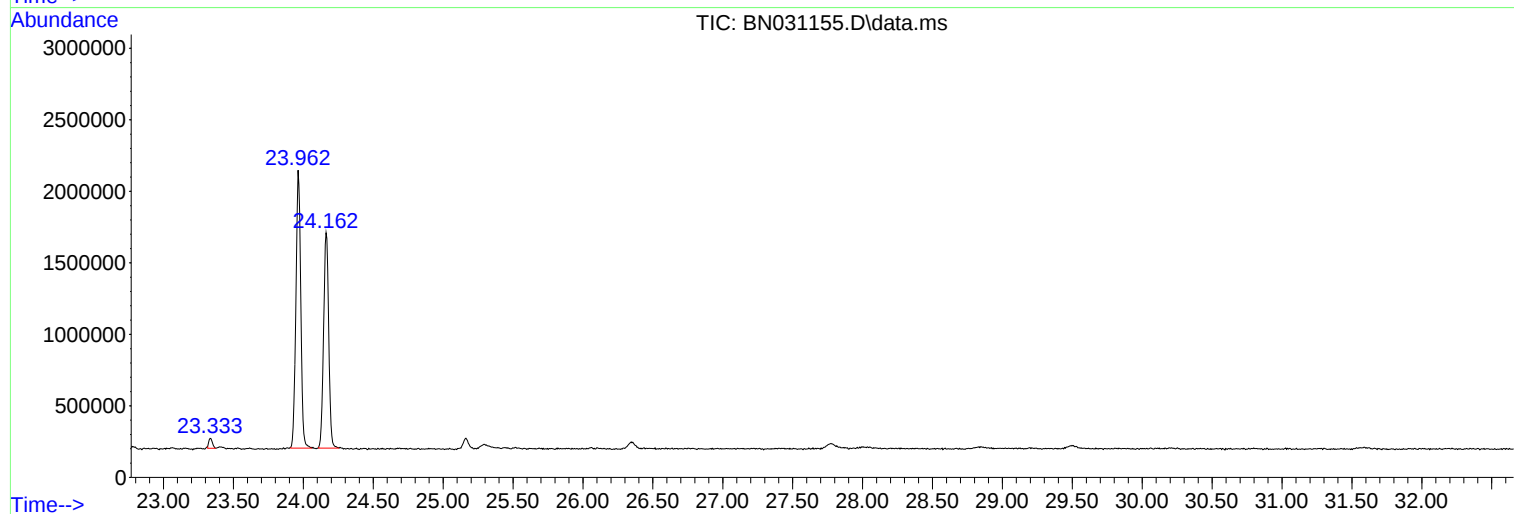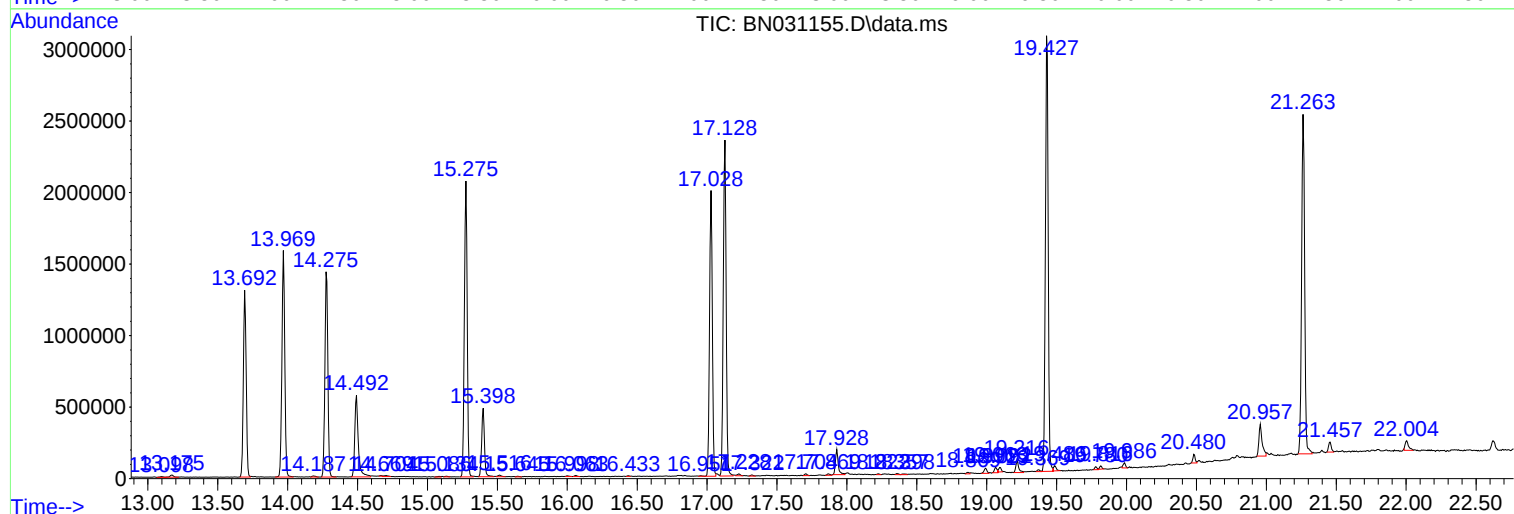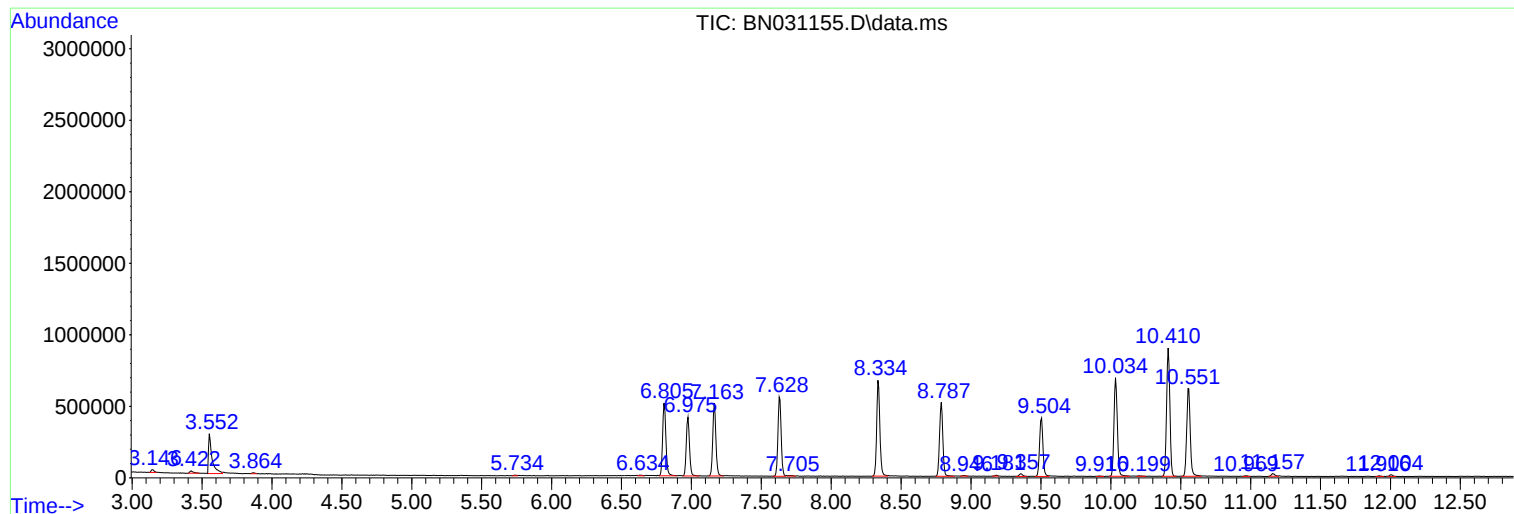

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031155.D
Acq On : 23 Apr 2024 14:58
Operator : MA/JU
Sample : P2164-02
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0SA0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Carbonic acid, decyl octade... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.957	2.03 ng/ul	357405	Chrysene-d12	21.263

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Carbonic acid, decyl octadecyl e...	454	C29H58O3	1000383-16-7	91
2			1-Decanol, 2-hexyl-	242	C16H34O	002425-77-6	91
3			Hexadecane	226	C16H34	000544-76-3	83
4			Eicosane	282	C20H42	000112-95-8	83
5			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	81

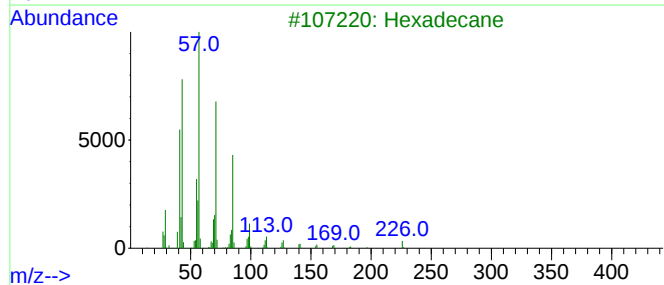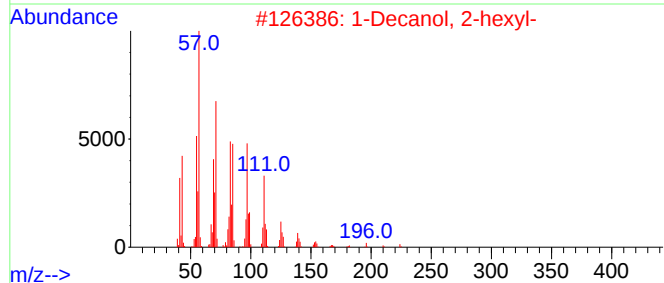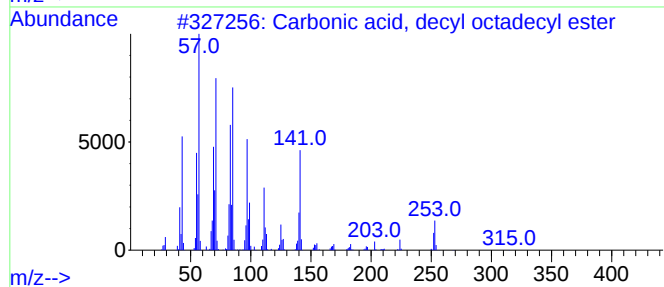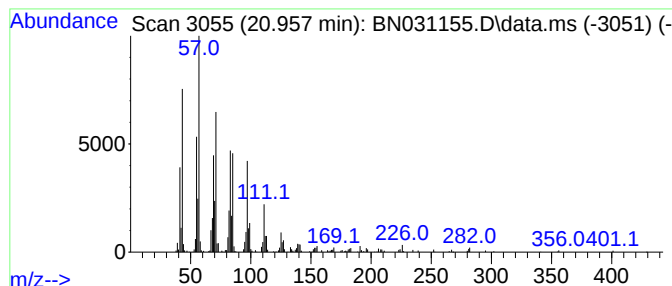

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031155.D
Acq On : 23 Apr 2024 14:58
Operator : MA/JU
Sample : P2164-02
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0SA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Carbonic acid, ...	20.957	2.0	ng/ul	357405	5	21.263	3525630	20.0