

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031162.D
 Acq On : 23 Apr 2024 20:16
 Operator : MA/JU
 Sample : PB160404BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK404

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	33	rBV	26219	41980	0.85%	0.099%
2	3.552	93	96	117	rBV	340127	605981	12.31%	1.431%
3	3.869	146	150	154	rVB4	4511	7106	0.14%	0.017%
4	6.804	643	649	662	rVB	548216	845515	17.18%	1.997%
5	6.975	671	678	687	rBV	429795	667944	13.57%	1.578%
6	7.163	703	710	726	rBV	535808	847198	17.21%	2.001%
7	7.628	782	789	798	rBV	489892	770223	15.65%	1.819%
8	8.334	902	909	919	rBV	684440	1110875	22.57%	2.624%
9	8.787	979	986	994	rBV	522780	852669	17.32%	2.014%
10	8.951	1009	1014	1021	rBV	3477	6387	0.13%	0.015%
11	9.504	1101	1108	1117	rBV	426021	693611	14.09%	1.638%
12	10.034	1191	1198	1210	rBV	716644	1168243	23.73%	2.759%
13	10.410	1254	1262	1270	rBV	765682	1253954	25.47%	2.962%
14	10.557	1280	1287	1305	rBV	687345	1171791	23.81%	2.768%
15	12.010	1527	1534	1538	rBV4	10613	19451	0.40%	0.046%
16	13.175	1725	1732	1736	rBV3	11151	17013	0.35%	0.040%
17	13.692	1814	1820	1828	rBV	1293630	1785742	36.28%	4.218%
18	13.969	1860	1867	1877	rBV2	1540479	2247114	45.65%	5.307%
19	14.274	1912	1919	1930	rBV	1234240	1838373	37.35%	4.342%
20	14.492	1948	1956	1972	rBV	547262	961102	19.52%	2.270%
21	15.274	2082	2089	2099	rBV	2068906	2850481	57.91%	6.732%
22	15.398	2104	2110	2124	rVV	540388	747805	15.19%	1.766%
23	15.510	2126	2129	2134	rVV4	7487	11132	0.23%	0.026%
24	16.063	2217	2223	2227	rBV6	6459	8170	0.17%	0.019%
25	17.027	2381	2387	2397	rVB	1754437	2405935	48.88%	5.682%
26	17.127	2397	2404	2415	rBV	2382508	3336691	67.79%	7.881%
27	17.927	2537	2540	2546	rBV7	4971	7272	0.15%	0.017%
28	18.992	2717	2721	2726	rBV2	27666	36952	0.75%	0.087%
29	19.062	2729	2733	2738	rVB	26573	36765	0.75%	0.087%
30	19.215	2758	2759	2764	rBV5	5095	7834	0.16%	0.019%
31	19.362	2782	2784	2789	rBV6	8971	12176	0.25%	0.029%
32	19.433	2789	2796	2803	rBV	3085096	4297871	87.31%	10.151%
33	21.262	3101	3107	3117	rBV	2314250	3189115	64.79%	7.532%
34	23.968	3557	3567	3580	rBV	2064312	4922445	100.00%	11.626%
35	24.162	3591	3600	3616	rVB2	1417938	3556920	72.26%	8.401%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031162.D
Acq On : 23 Apr 2024 20:16
Operator : MA/JU
Sample : PB160404BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK404

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 42339836

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031162.D
Acq On : 23 Apr 2024 20:16
Operator : MA/JU
Sample : PB160404BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK404

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

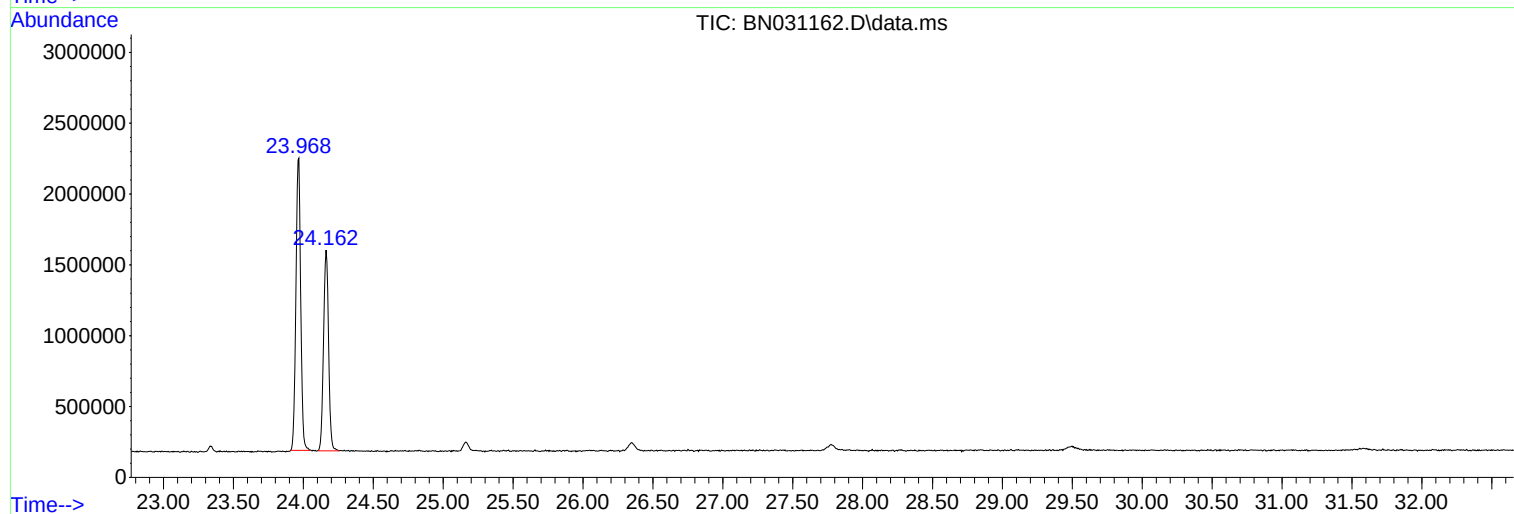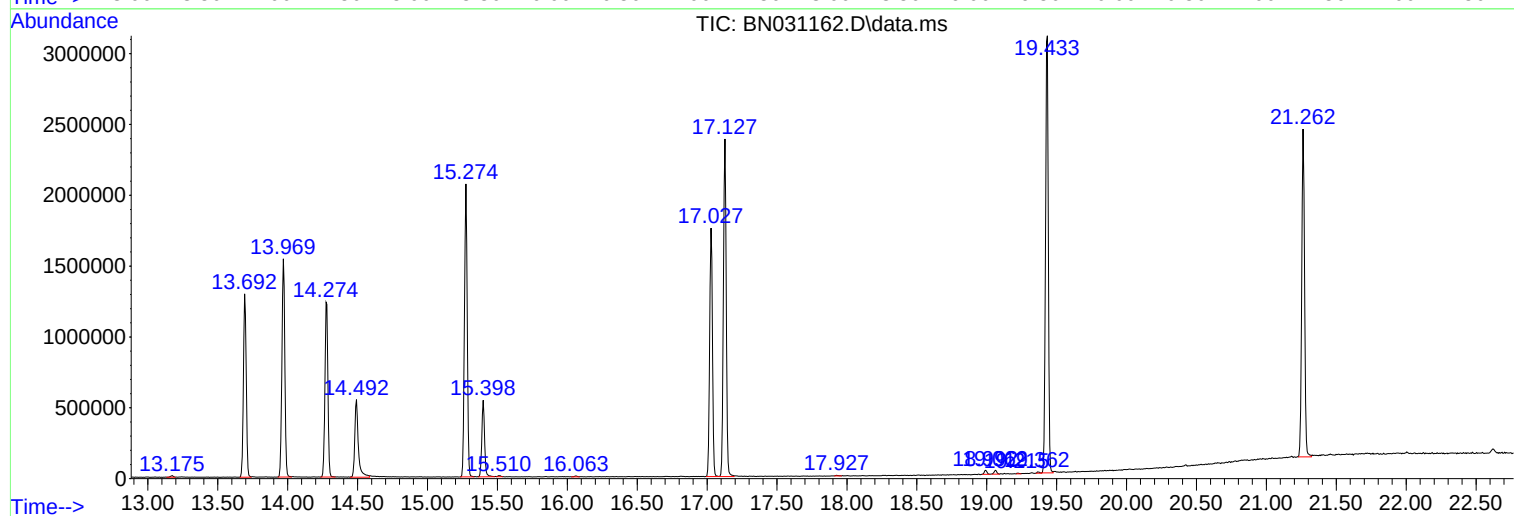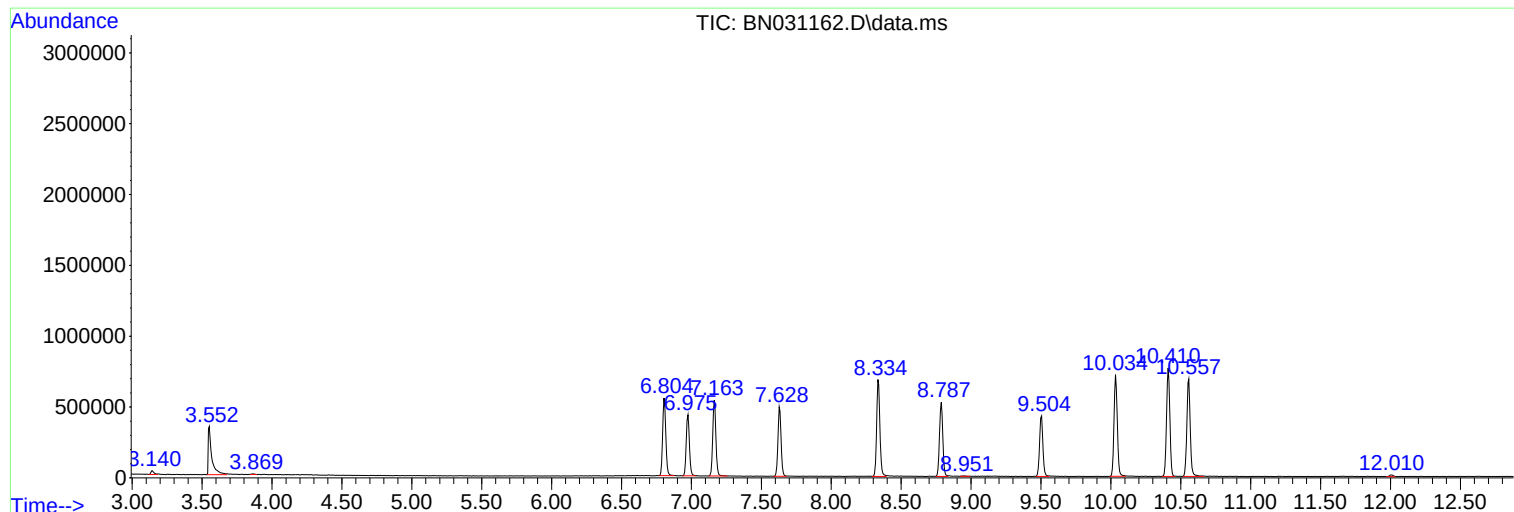

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031162.D
Acq On : 23 Apr 2024 20:16
Operator : MA/JU
Sample : PB160404BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK404

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031162.D
Acq On : 23 Apr 2024 20:16
Operator : MA/JU
Sample : PB160404BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK404

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc