

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031170.D
 Acq On : 24 Apr 2024 01:32
 Operator : MA/JU
 Sample : P2140-07
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031170.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.111	18	21	24	rBV3	9649	13063	0.15%	0.020%
2	3.146	24	27	37	rVB	31277	52357	0.59%	0.081%
3	3.552	95	96	111	rBV	160672	294160	3.31%	0.456%
4	5.699	457	461	473	rVB3	25431	48899	0.55%	0.076%
5	6.805	643	649	659	rBV	159343	257837	2.91%	0.400%
6	6.975	671	678	691	rBV	685469	1098386	12.38%	1.703%
7	7.163	702	710	720	rBV	638774	1009949	11.38%	1.566%
8	7.628	782	789	797	rBV	686253	1081985	12.19%	1.678%
9	8.334	901	909	922	rBV	515822	836116	9.42%	1.296%
10	8.787	977	986	996	rBV	880138	1455901	16.40%	2.257%
11	9.175	1047	1052	1058	rVB3	7646	12617	0.14%	0.020%
12	9.357	1079	1083	1088	rBV3	9260	14865	0.17%	0.023%
13	9.499	1100	1107	1119	rBV	679562	1115081	12.56%	1.729%
14	9.910	1169	1177	1183	rBV2	7167	11590	0.13%	0.018%
15	10.034	1189	1198	1212	rBV	1017354	1698270	19.13%	2.633%
16	10.410	1254	1262	1272	rBV	1037673	1742440	19.63%	2.702%
17	10.552	1277	1286	1301	rBV	1007465	1736686	19.57%	2.693%
18	11.163	1384	1390	1394	rBV3	9964	20256	0.23%	0.031%
19	12.004	1528	1533	1539	rBV2	22052	35186	0.40%	0.055%
20	13.122	1715	1723	1726	rBV4	7641	18411	0.21%	0.029%
21	13.169	1726	1731	1736	rVB2	13959	23078	0.26%	0.036%
22	13.693	1812	1820	1829	rBV	2202427	3039978	34.25%	4.714%
23	13.969	1860	1867	1878	rBV	2539817	3803712	42.86%	5.898%
24	14.275	1912	1919	1928	rBV	1764073	2542446	28.65%	3.942%
25	14.492	1950	1956	1970	rBV	156122	301919	3.40%	0.468%
26	14.840	2009	2015	2021	rBV2	14926	30479	0.34%	0.047%
27	15.275	2082	2089	2095	rBV	3547347	4952825	55.80%	7.680%
28	15.322	2095	2097	2104	rVB6	15806	19388	0.22%	0.030%
29	15.398	2104	2110	2121	rBV	1056549	1436124	16.18%	2.227%
30	15.516	2126	2130	2135	rVB2	17399	26535	0.30%	0.041%
31	16.057	2218	2222	2228	rVB4	12900	19047	0.21%	0.030%
32	17.028	2380	2387	2394	rBV	2342080	3285068	37.01%	5.094%
33	17.128	2397	2404	2415	rBV2	4214903	6061708	68.30%	9.399%
34	17.798	2514	2518	2522	rBV7	7527	12831	0.14%	0.020%
35	17.928	2535	2540	2547	rBV	80009	117728	1.33%	0.183%
36	18.363	2611	2614	2617	rVB5	7844	9752	0.11%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031170.D
 Acq On : 24 Apr 2024 01:32
 Operator : MA/JU
 Sample : P2140-07
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

37	18.992	2716	2721	2725	rBV	64348	85393	0.96%	0.132%
38	19.063	2728	2733	2737	rBV	64612	88374	1.00%	0.137%
39	19.216	2755	2759	2767	rBV5	40212	56666	0.64%	0.088%
40	19.369	2782	2785	2788	rVB2	22758	25064	0.28%	0.039%
41	19.433	2789	2796	2803	rBV	5328360	7614287	85.79%	11.806%
42	20.957	3051	3055	3064	rBV4	124025	224132	2.53%	0.348%
43	21.263	3101	3107	3119	rBV2	3003119	4322164	48.70%	6.702%
44	22.792	3363	3367	3372	rVB2	112324	188175	2.12%	0.292%
45	23.968	3557	3567	3585	rVB2	3582792	8875324	100.00%	13.762%
46	24.163	3591	3600	3617	rVB	1943309	4776244	53.81%	7.406%


Sum of corrected areas: 64492496

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031170.D
Acq On : 24 Apr 2024 01:32
Operator : MA/JU
Sample : P2140-07
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSR3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

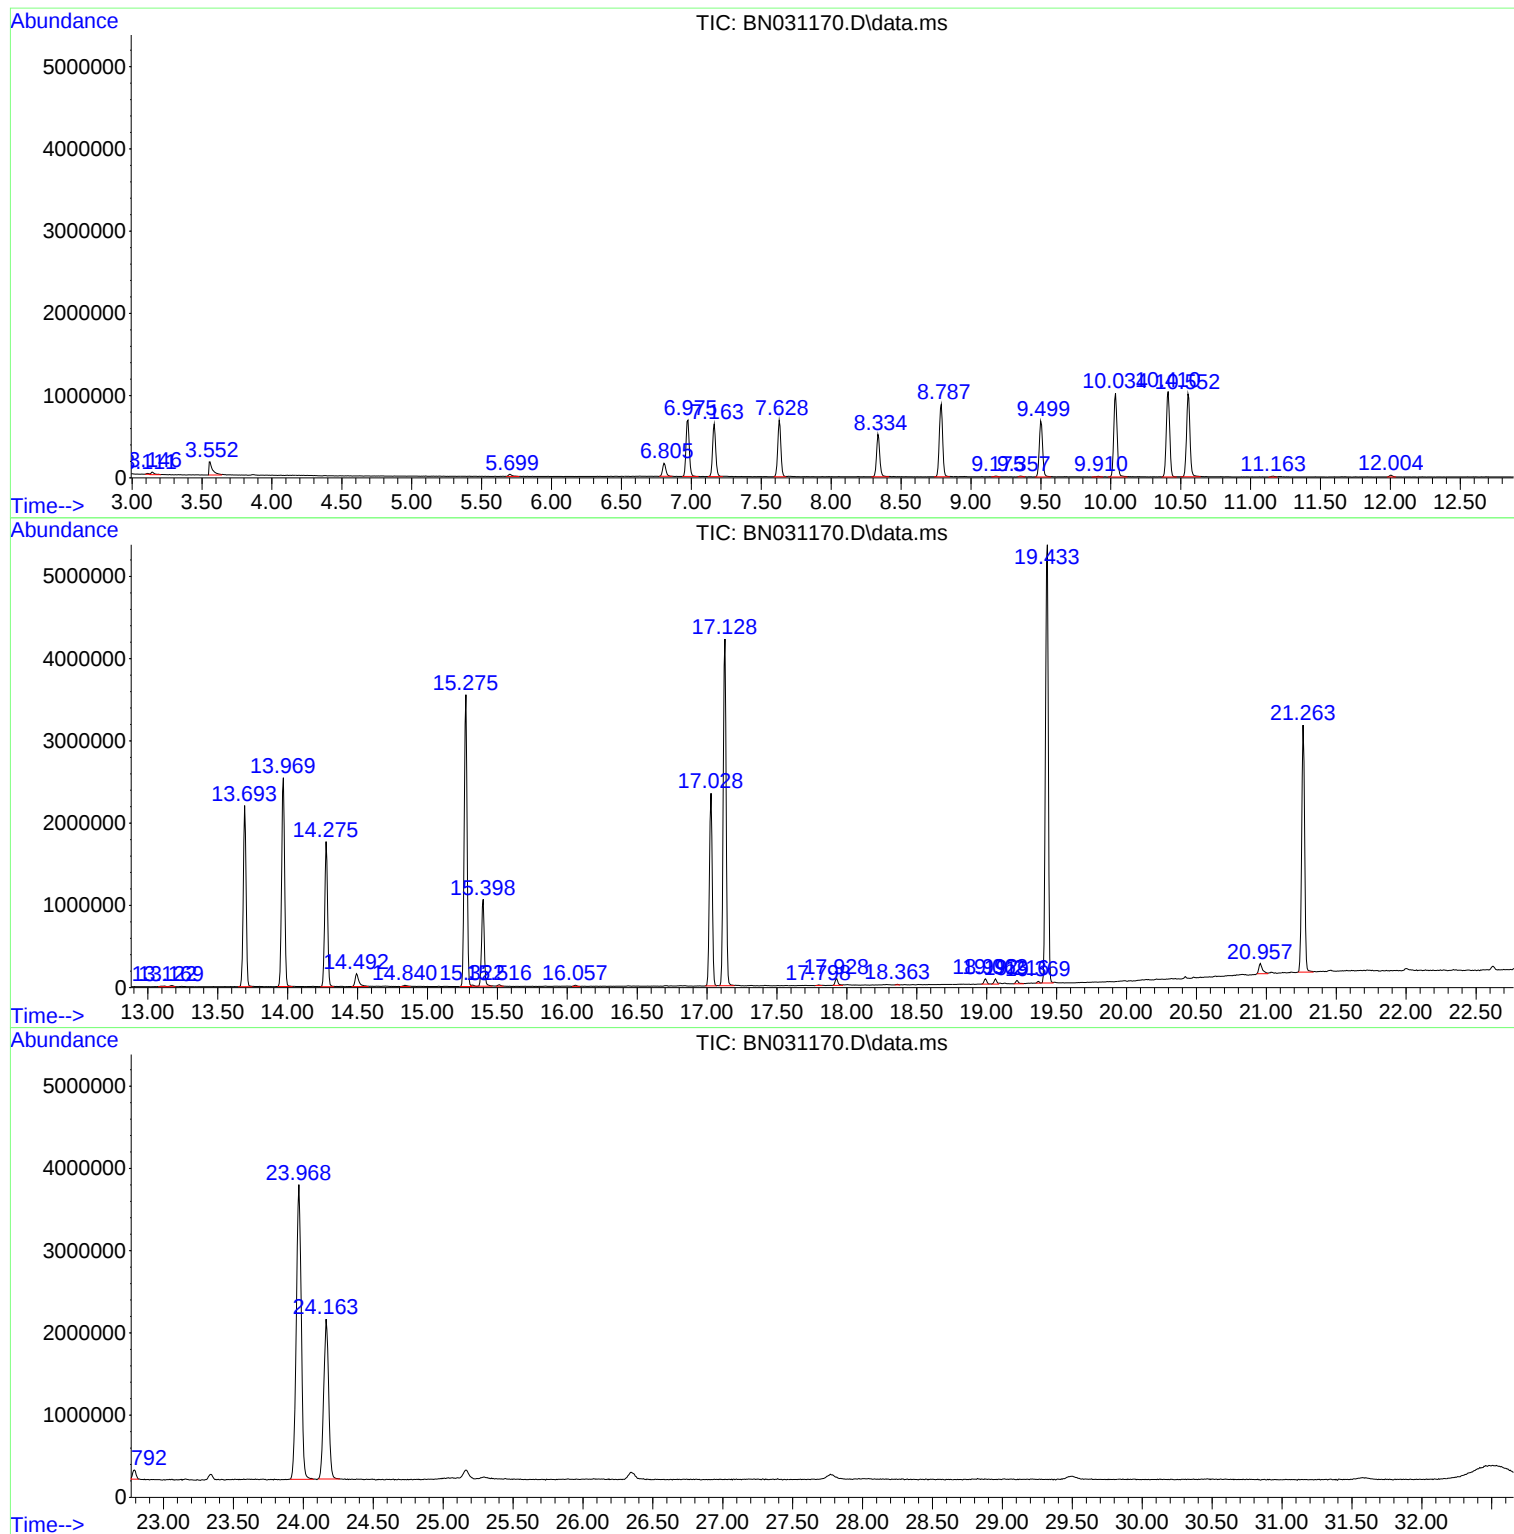

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031170.D
Acq On : 24 Apr 2024 01:32
Operator : MA/JU
Sample : P2140-07
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSR3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031170.D
Acq On : 24 Apr 2024 01:32
Operator : MA/JU
Sample : P2140-07
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSR3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc