

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031172.D
 Acq On : 24 Apr 2024 02:52
 Operator : MA/JU
 Sample : P2140-09
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSZ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031172.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	24	27	34	rVB	30485	45879	0.46%	0.059%
2	3.552	93	96	118	rBV	253090	450344	4.53%	0.576%
3	3.864	146	149	155	rVB3	9651	15839	0.16%	0.020%
4	4.375	231	236	246	rVB	51230	89485	0.90%	0.114%
5	5.699	457	461	467	rVB4	13695	20771	0.21%	0.027%
6	6.805	643	649	658	rBV	210113	336585	3.38%	0.430%
7	6.969	671	677	689	rBV	921662	1460512	14.68%	1.867%
8	7.163	702	710	719	rBV	853635	1366683	13.74%	1.747%
9	7.628	782	789	798	rBV	855350	1323785	13.31%	1.692%
10	8.334	903	909	918	rBV	688178	1074855	10.81%	1.374%
11	8.787	978	986	995	rBV	1186004	1921735	19.32%	2.456%
12	9.499	1099	1107	1122	rBV	937434	1544015	15.52%	1.973%
13	9.904	1171	1176	1186	rVB2	20011	35152	0.35%	0.045%
14	10.034	1190	1198	1218	rBV	1333388	2296579	23.09%	2.935%
15	10.410	1254	1262	1274	rBV	1246604	2108539	21.20%	2.695%
16	10.551	1278	1286	1301	rBV	1391809	2420021	24.33%	3.093%
17	11.204	1390	1397	1404	rBV9	9359	19704	0.20%	0.025%
18	11.951	1518	1524	1529	rBV2	14012	24847	0.25%	0.032%
19	12.004	1529	1533	1539	rVB2	26595	42382	0.43%	0.054%
20	13.169	1726	1731	1737	rBV4	21577	35588	0.36%	0.045%
21	13.692	1812	1820	1827	rBV	2782071	3904334	39.25%	4.990%
22	13.969	1860	1867	1878	rBV2	3300459	4937842	49.65%	6.311%
23	14.275	1912	1919	1932	rBV	2057924	3044076	30.61%	3.891%
24	14.492	1948	1956	1970	rBV	193335	371139	3.73%	0.474%
25	14.704	1987	1992	1996	rVB7	7504	11172	0.11%	0.014%
26	15.275	2082	2089	2103	rBV	4247055	6133703	61.67%	7.839%
27	15.398	2103	2110	2125	rVV	1379646	1846211	18.56%	2.360%
28	15.516	2125	2130	2138	rVB2	23821	38797	0.39%	0.050%
29	16.057	2218	2222	2226	rVB3	15259	19966	0.20%	0.026%
30	16.704	2327	2332	2336	rBV7	9460	14483	0.15%	0.019%
31	16.816	2347	2351	2353	rVV4	7812	10593	0.11%	0.014%
32	17.028	2381	2387	2397	rBV	2883822	3962977	39.84%	5.065%
33	17.128	2397	2404	2416	rVV2	4749191	6961387	69.99%	8.897%
34	17.922	2534	2539	2546	rBV	52061	77165	0.78%	0.099%
35	18.269	2592	2598	2599	rBV5	8527	15010	0.15%	0.019%
36	18.992	2716	2721	2726	rBV	74118	106037	1.07%	0.136%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031172.D
Acq On : 24 Apr 2024 02:52
Operator : MA/JU
Sample : P2140-09
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSZ2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION

37	19.063	2728	2733	2737	rBV	68636	98404	0.99%	0.126%
38	19.216	2755	2759	2767	rBV3	59251	81216	0.82%	0.104%
39	19.369	2781	2785	2789	rBV3	27208	33279	0.33%	0.043%
40	19.433	2789	2796	2803	rBV2	6059425	8778604	88.26%	11.220%
41	20.422	2962	2964	2967	rVB2	21168	14584	0.15%	0.019%
42	21.263	3101	3107	3119	rBV	3579005	5051970	50.79%	6.457%
43	23.333	3455	3459	3467	rVB2	103755	197656	1.99%	0.253%
44	23.974	3557	3568	3585	rVB2	3986646	9946109	100.00%	12.712%
45	24.168	3591	3601	3612	rVB	2315514	5580051	56.10%	7.132%
46	25.162	3765	3770	3780	rVB2	152691	373638	3.76%	0.478%




Sum of corrected areas: 78243703

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031172.D
Acq On : 24 Apr 2024 02:52
Operator : MA/JU
Sample : P2140-09
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSZ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

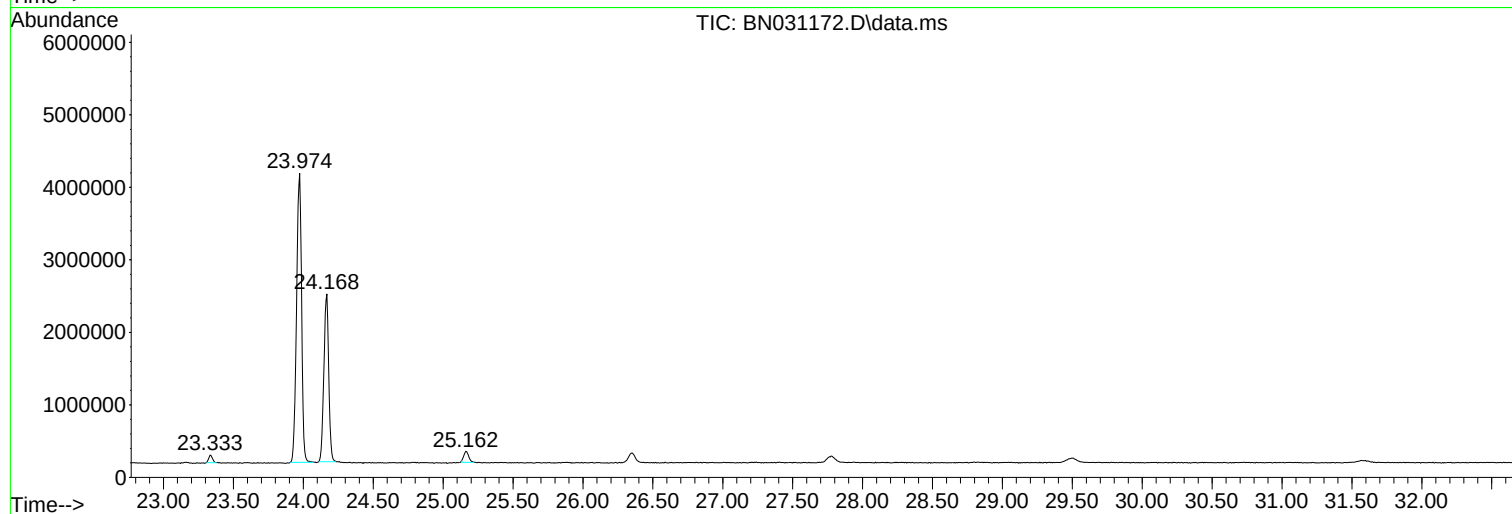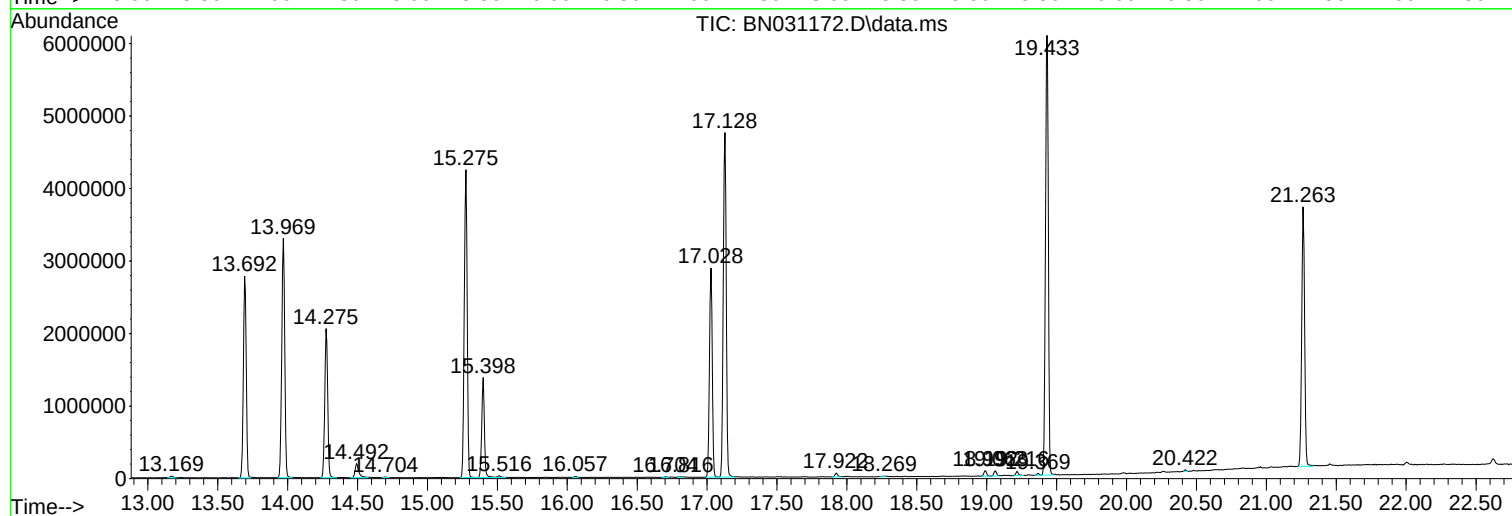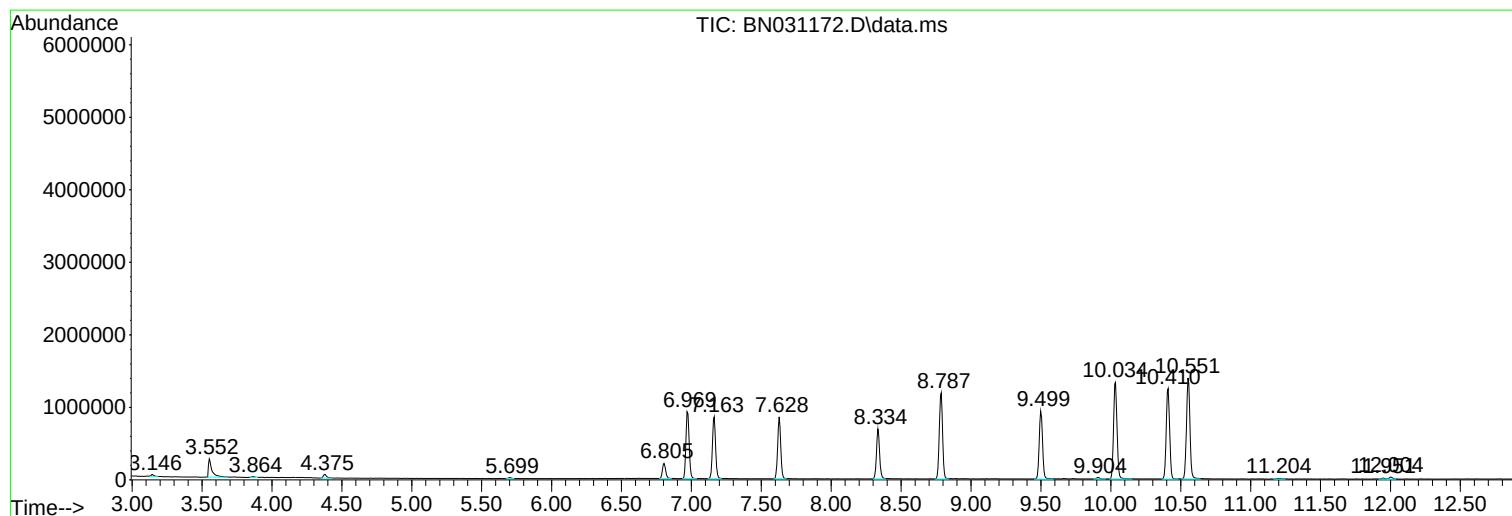

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031172.D
Acq On : 24 Apr 2024 02:52
Operator : MA/JU
Sample : P2140-09
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSZ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031172.D
Acq On : 24 Apr 2024 02:52
Operator : MA/JU
Sample : P2140-09
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSZ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc