

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031173.D
Acq On : 24 Apr 2024 03:32
Operator : MA/JU
Sample : P2140-10
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION

Signal : TIC: BN031173.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	18	22	24	rBV4	6366	10022	0.12%	0.017%
2	3.140	24	26	40	rVB	24069	42758	0.50%	0.072%
3	3.552	94	96	109	rBV	151629	272250	3.18%	0.457%
4	3.858	146	148	152	rVB4	7083	9004	0.11%	0.015%
5	4.381	232	237	242	rBV5	15736	26559	0.31%	0.045%
6	5.705	455	462	467	rBV8	8984	17800	0.21%	0.030%
7	6.805	643	649	656	rBV	159586	254221	2.97%	0.427%
8	6.969	668	677	689	rBV	641929	1055453	12.31%	1.773%
9	7.163	703	710	719	rBV	623214	998512	11.65%	1.677%
10	7.628	782	789	798	rBV	624099	992893	11.58%	1.668%
11	8.334	902	909	918	rBV	474464	752551	8.78%	1.264%
12	8.787	977	986	997	rBV	825883	1357088	15.83%	2.279%
13	9.175	1047	1052	1057	rBV7	4738	9937	0.12%	0.017%
14	9.499	1100	1107	1118	rBV	651878	1056158	12.32%	1.774%
15	9.910	1171	1177	1182	rBV	21913	36417	0.42%	0.061%
16	10.034	1190	1198	1208	rBV	971408	1626009	18.97%	2.731%
17	10.410	1254	1262	1273	rVB	933734	1573552	18.36%	2.643%
18	10.552	1277	1286	1303	rBV	941272	1629929	19.02%	2.738%
19	11.199	1393	1396	1402	rVB6	6765	10826	0.13%	0.018%
20	12.004	1529	1533	1539	rVB	20028	29708	0.35%	0.050%
21	13.175	1724	1732	1738	rBV3	16110	26727	0.31%	0.045%
22	13.693	1811	1820	1832	rBV	2025501	2708241	31.60%	4.549%
23	13.969	1858	1867	1879	rBV	2368291	3440410	40.14%	5.779%
24	14.275	1912	1919	1932	rBV	1548723	2276971	26.57%	3.825%
25	14.492	1949	1956	1975	rBV	140094	297340	3.47%	0.499%
26	14.704	1988	1992	1998	rVB8	7623	12329	0.14%	0.021%
27	15.275	2082	2089	2100	rBV	3064347	4335058	50.58%	7.282%
28	15.398	2104	2110	2125	rVV	867942	1207030	14.08%	2.027%
29	15.510	2125	2129	2136	rVB3	15847	23839	0.28%	0.040%
30	16.057	2219	2222	2226	rVB4	11315	15101	0.18%	0.025%
31	17.028	2380	2387	2397	rBV	2200947	3014376	35.17%	5.063%
32	17.128	2397	2404	2415	rVV2	3642869	5157491	60.18%	8.663%
33	17.822	2516	2522	2526	rBV	9335	15729	0.18%	0.026%
34	17.928	2535	2540	2547	rBV3	79072	113849	1.33%	0.191%
35	17.992	2549	2551	2557	rVB3	5559	9928	0.12%	0.017%
36	18.192	2581	2585	2592	rBV	53099	70879	0.83%	0.119%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031173.D
Acq On : 24 Apr 2024 03:32
Operator : MA/JU
Sample : P2140-10
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION

37	18.992	2716	2721	2726	rVB	53398	69304	0.81%	0.116%
38	19.063	2728	2733	2737	rBV	52910	72617	0.85%	0.122%
39	19.151	2745	2748	2755	rVB	29700	35598	0.42%	0.060%
40	19.216	2755	2759	2767	rBV3	59848	84439	0.99%	0.142%
41	19.298	2770	2773	2776	rBV4	8783	12571	0.15%	0.021%
42	19.369	2782	2785	2789	rBV3	17400	20945	0.24%	0.035%
43	19.433	2789	2796	2802	rBV	4868411	6858416	80.02%	11.520%
44	20.263	2934	2937	2941	rBV	52228	63682	0.74%	0.107%
45	21.263	3101	3107	3116	rBV2	2917531	4271436	49.84%	7.175%
46	23.974	3557	3568	3578	rBV3	3426024	8570689	100.00%	14.396%
47	24.163	3591	3600	3617	rVB	2009867	4988241	58.20%	8.379%




Sum of corrected areas: 59534883

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031173.D
Acq On : 24 Apr 2024 03:32
Operator : MA/JU
Sample : P2140-10
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSZ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

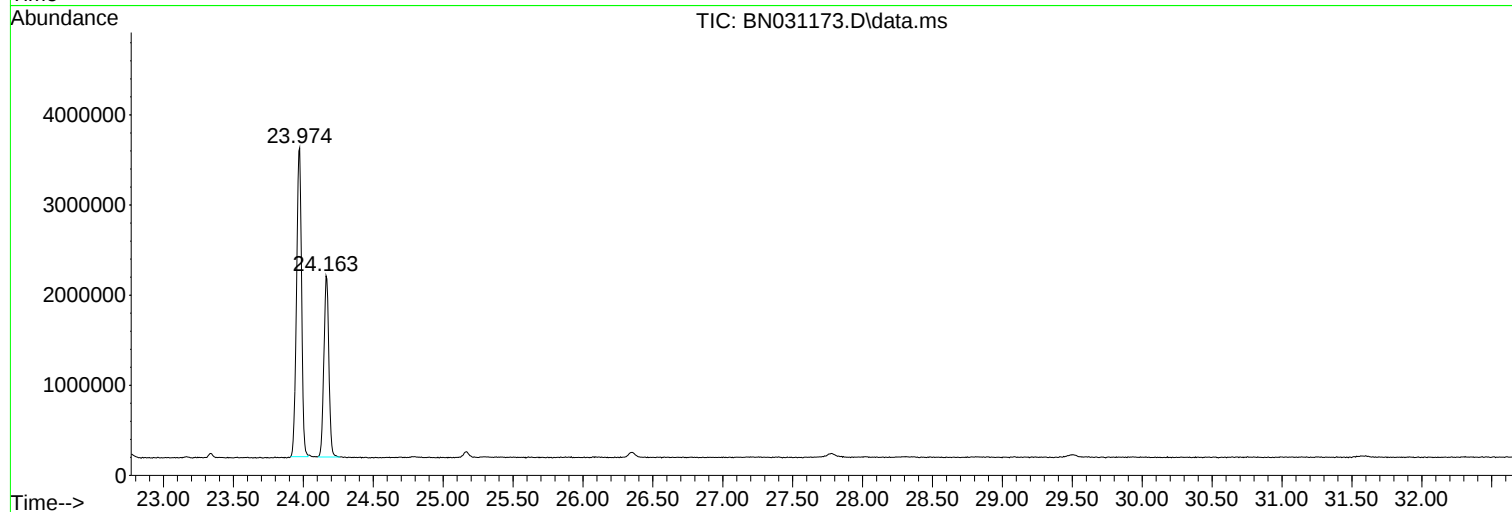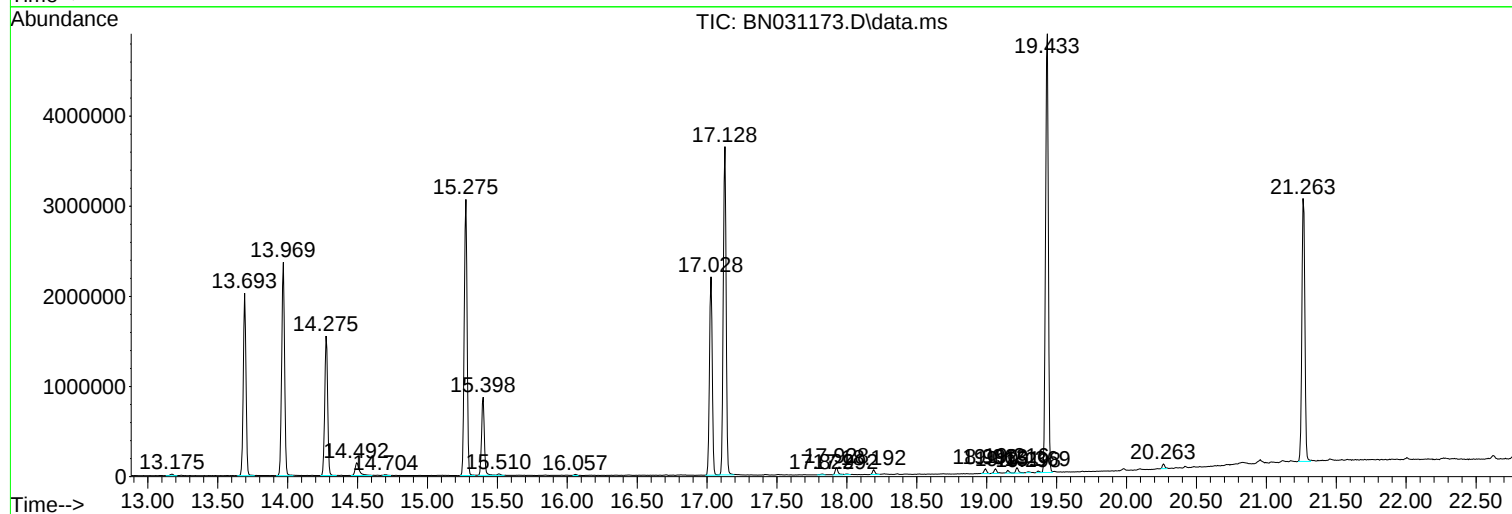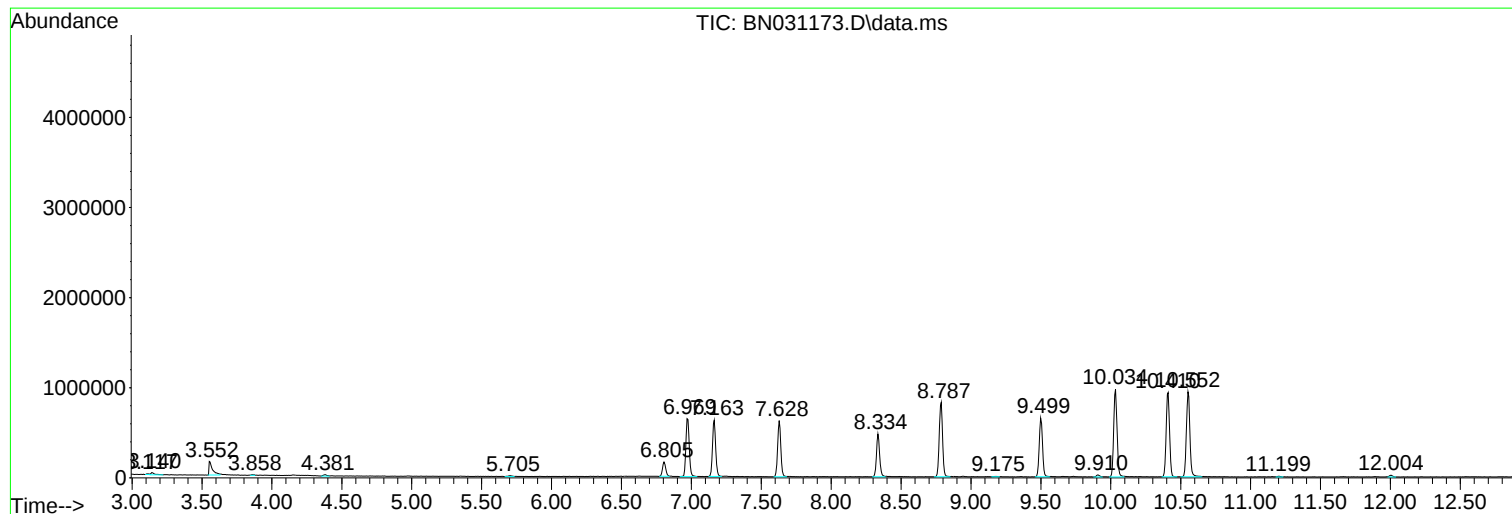

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031173.D
Acq On : 24 Apr 2024 03:32
Operator : MA/JU
Sample : P2140-10
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSZ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031173.D
Acq On : 24 Apr 2024 03:32
Operator : MA/JU
Sample : P2140-10
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSZ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
