

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031178.D
 Acq On : 24 Apr 2024 07:29
 Operator : MA/JU
 Sample : PB160407BL
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK407

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031178.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	23	26	36	rBV	30676	43842	0.78%	0.088%
2	3.546	93	95	119	rVV	434651	808652	14.38%	1.622%
3	3.864	144	149	155	rBV2	9888	17443	0.31%	0.035%
4	6.805	642	649	659	rBV	673441	1055483	18.77%	2.117%
5	6.969	671	677	690	rVB	538703	833211	14.81%	1.672%
6	7.163	702	710	720	rBV	667203	1082576	19.25%	2.172%
7	7.628	782	789	797	rBV	559868	892028	15.86%	1.790%
8	8.334	903	909	919	rBV	869817	1377423	24.49%	2.763%
9	8.781	978	985	993	rBV	648114	1068008	18.99%	2.143%
10	9.499	1100	1107	1120	rBV	551364	898548	15.98%	1.803%
11	10.034	1191	1198	1210	rBV	850574	1455186	25.87%	2.919%
12	10.410	1253	1262	1271	rBV	840734	1421814	25.28%	2.852%
13	10.551	1278	1286	1299	rBV	851452	1448270	25.75%	2.906%
14	12.004	1524	1533	1540	rVB3	15204	27433	0.49%	0.055%
15	13.169	1726	1731	1735	rBV5	11668	19422	0.35%	0.039%
16	13.692	1813	1820	1826	rBV	1666769	2216636	39.41%	4.447%
17	13.969	1860	1867	1879	rBV	1834735	2773963	49.32%	5.565%
18	14.275	1912	1919	1928	rBV	1429713	2071550	36.83%	4.156%
19	14.492	1950	1956	1978	rBV	681580	1210155	21.52%	2.428%
20	14.687	1987	1989	1994	rVB5	4655	7059	0.13%	0.014%
21	15.275	2082	2089	2097	rBV	2441758	3498053	62.20%	7.018%
22	15.398	2104	2110	2125	rBV	673504	956498	17.01%	1.919%
23	15.516	2125	2130	2133	rVB5	10434	15866	0.28%	0.032%
24	16.063	2217	2223	2228	rBV7	7371	13176	0.23%	0.026%
25	16.704	2329	2332	2337	rBV6	5601	8244	0.15%	0.017%
26	17.028	2380	2387	2397	rBV	1939228	2690716	47.84%	5.398%
27	17.122	2397	2403	2418	rVV	2745624	4047351	71.96%	8.120%
28	17.933	2537	2541	2543	rBV5	4366	5687	0.10%	0.011%
29	18.257	2593	2596	2600	rBV6	4232	6172	0.11%	0.012%
30	18.992	2716	2721	2725	rBV	36869	49684	0.88%	0.100%
31	19.063	2729	2733	2740	rVV	32115	45000	0.80%	0.090%
32	19.210	2754	2758	2760	rBV5	7078	11044	0.20%	0.022%
33	19.369	2782	2785	2789	rBV6	9833	12869	0.23%	0.026%
34	19.427	2789	2795	2802	rBV2	3865074	5164936	91.83%	10.362%
35	21.263	3101	3107	3115	rBV	2359244	3416662	60.75%	6.854%
36	23.963	3557	3566	3578	rBV2	2331100	5624257	100.00%	11.283%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031178.D
Acq On : 24 Apr 2024 07:29
Operator : MA/JU
Sample : PB160407BL
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK407

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION

37 24.163 3591 3600 3610 rBV 1477161 3550801 63.13% 7.124%




Sum of corrected areas: 49845718

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031178.D
Acq On : 24 Apr 2024 07:29
Operator : MA/JU
Sample : PB160407BL
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK407

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

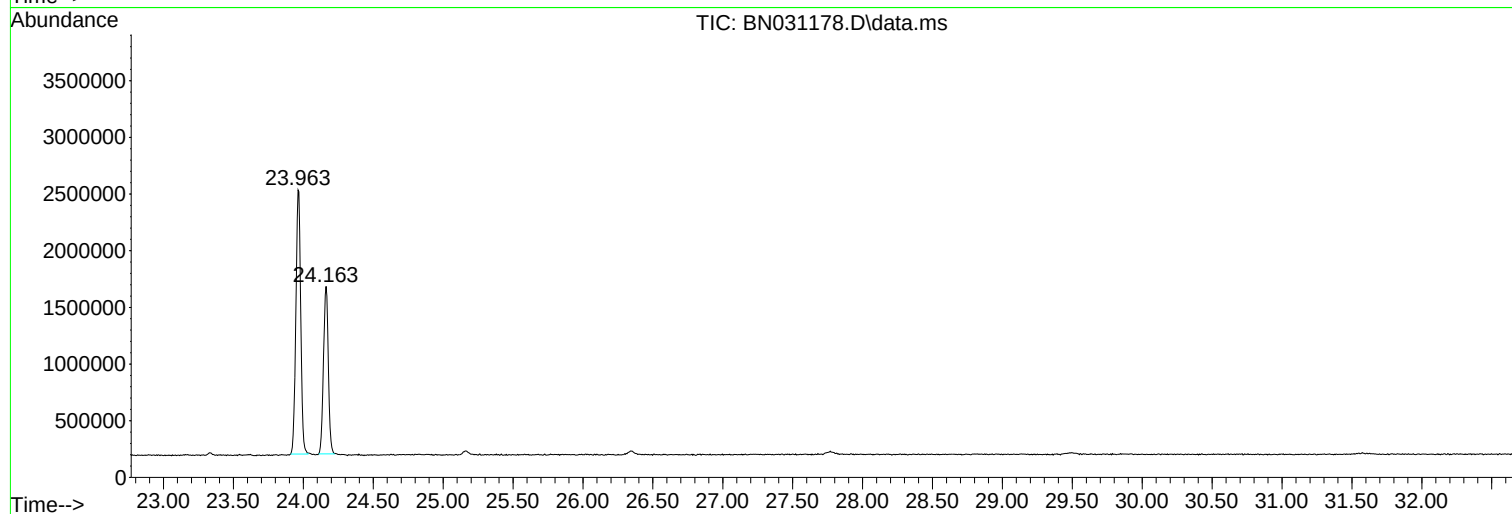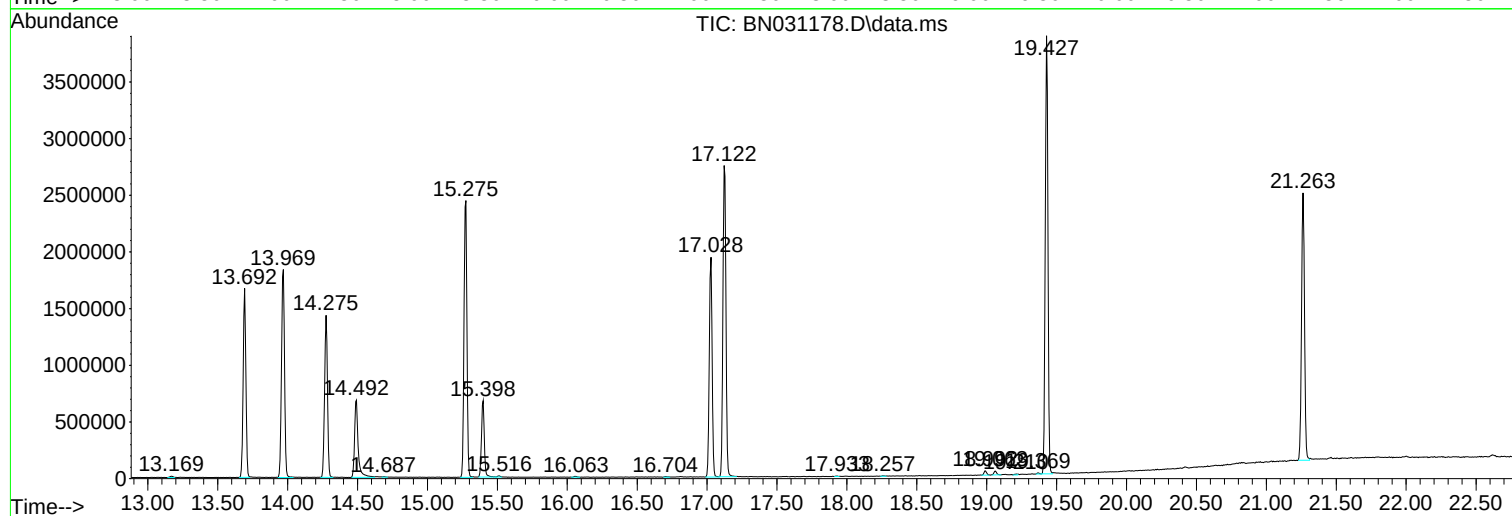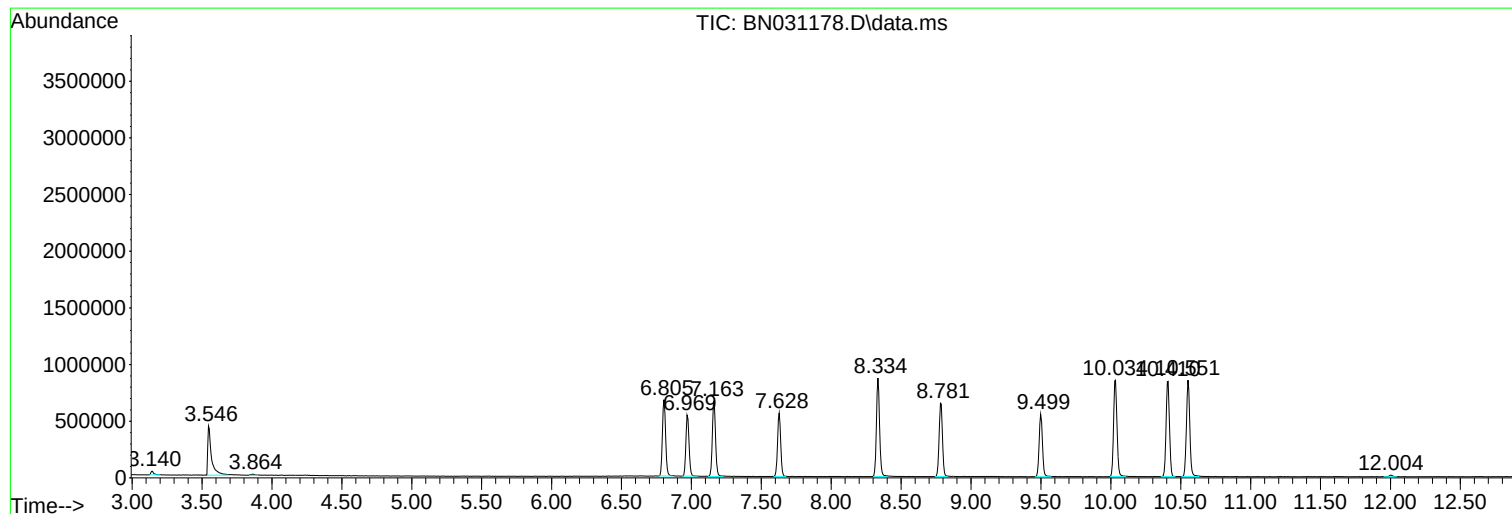

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031178.D
Acq On : 24 Apr 2024 07:29
Operator : MA/JU
Sample : PB160407BL
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK407

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031178.D
Acq On : 24 Apr 2024 07:29
Operator : MA/JU
Sample : PB160407BL
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK407

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc