

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031182.D
 Acq On : 24 Apr 2024 10:07
 Operator : MA/JU
 Sample : P2141-03
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031182.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.111	17	21	43	rVB2	160175	315341	4.69%	0.650%
2	3.558	95	97	115	rBV	136281	258474	3.85%	0.533%
3	3.869	145	150	151	rBV4	7351	9247	0.14%	0.019%
4	4.375	231	236	247	rBV	101838	169879	2.53%	0.350%
5	6.628	615	619	623	rBV4	8660	12760	0.19%	0.026%
6	6.757	636	641	644	rBV3	6828	10773	0.16%	0.022%
7	6.805	644	649	658	rVB	142971	227669	3.39%	0.469%
8	6.975	671	678	687	rBV	541614	875708	13.03%	1.805%
9	7.163	703	710	721	rBV	543730	845613	12.59%	1.743%
10	7.628	780	789	797	rBV	462688	730756	10.88%	1.506%
11	7.687	797	799	804	rVB4	4925	7739	0.12%	0.016%
12	8.334	902	909	923	rBV	443365	714688	10.64%	1.473%
13	8.787	978	986	999	rBV	677224	1136445	16.91%	2.342%
14	8.899	999	1005	1010	rVV4	10266	18632	0.28%	0.038%
15	8.946	1010	1013	1017	rVB5	7383	10180	0.15%	0.021%
16	9.181	1046	1053	1060	rVV	25402	43361	0.65%	0.089%
17	9.357	1079	1083	1087	rVB6	6001	10035	0.15%	0.021%
18	9.498	1099	1107	1116	rBV	536681	879599	13.09%	1.813%
19	9.734	1142	1147	1153	rBV4	10193	16893	0.25%	0.035%
20	10.034	1191	1198	1216	rBV	812787	1380117	20.54%	2.844%
21	10.404	1255	1261	1271	rVB	691295	1166027	17.35%	2.403%
22	10.551	1278	1286	1298	rBV	706940	1232566	18.34%	2.540%
23	11.198	1393	1396	1404	rVB7	6895	13987	0.21%	0.029%
24	11.669	1471	1476	1480	rVB	23358	34482	0.51%	0.071%
25	12.004	1528	1533	1540	rBV2	15120	26006	0.39%	0.054%
26	13.169	1725	1731	1737	rBV3	14542	22589	0.34%	0.047%
27	13.692	1812	1820	1828	rBV	1786878	2406039	35.81%	4.959%
28	13.969	1860	1867	1879	rVB	1955872	2908507	43.29%	5.994%
29	14.275	1912	1919	1927	rBV	1178142	1685770	25.09%	3.474%
30	14.492	1951	1956	1968	rBV	119278	242750	3.61%	0.500%
31	15.110	2058	2061	2070	rVB6	4539	8756	0.13%	0.018%
32	15.275	2080	2089	2096	rBV	2552661	3742861	55.70%	7.714%
33	15.398	2104	2110	2120	rBV	705852	993892	14.79%	2.048%
34	15.516	2125	2130	2134	rVB3	15047	22672	0.34%	0.047%
35	16.051	2219	2221	2226	rVB5	6367	9070	0.13%	0.019%
36	16.951	2369	2374	2378	rBV4	15939	19413	0.29%	0.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
 Data File : BN031182.D
 Acq On : 24 Apr 2024 10:07
 Operator : MA/JU
 Sample : P2141-03
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

37	17.028	2380	2387	2397	rBV	1558638	2206806	32.84%	4.548%
38	17.127	2397	2404	2416	rBV2	3086128	4506611	67.07%	9.288%
39	17.422	2449	2454	2455	rBV5	6494	9358	0.14%	0.019%
40	17.698	2496	2501	2510	rVB2	104768	142387	2.12%	0.293%
41	17.869	2527	2530	2534	rBV3	15605	20531	0.31%	0.042%
42	17.927	2534	2540	2542	rBV	98597	145872	2.17%	0.301%
43	18.022	2553	2556	2561	rVB6	12189	15372	0.23%	0.032%
44	18.139	2571	2576	2582	rBV	137678	210445	3.13%	0.434%
45	18.257	2594	2596	2602	rVB7	6286	7162	0.11%	0.015%
46	18.798	2685	2688	2690	rBV4	6291	8882	0.13%	0.018%
47	18.992	2717	2721	2726	rVB	43964	62320	0.93%	0.128%
48	19.063	2728	2733	2736	rBV	44338	66688	0.99%	0.137%
49	19.098	2736	2739	2741	rVV4	16698	16620	0.25%	0.034%
50	19.216	2755	2759	2767	rBV2	76104	107045	1.59%	0.221%
51	19.369	2782	2785	2789	rVB	28228	28569	0.43%	0.059%
52	19.427	2789	2795	2803	rBV	4146225	5859610	87.21%	12.077%
53	20.957	3052	3055	3060	rBV2	70935	85764	1.28%	0.177%
54	21.263	3101	3107	3117	rBV	1981170	2902035	43.19%	5.981%
55	23.968	3557	3567	3580	rBV2	2808630	6719111	100.00%	13.848%
56	24.162	3591	3600	3613	rVB2	1258504	3189148	47.46%	6.573%




Sum of corrected areas: 48519632

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031182.D
Acq On : 24 Apr 2024 10:07
Operator : MA/JU
Sample : P2141-03
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSR6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

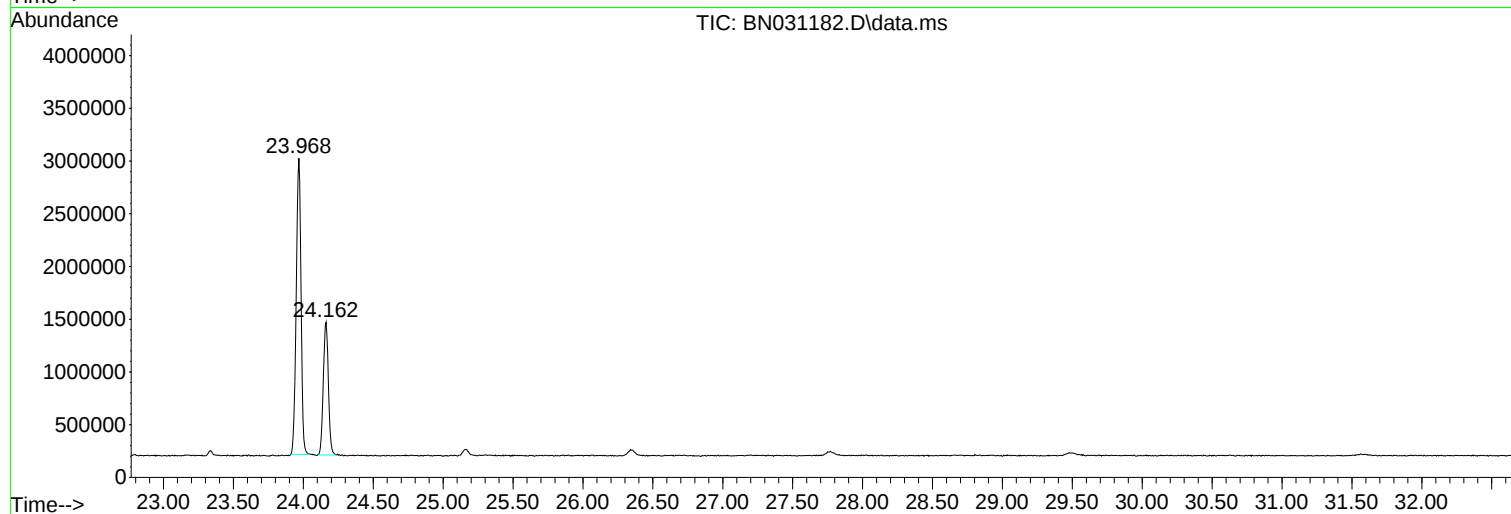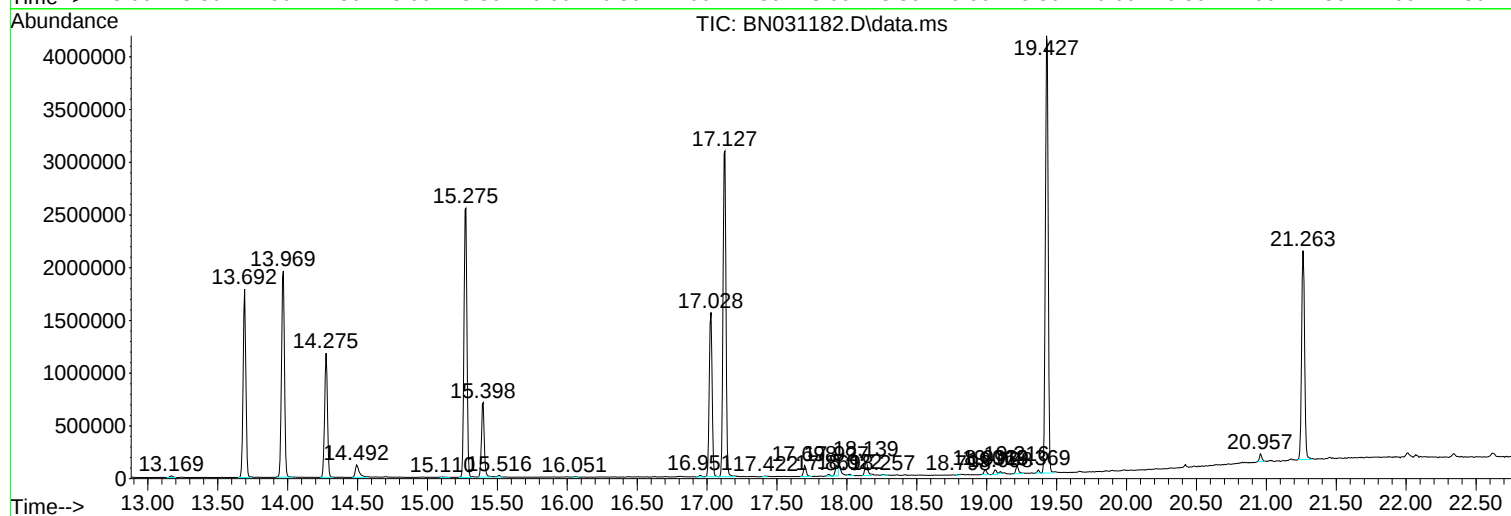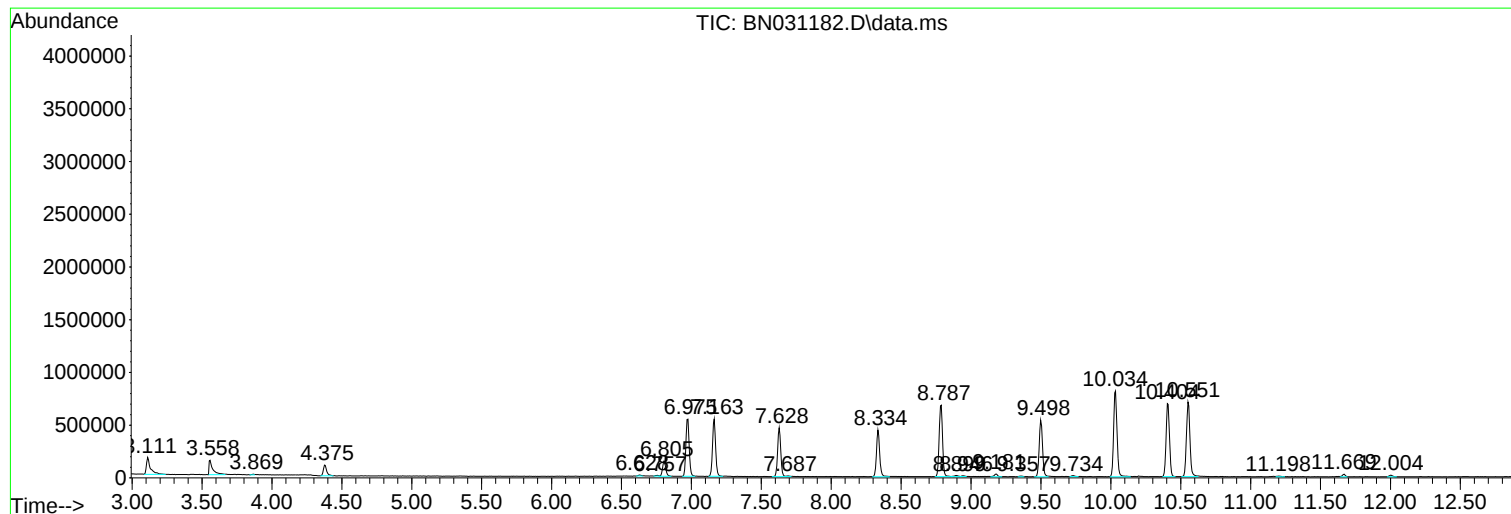

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031182.D
Acq On : 24 Apr 2024 10:07
Operator : MA/JU
Sample : P2141-03
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSR6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.375	4.65 ng/ul	169879	1,4-Dichlorobenzene-d4	7.628

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	32

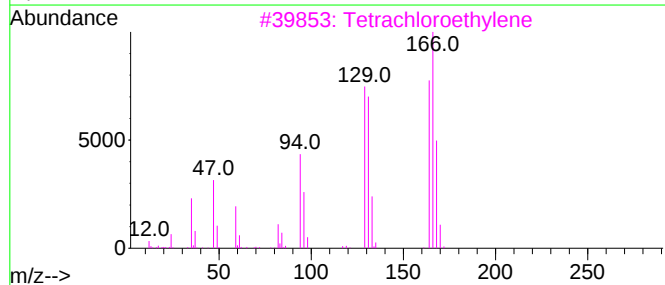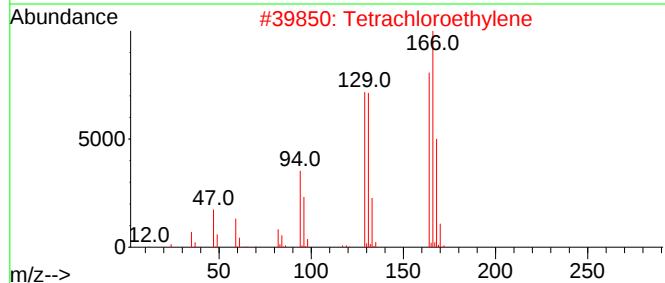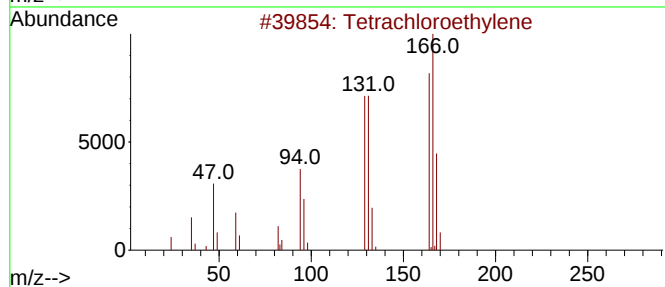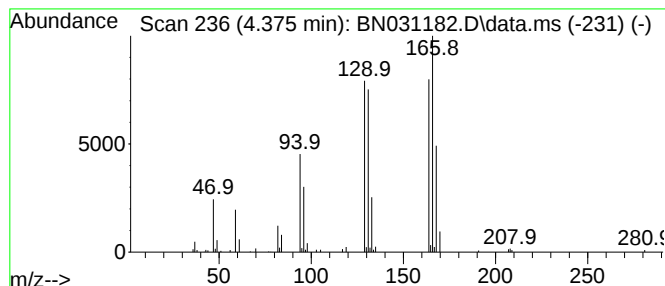

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042224\
Data File : BN031182.D
Acq On : 24 Apr 2024 10:07
Operator : MA/JU
Sample : P2141-03
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSR6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.375	4.7	ng/u1	169879	1	7.628	730756	20.0