

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042319\
 Data File : BN005217.D
 Acq On : 23 Apr 2019 16:39
 Operator : JU/SJ
 Sample : K2403-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5102

Quant Time: Apr 24 08:53:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 23 03:50:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	602498	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	2578943	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	1466973	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	3075778	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	2527205	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	2767274	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	82167	6.58	ng/uL	0.00
5) Phenol-d5	6.78	99	1069186	22.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	664311	22.50	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	850317	23.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	863865	23.35	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	412256	25.97	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	454996	28.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	847536	22.98	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	1113540	29.27	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	2525031	23.71	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	3093428	23.65	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	343326	20.42	ng/ul	0.00
57) Fluorene-d10	15.23	176	2061545	23.07	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	156813	11.34	ng/ul	0.00
70) Anthracene-d10	17.08	188	3036070	23.55	ng/ul	0.00
78) Pyrene-d10	19.40	212	3136732	24.26	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.28	264	2911877	24.08	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.70	163	716744	6.755	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042319\
Data File : BN005217.D
Acq On : 23 Apr 2019 16:39
Operator : JU/SJ
Sample : K2403-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5102

Quant Time: Apr 24 08:53:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 03:50:45 2019
Response via : Initial Calibration

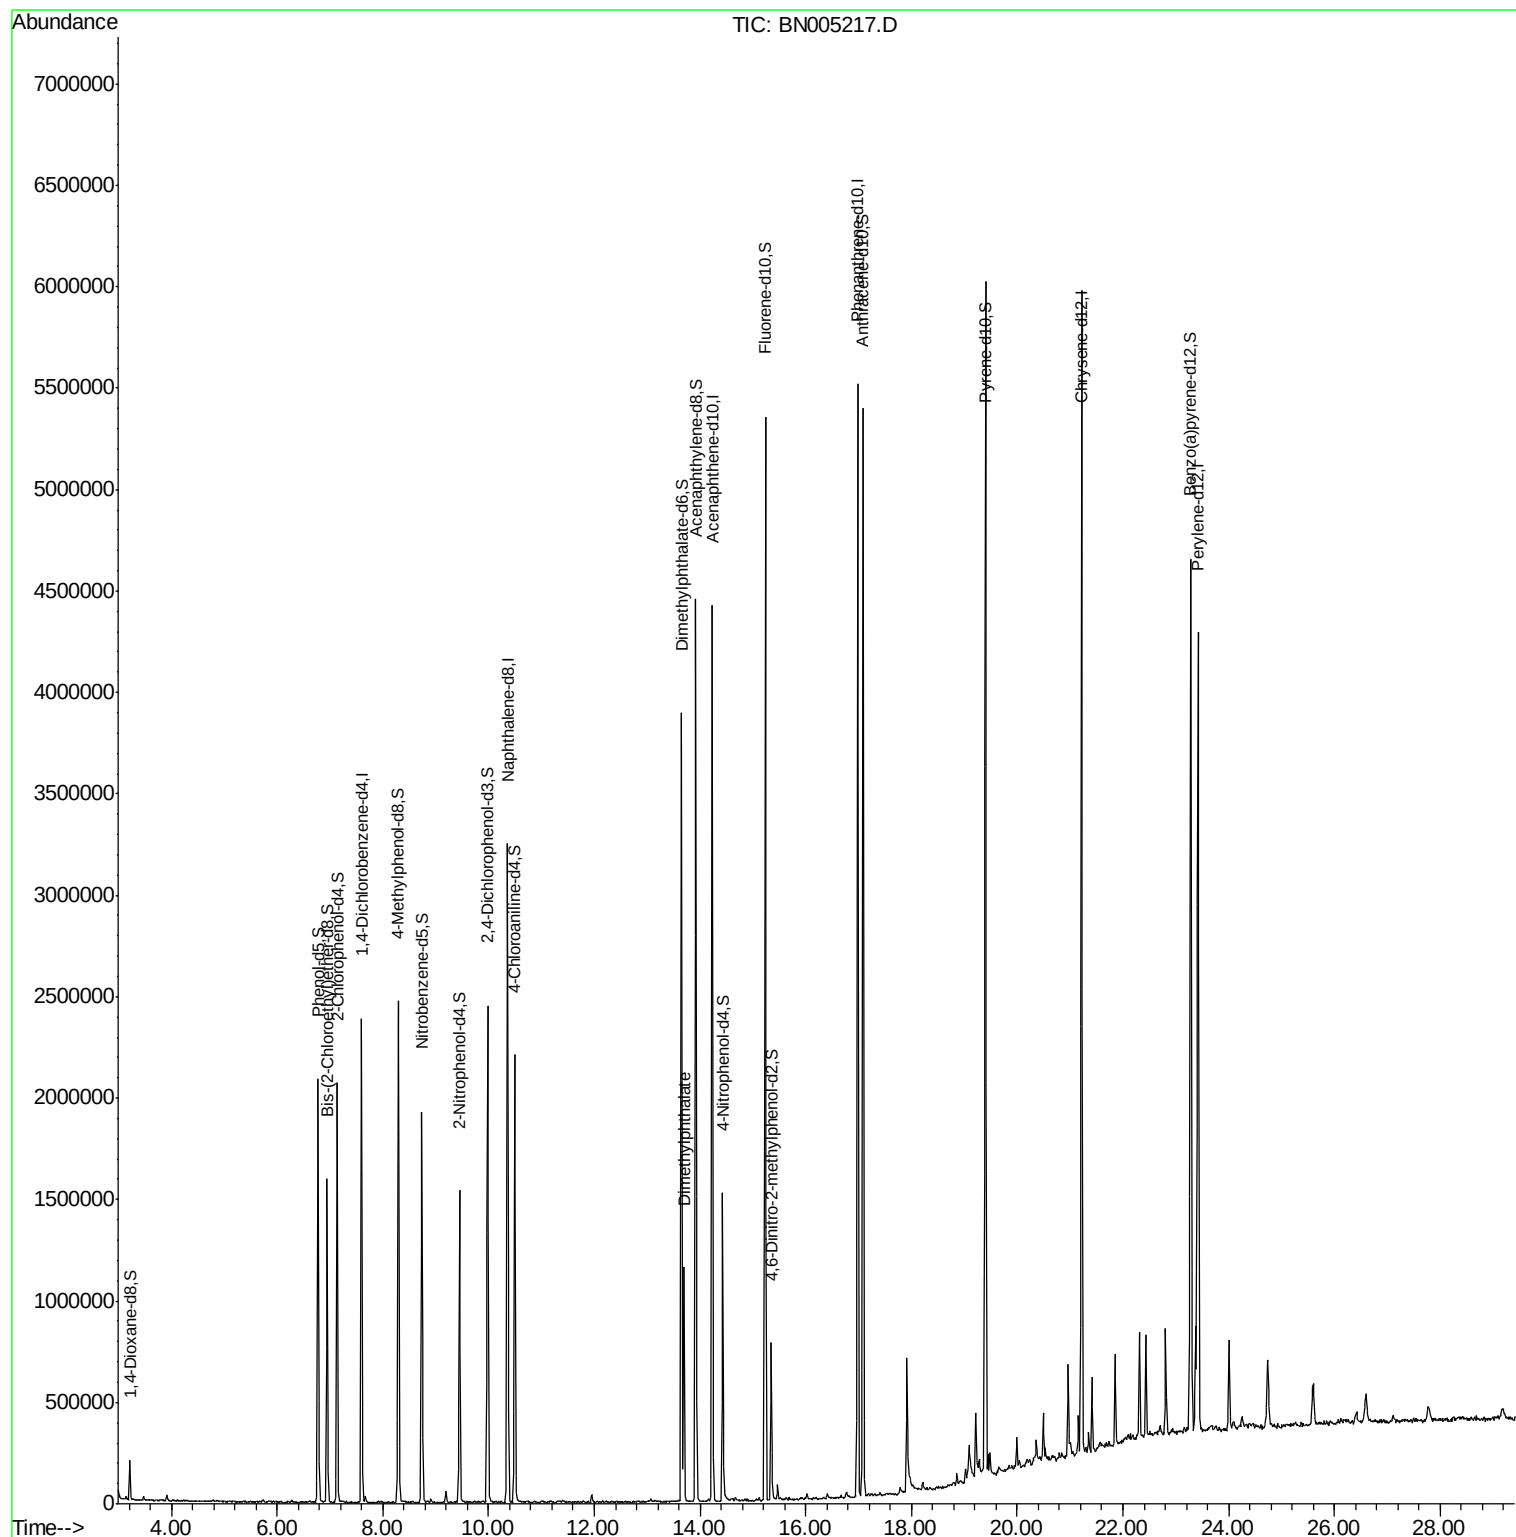

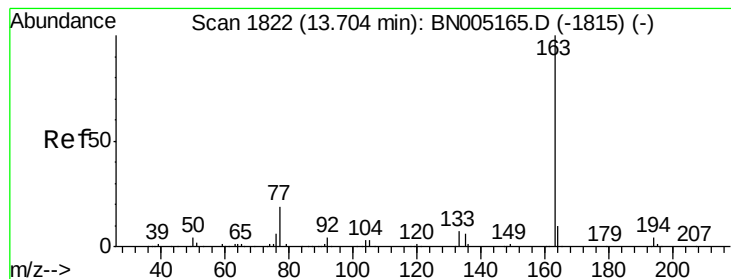

#44

Dimethylphthalate

Concen: 6.755 ng/ul

RT: 13.70 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BN005217.D

Acq: 23 Apr 2019 16:39

Instrument :

BNA_N

ClientSampleId :

A5102


Tgt Ion:163 Resp: 716744

Ion Ratio Lower Upper

163 100

194 3.9 3.4 5.0

164 9.3 8.1 12.1

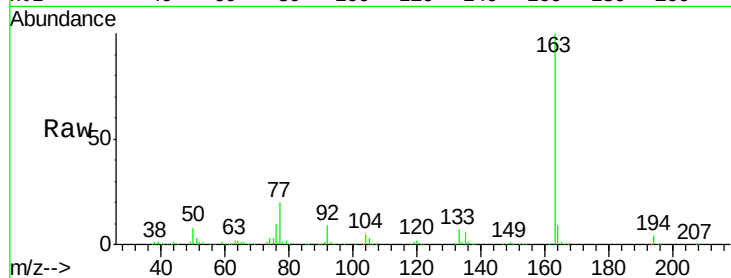

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

