
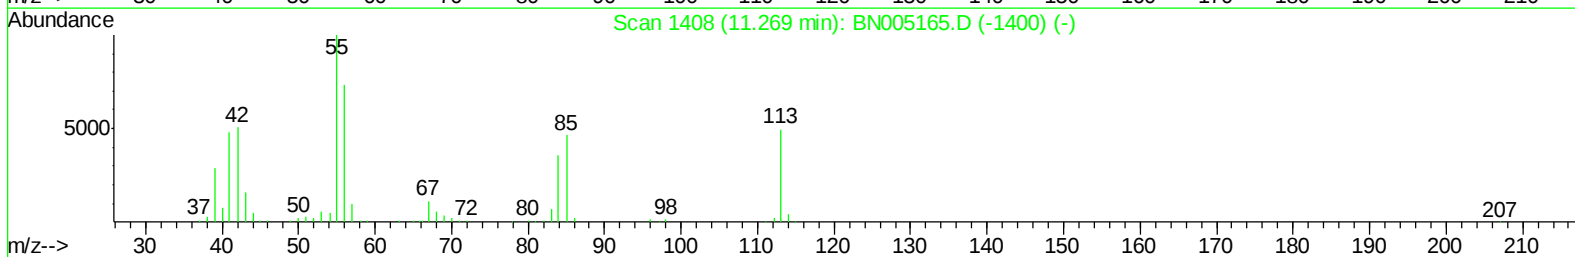
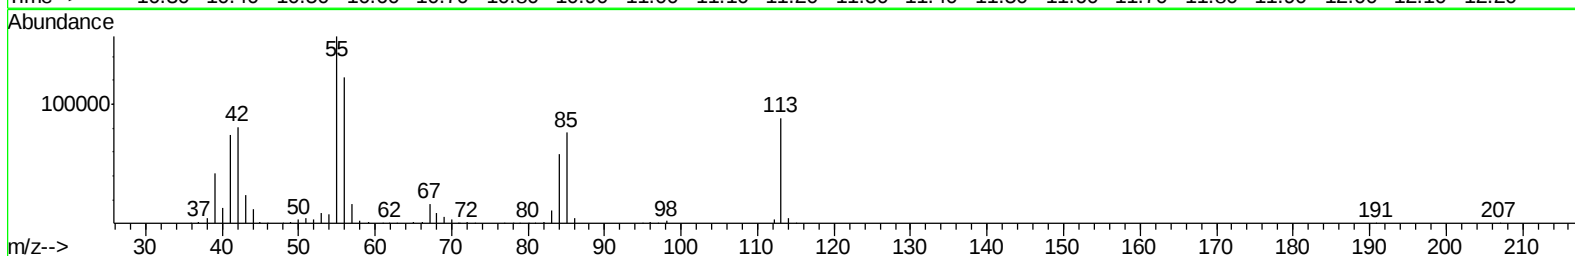


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042319\
Data File : BN005228.D
Acq On : 23 Apr 2019 23:02
Operator : JU/SJ
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP54

Quant Time: Apr 24 08:44:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 03:50:45 2019
Response via : Initial Calibration

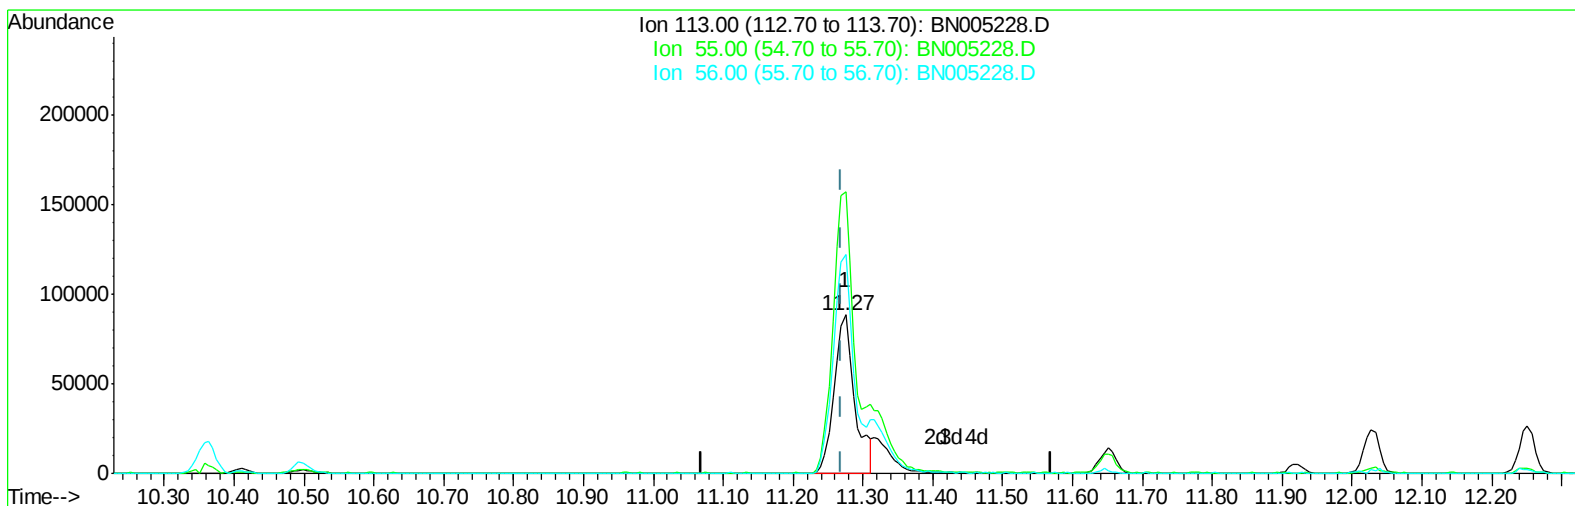

TIC: BN005228.D

(32) Caprolactam

11.275min (+0.006) 17.98ng/ul




response 179052

Ion	Exp%	Act%
113.00	100	100
55.00	196.20	177.71
56.00	148.90	138.29
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042319\
Data File : BN005228.D
Acq On : 23 Apr 2019 23:02
Operator : JU/SJ
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP54

Quant Time: Apr 24 08:44:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 03:50:45 2019
Response via : Initial Calibration

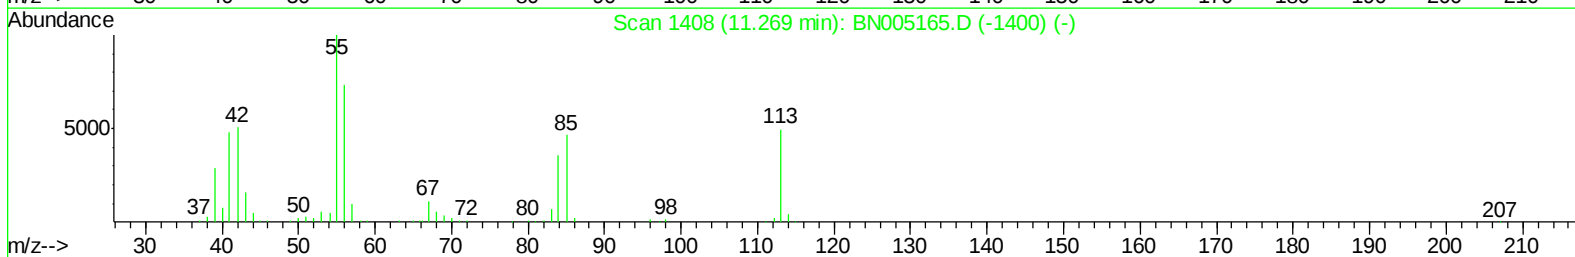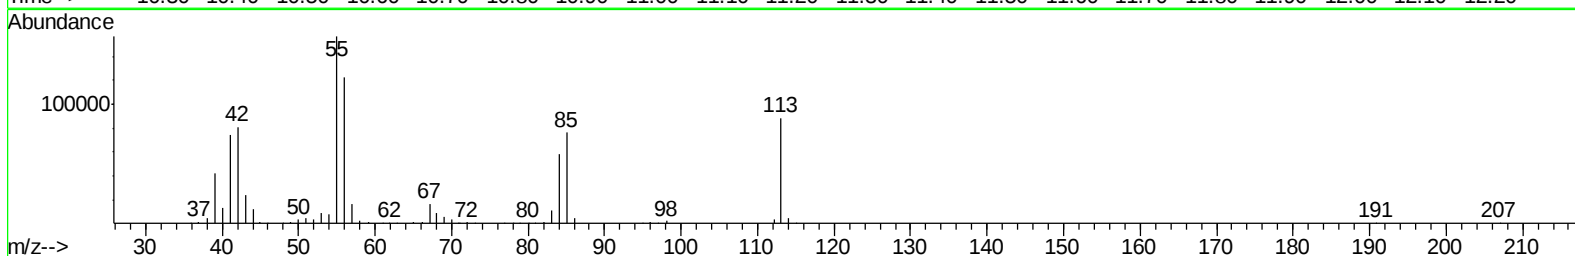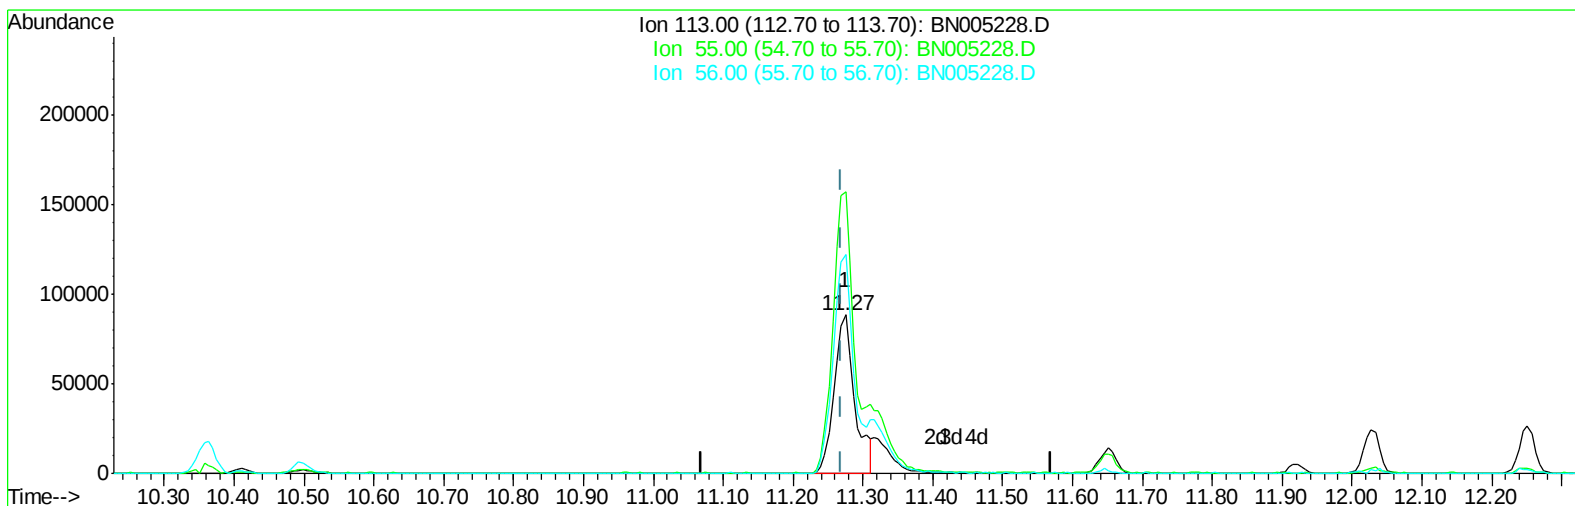

TIC: BN005228.D

(32) Caprolactam

11.275min (+0.006) 17.98ng/ul

response 179052

Ion	Exp%	Act%
113.00	100	100
55.00	196.20	177.71
56.00	148.90	138.29
0.00	0.00	0.00