

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042319\
 Data File : BN005222.D
 Acq On : 23 Apr 2019 19:32
 Operator : JU/SJ
 Sample : K2403-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5127

Quant Time: Apr 24 08:53:52 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 23 03:50:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	1145646	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	4914699	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	2771837	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	5530476	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	4350503	20.00	ng/ul	0.00
85) Perylene-d12	23.43	264	4632786	20.00	ng/ul	0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	94645	3.99	ng/uL	0.00
5) Phenol-d5	6.78	99	1267128	14.08	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	771365	13.74	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	991444	14.40	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	1029914	14.64	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	493086	16.30	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	555010	18.10	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	1021532	14.53	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	1379786	19.03	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	3128534	15.55	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	3764094	15.23	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	437621	13.77	ng/ul	0.00
57) Fluorene-d10	15.23	176	2524022	14.95	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	197900	7.96	ng/ul	0.00
70) Anthracene-d10	17.08	188	3581693	15.45	ng/ul	0.00
78) Pyrene-d10	19.40	212	3566847	16.03	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.30	264	3252821	16.07	ng/ul	0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.70	163	984111	4.908	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042319\
Data File : BN005222.D
Acq On : 23 Apr 2019 19:32
Operator : JU/SJ
Sample : K2403-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5127

Quant Time: Apr 24 08:53:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 03:50:45 2019
Response via : Initial Calibration

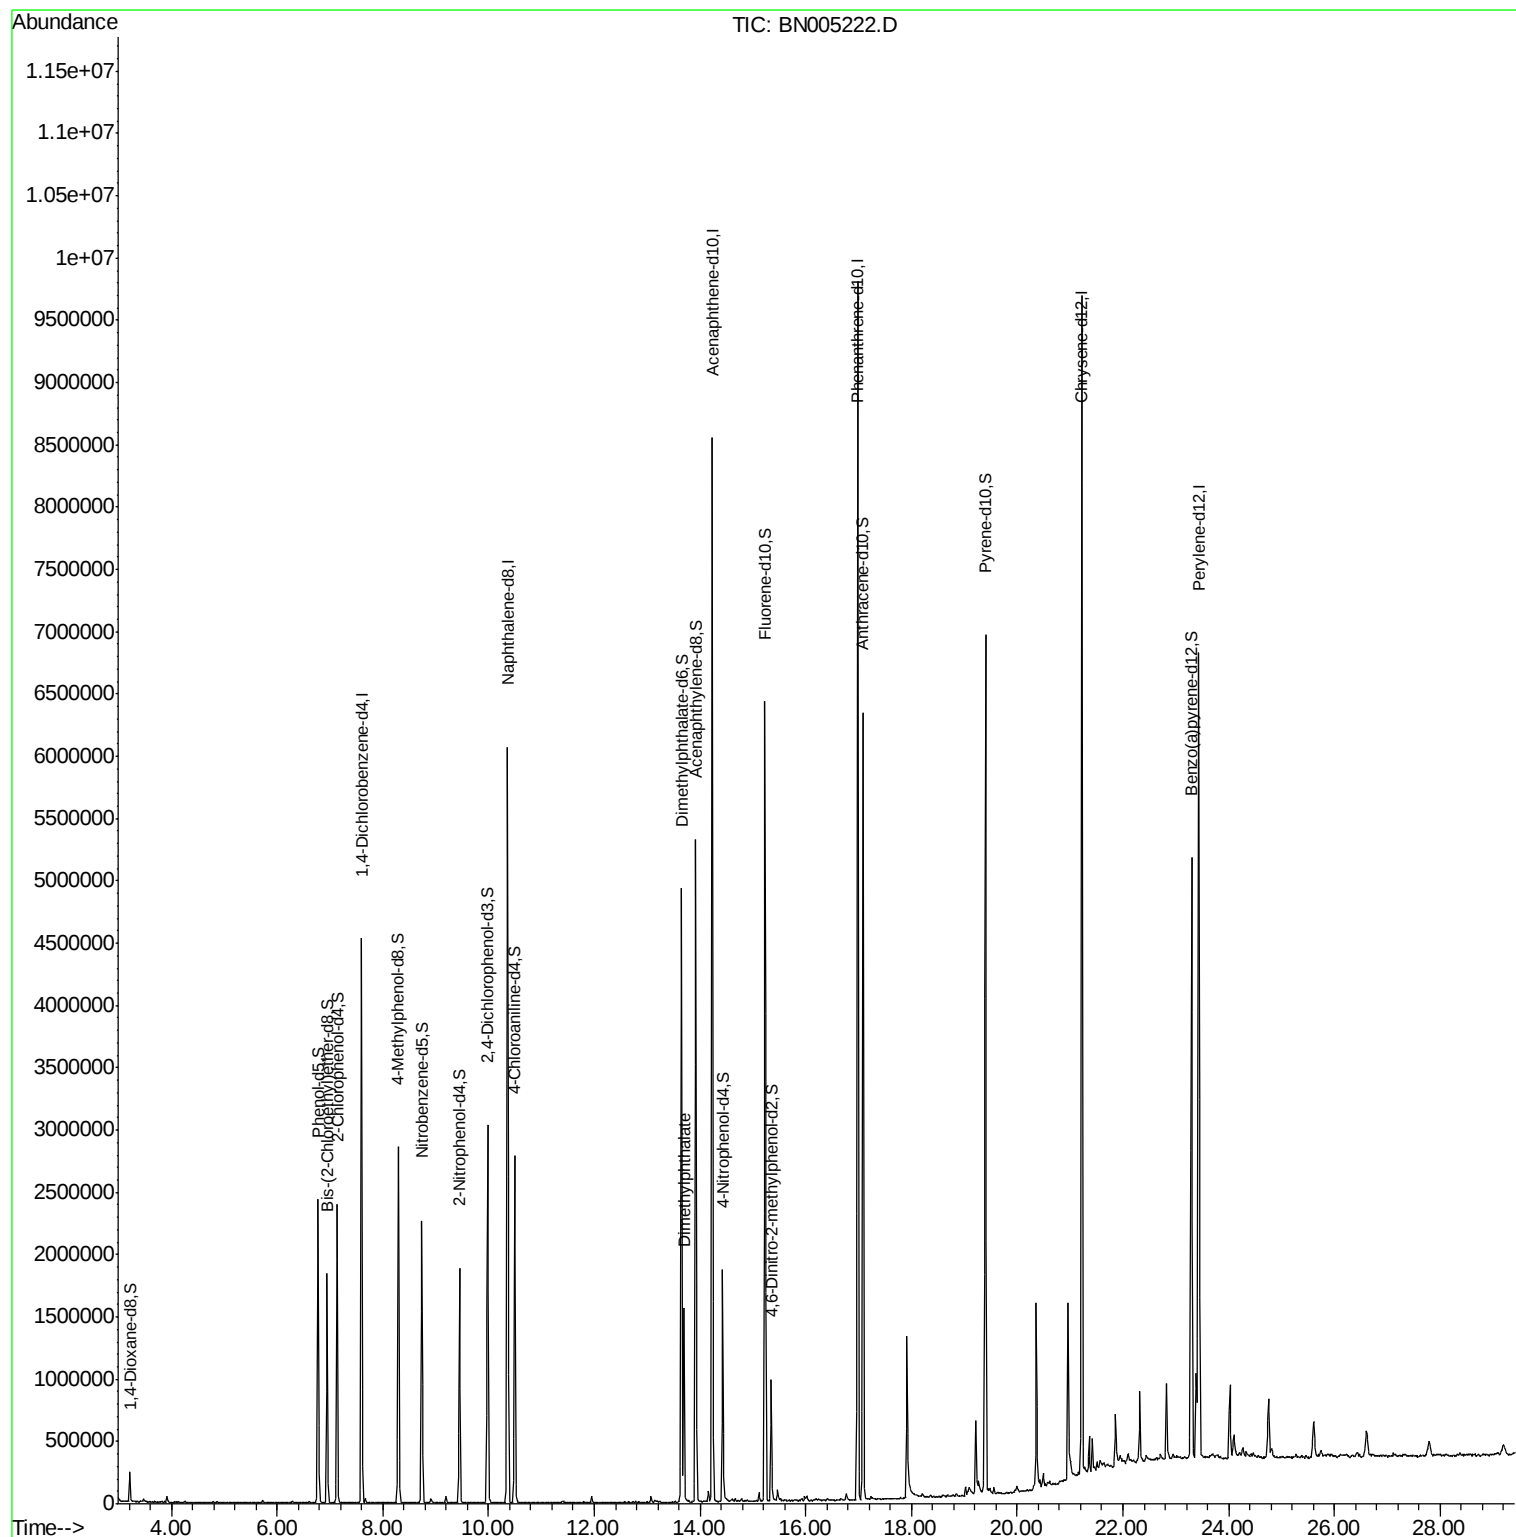


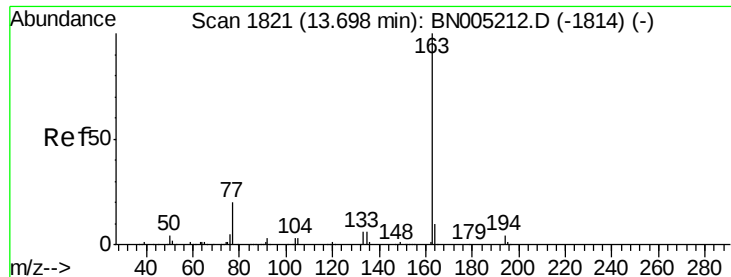

#44
 Dimethylphthalate
 Concen: 4.908 ng/ul
 RT: 13.70 min Scan# 1821
 Delta R.T. -0.01 min
 Lab File: BN005222.D
 Acq: 23 Apr 2019 19:32

Instrument :
 BNA_N
 ClientSampleId :
 A5127

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.4	3.4	5.0
164	10.4	8.1	12.1

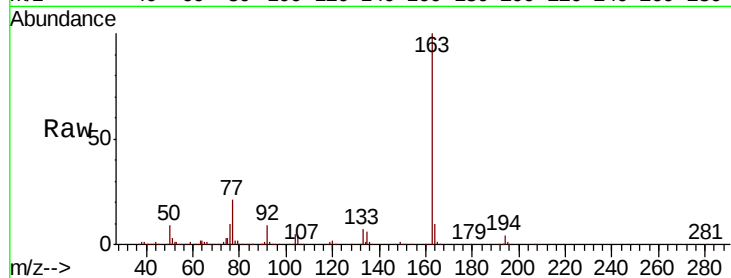

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

