

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042319\
 Data File : BN005232.D
 Acq On : 24 Apr 2019 01:56
 Operator : JU/SJ
 Sample : K2403-16
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5130

Quant Time: Apr 24 08:54:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 23 03:50:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	481385	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	2024918	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	1142787	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	2214702	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	1747115	20.00	ng/ul	0.00
85) Perylene-d12	23.41	264	1891020	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	70683	7.09	ng/uL	0.00
5) Phenol-d5	6.78	99	1016327	26.88	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	613109	26.00	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	803989	27.79	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	781520	26.44	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	384789	30.87	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	416994	33.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	836182	28.87	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	768355	25.73	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	2467008	29.74	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	2942048	28.88	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	297029	22.68	ng/ul	0.00
57) Fluorene-d10	15.23	176	1975381	28.37	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	139225	13.98	ng/ul	0.00
70) Anthracene-d10	17.08	188	2742995	29.54	ng/ul	0.00
78) Pyrene-d10	19.39	212	2701572	30.23	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.27	264	2415229	29.23	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.69	163	509885	6.168	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042319\
Data File : BN005232.D
Acq On : 24 Apr 2019 01:56
Operator : JU/SJ
Sample : K2403-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5130

Quant Time: Apr 24 08:54:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 03:50:45 2019
Response via : Initial Calibration

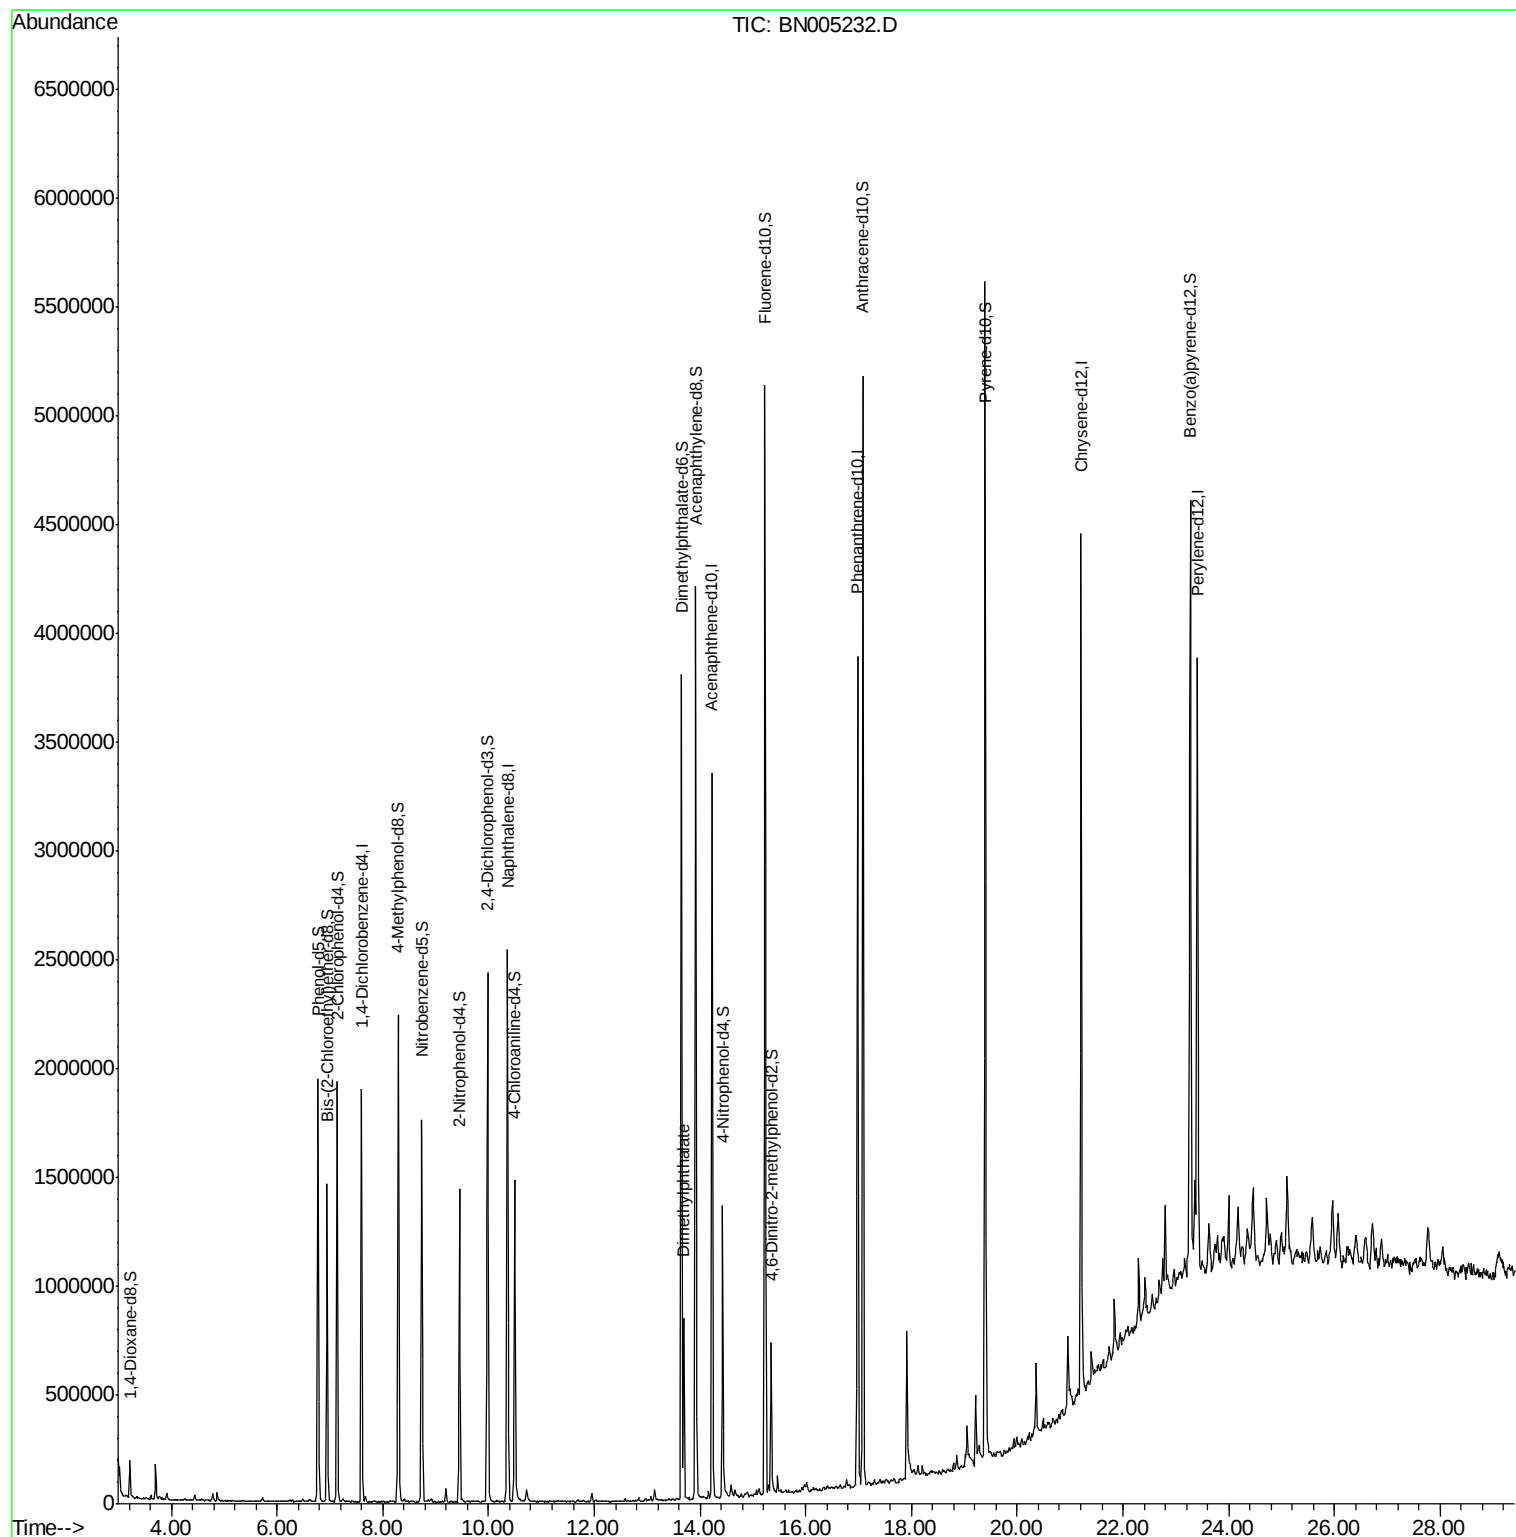

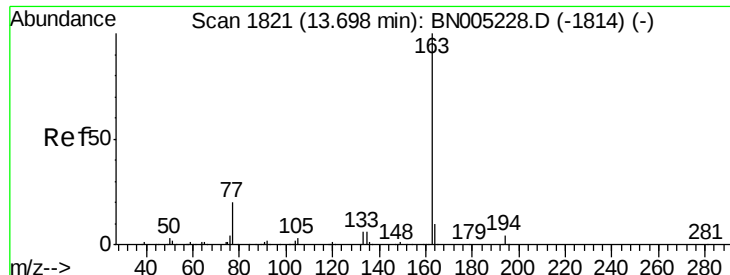

#44

Dimethylphthalate

Concen: 6.168 ng/ul

RT: 13.69 min Scan# 1820

Delta R.T. -0.01 min

Lab File: BN005232.D

Acq: 24 Apr 2019 01:56

Instrument :

BNA_N

ClientSampleId :

A5130


Tot Ion:163 Resp: 509885

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 10.3 8.1 12.1

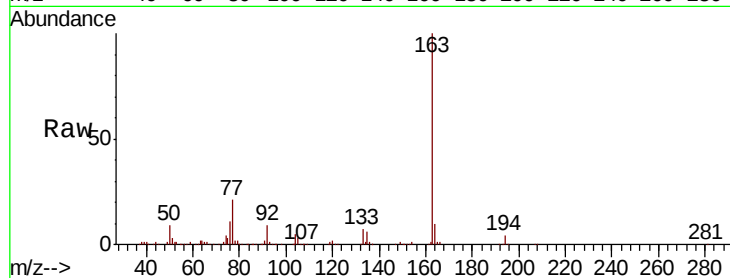

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

