

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042319\
 Data File : BN005223.D
 Acq On : 23 Apr 2019 20:07
 Operator : JU/SJ
 Sample : PB118951BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	34	39	47	rBV	154828	189643	2.09%	0.163%
2	3.916	153	158	164	rBV	27546	32872	0.36%	0.028%
3	4.869	315	320	324	rVB2	7556	12078	0.13%	0.010%
4	6.775	637	644	656	rBV	2352500	3641004	40.07%	3.131%
5	6.946	666	673	682	rVB	1857163	2765508	30.43%	2.378%
6	7.134	698	705	721	rVB	2412929	3702865	40.75%	3.184%
7	7.599	776	784	794	rBV	2091984	3266802	35.95%	2.809%
8	8.293	894	902	913	rBV	2834812	4566666	50.25%	3.927%
9	8.740	970	978	987	rBV	2302547	3670193	40.39%	3.156%
10	9.451	1092	1099	1111	rBV	1867530	2974645	32.73%	2.558%
11	9.981	1181	1189	1201	rBV	2919337	4774256	52.54%	4.105%
12	10.357	1246	1253	1263	rVB	2854439	4802030	52.84%	4.129%
13	10.493	1269	1276	1290	rBV	2790445	4790934	52.72%	4.120%
14	11.951	1519	1524	1534	rBV2	44252	75262	0.83%	0.065%
15	13.192	1730	1735	1741	rBV5	8943	16345	0.18%	0.014%
16	13.598	1798	1804	1806	rBV5	10101	15484	0.17%	0.013%
17	13.651	1806	1813	1821	rVV	4807474	6455133	71.04%	5.551%
18	13.922	1851	1859	1872	rBV	5147238	7819108	86.05%	6.724%
19	14.234	1904	1912	1920	rBV2	3913963	6040680	66.48%	5.194%
20	14.428	1938	1945	1957	rBV	1698362	2575111	28.34%	2.214%
21	14.892	2019	2024	2029	rBV6	8378	17363	0.19%	0.015%
22	15.228	2074	2081	2090	rBV	6231274	9087086	100.00%	7.814%
23	15.345	2095	2101	2112	rVV	735826	1055359	11.61%	0.908%
24	15.469	2117	2122	2127	rVB2	83384	120888	1.33%	0.104%
25	16.016	2211	2215	2220	rBV2	28210	36496	0.40%	0.031%
26	16.186	2240	2244	2247	rVB2	8755	9734	0.11%	0.008%
27	16.663	2321	2325	2329	rBV4	12789	16095	0.18%	0.014%
28	16.769	2338	2343	2349	rBV4	19443	28179	0.31%	0.024%
29	16.986	2373	2380	2390	rBV2	4345996	6399516	70.42%	5.503%
30	17.080	2390	2396	2408	rVB2	6074703	8669534	95.40%	7.455%
31	17.975	2545	2548	2552	rVB3	9412	13393	0.15%	0.012%
32	19.027	2723	2727	2731	rBV	61558	82870	0.91%	0.071%
33	19.280	2766	2770	2775	rVB	56056	75262	0.83%	0.065%
34	19.398	2783	2790	2802	rBV	6198470	8691526	95.65%	7.474%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042319\
Data File : BN005223.D
Acq On : 23 Apr 2019 20:07
Operator : JU/SJ
Sample : PB118951BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK51

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Title : SVOA CALIBRATION

35	21.216	3094	3099	3110	rBV	4292969	5564282	61.23%	4.785%
36	21.357	3120	3123	3127	rVB4	76398	85143	0.94%	0.073%
37	21.857	3205	3208	3211	rBV3	58954	70537	0.78%	0.061%
38	22.315	3283	3286	3293	rVB2	117389	163059	1.79%	0.140%
39	22.815	3368	3371	3378	rVB2	148377	217855	2.40%	0.187%
40	23.286	3444	3451	3461	rBV2	4178415	7549156	83.08%	6.492%
41	23.380	3463	3467	3468	rVV	193079	260805	2.87%	0.224%
42	23.421	3468	3474	3486	rVB2	3042488	5585545	61.47%	4.803%
43	24.015	3571	3575	3582	rVB	175108	304574	3.35%	0.262%


Sum of corrected areas: 116290876

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042319\
Data File : BN005223.D
Acq On : 23 Apr 2019 20:07
Operator : JU/SJ
Sample : PB118951BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK51

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

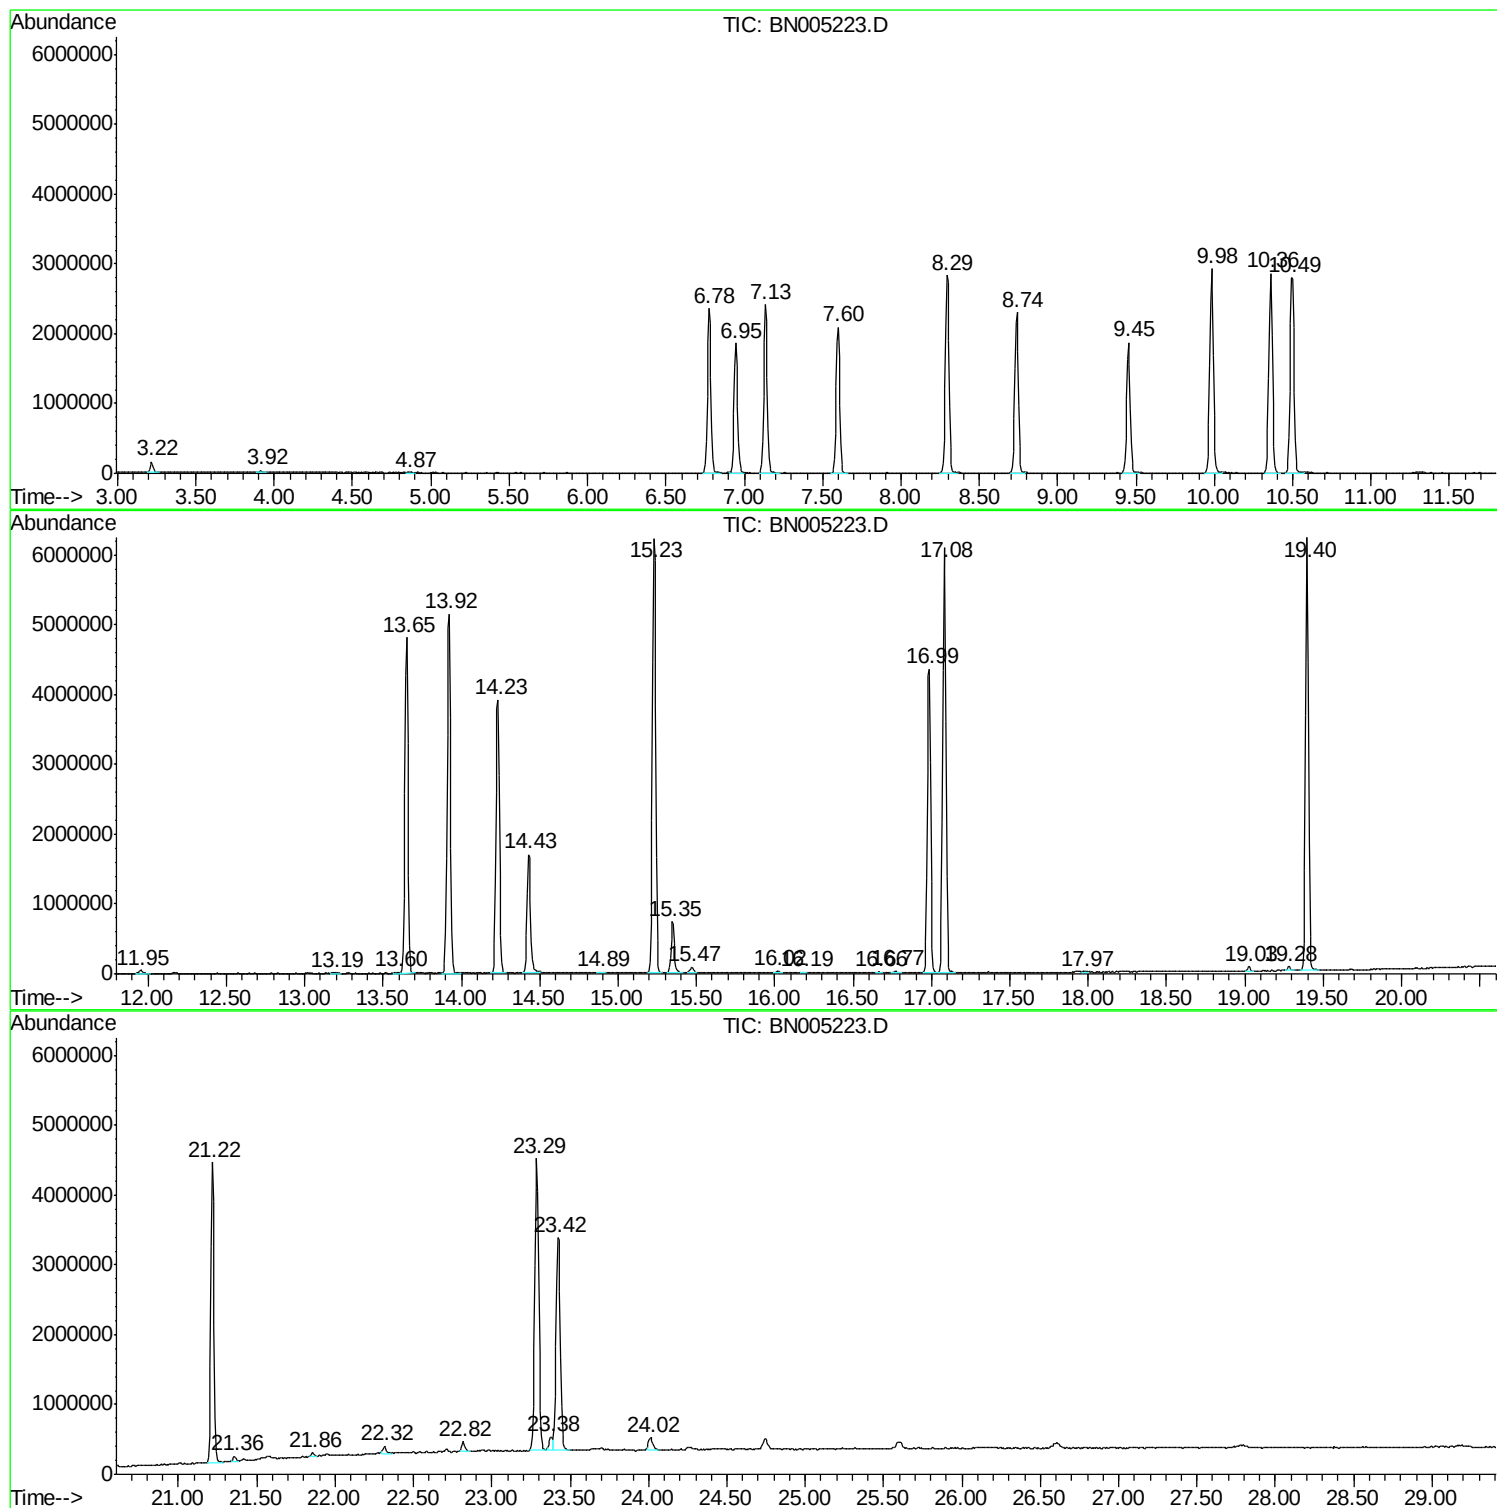

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042319\
Data File : BN005223.D
Acq On : 23 Apr 2019 20:07
Operator : JU/SJ
Sample : PB118951BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK51

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042319\
Data File : BN005223.D
Acq On : 23 Apr 2019 20:07
Operator : JU/SJ
Sample : PB118951BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK51

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc