


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN042321\
Data File : BN014384.D
Acq On : 23 Apr 2021 19:15
Operator : CG/JU
Sample : M2065-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG564

Manual Integrations
APPROVED

mohammad
4/26/2021 11:37:46 AM

Quant Time: Apr 24 00:02:40 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 23 12:06:34 2021
Response via : Initial Calibration

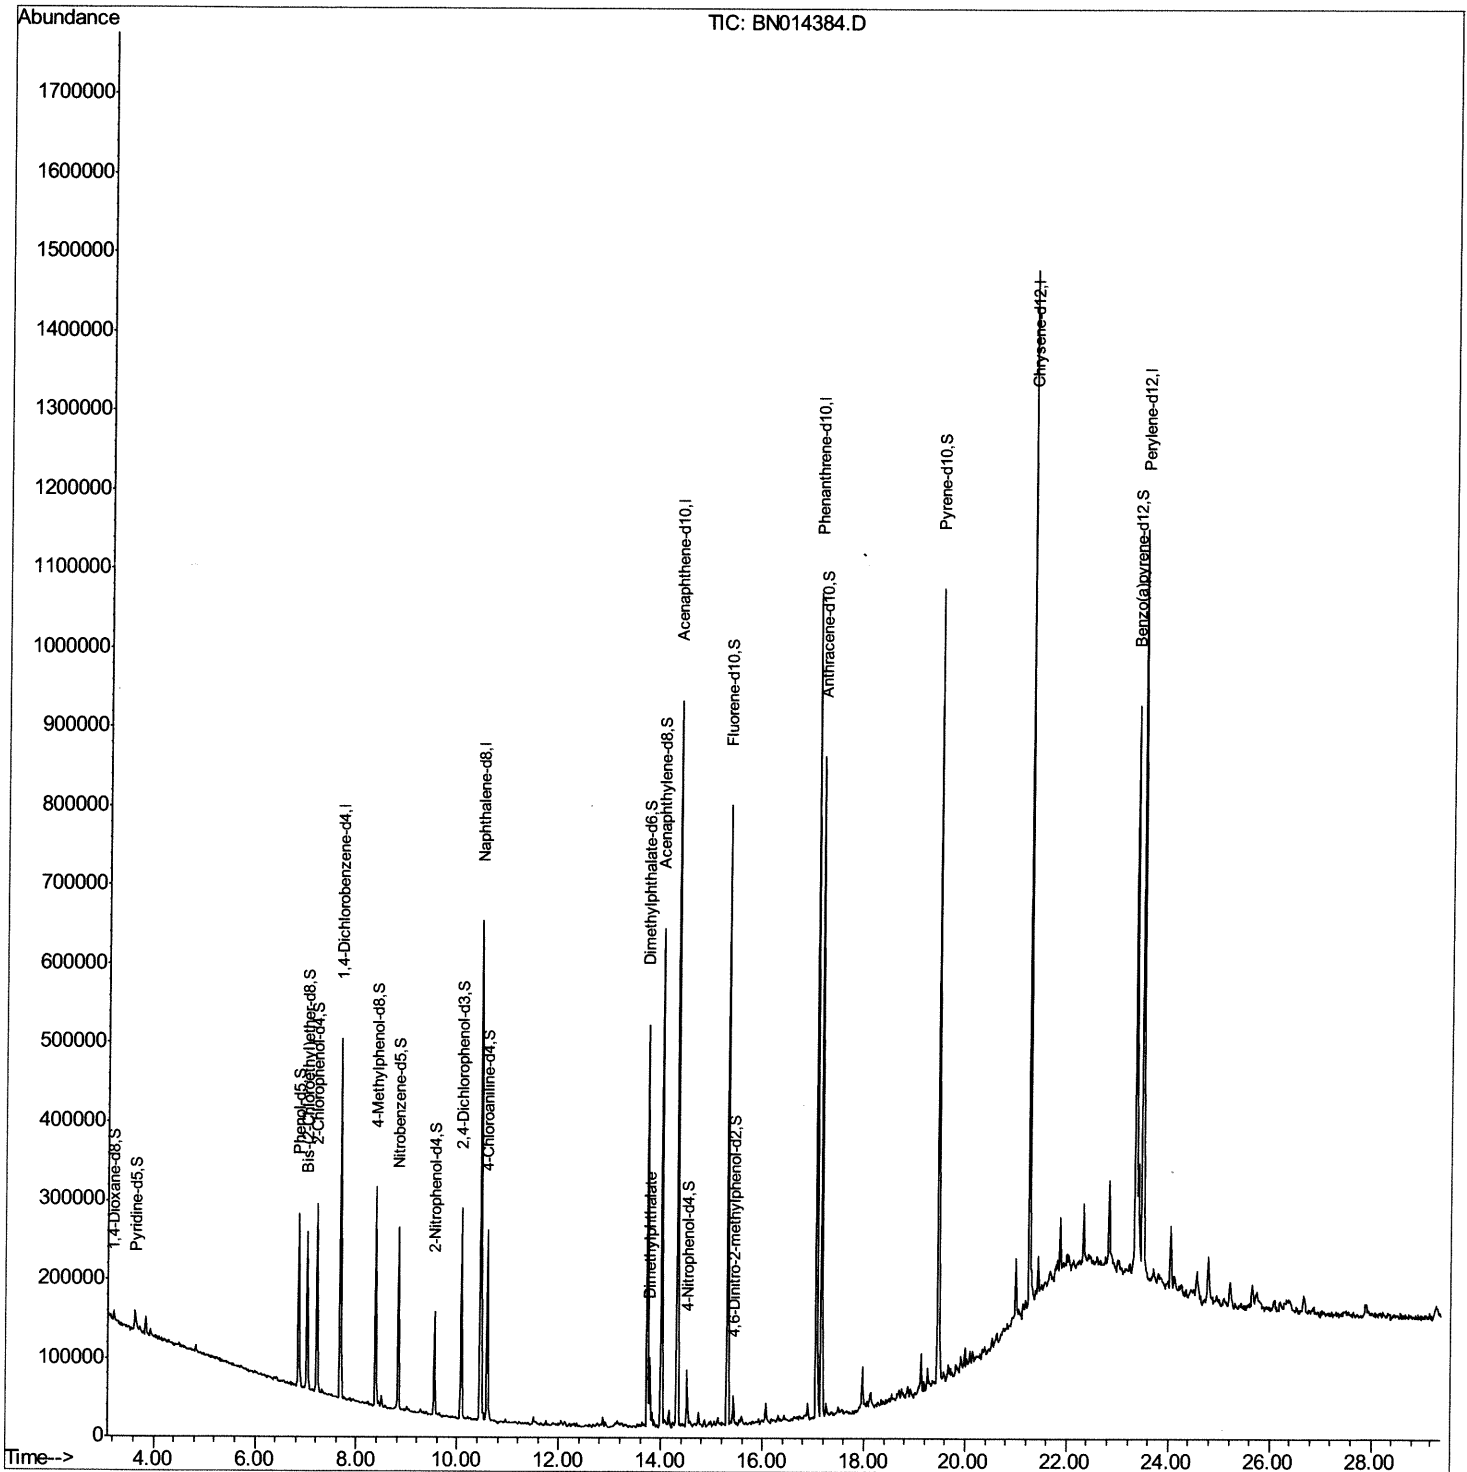

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN042321\
 Data File : BN014384.D
 Acq On : 23 Apr 2021 19:15
 Operator : CG/JU
 Sample : M2065-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG564

Manual Integrations
 APPROVED

mohammad
 4/26/2021 11:37:46 AM

Quant Time: Apr 23 23:19:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 23 12:06:34 2021
 Response via : Initial Calibration

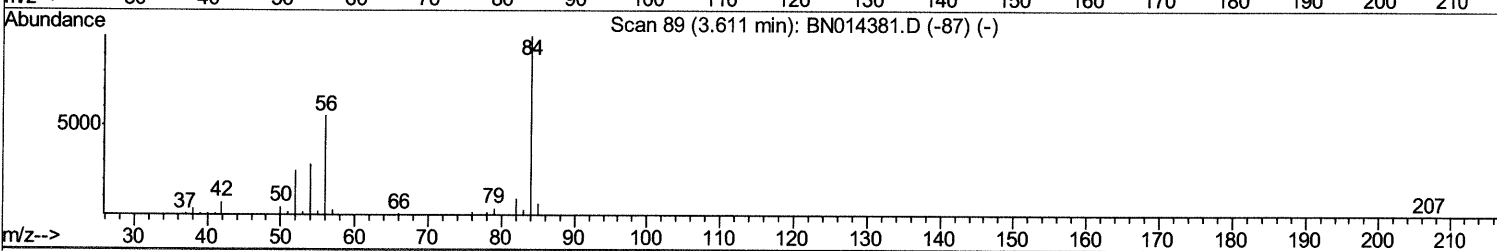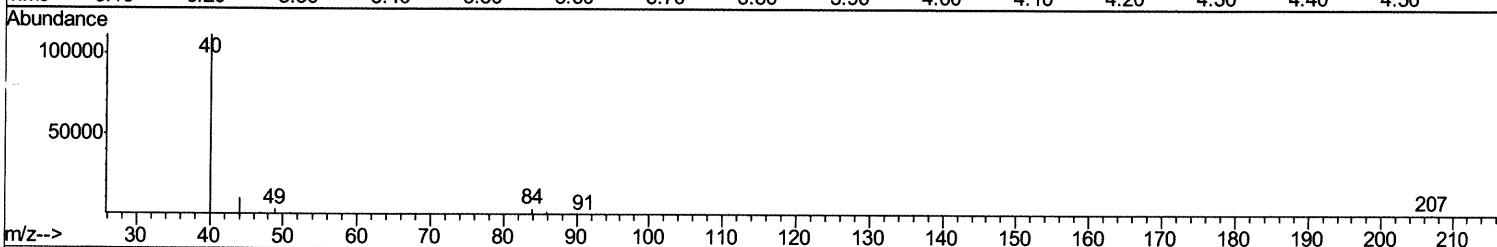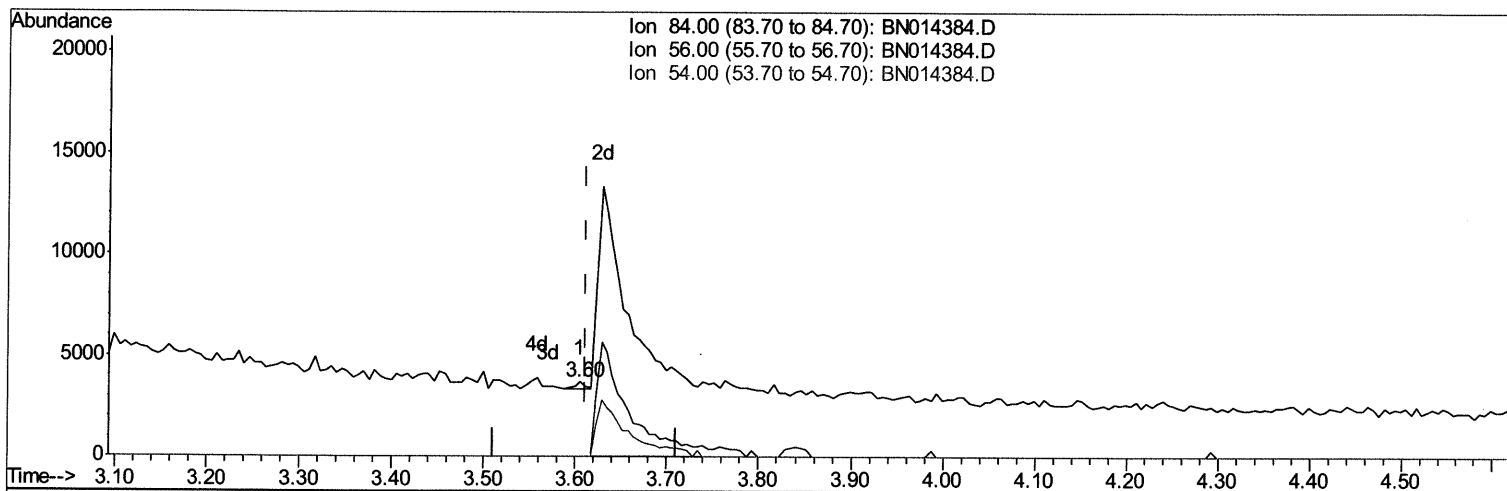

TIC: BN014384.D

(4) Pyridine-d5 (S)

3.605min (-0.006) 0.03ng/ul

response 276

Ion	Exp%	Act%
84.00	100	100
56.00	55.90	0.00#
54.00	27.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN042321\
 Data File : BN014384.D
 Acq On : 23 Apr 2021 19:15
 Operator : CG/JU
 Sample : M2065-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG564

Manual Integrations
 APPROVED

mohammad
 4/26/2021 11:37:46 AM

Quant Time: Apr 23 23:19:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 23 12:06:34 2021
 Response via : Initial Calibration

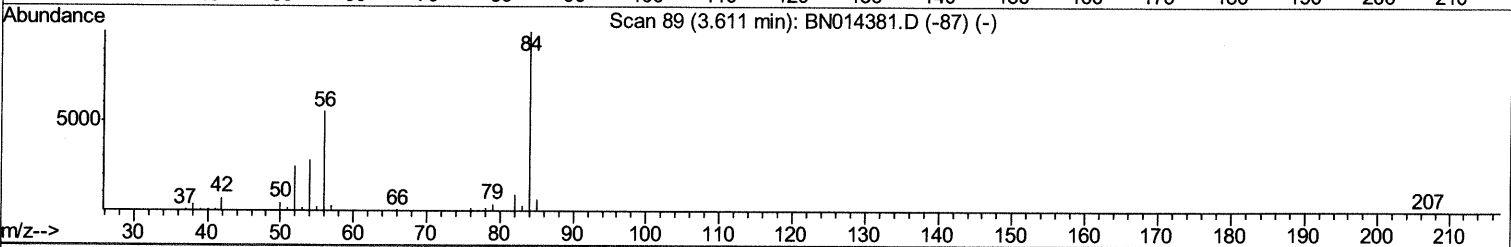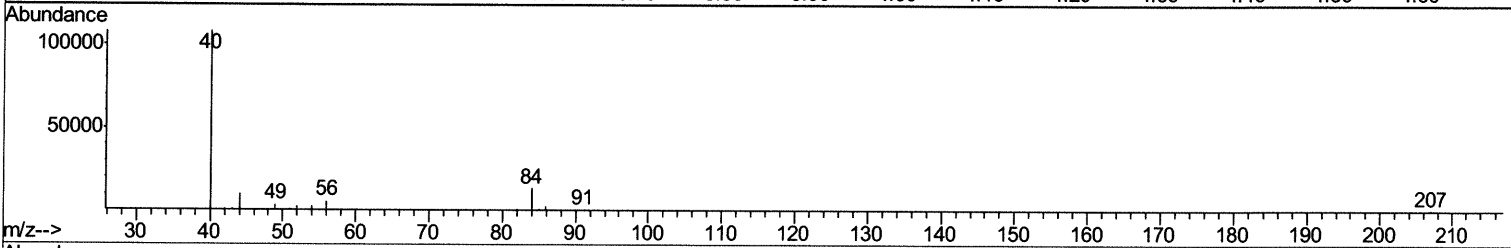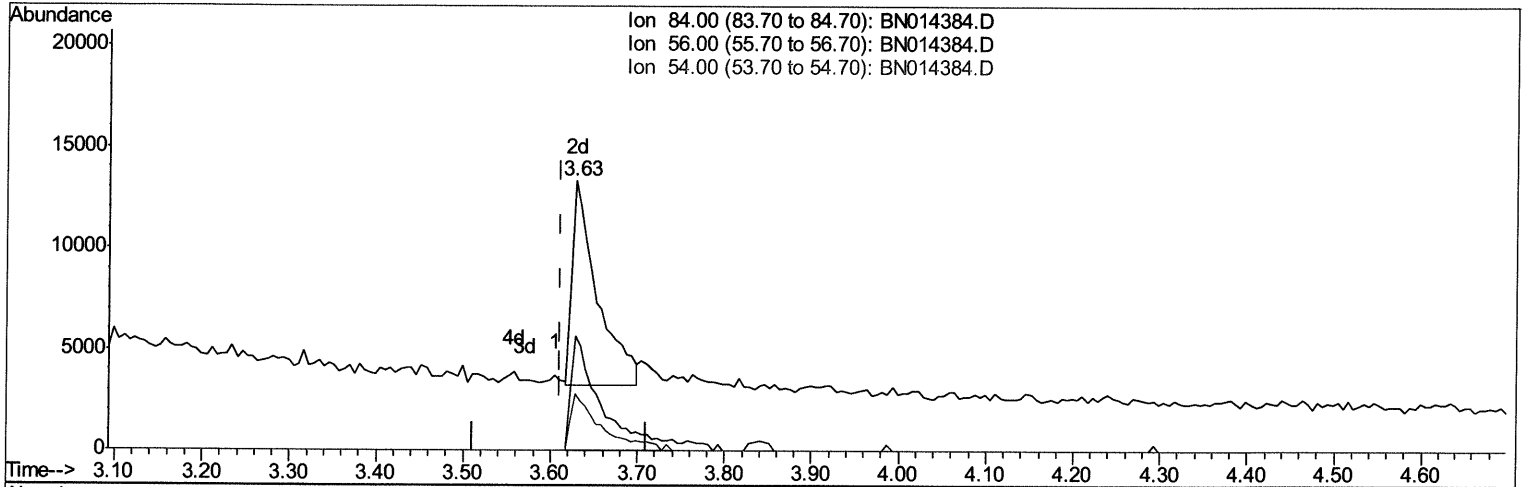

TIC: BN014384.D

(4) Pyridine-d5 (S)

3.628min (+0.018) 2.30ng/ul m 04/20/21 54

response 20427

Ion	Exp%	Act%
84.00	100	100
56.00	55.90	42.29#
54.00	27.50	20.85#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042321\
 Data File : BN014384.D
 Acq On : 23 Apr 2021 19:15
 Operator : CG/JU
 Sample : M2065-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG564

Manual Integrations
 APPROVED

mohammad
 4/26/2021 11:37:46 AM

Quant Time: Apr 24 00:02:40 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 23 12:06:34 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	127717	20.00	ng/ul	0.00
20) Naphthalene-d8	10.46	136	528299	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.32	164	300623	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.07	188	617930	20.00	ng/ul	0.00
79) Chrysene-d12	21.26	240	611352	20.00	ng/ul	0.00
88) Perylene-d12	23.49	264	618168	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.21	96	6665	1.99	ng/uL	0.00
4) Pyridine-d5	3.63	84	20427m	2.30	ng/ul	0.02
7) Phenol-d5	6.85	99	127309	11.92	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.02	67	86814	13.58	ng/ul	0.00
11) 2-Chlorophenol-d4	7.22	132	112599	13.41	ng/ul	0.00
15) 4-Methylphenol-d8	8.38	113	101663	12.56	ng/ul	0.00
21) Nitrobenzene-d5	8.83	128	57105	14.96	ng/ul	0.00
24) 2-Nitrophenol-d4	9.55	143	42038	11.24	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.08	165	93015	11.55	ng/ul	0.00
31) 4-Chloroaniline-d4	10.59	131	128563	10.76	ng/ul	0.00
46) Dimethylphthalate-d6	13.73	166	326546	14.99	ng/ul	0.00
49) Acenaphthylene-d8	14.01	160	429735	16.40	ng/ul	0.00
54) 4-Nitrophenol-d4	14.51	143	15421	3.65	ng/ul	0.00
60) Fluorene-d10	15.32	176	296452	15.40	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.43	200	6407	1.94	ng/ul	0.00
73) Anthracene-d10	17.16	188	441516	15.31	ng/ul	0.00
81) Pyrene-d10	19.46	212	495083	16.68	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.34	264	491965	15.00	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.77	163	51417	2.274	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed