




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN042321\
 Data File : BN014393.D
 Acq On : 24 Apr 2021 00:36
 Operator : CG/JU
 Sample : M2065-12
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG565

Manual Integrations
 APPROVED

mohammad
 4/26/2021 11:37:53 AM

Quant Time: Apr 24 01:22:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 23 23:19:59 2021
 Response via : Initial Calibration

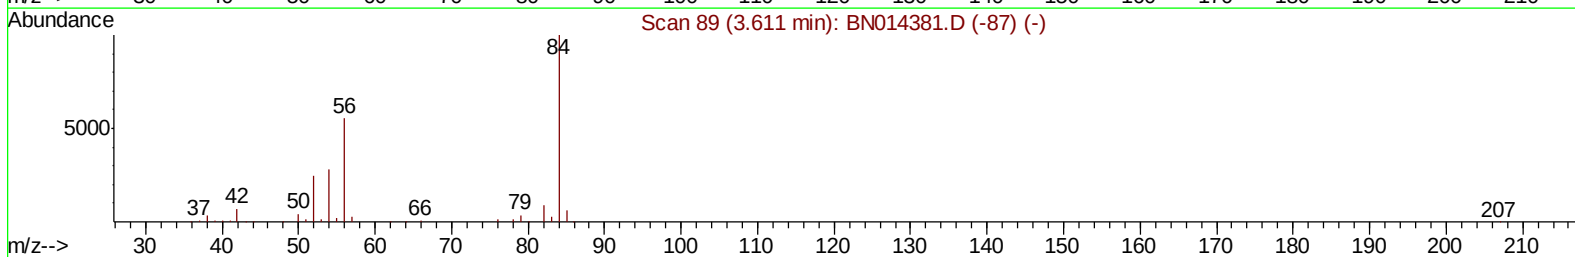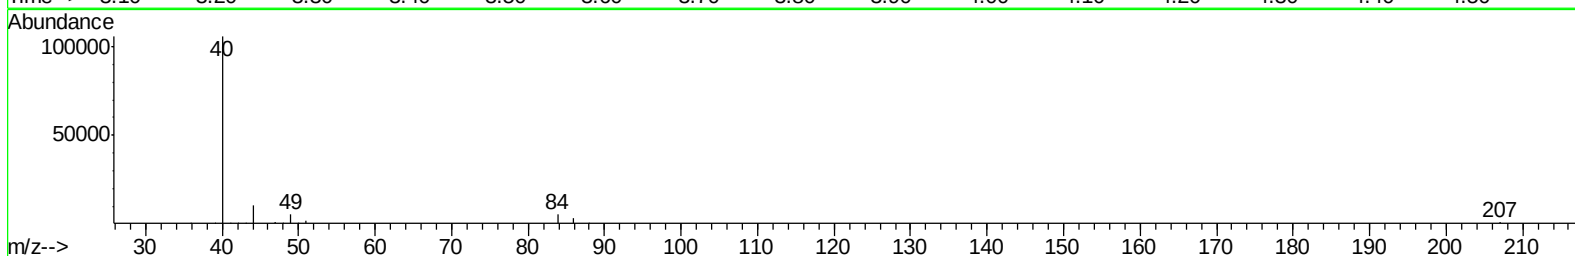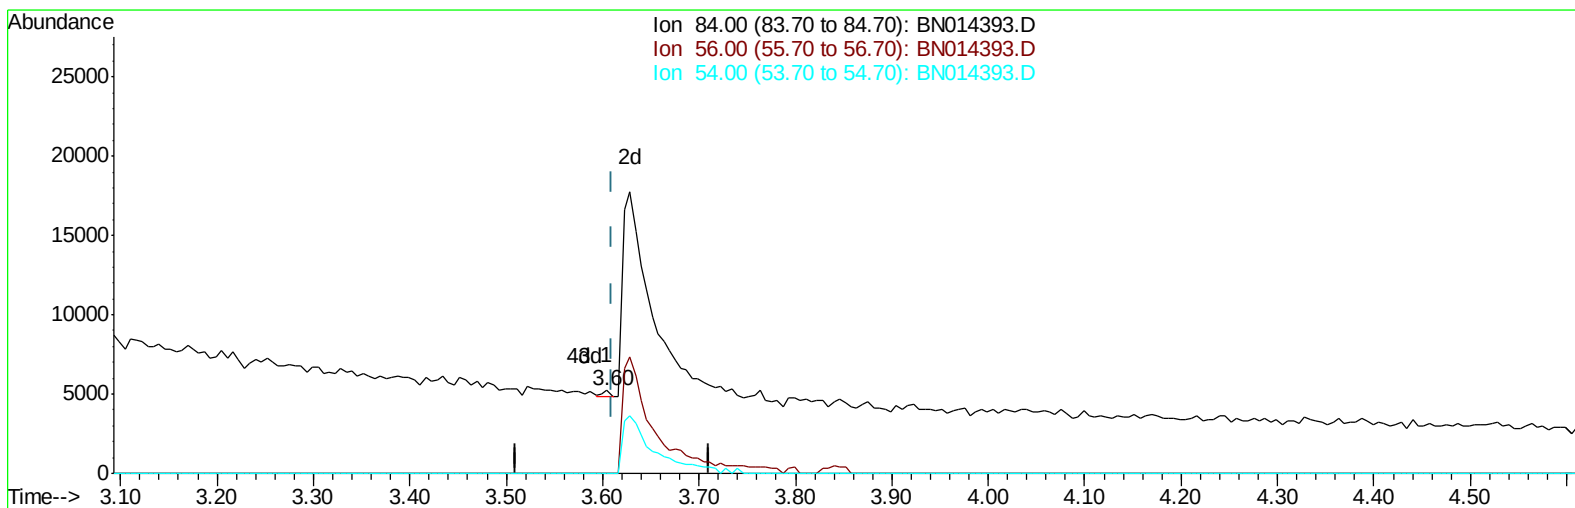

TIC: BN014393.D

(4) Pyridine-d5 (S)

3.605min (-0.006) 0.02ng/ul

response 182

Ion	Exp%	Act%
84.00	100	100
56.00	55.90	0.00#
54.00	27.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN042321\
Data File : BN014393.D
Acq On : 24 Apr 2021 00:36
Operator : CG/JU
Sample : M2065-12
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG565

Manual Integrations
APPROVED

mohammad
4/26/2021 11:37:53 AM

Quant Time: Apr 24 01:22:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 23 23:19:59 2021
Response via : Initial Calibration

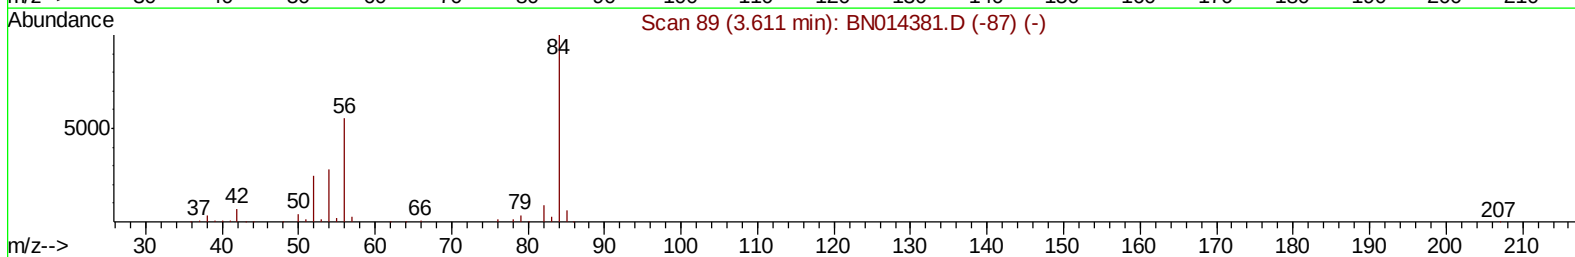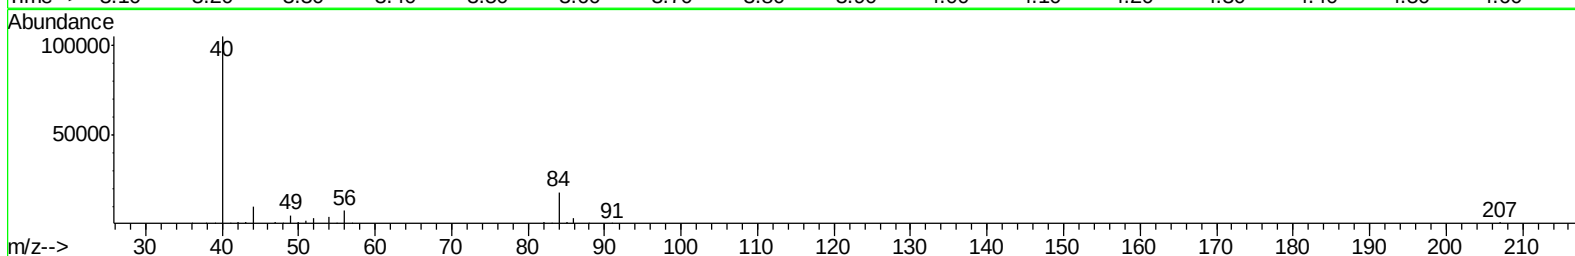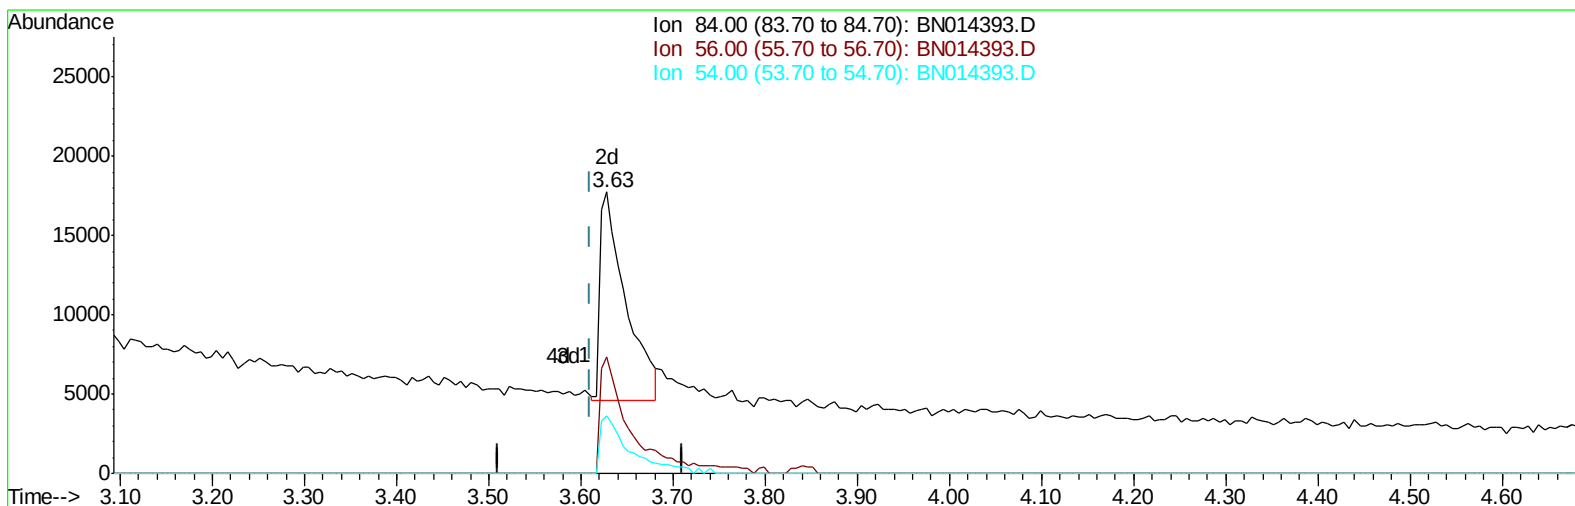

TIC: BN014393.D

(4) Pyridine-d5 (S)

3.628min (+0.018) 2.57ng/ul m

response 25542

Ion	Exp%	Act%
84.00	100	100
56.00	55.90	41.22#
54.00	27.50	20.66#
0.00	0.00	0.00