

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042321\
 Data File : BN014376.D
 Acq On : 23 Apr 2021 14:29
 Operator : CG/JU
 Sample : M2031-18
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG534

Quant Time: Apr 23 14:58:47 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 23 12:06:34 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	126492	20.00	ng/ul	0.00
20) Naphthalene-d8	10.46	136	510961	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.32	164	292095	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.07	188	608536	20.00	ng/ul	0.00
79) Chrysene-d12	21.26	240	605434	20.00	ng/ul	0.00
88) Perylene-d12	23.49	264	621138	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.21	96	14992	4.51	ng/uL	0.00
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	6.85	99	75516	7.14	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.02	67	181024	28.59	ng/ul	0.00
11) 2-Chlorophenol-d4	7.22	132	201499	24.23	ng/ul	0.00
15) 4-Methylphenol-d8	8.38	113	126861	15.83	ng/ul	0.00
21) Nitrobenzene-d5	8.83	128	124558	33.73	ng/ul	0.00
24) 2-Nitrophenol-d4	9.55	143	102351	28.31	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.08	165	204076	26.20	ng/ul	0.00
31) 4-Chloroaniline-d4	10.59	131	13255	1.15	ng/ul	0.00
46) Dimethylphthalate-d6	13.73	166	744943	35.20	ng/ul	0.00
49) Acenaphthylene-d8	14.01	160	963900	37.86	ng/ul	0.00
54) 4-Nitrophenol-d4	14.52	143	16729	4.08	ng/ul	0.00
60) Fluorene-d10	15.32	176	660480	35.31	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.43	200	64863	19.92	ng/ul	0.00
73) Anthracene-d10	17.16	188	1056299	37.19	ng/ul	0.00
81) Pyrene-d10	19.47	212	1261378	42.92	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.35	264	1295741	39.32	ng/ul	0.00
Target Compounds						
30) Naphthalene	10.51	128	28586	1.009	ng/ul	Ovalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
Data File : BN014376.D
Acq On : 23 Apr 2021 14:29
Operator : CG/JU
Sample : M2031-18
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG534

Quant Time: Apr 23 14:58:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 23 12:06:34 2021
Response via : Initial Calibration

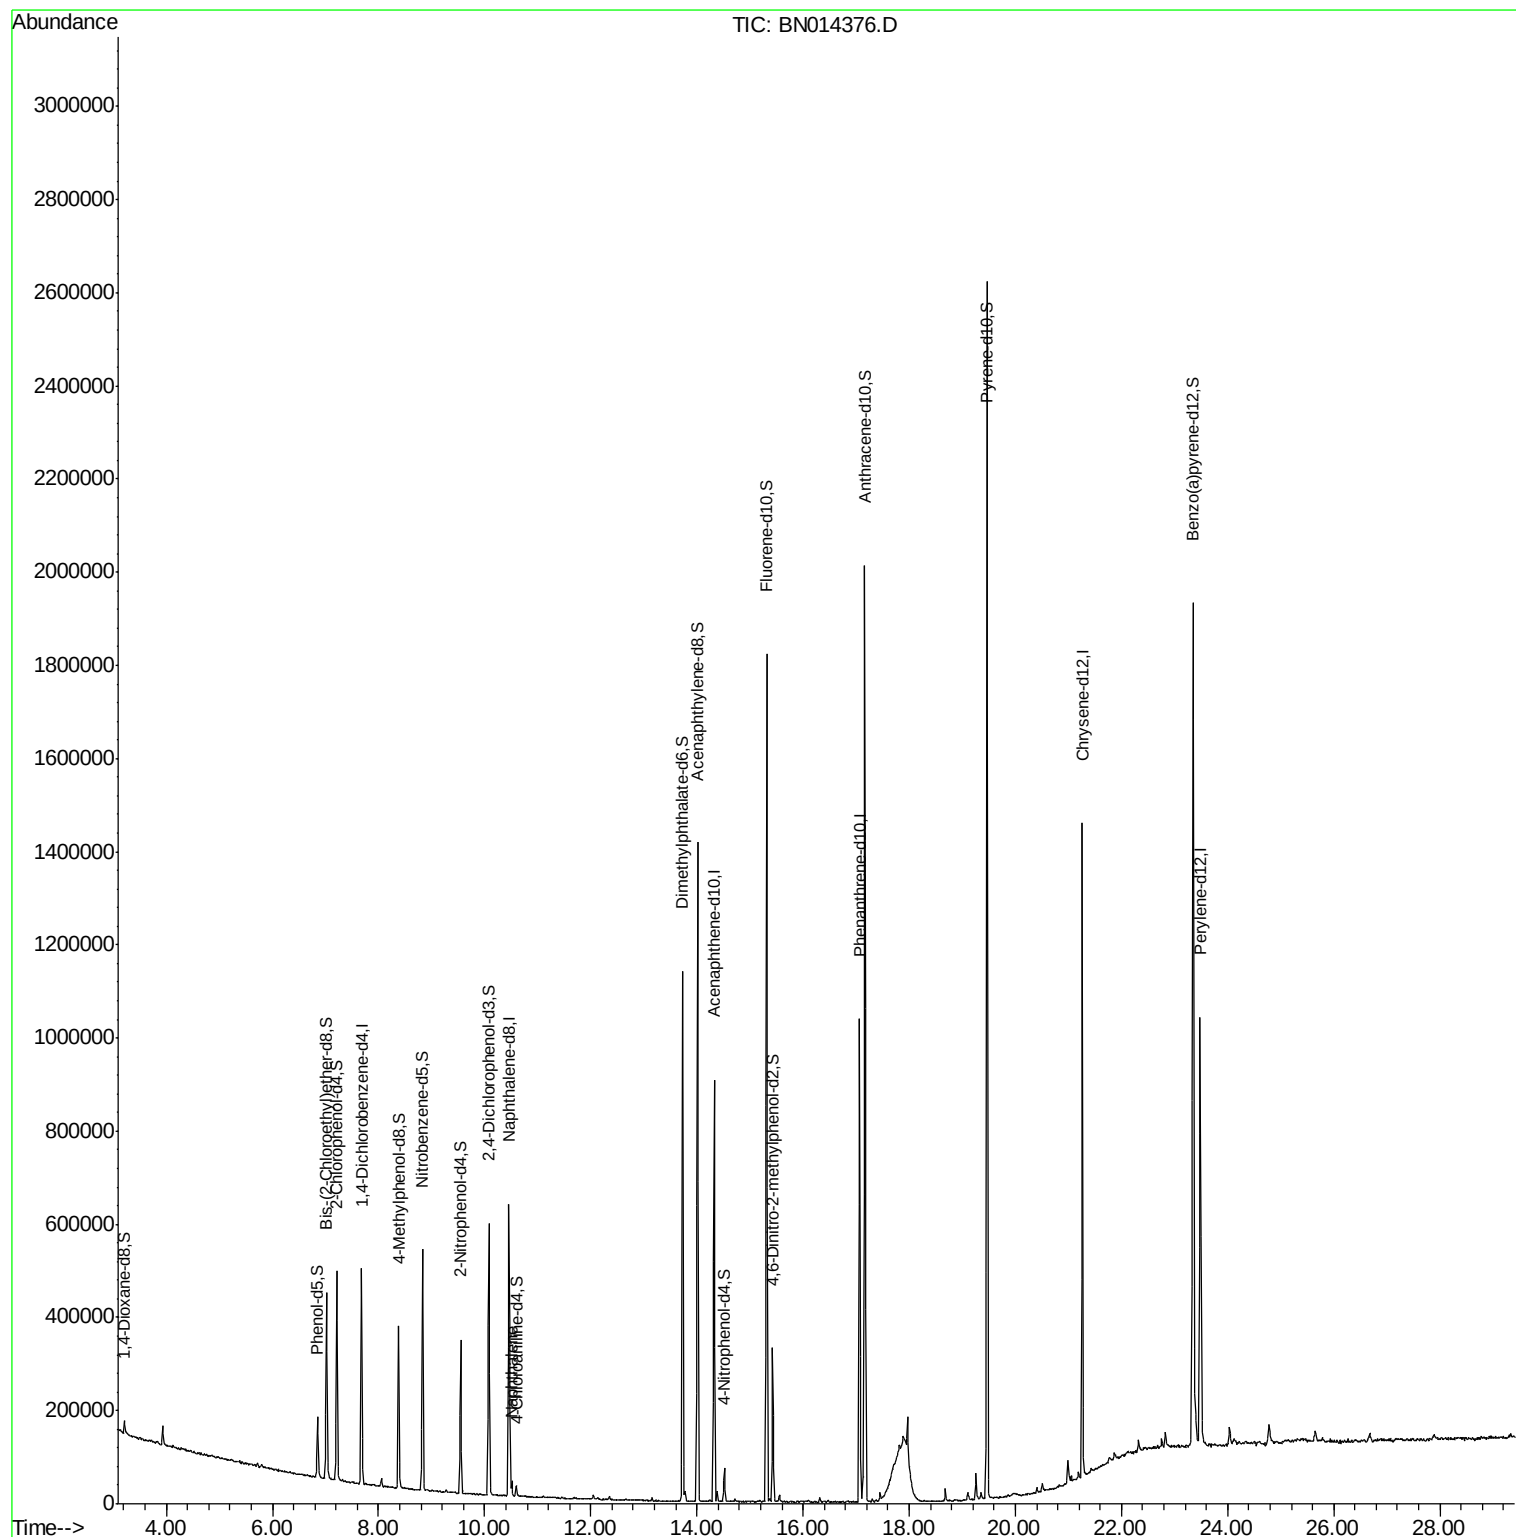

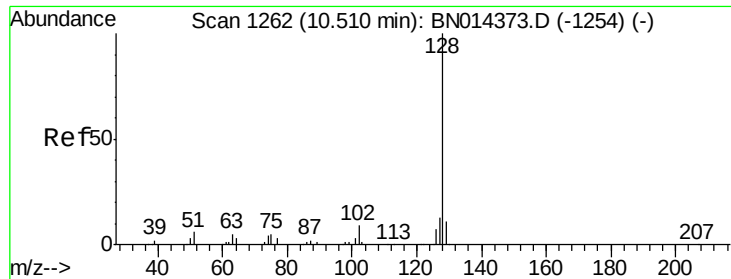

#30

Naphthalene

Concen: 1.009 ng/ul

RT: 10.51 min Scan# 1262

Delta R.T. 0.00 min

Lab File: BN014376.D

Acq: 23 Apr 2021 14:29

Instrument :

BNA_N

ClientSampleId :

BG534

Tot Ion:128 Resp: 28586

Ion Ratio Lower Upper

128 100

129 11.0 8.7 13.1

127 11.0 10.6 15.8

