

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
 Data File : BN014377.D
 Acq On : 23 Apr 2021 15:04
 Operator : CG/JU
 Sample : M2031-20
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG545

Quant Time: Apr 23 15:34:25 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 23 12:06:34 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	123825	20.00	ng/ul	0.00
20) Naphthalene-d8	10.46	136	501354	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.32	164	284103	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.07	188	605139	20.00	ng/ul	0.00
79) Chrysene-d12	21.26	240	617225	20.00	ng/ul	0.00
88) Perylene-d12	23.49	264	609727	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.21	96	12146	3.73	ng/uL	0.00
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.85	99	64454	6.23	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.02	67	182793	29.49	ng/ul	0.00
11) 2-Chlorophenol-d4	7.22	132	195131	23.97	ng/ul	0.00
15) 4-Methylphenol-d8	8.38	113	115862	14.77	ng/ul	0.00
21) Nitrobenzene-d5	8.83	128	126719	34.98	ng/ul	0.00
24) 2-Nitrophenol-d4	9.55	143	103003	29.03	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.08	165	202751	26.53	ng/ul	0.00
31) 4-Chloroaniline-d4	10.60	131	11744	1.04	ng/ul	0.00
46) Dimethylphthalate-d6	13.73	166	790365	38.40	ng/ul	0.00
49) Acenaphthylene-d8	14.01	160	997915	40.30	ng/ul	0.00
54) 4-Nitrophenol-d4	14.52	143	15076	3.78	ng/ul	0.00
60) Fluorene-d10	15.32	176	713197	39.20	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.43	200	67917	20.97	ng/ul	0.00
73) Anthracene-d10	17.16	188	1150982	40.75	ng/ul	0.00
81) Pyrene-d10	19.46	212	1298865	43.35	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.34	264	1384081	42.79	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	11.75	107	13815	1.782	ng/ul	98
47) Dimethylphthalate	13.78	163	22587	1.057	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
Data File : BN014377.D
Acq On : 23 Apr 2021 15:04
Operator : CG/JU
Sample : M2031-20
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG545

Quant Time: Apr 23 15:34:25 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 23 12:06:34 2021
Response via : Initial Calibration




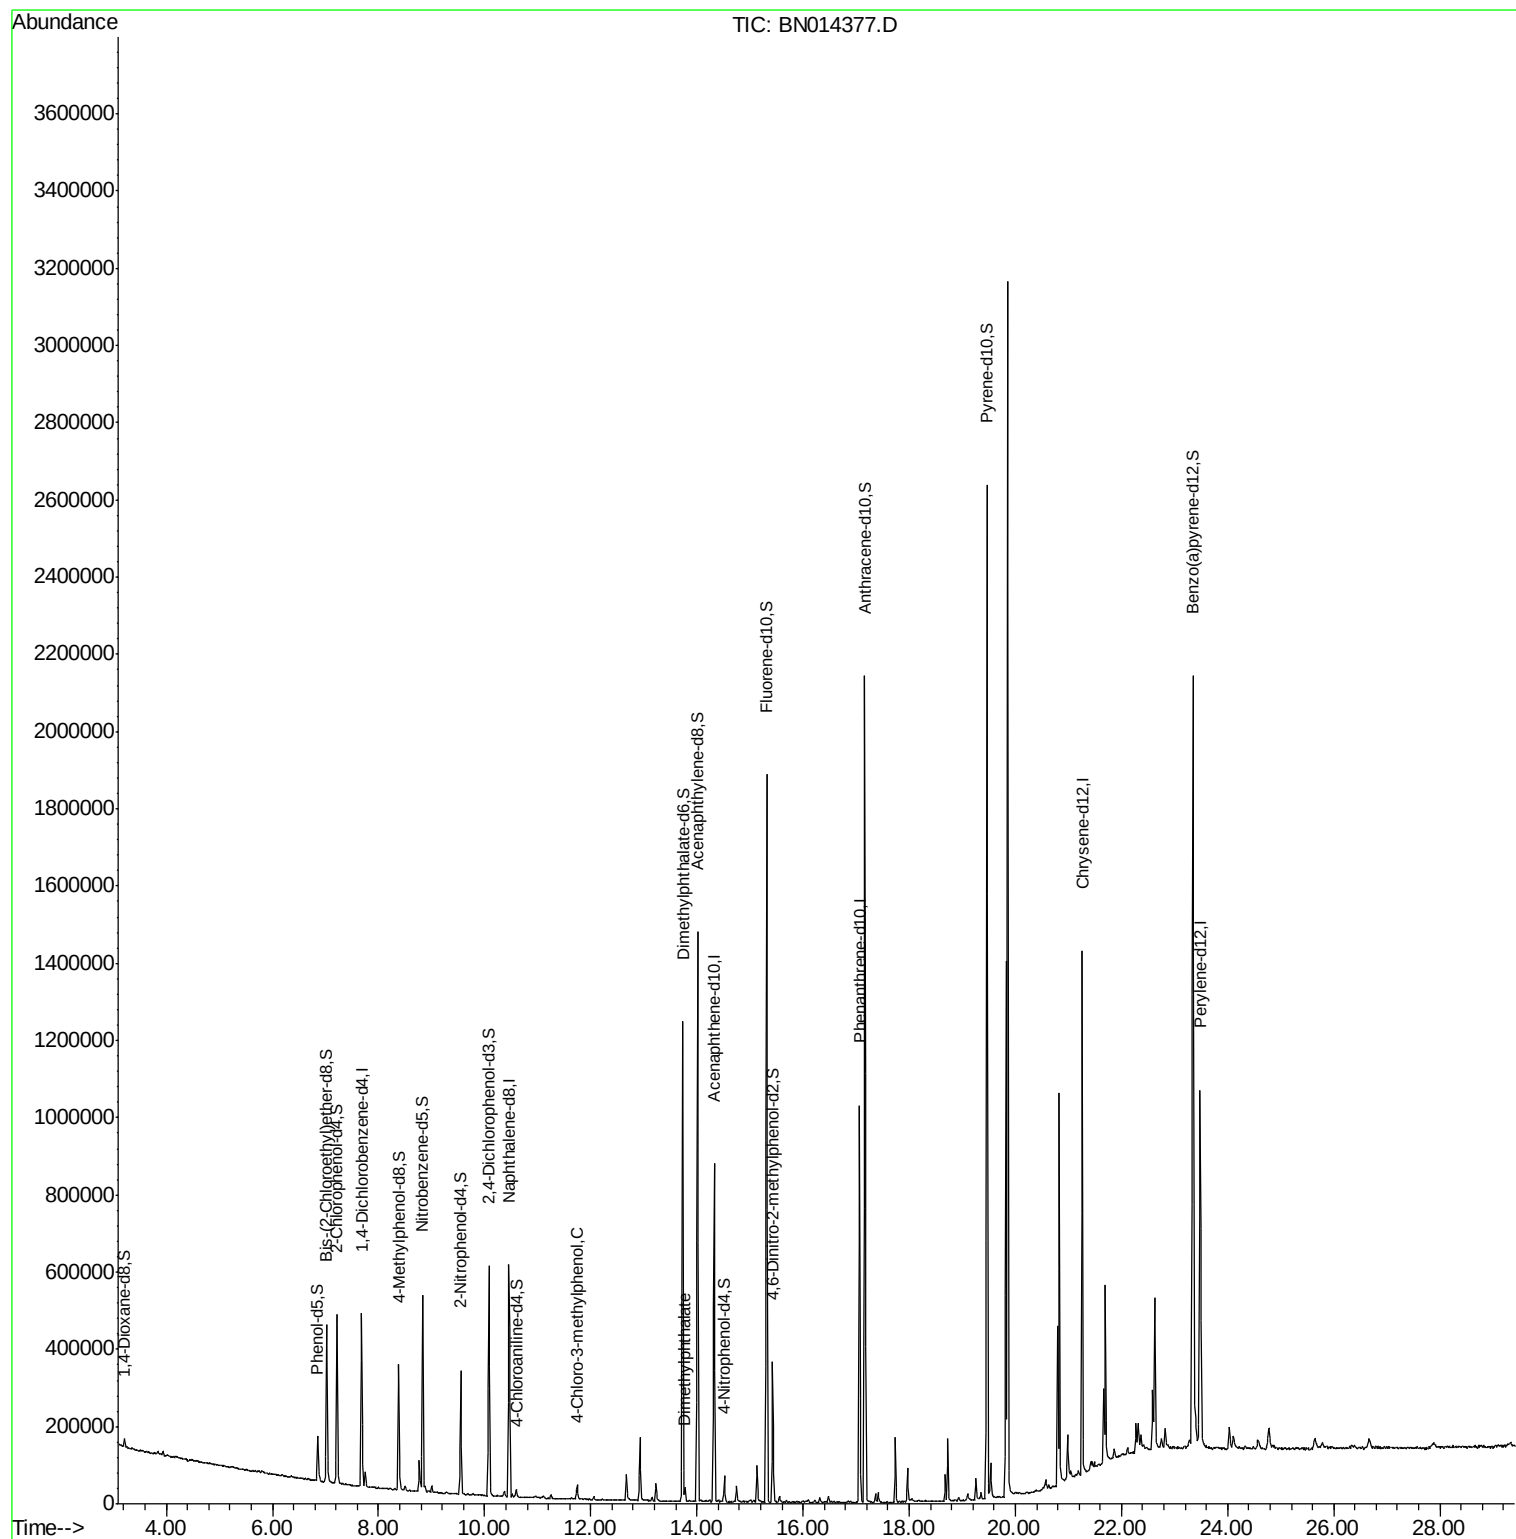


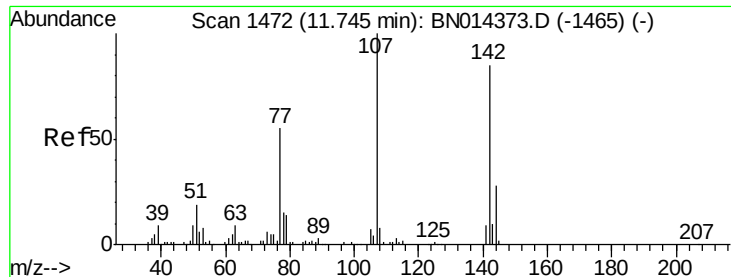

#35
 4-Chloro-3-methylphenol
 Concen: 1.782 ng/ul
 RT: 11.75 min Scan# 1472
 Delta R.T. 0.00 min
 Lab File: BN014377.D
 Acq: 23 Apr 2021 15:04

Instrument :
 BNA_N
 ClientSampled :
 BG545

Tot Ion	Ratio	Lower	Upper
107	100		
144	26.6	21.0	31.4
142	81.3	66.4	99.6

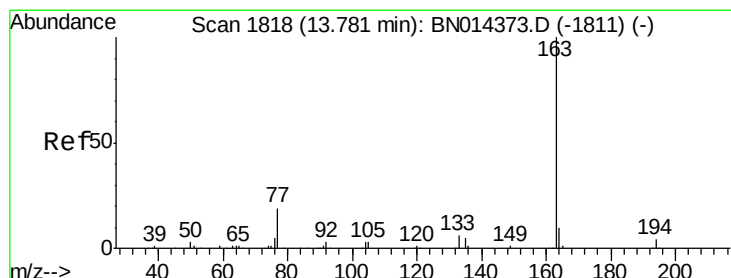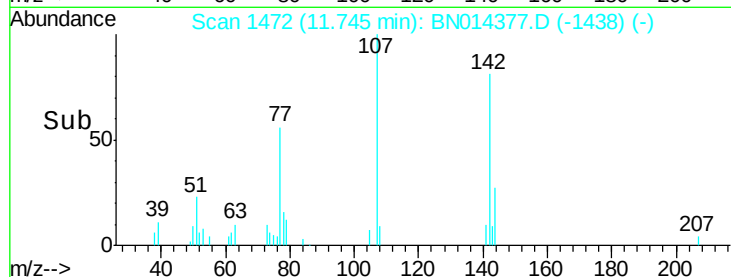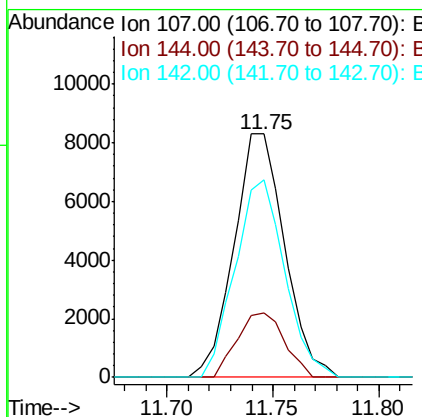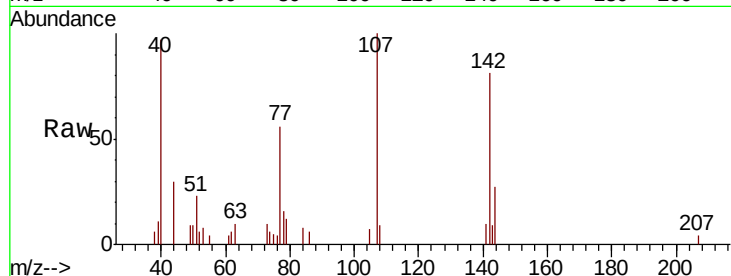

#47
 Dimethylphthalate
 Concen: 1.057 ng/ul
 RT: 13.78 min Scan# 1818
 Delta R.T. 0.00 min
 Lab File: BN014377.D
 Acq: 23 Apr 2021 15:04

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.3	4.9
164	10.0	7.8	11.8

