

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
 Data File : BN014390.D
 Acq On : 23 Apr 2021 22:49
 Operator : CG/JU
 Sample : M2065-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG566

Quant Time: Apr 24 00:47:04 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 23 23:19:59 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	163911	20.00	ng/ul	0.00
20) Naphthalene-d8	10.46	136	692132	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.32	164	405503	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.06	188	841447	20.00	ng/ul	0.00
79) Chrysene-d12	21.26	240	809881	20.00	ng/ul	0.00
88) Perylene-d12	23.49	264	845755	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.21	96	7859	1.82	ng/uL	0.00
4) Pyridine-d5	3.62	84	35364	3.10	ng/ul	0.01
7) Phenol-d5	6.85	99	164025	11.97	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.02	67	107672	13.12	ng/ul	0.00
11) 2-Chlorophenol-d4	7.22	132	143513	13.32	ng/ul	0.00
15) 4-Methylphenol-d8	8.38	113	131654	12.67	ng/ul	0.00
21) Nitrobenzene-d5	8.83	128	75001	15.00	ng/ul	0.00
24) 2-Nitrophenol-d4	9.55	143	61383	12.53	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.08	165	124746	11.82	ng/ul	0.00
31) 4-Chloroaniline-d4	10.59	131	179072	11.44	ng/ul	0.00
46) Dimethylphthalate-d6	13.73	166	434077	14.78	ng/ul	0.00
49) Acenaphthylene-d8	14.01	160	549322	15.54	ng/ul	0.00
54) 4-Nitrophenol-d4	14.52	143	34568	6.07	ng/ul	0.00
60) Fluorene-d10	15.32	176	366543	14.11	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.43	200	17740	3.94	ng/ul	0.00
73) Anthracene-d10	17.16	188	574236	14.62	ng/ul	0.00
81) Pyrene-d10	19.46	212	653934	16.63	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.34	264	674869	15.04	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.77	163	77232	2.532	ng/ul	Ovalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
Data File : BN014390.D
Acq On : 23 Apr 2021 22:49
Operator : CG/JU
Sample : M2065-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG566

Quant Time: Apr 24 00:47:04 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 23 23:19:59 2021
Response via : Initial Calibration

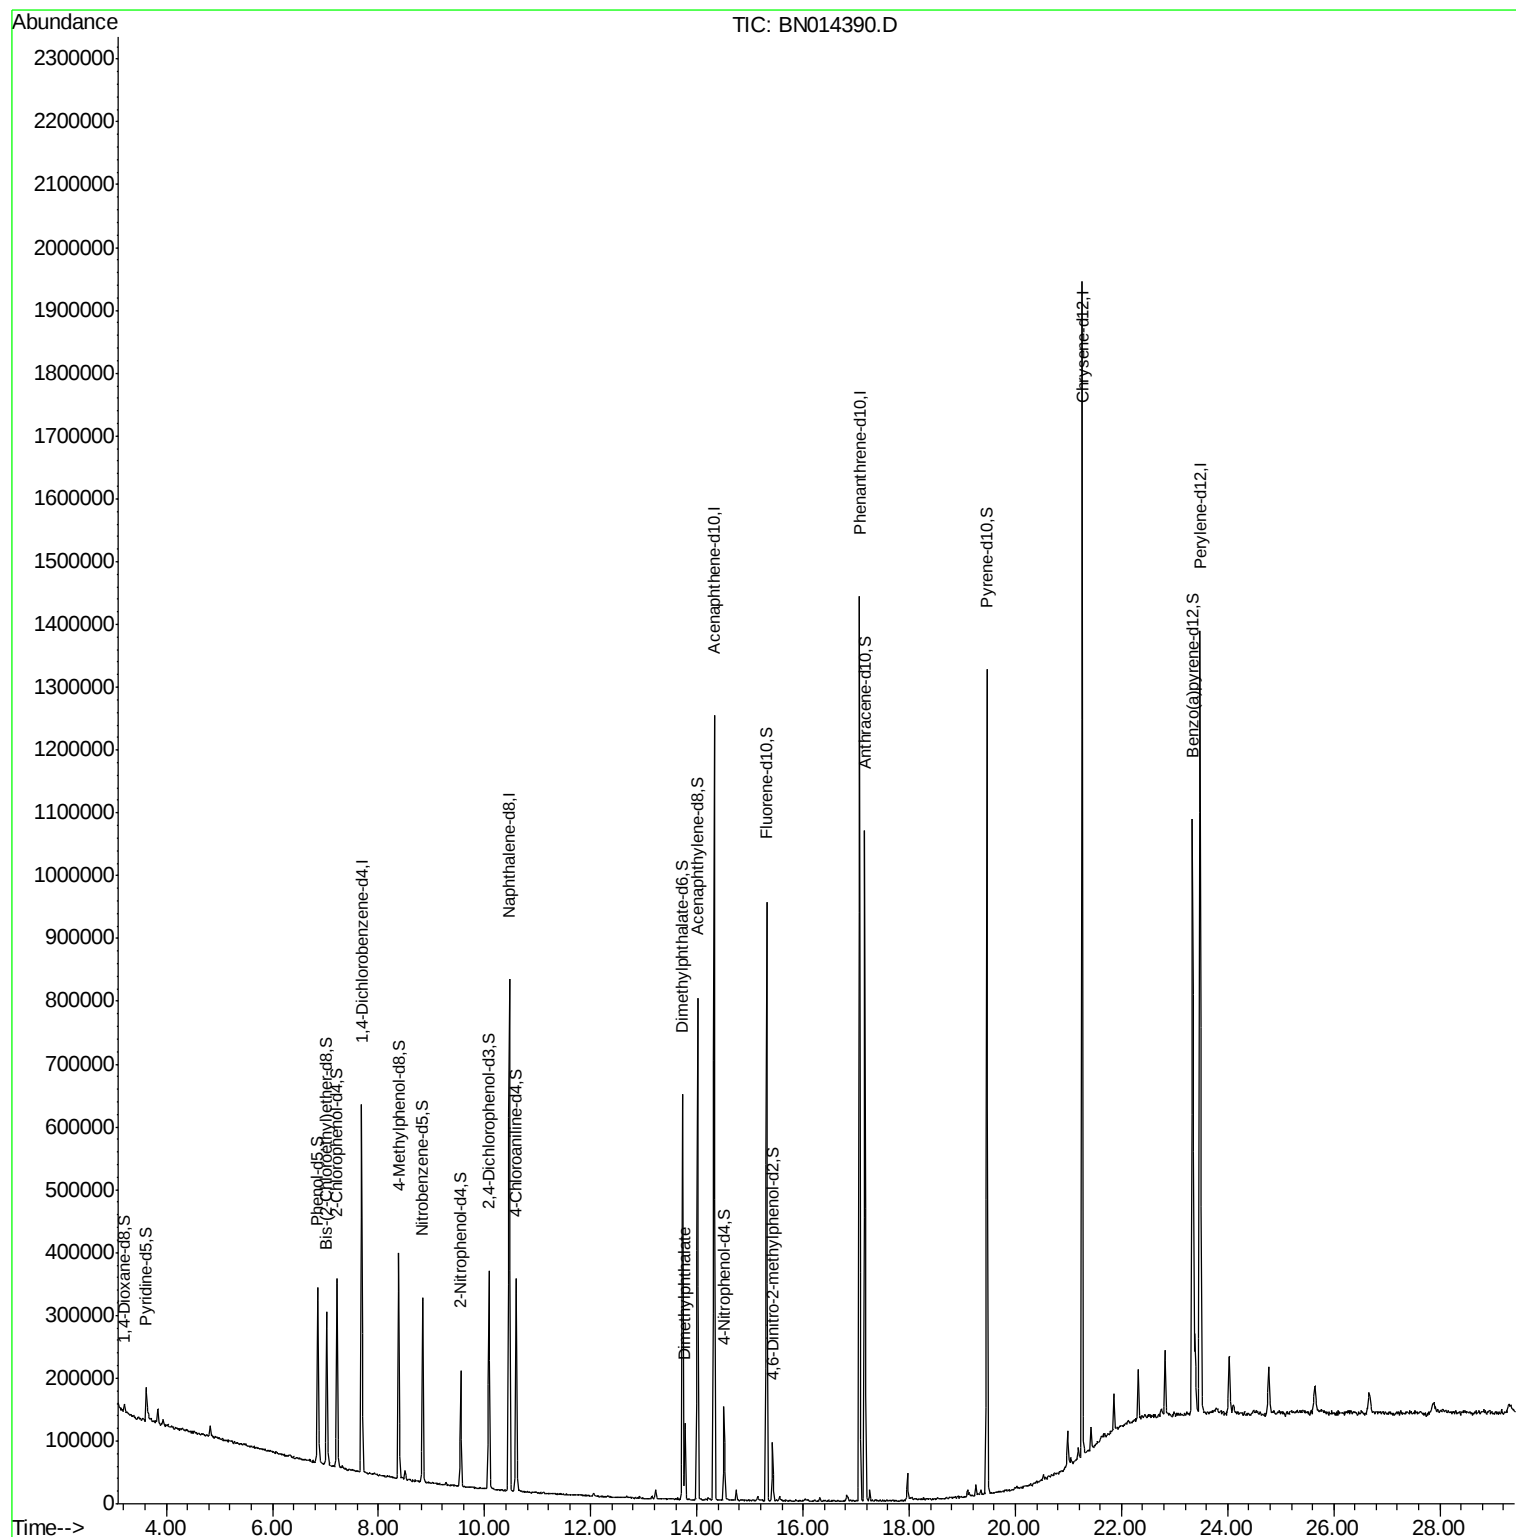

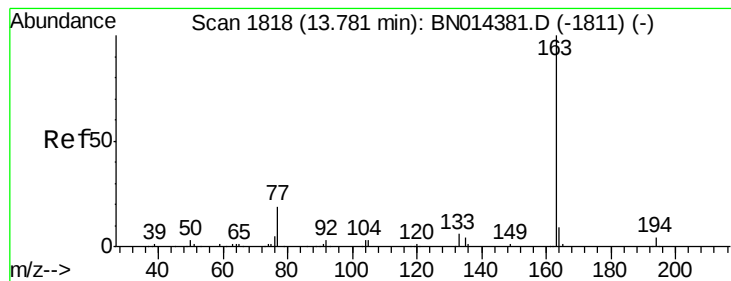

#47

Dimethylphthalate

Concen: 2.532 ng/ul

RT: 13.77 min Scan# 1817

Delta R.T. -0.01 min

Lab File: BN014390.D

Acq: 23 Apr 2021 22:49

Instrument :

BNA_N

ClientSampleId :

BG566


Tot Ion:163 Resp: 77232

Ion Ratio Lower Upper

163 100

194 4.0 3.3 4.9

164 9.6 7.8 11.8

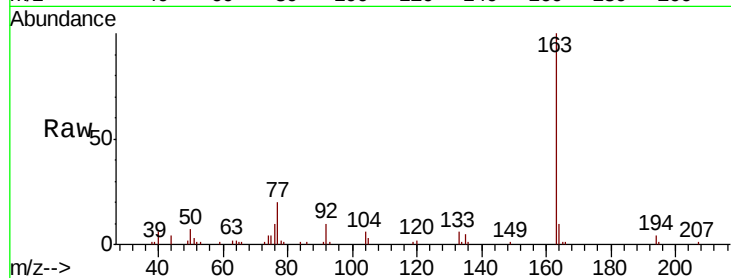

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

