

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042321\
 Data File : BN014374.D
 Acq On : 23 Apr 2021 11:46
 Operator : CG/JU
 Sample : PB135824BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK824

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.611	86	89	109	rBV	410374	653701	16.44%	1.718%
2	6.852	635	640	652	rVB	661117	1036172	26.07%	2.724%
3	7.022	664	669	686	rVB	568259	919692	23.14%	2.417%
4	7.222	696	703	716	rVB	710392	1135534	28.56%	2.985%
5	7.687	776	782	790	rVB	482449	770350	19.38%	2.025%
6	8.381	894	900	910	rBV	824499	1268278	31.90%	3.334%
7	8.834	970	977	988	rVB	684162	1121006	28.20%	2.947%
8	9.552	1092	1099	1108	rVB	445449	718793	18.08%	1.889%
9	10.081	1183	1189	1208	rVB	818889	1289233	32.43%	3.389%
10	10.463	1247	1254	1262	rVB	650616	1088288	27.38%	2.861%
11	10.593	1270	1276	1288	rBV	844744	1392668	35.03%	3.661%
12	12.051	1520	1524	1532	rVB2	10687	17116	0.43%	0.045%
13	13.734	1804	1810	1820	rVB	1522471	2009728	50.56%	5.283%
14	14.010	1850	1857	1864	rBV	1882010	2635384	66.29%	6.927%
15	14.322	1903	1910	1917	rBV	965157	1389277	34.95%	3.652%
16	14.516	1937	1943	1953	rBV	549403	735973	18.51%	1.935%
17	15.316	2072	2079	2087	rBB	2242059	3077767	77.42%	8.090%
18	15.434	2093	2099	2109	rBV	426309	585571	14.73%	1.539%
19	15.557	2115	2120	2125	rVB2	19912	25342	0.64%	0.067%
20	16.104	2209	2213	2219	rVB2	4489	5438	0.14%	0.014%
21	17.069	2370	2377	2384	rVB	1117357	1562330	39.30%	4.107%
22	17.163	2387	2393	2408	rVB	2358974	3328340	83.73%	8.749%
23	19.098	2718	2722	2728	rVB2	14721	18504	0.47%	0.049%
24	19.351	2759	2765	2770	rBV	13320	18687	0.47%	0.049%
25	19.469	2779	2785	2795	rBV	2848230	3902567	98.17%	10.258%
26	21.263	3085	3090	3097	rBV	1361594	1641274	41.29%	4.314%
27	23.345	3437	3444	3459	rBV	2206575	3975303	100.00%	10.449%
28	23.486	3461	3468	3480	rVB2	948546	1721953	43.32%	4.526%


Sum of corrected areas: 38044269

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042321\
Data File : BN014374.D
Acq On : 23 Apr 2021 11:46
Operator : CG/JU
Sample : PB135824BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK824

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

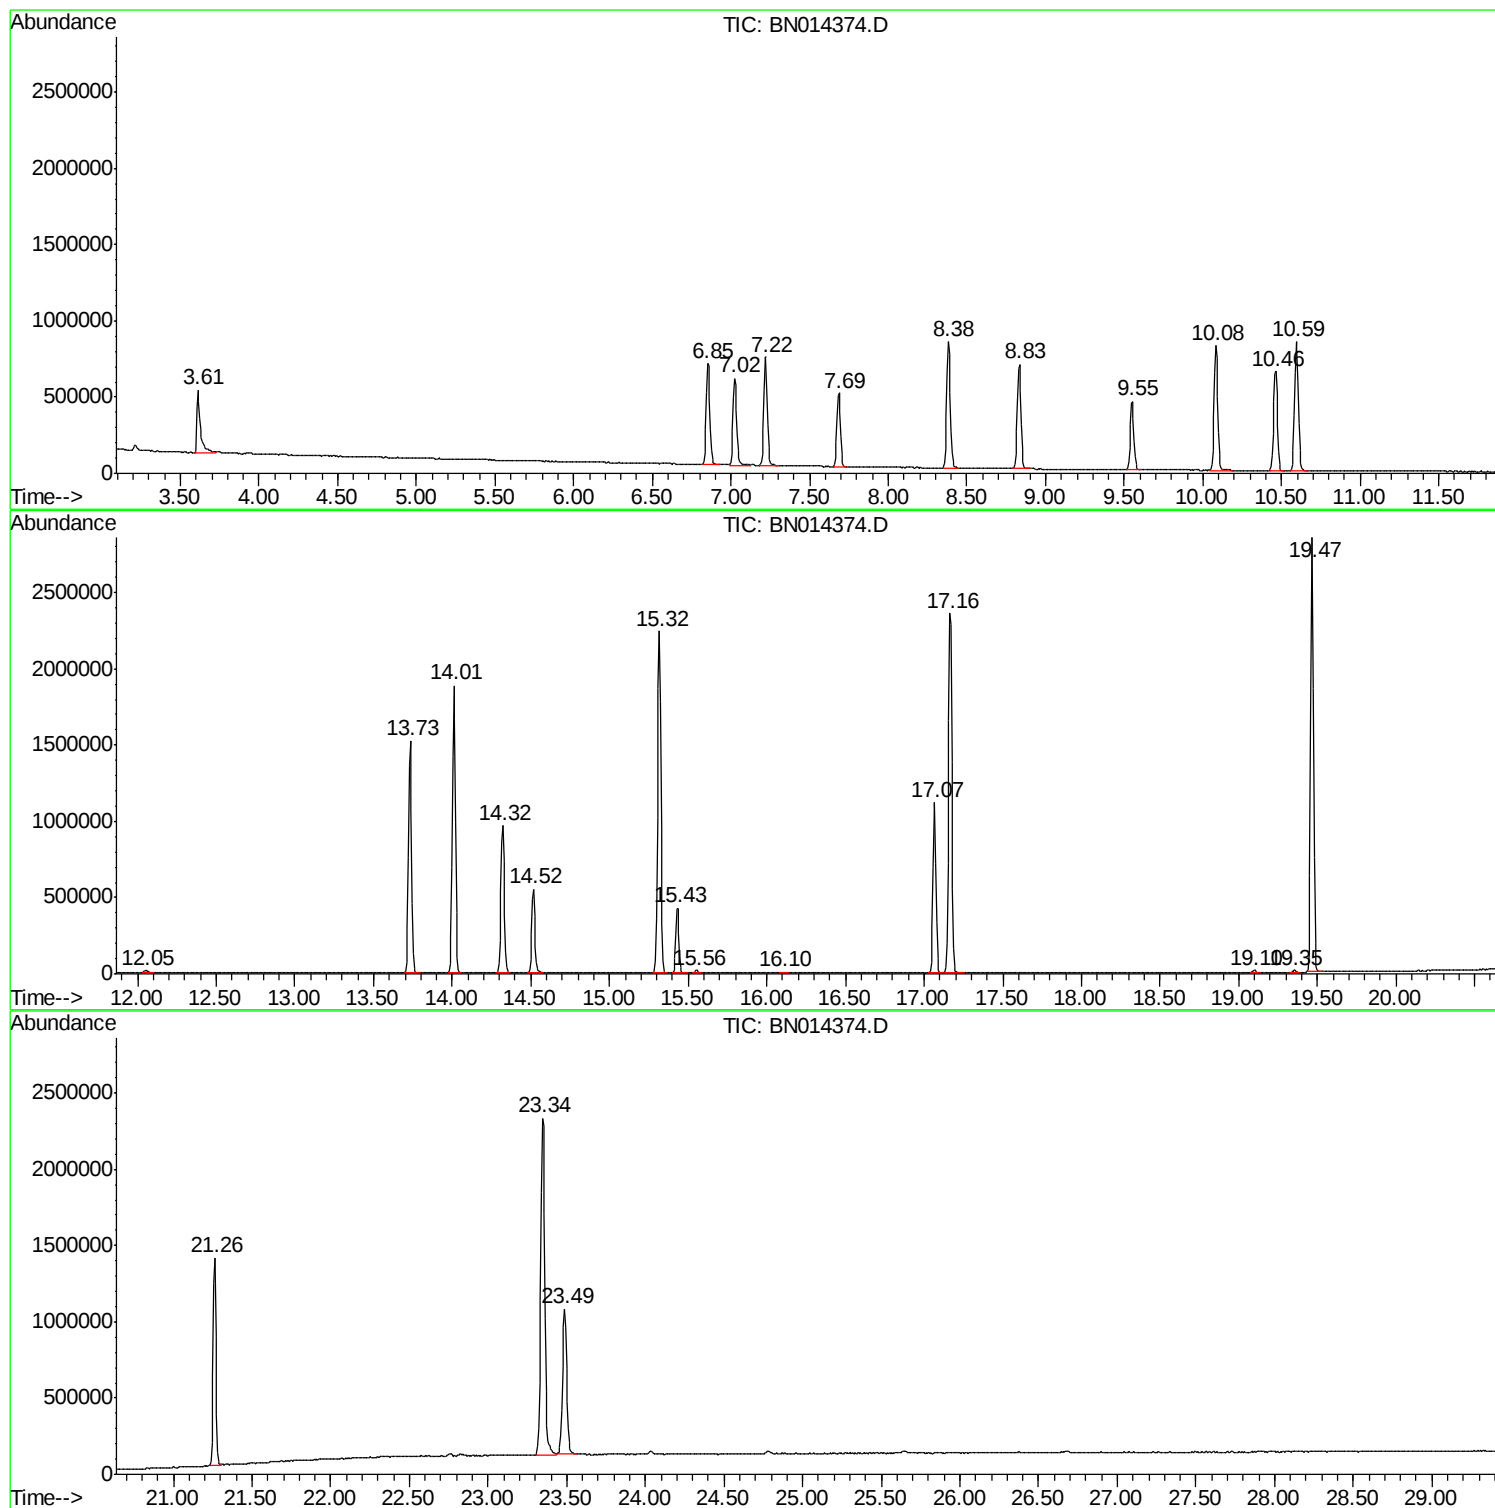

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
Data File : BN014374.D
Acq On : 23 Apr 2021 11:46
Operator : CG/JU
Sample : PB135824BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK824

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
Data File : BN014374.D
Acq On : 23 Apr 2021 11:46
Operator : CG/JU
Sample : PB135824BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK824

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc