

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042321\
 Data File : BN014382.D
 Acq On : 23 Apr 2021 18:03
 Operator : CG/JU
 Sample : M2065-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG4Z8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.628	90	92	97	rBV2	31368	46962	2.19%	0.215%
2	6.852	635	640	653	rVB	215864	369259	17.19%	1.691%
3	7.022	664	669	679	rVB	201185	315745	14.70%	1.446%
4	7.216	697	702	711	rVB	232252	372823	17.36%	1.707%
5	7.687	776	782	789	rVB	473173	750193	34.92%	3.435%
6	8.381	894	900	907	rBV	264384	403598	18.79%	1.848%
7	8.499	918	920	927	rVB3	13567	18480	0.86%	0.085%
8	8.828	970	976	987	rVB	227203	378907	17.64%	1.735%
9	9.269	1048	1051	1055	rVB2	7434	11180	0.52%	0.051%
10	9.552	1093	1099	1105	rVB	125926	204688	9.53%	0.937%
11	10.081	1182	1189	1199	rBV	245937	393560	18.32%	1.802%
12	10.463	1246	1254	1266	rBV	631348	1066676	49.66%	4.884%
13	10.593	1270	1276	1288	rVB	196138	333792	15.54%	1.528%
14	12.051	1521	1524	1528	rVB4	4171	7049	0.33%	0.032%
15	12.757	1643	1644	1650	rVB4	1747	2168	0.10%	0.010%
16	12.816	1650	1654	1660	rVV3	2289	3428	0.16%	0.016%
17	12.857	1660	1661	1668	rVB4	2152	3753	0.17%	0.017%
18	12.922	1668	1672	1676	rBV6	3020	5132	0.24%	0.023%
19	13.110	1700	1704	1705	rBV3	2057	2501	0.12%	0.011%
20	13.157	1708	1712	1716	rVV2	5182	7424	0.35%	0.034%
21	13.222	1720	1723	1726	rBV3	3099	3788	0.18%	0.017%
22	13.287	1732	1734	1739	rVB6	1569	2295	0.11%	0.011%
23	13.634	1790	1793	1798	rBV4	3679	5235	0.24%	0.024%
24	13.728	1803	1809	1815	rBV	457710	650154	30.27%	2.977%
25	13.775	1815	1817	1822	rVB	27948	33468	1.56%	0.153%
26	13.863	1830	1832	1834	rBV2	2433	2561	0.12%	0.012%
27	14.010	1848	1857	1870	rBV	596141	870046	40.50%	3.984%
28	14.116	1874	1875	1878	rVV2	4361	3198	0.15%	0.015%
29	14.157	1878	1882	1889	rVB4	8353	12877	0.60%	0.059%
30	14.240	1889	1896	1899	rBV4	4118	8271	0.39%	0.038%
31	14.322	1899	1910	1917	rBV	932334	1363229	63.46%	6.242%
32	14.381	1917	1920	1925	rVV	13252	19010	0.88%	0.087%
33	14.516	1936	1943	1950	rBV	69542	113310	5.28%	0.519%
34	14.716	1974	1977	1978	rBV3	4431	4665	0.22%	0.021%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042321\
 Data File : BN014382.D
 Acq On : 23 Apr 2021 18:03
 Operator : CG/JU
 Sample : M2065-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG4Z8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

35	14.740	1978	1981	1984	rVB3	7494	10560	0.49%	0.048%
36	14.857	1999	2001	2004	rBV4	3079	3030	0.14%	0.014%
37	14.951	2009	2017	2020	rBV6	4081	10818	0.50%	0.050%
38	14.987	2020	2023	2027	rVB3	4572	6519	0.30%	0.030%
39	15.051	2030	2034	2040	rVB6	3035	5744	0.27%	0.026%
40	15.116	2040	2045	2047	rBV4	8478	11085	0.52%	0.051%
41	15.145	2047	2050	2054	rVB4	9953	12503	0.58%	0.057%
42	15.192	2054	2058	2060	rBV4	2417	3467	0.16%	0.016%
43	15.316	2073	2079	2085	rBV	777725	1040198	48.43%	4.763%
44	15.369	2085	2088	2092	rVV	7067	8157	0.38%	0.037%
45	15.428	2093	2098	2103	rVV	54504	76571	3.56%	0.351%
46	15.498	2106	2110	2112	rVB5	4130	5903	0.27%	0.027%
47	15.551	2112	2119	2123	rBV5	7466	13803	0.64%	0.063%
48	15.581	2123	2124	2129	rVB4	2557	3167	0.15%	0.015%
49	15.669	2135	2139	2142	rBV3	4632	7265	0.34%	0.033%
50	15.810	2160	2163	2170	rBV5	6491	11955	0.56%	0.055%
51	15.969	2186	2190	2193	rBV4	3939	7146	0.33%	0.033%
52	16.039	2199	2202	2205	rBV5	5254	7996	0.37%	0.037%
53	16.104	2211	2213	2218	rVB6	4753	5972	0.28%	0.027%
54	16.163	2218	2223	2225	rBV3	5014	6596	0.31%	0.030%
55	16.186	2225	2227	2229	rVB2	4876	3829	0.18%	0.018%
56	16.228	2229	2234	2237	rBV5	6113	10644	0.50%	0.049%
57	16.281	2240	2243	2246	rVV5	4471	4561	0.21%	0.021%
58	16.316	2246	2249	2254	rVV5	7571	11974	0.56%	0.055%
59	16.375	2254	2259	2261	rVV6	6494	9522	0.44%	0.044%
60	16.428	2264	2268	2271	rVB4	9144	12013	0.56%	0.055%
61	16.475	2272	2276	2280	rBV6	7580	11822	0.55%	0.054%
62	16.604	2296	2298	2299	rBV2	4484	3358	0.16%	0.015%
63	16.645	2303	2305	2310	rVB5	5838	6253	0.29%	0.029%
64	16.722	2312	2318	2320	rBV6	8326	15878	0.74%	0.073%
65	16.822	2328	2335	2342	rBV9	16440	39464	1.84%	0.181%
66	16.886	2343	2346	2354	rVB5	10473	21279	0.99%	0.097%
67	17.063	2370	2376	2381	rBV	1106963	1601422	74.55%	7.333%
68	17.104	2381	2383	2388	rVV	120262	158814	7.39%	0.727%
69	17.163	2388	2393	2405	rVB	806604	1155780	53.81%	5.292%
70	17.257	2405	2409	2415	rBV6	11973	24113	1.12%	0.110%
71	17.439	2438	2440	2442	rBV3	4587	3735	0.17%	0.017%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
 Data File : BN014382.D
 Acq On : 23 Apr 2021 18:03
 Operator : CG/JU
 Sample : M2065-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG4Z8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

72	17.469	2443	2445	2447	rBV2	5605	6314	0.29%	0.029%
73	17.645	2473	2475	2479	rVB3	7736	8428	0.39%	0.039%
74	17.851	2508	2510	2514	rBV5	6224	9335	0.43%	0.043%
75	17.939	2522	2525	2527	rBV	21155	25585	1.19%	0.117%
76	17.969	2527	2530	2539	rVB3	77944	145197	6.76%	0.665%
77	18.139	2554	2559	2563	rBV2	42401	67917	3.16%	0.311%
78	18.445	2608	2611	2614	rBV	27278	32800	1.53%	0.150%
79	18.480	2614	2617	2620	rVV3	18991	23324	1.09%	0.107%
80	18.698	2651	2654	2659	rVB5	27206	33325	1.55%	0.153%
81	18.745	2659	2662	2665	rBV2	13986	17118	0.80%	0.078%
82	18.869	2679	2683	2687	rBV	31786	46430	2.16%	0.213%
83	19.004	2703	2706	2709	rBV2	17810	24945	1.16%	0.114%
84	19.128	2722	2727	2733	rVB	595740	773127	35.99%	3.540%
85	19.257	2746	2749	2756	rBV2	46569	60728	2.83%	0.278%
86	19.463	2779	2784	2787	rBV	1032383	1494322	69.57%	6.843%
87	19.492	2787	2789	2799	rVB	462201	558869	26.02%	2.559%
88	19.992	2871	2874	2878	rVB	71401	85181	3.97%	0.390%
89	20.092	2888	2891	2895	rVB	50613	58413	2.72%	0.267%
90	20.992	3040	3044	3048	rBV3	92220	136339	6.35%	0.624%
91	21.186	3075	3077	3081	rVB	73752	67593	3.15%	0.310%
92	21.257	3084	3089	3094	rVV	1472544	2148035	100.00%	9.836%
93	21.298	3094	3096	3104	rVB	233968	269100	12.53%	1.232%
94	22.821	3351	3355	3368	rVB2	301094	673000	31.33%	3.082%
95	23.345	3438	3444	3449	rBV	643683	1114588	51.89%	5.104%
96	23.486	3462	3468	3477	rVB2	987456	1816132	84.55%	8.316%


Sum of corrected areas: 21838486

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
Data File : BN014382.D
Acq On : 23 Apr 2021 18:03
Operator : CG/JU
Sample : M2065-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG4Z8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

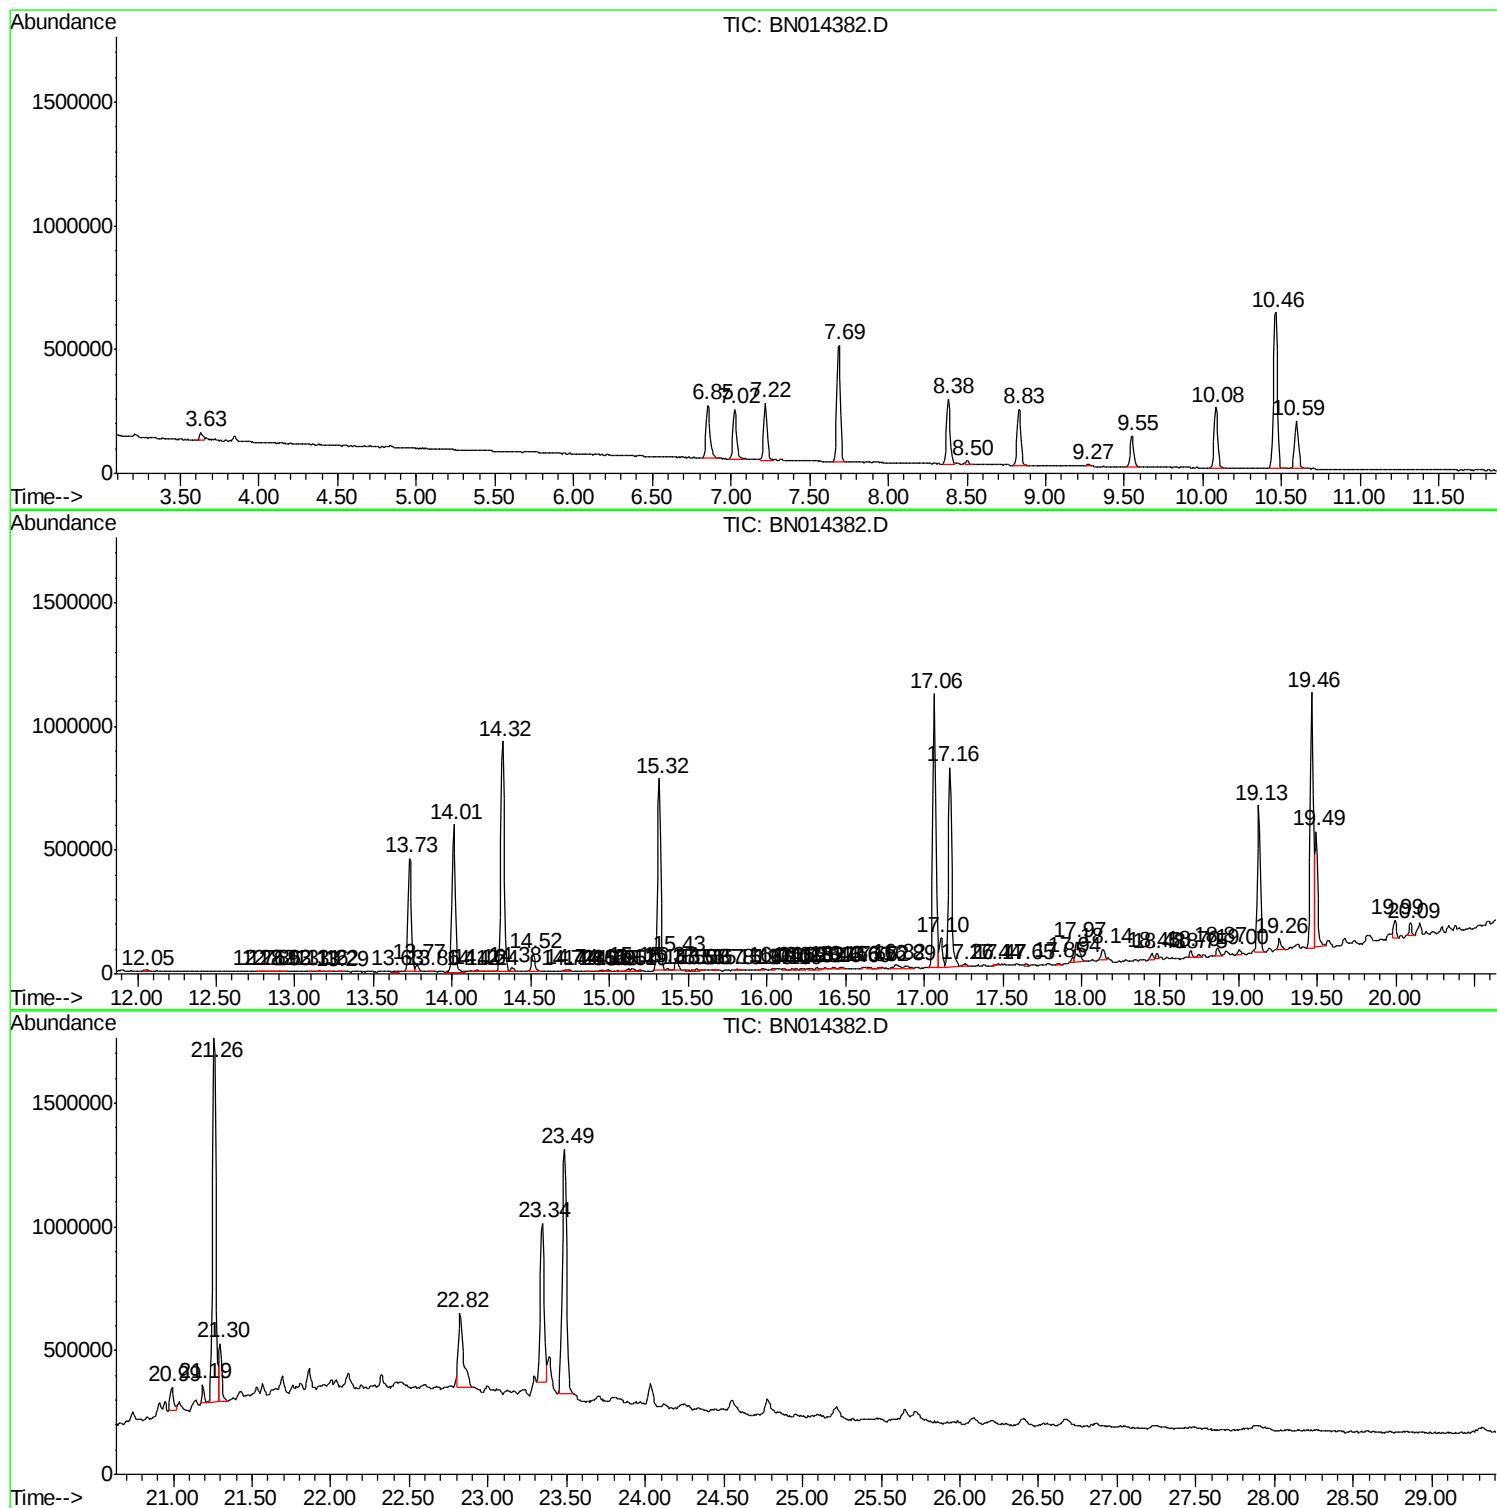

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
Data File : BN014382.D
Acq On : 23 Apr 2021 18:03
Operator : CG/JU
Sample : M2065-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG4Z8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
Data File : BN014382.D
Acq On : 23 Apr 2021 18:03
Operator : CG/JU
Sample : M2065-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG4Z8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc