

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042321\
 Data File : BN014384.D
 Acq On : 23 Apr 2021 19:15
 Operator : CG/JU
 Sample : M2065-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG564

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.628	90	92	100	rBV2	23699	43084	2.37%	0.221%
2	6.852	635	640	654	rVB	220364	366183	20.16%	1.874%
3	7.022	664	669	676	rVB	197786	305952	16.85%	1.566%
4	7.216	697	702	714	rVB	240540	391247	21.54%	2.003%
5	7.687	776	782	791	rVB	456554	733232	40.37%	3.753%
6	8.381	894	900	907	rBV	276777	424503	23.37%	2.173%
7	8.499	917	920	926	rVB2	14406	22053	1.21%	0.113%
8	8.828	970	976	985	rVB	232010	384431	21.17%	1.968%
9	9.004	1003	1006	1009	rBV4	5397	5574	0.31%	0.029%
10	9.551	1093	1099	1106	rBV	130769	215841	11.88%	1.105%
11	9.651	1114	1116	1119	rVB4	3761	4254	0.23%	0.022%
12	10.081	1183	1189	1197	rBV	266597	413410	22.76%	2.116%
13	10.457	1246	1253	1260	rBV	632958	1061572	58.45%	5.434%
14	10.510	1260	1262	1267	rVV	9026	9718	0.54%	0.050%
15	10.593	1270	1276	1289	rVB	242536	412289	22.70%	2.110%
16	10.957	1334	1338	1342	rVB4	4779	7095	0.39%	0.036%
17	11.234	1378	1385	1387	rBV7	2917	4947	0.27%	0.025%
18	11.398	1411	1413	1418	rVB4	2970	4699	0.26%	0.024%
19	11.504	1426	1431	1434	rBV3	8280	11989	0.66%	0.061%
20	11.657	1452	1457	1463	rVB5	3507	6460	0.36%	0.033%
21	11.757	1472	1474	1479	rVB5	5735	7627	0.42%	0.039%
22	12.045	1516	1523	1529	rVV6	6812	12761	0.70%	0.065%
23	12.104	1529	1533	1534	rVV3	3007	4385	0.24%	0.022%
24	12.122	1534	1536	1543	rVB3	6001	10159	0.56%	0.052%
25	12.198	1543	1549	1550	rBV3	3671	4961	0.27%	0.025%
26	12.210	1550	1551	1557	rVB5	3844	4290	0.24%	0.022%
27	12.351	1570	1575	1579	rVB5	3954	5201	0.29%	0.027%
28	12.681	1626	1631	1632	rBV5	3710	4747	0.26%	0.024%
29	12.728	1636	1639	1641	rVV3	2859	4305	0.24%	0.022%
30	12.757	1641	1644	1647	rVV5	5208	9044	0.50%	0.046%
31	12.822	1651	1655	1659	rVV5	4447	9086	0.50%	0.047%
32	12.869	1659	1663	1667	rVV3	13351	21538	1.19%	0.110%
33	12.922	1667	1672	1681	rVB4	8137	17198	0.95%	0.088%
34	13.104	1695	1703	1706	rBV7	5793	12024	0.66%	0.062%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042321\
 Data File : BN014384.D
 Acq On : 23 Apr 2021 19:15
 Operator : CG/JU
 Sample : M2065-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG564

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

35	13.151	1706	1711	1715	rVB6	4619	10439	0.57%	0.053%
36	13.287	1730	1734	1737	rBV5	3572	4518	0.25%	0.023%
37	13.322	1737	1740	1747	rVB7	4491	7412	0.41%	0.038%
38	13.387	1749	1751	1758	rVB5	2654	3979	0.22%	0.020%
39	13.469	1760	1765	1768	rBV7	2914	3894	0.21%	0.020%
40	13.540	1773	1777	1778	rBV3	4250	5456	0.30%	0.028%
41	13.581	1781	1784	1789	rBV7	3131	4631	0.25%	0.024%
42	13.645	1789	1795	1797	rBV5	5171	7583	0.42%	0.039%
43	13.681	1799	1801	1804	rVB3	3626	3715	0.20%	0.019%
44	13.728	1804	1809	1814	rBV	510854	738757	40.68%	3.781%
45	13.775	1814	1817	1822	rVV	83495	113779	6.27%	0.582%
46	13.816	1822	1824	1828	rVB	16483	19745	1.09%	0.101%
47	13.863	1828	1832	1840	rVB7	9395	17593	0.97%	0.090%
48	13.934	1842	1844	1848	rVB5	3812	4331	0.24%	0.022%
49	14.010	1848	1857	1863	rBV	634484	924242	50.89%	4.731%
50	14.069	1863	1867	1869	rBV4	3463	4112	0.23%	0.021%
51	14.157	1877	1882	1890	rVB3	22408	41969	2.31%	0.215%
52	14.228	1890	1894	1899	rBV7	8294	17606	0.97%	0.090%
53	14.322	1899	1910	1918	rVV	920401	1379725	75.97%	7.062%
54	14.510	1936	1942	1950	rBV	72750	121222	6.67%	0.620%
55	14.663	1961	1968	1970	rBV6	4625	8910	0.49%	0.046%
56	14.739	1977	1981	1985	rVB5	15468	19632	1.08%	0.100%
57	14.863	1996	2002	2008	rVB6	9041	17987	0.99%	0.092%
58	14.939	2008	2015	2016	rBV7	4251	7737	0.43%	0.040%
59	14.957	2016	2018	2019	rVV2	4240	3706	0.20%	0.019%
60	14.986	2019	2023	2026	rVB5	7123	11021	0.61%	0.056%
61	15.051	2026	2034	2040	rBV7	7633	16682	0.92%	0.085%
62	15.122	2040	2046	2054	rBV4	11690	24774	1.36%	0.127%
63	15.198	2055	2059	2060	rVB4	4110	4381	0.24%	0.022%
64	15.316	2072	2079	2085	rBV	787066	1109682	61.10%	5.680%
65	15.369	2085	2088	2091	rVV4	5813	8986	0.49%	0.046%
66	15.398	2091	2093	2094	rVV2	4289	4190	0.23%	0.021%
67	15.428	2094	2098	2104	rVV	37896	58109	3.20%	0.297%
68	15.551	2113	2119	2122	rBV3	7548	13793	0.76%	0.071%
69	15.598	2122	2127	2136	rVB6	11142	24132	1.33%	0.124%
70	15.692	2136	2143	2144	rBV7	3920	6022	0.33%	0.031%
71	15.810	2159	2163	2167	rBV6	4829	7545	0.42%	0.039%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
 Data File : BN014384.D
 Acq On : 23 Apr 2021 19:15
 Operator : CG/JU
 Sample : M2065-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG564

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

72	15.934	2180	2184	2188	rVB6	6444	9882	0.54%	0.051%
73	15.992	2188	2194	2197	rBV7	5600	12725	0.70%	0.065%
74	16.075	2205	2208	2222	rVB4	25578	45312	2.50%	0.232%
75	16.181	2222	2226	2230	rBV7	6207	9527	0.52%	0.049%
76	16.316	2241	2249	2253	rBV6	8058	14178	0.78%	0.073%
77	16.351	2253	2255	2259	rVB4	2729	3835	0.21%	0.020%
78	16.422	2265	2267	2273	rBV6	6798	9564	0.53%	0.049%
79	16.633	2299	2303	2304	rBV4	4073	5025	0.28%	0.026%
80	16.728	2316	2319	2322	rBV5	5388	7639	0.42%	0.039%
81	16.898	2344	2348	2354	rVB5	21167	34256	1.89%	0.175%
82	17.069	2370	2377	2382	rBV	1046515	1533526	84.44%	7.849%
83	17.163	2387	2393	2405	rVB	836925	1164124	64.10%	5.958%
84	17.257	2406	2409	2415	rBV6	16714	28783	1.58%	0.147%
85	17.504	2448	2451	2454	rVB5	7958	10149	0.56%	0.052%
86	17.969	2526	2530	2537	rVB2	47880	65682	3.62%	0.336%
87	18.280	2580	2583	2587	rBV5	6693	12231	0.67%	0.063%
88	18.339	2591	2593	2598	rVV5	6230	9130	0.50%	0.047%
89	18.551	2626	2629	2634	rBV7	9291	12712	0.70%	0.065%
90	18.922	2688	2692	2697	rBV6	9577	20563	1.13%	0.105%
91	19.127	2724	2727	2732	rVB	48357	64281	3.54%	0.329%
92	19.257	2746	2749	2752	rBV4	25437	28514	1.57%	0.146%
93	19.463	2779	2784	2793	rBV	1007395	1445815	79.61%	7.400%
94	20.986	3040	3043	3050	rVB3	70598	109443	6.03%	0.560%
95	21.263	3084	3090	3095	rBV	1307517	1774911	97.73%	9.085%
96	21.863	3189	3192	3197	rVB	64683	78414	4.32%	0.401%
97	22.321	3267	3270	3274	rVB2	68846	80156	4.41%	0.410%
98	22.827	3352	3356	3361	rVB2	92225	141862	7.81%	0.726%
99	23.345	3438	3444	3449	rBV	698056	1251210	68.90%	6.404%
100	23.486	3462	3468	3487	rVB2	950638	1816102	100.00%	9.296%


Sum of corrected areas: 19537407

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042321\
Data File : BN014384.D
Acq On : 23 Apr 2021 19:15
Operator : CG/JU
Sample : M2065-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG564

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

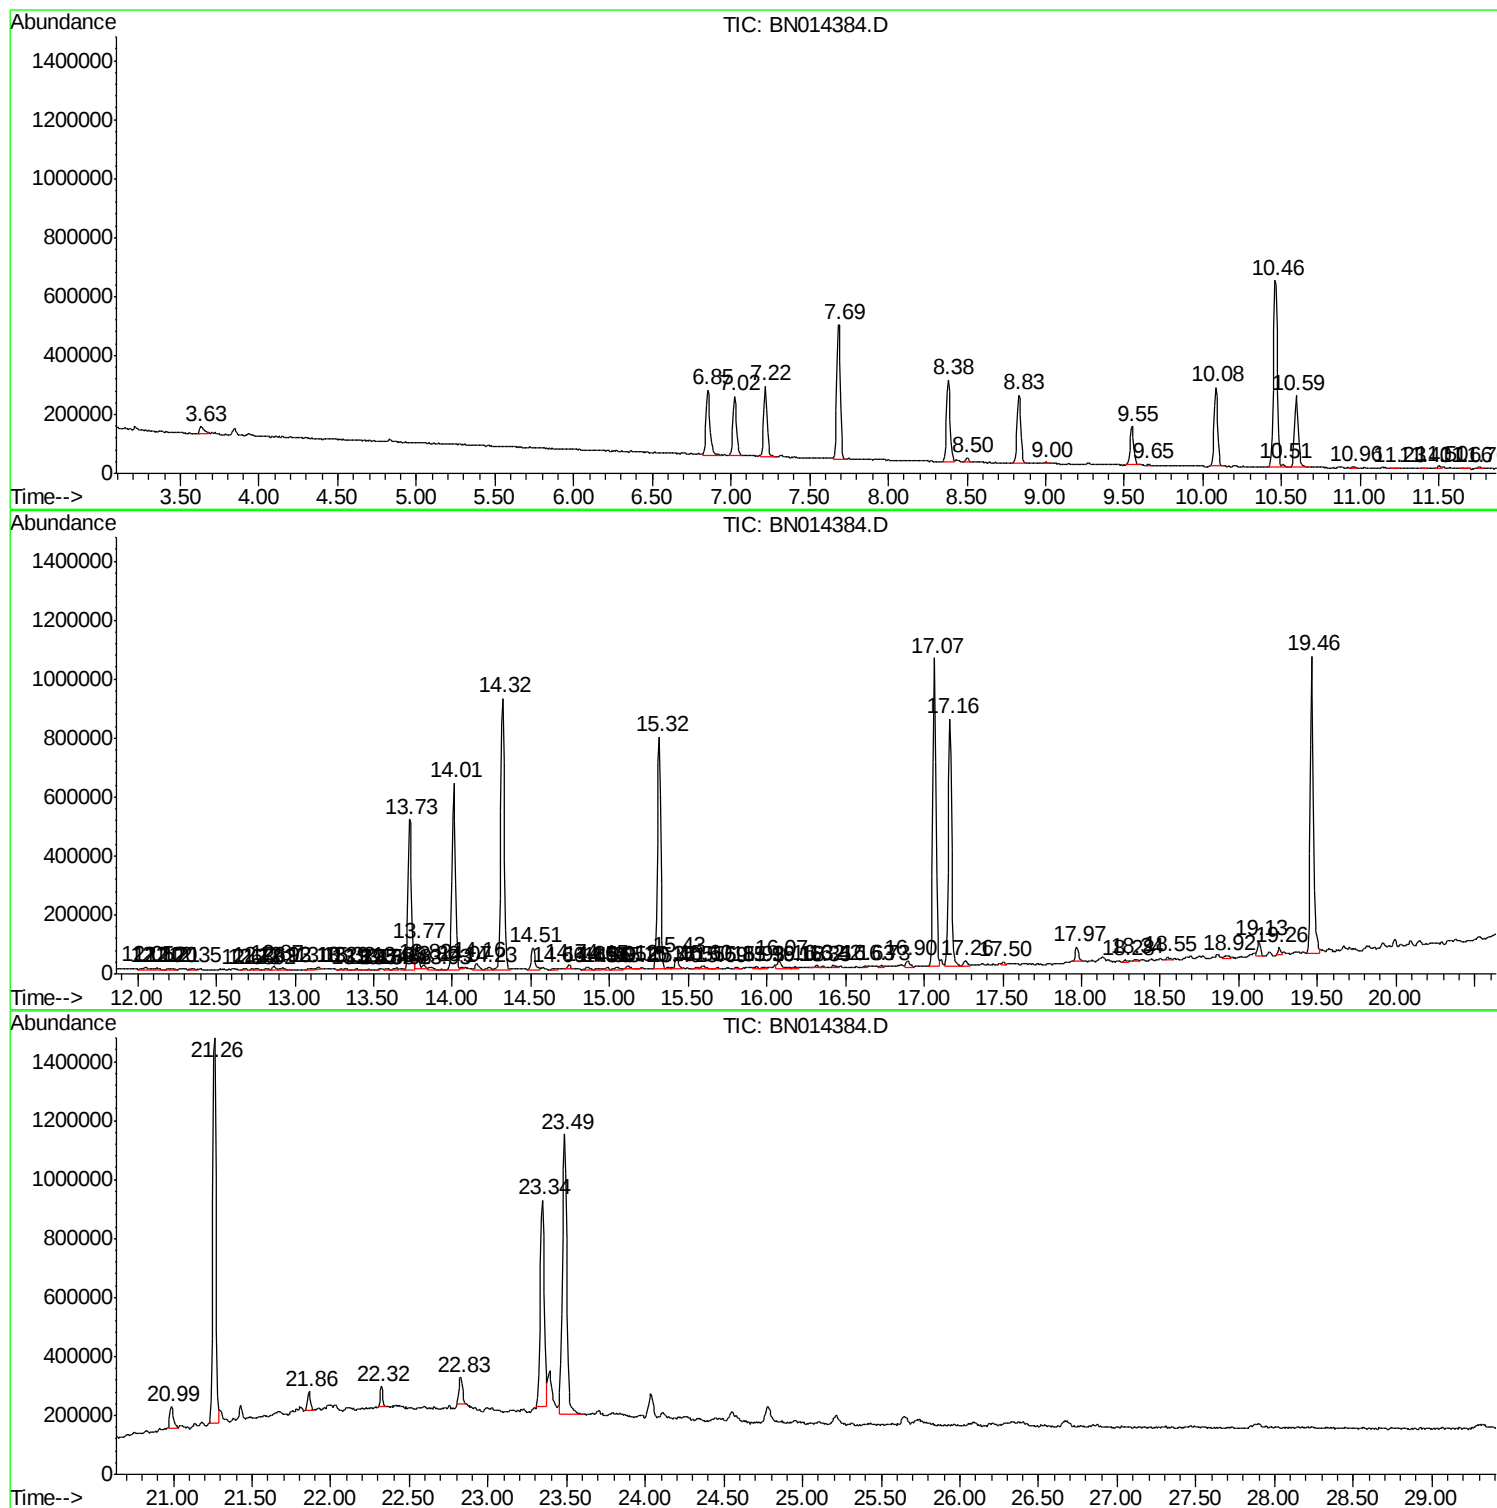

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
Data File : BN014384.D
Acq On : 23 Apr 2021 19:15
Operator : CG/JU
Sample : M2065-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG564

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
Data File : BN014384.D
Acq On : 23 Apr 2021 19:15
Operator : CG/JU
Sample : M2065-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG564

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc