

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042321\
 Data File : BN014385.D
 Acq On : 23 Apr 2021 19:51
 Operator : CG/JU
 Sample : M2065-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG562

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.628	90	92	101	rVB2	28998	49054	2.64%	0.223%
2	6.851	635	640	649	rVB	268418	442728	23.86%	2.013%
3	7.022	664	669	678	rVB	243934	386222	20.81%	1.756%
4	7.216	697	702	712	rVB	293225	469758	25.31%	2.136%
5	7.687	776	782	789	rVB	457238	733073	39.50%	3.333%
6	7.910	817	820	832	rVB6	21479	43885	2.36%	0.200%
7	8.228	872	874	879	rVB3	7962	9720	0.52%	0.044%
8	8.381	894	900	908	rBV	328429	511537	27.56%	2.326%
9	8.498	916	920	928	rVB2	22766	35024	1.89%	0.159%
10	8.828	970	976	984	rVB	287200	471184	25.39%	2.142%
11	8.998	1003	1005	1010	rBV4	4901	5144	0.28%	0.023%
12	9.275	1046	1052	1056	rVB3	8571	14943	0.81%	0.068%
13	9.551	1093	1099	1106	rBV	169283	283445	15.27%	1.289%
14	10.081	1182	1189	1197	rBV	322819	523402	28.20%	2.380%
15	10.204	1207	1210	1214	rVB3	3597	5315	0.29%	0.024%
16	10.463	1247	1254	1260	rVB	641545	1050043	56.58%	4.775%
17	10.592	1269	1276	1290	rVB	295494	527414	28.42%	2.398%
18	10.769	1303	1306	1310	rVB3	2650	3420	0.18%	0.016%
19	10.869	1320	1323	1329	rVB6	2985	4491	0.24%	0.020%
20	10.957	1334	1338	1344	rVB5	5673	10270	0.55%	0.047%
21	11.134	1365	1368	1370	rBV3	2396	3435	0.19%	0.016%
22	11.257	1382	1389	1393	rBV5	10068	17381	0.94%	0.079%
23	11.298	1393	1396	1400	rVB4	2269	3750	0.20%	0.017%
24	11.498	1425	1430	1435	rBV4	12443	22930	1.24%	0.104%
25	11.657	1452	1457	1460	rBV6	2940	4329	0.23%	0.020%
26	11.757	1470	1474	1479	rVB4	6762	11471	0.62%	0.052%
27	11.816	1482	1484	1490	rVB6	2486	3775	0.20%	0.017%
28	12.051	1518	1524	1528	rVV3	7579	14207	0.77%	0.065%
29	12.128	1532	1537	1542	rVB7	6914	15462	0.83%	0.070%
30	12.204	1544	1550	1558	rVB8	5333	14746	0.79%	0.067%
31	12.269	1558	1561	1564	rBV4	4658	5979	0.32%	0.027%
32	12.304	1564	1567	1570	rBV3	3717	3827	0.21%	0.017%
33	12.345	1570	1574	1579	rBV4	3945	7585	0.41%	0.034%
34	12.392	1579	1582	1589	rVB7	3530	6213	0.33%	0.028%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042321\
 Data File : BN014385.D
 Acq On : 23 Apr 2021 19:51
 Operator : CG/JU
 Sample : M2065-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG562

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

35	12.545	1598	1608	1610	rBV10	4413	10360	0.56%	0.047%
36	12.604	1610	1618	1620	rBV6	3296	6139	0.33%	0.028%
37	12.681	1627	1631	1634	rBV5	4001	5407	0.29%	0.025%
38	12.757	1640	1644	1649	rVB6	8564	13512	0.73%	0.061%
39	12.828	1651	1656	1658	rVV5	4113	7355	0.40%	0.033%
40	12.869	1658	1663	1667	rVB	22423	32395	1.75%	0.147%
41	12.916	1667	1671	1677	rVB5	8311	14864	0.80%	0.068%
42	13.104	1696	1703	1706	rBV7	11080	19638	1.06%	0.089%
43	13.139	1706	1709	1711	rVV3	5093	7674	0.41%	0.035%
44	13.181	1714	1716	1719	rVB4	5472	6089	0.33%	0.028%
45	13.216	1719	1722	1724	rBV4	3941	4979	0.27%	0.023%
46	13.292	1731	1735	1737	rBV5	3906	5328	0.29%	0.024%
47	13.322	1737	1740	1746	rVB5	8256	12383	0.67%	0.056%
48	13.386	1746	1751	1757	rBV9	5805	14816	0.80%	0.067%
49	13.469	1757	1765	1768	rBV10	5920	9857	0.53%	0.045%
50	13.539	1773	1777	1781	rBV5	4462	7664	0.41%	0.035%
51	13.592	1783	1786	1789	rBV6	3712	5013	0.27%	0.023%
52	13.645	1792	1795	1797	rBV4	4390	5064	0.27%	0.023%
53	13.728	1804	1809	1815	rBV	614748	903494	48.69%	4.108%
54	13.775	1815	1817	1821	rVV	52591	66790	3.60%	0.304%
55	13.816	1821	1824	1829	rVV2	39135	55153	2.97%	0.251%
56	13.863	1829	1832	1837	rVV7	8803	16164	0.87%	0.073%
57	14.010	1848	1857	1864	rBV	745227	1123101	60.52%	5.107%
58	14.069	1864	1867	1870	rVV4	8295	15072	0.81%	0.069%
59	14.104	1870	1873	1874	rVV3	8447	10975	0.59%	0.050%
60	14.157	1878	1882	1890	rVB4	27164	50488	2.72%	0.230%
61	14.228	1890	1894	1900	rBV7	12177	25865	1.39%	0.118%
62	14.322	1901	1910	1919	rVB	933144	1391702	74.99%	6.328%
63	14.433	1924	1929	1930	rBV5	4267	6030	0.32%	0.027%
64	14.516	1937	1943	1951	rBV	112907	187499	10.10%	0.853%
65	14.575	1951	1953	1957	rVB5	6369	7480	0.40%	0.034%
66	14.657	1959	1967	1971	rBV6	7797	18114	0.98%	0.082%
67	14.739	1976	1981	1985	rVV7	19595	29515	1.59%	0.134%
68	14.863	1997	2002	2008	rBV6	17339	27911	1.50%	0.127%
69	14.986	2020	2023	2028	rVB4	12222	18023	0.97%	0.082%
70	15.051	2030	2034	2039	rBV6	9679	14793	0.80%	0.067%
71	15.116	2040	2045	2048	rBV3	15333	24893	1.34%	0.113%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
 Data File : BN014385.D
 Acq On : 23 Apr 2021 19:51
 Operator : CG/JU
 Sample : M2065-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG562

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION




72	15.145	2048	2050	2054	rVB2	9127	11117	0.60%	0.051%
73	15.316	2073	2079	2085	rVB	965447	1365931	73.61%	6.211%
74	15.375	2085	2089	2091	rBV5	7744	8898	0.48%	0.040%
75	15.427	2093	2098	2104	rVB	75722	106252	5.73%	0.483%
76	15.492	2107	2109	2112	rVB2	11005	10137	0.55%	0.046%
77	15.533	2112	2116	2118	rBV	12114	18045	0.97%	0.082%
78	15.598	2122	2127	2131	rBV2	30443	50311	2.71%	0.229%
79	15.751	2148	2153	2159	rBV9	6384	15939	0.86%	0.072%
80	15.839	2165	2168	2170	rVB3	6817	7533	0.41%	0.034%
81	15.886	2174	2176	2181	rVV6	5926	9840	0.53%	0.045%
82	16.075	2201	2208	2212	rBV	59820	96030	5.17%	0.437%
83	16.180	2220	2226	2227	rBV5	11332	18862	1.02%	0.086%
84	16.222	2231	2233	2236	rVV3	9774	10418	0.56%	0.047%
85	16.322	2246	2250	2253	rVV2	19773	27038	1.46%	0.123%
86	16.363	2253	2257	2260	rVB	17857	22622	1.22%	0.103%
87	16.422	2265	2267	2272	rVV5	18469	27475	1.48%	0.125%
88	16.474	2272	2276	2285	rVB4	20571	38369	2.07%	0.174%
89	16.816	2332	2334	2337	rVB3	13649	13303	0.72%	0.060%
90	16.898	2344	2348	2355	rVB	47130	79749	4.30%	0.363%
91	17.063	2370	2376	2387	rBV	1060029	1582596	85.28%	7.196%
92	17.163	2387	2393	2402	rVB	977746	1394520	75.15%	6.341%
93	17.969	2527	2530	2536	rVB4	44242	62022	3.34%	0.282%
94	19.127	2724	2727	2735	rVB	57696	84929	4.58%	0.386%
95	19.463	2779	2784	2797	rBV	1152381	1695587	91.37%	7.710%
96	20.986	3040	3043	3051	rVB2	80341	118395	6.38%	0.538%
97	21.186	3074	3077	3081	rBV	135588	158088	8.52%	0.719%
98	21.262	3085	3090	3094	rBV	1373368	1717480	92.55%	7.809%
99	23.345	3438	3444	3450	rBV	771516	1488537	80.21%	6.768%
100	23.486	3462	3468	3483	rVB2	923670	1855751	100.00%	8.438%

Sum of corrected areas: 21992535

Instrument :
BNA_N
ClientSampleId :
BG562

Quant Method : Z:\SV0ASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SV0A CALIBRATION

```
TIC Library      : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P
```

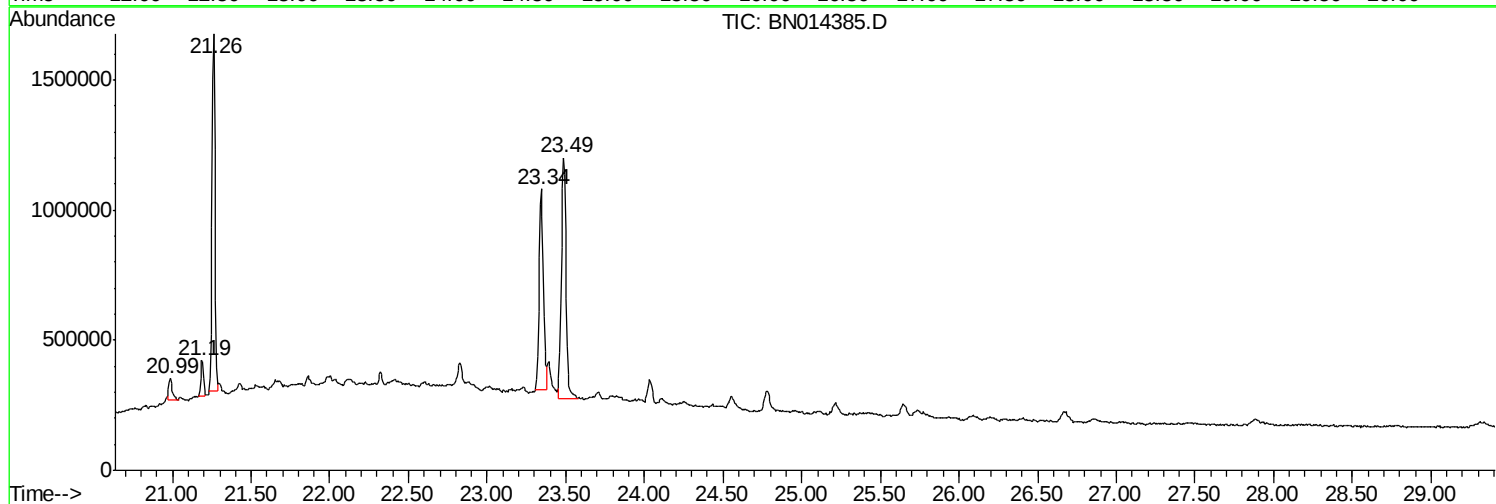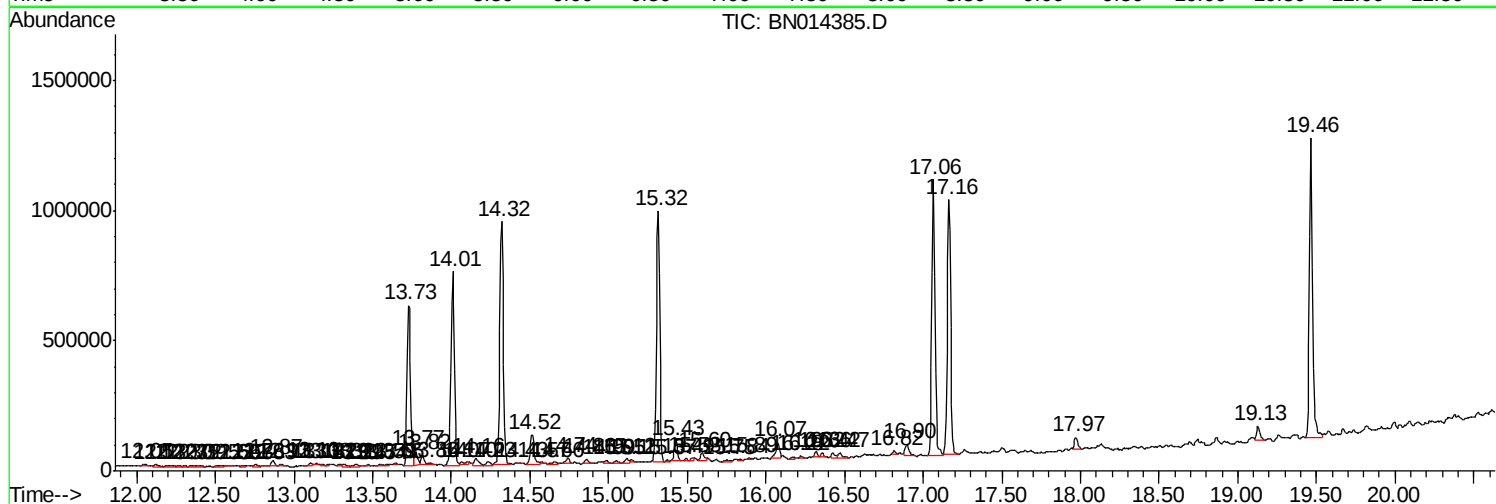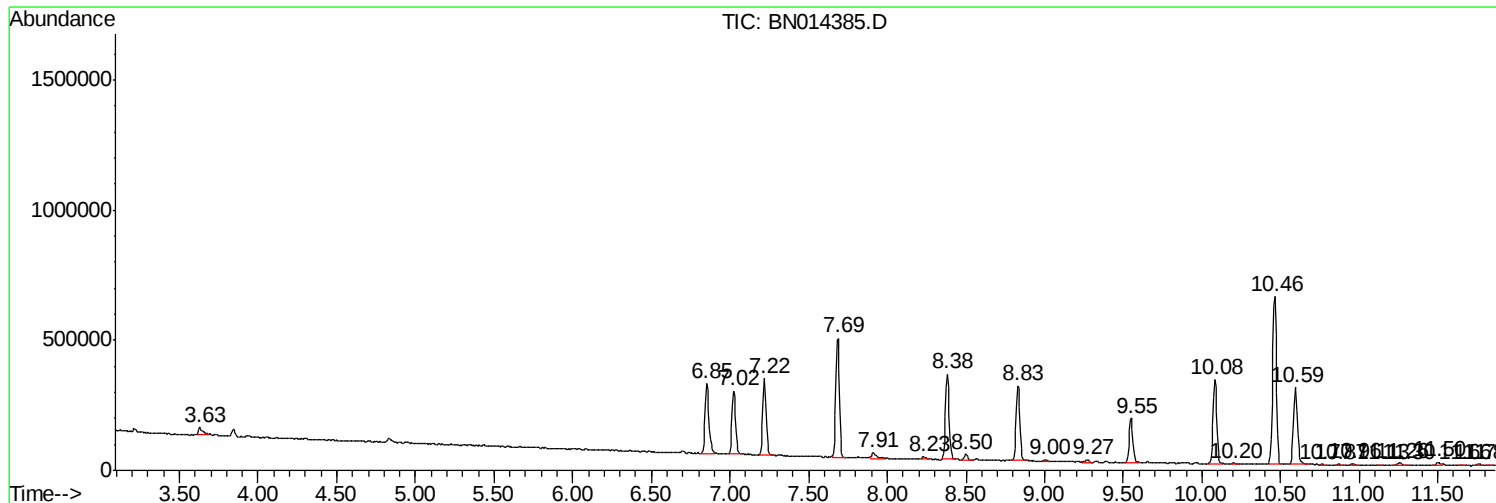

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
Data File : BN014385.D
Acq On : 23 Apr 2021 19:51
Operator : CG/JU
Sample : M2065-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG562

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
Data File : BN014385.D
Acq On : 23 Apr 2021 19:51
Operator : CG/JU
Sample : M2065-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG562

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc