

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042321\
 Data File : BN014390.D
 Acq On : 23 Apr 2021 22:49
 Operator : CG/JU
 Sample : M2065-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG566

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.622	89	91	98	rBV	53623	87806	3.76%	0.357%
2	6.852	635	640	655	rVB	280382	470040	20.11%	1.909%
3	7.022	664	669	679	rVB	243804	386712	16.55%	1.571%
4	7.216	697	702	713	rVB	302402	492786	21.09%	2.001%
5	7.687	775	782	790	rVB	584258	929066	39.76%	3.773%
6	8.381	894	900	908	rVB	358069	551951	23.62%	2.242%
7	8.499	917	920	927	rVB4	15454	26754	1.14%	0.109%
8	8.828	970	976	983	rBV	292368	486312	20.81%	1.975%
9	9.546	1093	1098	1107	rVB	185158	307623	13.16%	1.249%
10	10.081	1183	1189	1198	rBV	347588	555718	23.78%	2.257%
11	10.463	1246	1254	1266	rVB	814737	1376587	58.91%	5.591%
12	10.593	1270	1276	1284	rVB	337638	550898	23.57%	2.237%
13	12.051	1520	1524	1529	rVB3	5372	9090	0.39%	0.037%
14	12.922	1670	1672	1678	rVB3	3130	4181	0.18%	0.017%
15	13.151	1708	1711	1715	rVB3	4322	5812	0.25%	0.024%
16	13.222	1719	1723	1728	rVB2	14650	20171	0.86%	0.082%
17	13.728	1802	1809	1814	rVV	644589	904323	38.70%	3.673%
18	13.775	1814	1817	1823	rVB	122331	162729	6.96%	0.661%
19	14.010	1848	1857	1864	rBV	798657	1135252	48.58%	4.611%
20	14.210	1887	1891	1893	rBV3	4964	5275	0.23%	0.021%
21	14.234	1893	1895	1899	rVV3	3020	3103	0.13%	0.013%
22	14.322	1903	1910	1917	rBV	1249159	1800151	77.03%	7.311%
23	14.510	1937	1942	1950	rBV	149290	222992	9.54%	0.906%
24	14.740	1977	1981	1987	rVB3	17110	20673	0.88%	0.084%
25	15.145	2043	2050	2055	rBV2	7376	11399	0.49%	0.046%
26	15.316	2072	2079	2086	rBV	953529	1346488	57.62%	5.469%
27	15.428	2093	2098	2105	rVB	93697	127537	5.46%	0.518%
28	15.557	2117	2120	2124	rVB	6912	7608	0.33%	0.031%
29	15.863	2169	2172	2176	rBV4	1441	2610	0.11%	0.011%
30	16.039	2196	2202	2205	rBV2	2521	4561	0.20%	0.019%
31	16.104	2210	2213	2216	rVB2	2535	2731	0.12%	0.011%
32	16.216	2228	2232	2236	rVB3	1800	3135	0.13%	0.013%
33	16.316	2244	2249	2253	rBV4	5693	8384	0.36%	0.034%
34	16.828	2331	2336	2343	rBV4	9006	17699	0.76%	0.072%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
 Data File : BN014390.D
 Acq On : 23 Apr 2021 22:49
 Operator : CG/JU
 Sample : M2065-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG566

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

35	17.063	2370	2376	2384	rVV	1440780	2025781	86.69%	8.228%
36	17.163	2387	2393	2402	rVV	1067081	1464436	62.67%	5.948%
37	17.263	2405	2410	2414	rVB3	17267	21703	0.93%	0.088%
38	17.363	2423	2427	2432	rBV3	2939	4391	0.19%	0.018%
39	17.586	2460	2465	2466	rBV4	2161	2508	0.11%	0.010%
40	17.969	2526	2530	2536	rBV2	43094	58428	2.50%	0.237%
41	18.039	2540	2542	2549	rVB	4170	6911	0.30%	0.028%
42	18.275	2579	2582	2586	rBV3	3355	3999	0.17%	0.016%
43	18.475	2615	2616	2620	rVB4	2187	2481	0.11%	0.010%
44	18.539	2625	2627	2630	rVB2	2738	2611	0.11%	0.011%
45	18.910	2685	2690	2696	rBV7	3755	7248	0.31%	0.029%
46	19.098	2718	2722	2725	rBV	10969	14614	0.63%	0.059%
47	19.133	2725	2728	2731	rVB3	6401	8050	0.34%	0.033%
48	19.257	2745	2749	2754	rBV2	17422	24588	1.05%	0.100%
49	19.351	2762	2765	2769	rVB	8183	10542	0.45%	0.043%
50	19.463	2778	2784	2794	rBV2	1313339	1766866	75.61%	7.176%
51	20.028	2878	2880	2883	rBV3	4415	2958	0.13%	0.012%
52	20.527	2962	2965	2968	rBV5	8616	10516	0.45%	0.043%
53	20.986	3038	3043	3050	rBV3	56859	102510	4.39%	0.416%
54	21.186	3074	3077	3083	rBV	19476	27162	1.16%	0.110%
55	21.257	3084	3089	3096	rBV	1871296	2271745	97.22%	9.227%
56	21.427	3115	3118	3121	rBV	32486	36293	1.55%	0.147%
57	21.857	3188	3191	3197	rBV	56049	66563	2.85%	0.270%
58	22.316	3266	3269	3274	rVB2	76894	95331	4.08%	0.387%
59	22.821	3352	3355	3361	rVB2	98529	134067	5.74%	0.545%
60	23.339	3437	3443	3449	rBV	940364	1741096	74.51%	7.071%
61	23.486	3461	3468	3480	rVB2	1244512	2336802	100.00%	9.491%
62	24.027	3556	3560	3567	rVB2	87308	169069	7.24%	0.687%
63	24.774	3683	3687	3695	rVB3	73795	154468	6.61%	0.627%


Sum of corrected areas: 24621894

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042321\
Data File : BN014390.D
Acq On : 23 Apr 2021 22:49
Operator : CG/JU
Sample : M2065-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG566

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

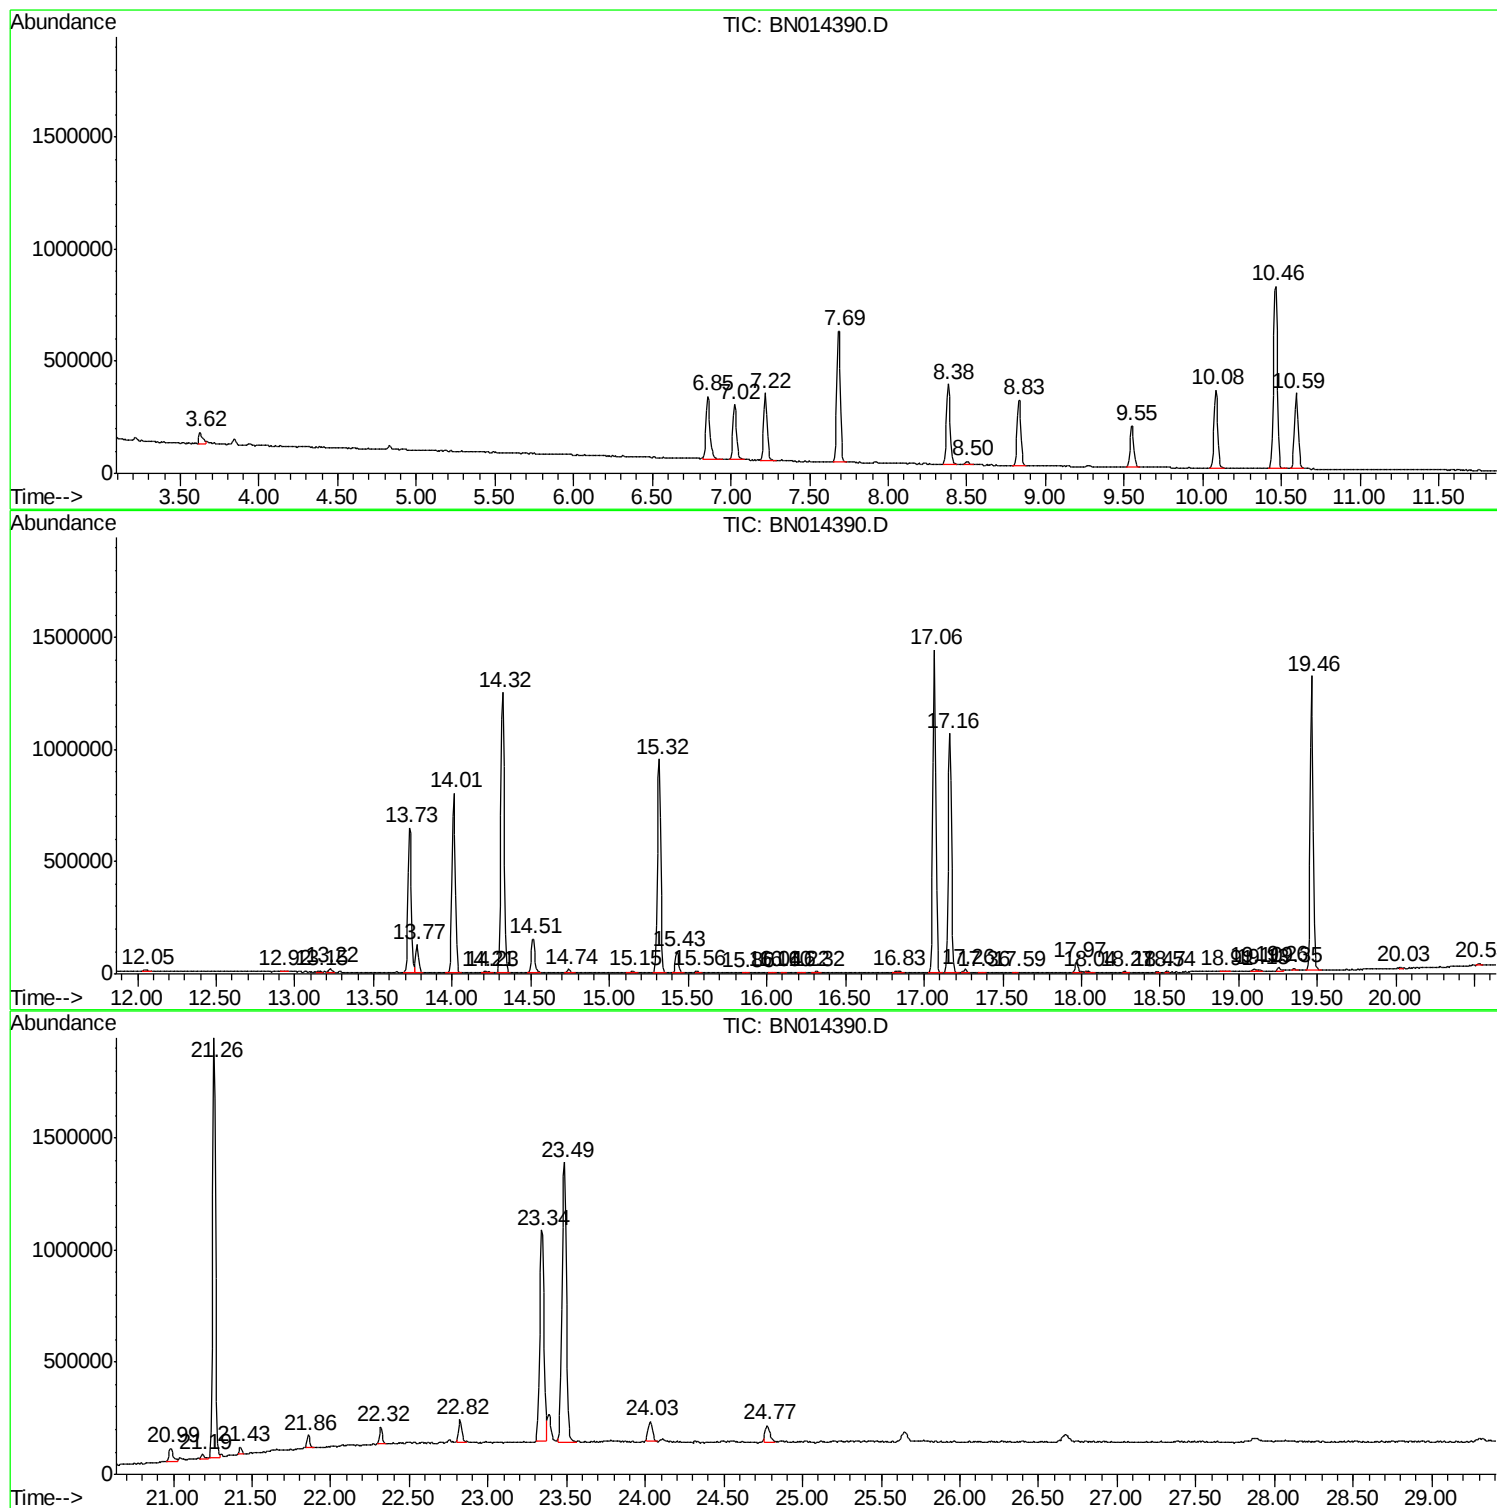

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
Data File : BN014390.D
Acq On : 23 Apr 2021 22:49
Operator : CG/JU
Sample : M2065-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG566

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042321\
Data File : BN014390.D
Acq On : 23 Apr 2021 22:49
Operator : CG/JU
Sample : M2065-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG566

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc
