

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042419\
 Data File : BN005251.D
 Acq On : 24 Apr 2019 15:15
 Operator : JU/SJ
 Sample : K2403-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5126

Quant Time: Apr 25 03:51:26 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 25 03:19:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	403350	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	1749538	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	1037177	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	2101310	20.00	ng/ul	0.00
77) Chrysene-d12	21.23	240	1431349	20.00	ng/ul	0.00
85) Perylene-d12	23.44	264	1525497	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	45951	5.50	ng/uL	0.00
5) Phenol-d5	6.78	99	1032889	32.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	619935	31.37	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	812375	33.51	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	858872	34.68	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	415804	38.61	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	464339	42.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	863211	34.50	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	1118089	43.33	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	2764091	36.71	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	3323263	35.94	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	387760	32.62	ng/ul	0.00
57) Fluorene-d10	15.23	176	2265661	35.86	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	219619	23.24	ng/ul	0.00
70) Anthracene-d10	17.08	188	3211918	36.46	ng/ul	0.00
78) Pyrene-d10	19.40	212	3023214	41.29	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.30	264	2522810	37.84	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.69	163	899564	11.991	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042419\
Data File : BN005251.D
Acq On : 24 Apr 2019 15:15
Operator : JU/SJ
Sample : K2403-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5126

Quant Time: Apr 25 03:51:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 25 03:19:34 2019
Response via : Initial Calibration

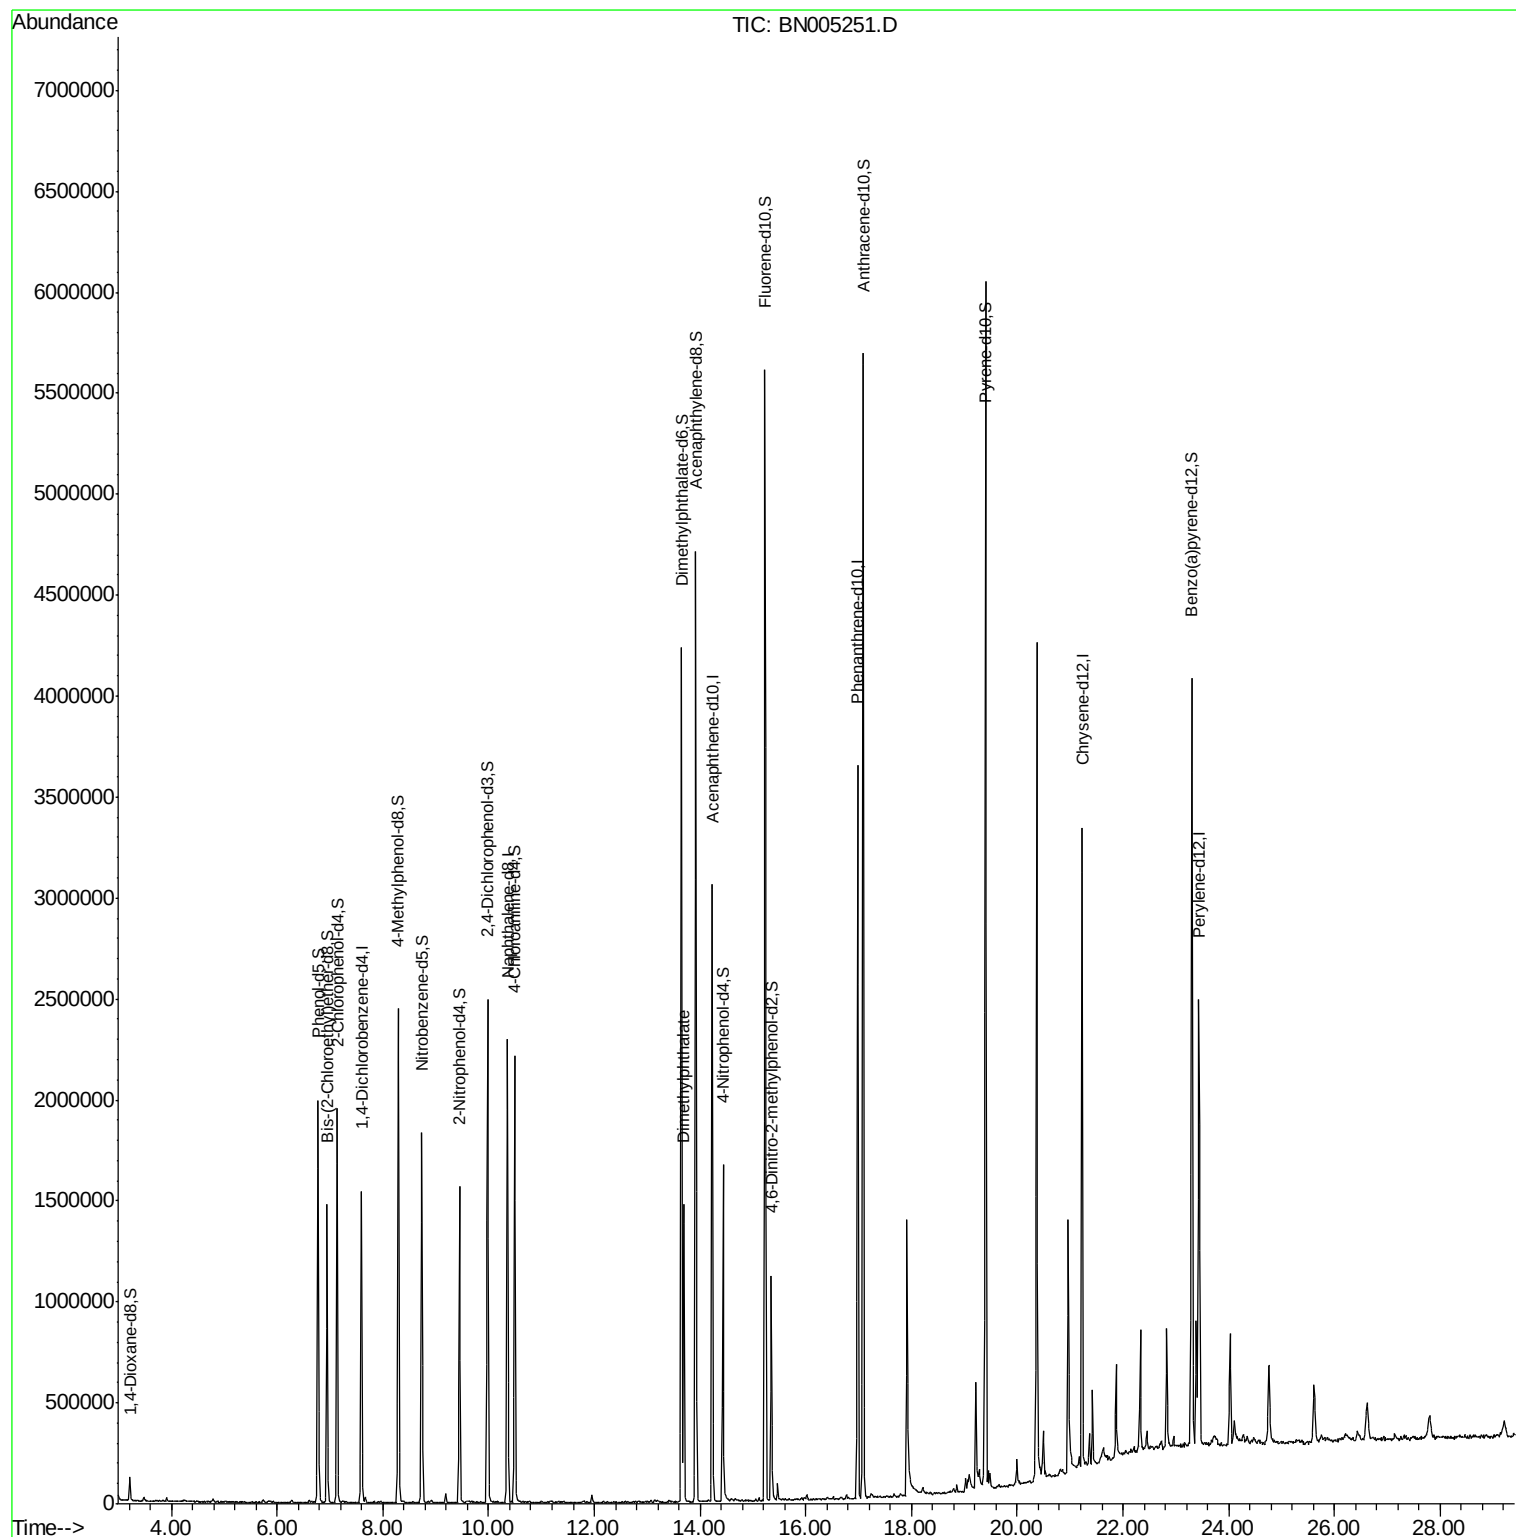

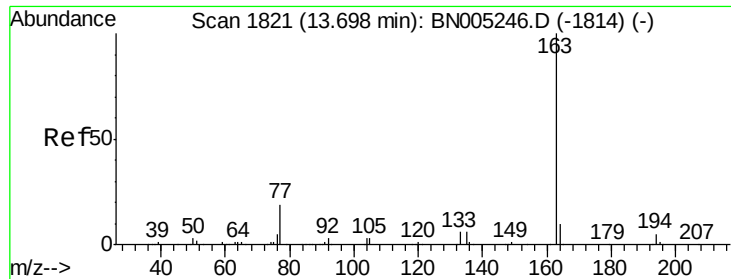

#44

Dimethylphthalate

Concen: 11.991 ng/ul

RT: 13.69 min Scan# 1820

Delta R.T. -0.01 min

Lab File: BN005251.D

Acq: 24 Apr 2019 15:15

Instrument :

BNA_N

ClientSampleId :

A5126


Tot Ion:163 Resp: 899564

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 9.9 8.1 12.1

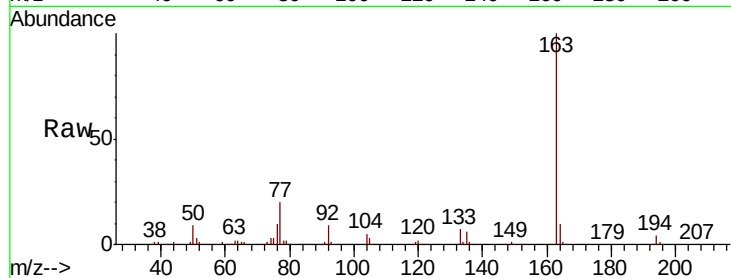

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

