

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042419\
 Data File : BN005252.D
 Acq On : 24 Apr 2019 15:49
 Operator : JU/SJ
 Sample : K2403-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5127

Quant Time: Apr 25 03:28:00 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 25 03:19:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	404649	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	1736876	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	1028639	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	2060899	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	1476142	20.00	ng/ul	0.00
85) Perylene-d12	23.43	264	1576858	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	58654	7.00	ng/uL	0.00
5) Phenol-d5	6.78	99	1251641	39.38	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	750356	37.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	983333	40.43	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	1033898	41.62	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	504953	47.24	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	568226	52.43	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	1042326	41.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	1424866	55.62	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	3300993	44.21	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	3994373	43.55	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	466568	39.57	ng/ul	0.00
57) Fluorene-d10	15.23	176	2681929	42.80	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	273461	29.50	ng/ul	0.00
70) Anthracene-d10	17.09	188	3758149	43.50	ng/ul	0.00
78) Pyrene-d10	19.40	212	3597008	47.63	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.30	264	3132622	45.46	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.70	163	1032596	13.878	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042419\
Data File : BN005252.D
Acq On : 24 Apr 2019 15:49
Operator : JU/SJ
Sample : K2403-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5127

Quant Time: Apr 25 03:28:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 25 03:19:34 2019
Response via : Initial Calibration

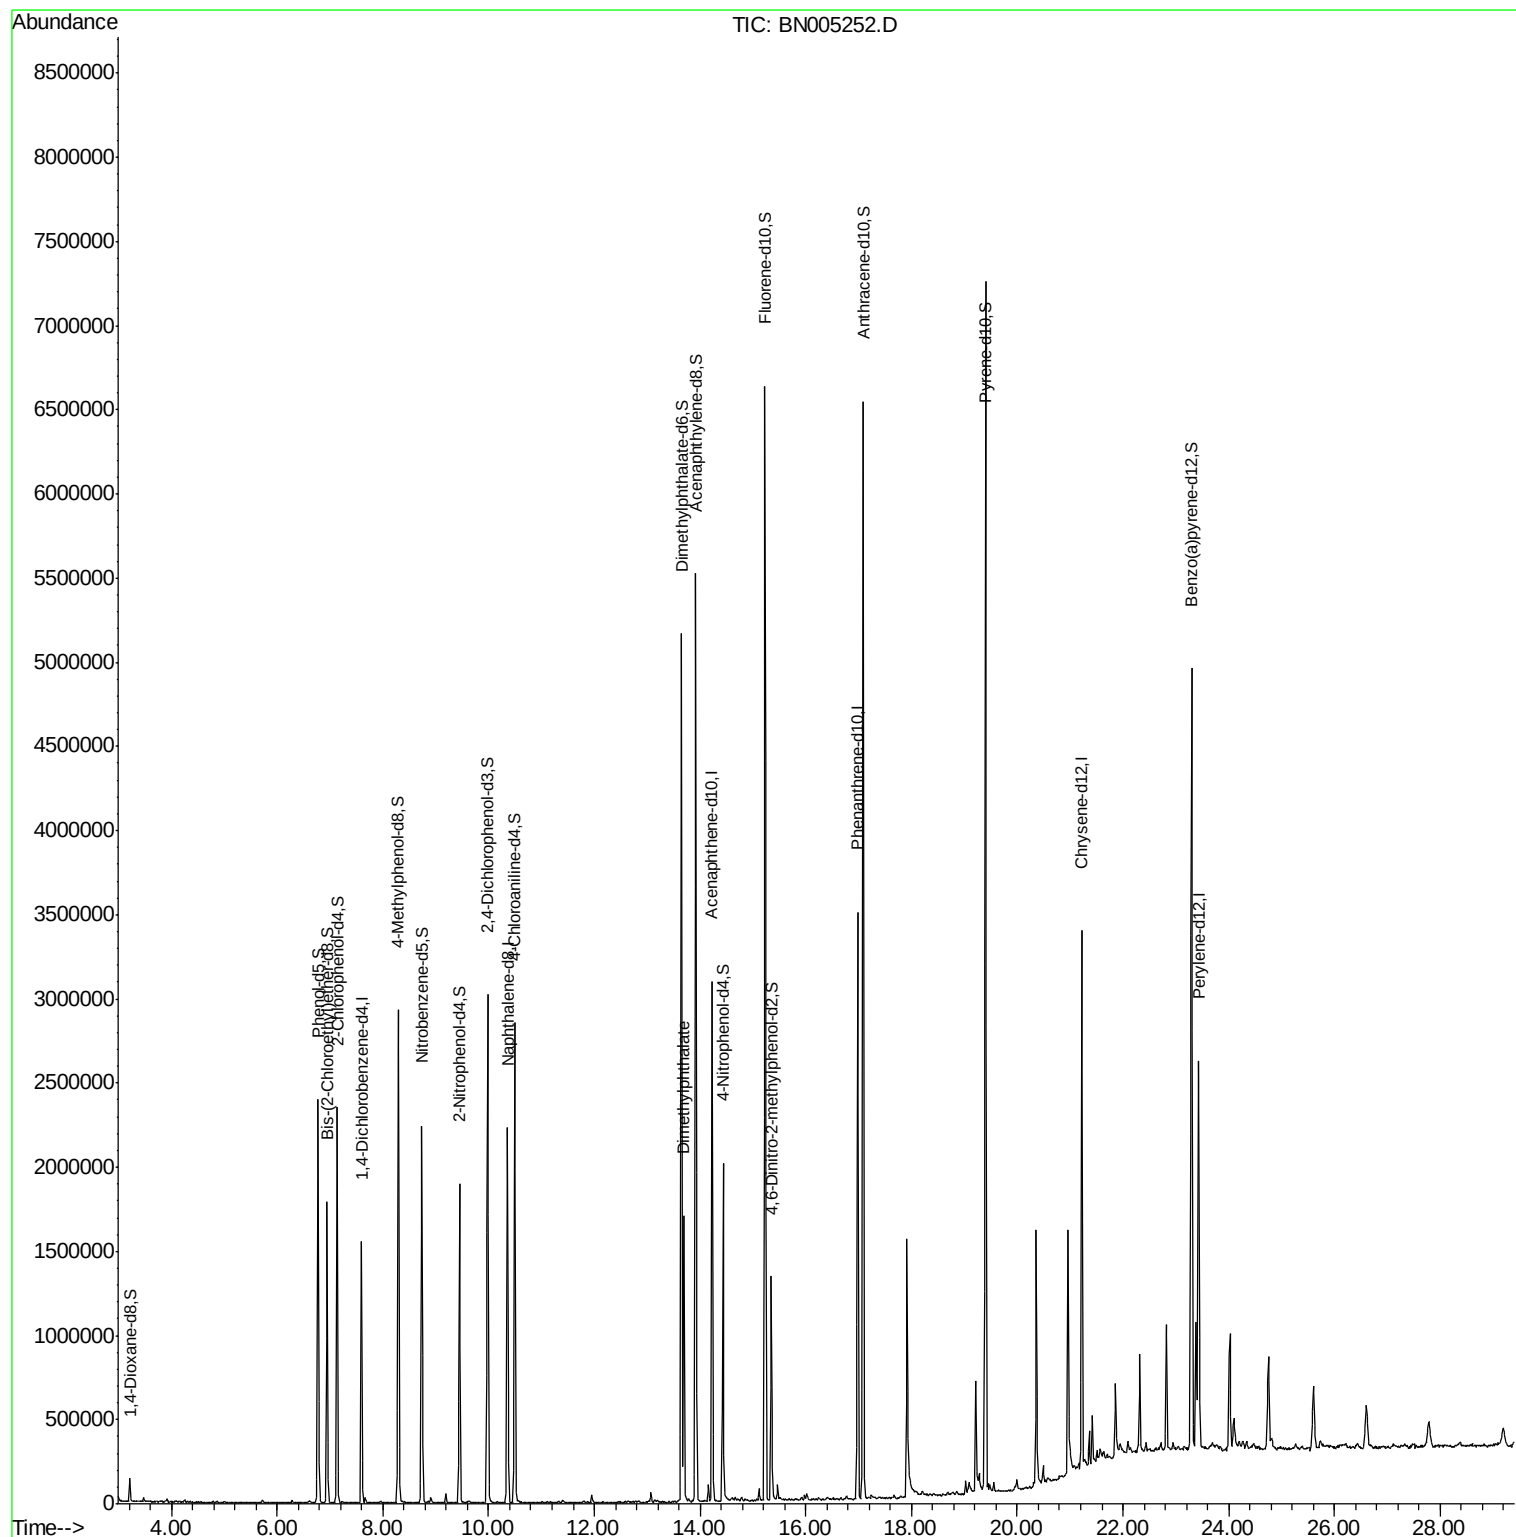


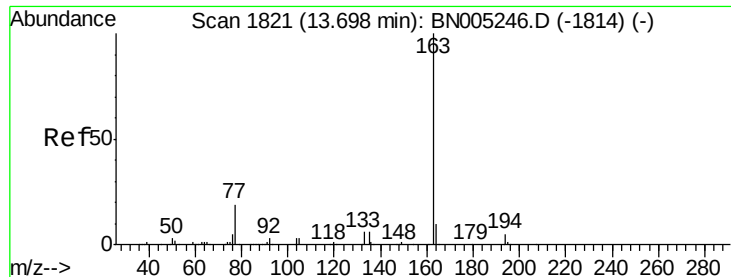

#44
 Dimethylphthalate
 Concen: 13.878 ng/ul
 RT: 13.70 min Scan# 1821
 Delta R.T. 0.00 min
 Lab File: BN005252.D
 Acq: 24 Apr 2019 15:49

Instrument :
 BNA_N
 ClientSampleId :
 A5127

Tot Ion:163 Resp: 1032596
 Ion Ratio Lower Upper
 163 100
 194 4.4 3.4 5.0
 164 9.9 8.1 12.1

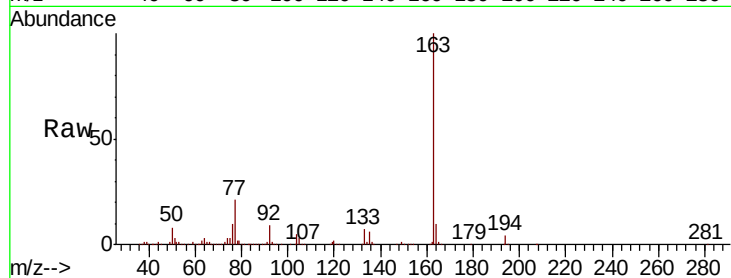

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

